
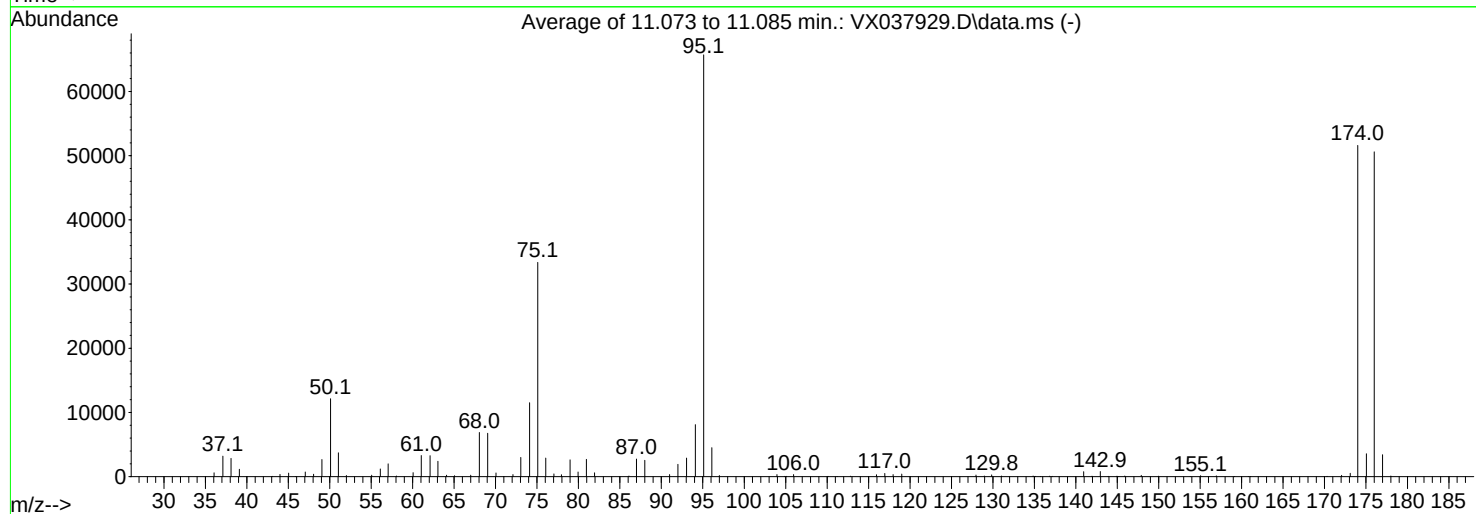


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092723\
Data File : VX037929.D
Acq On : 27 Sep 2023 17:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X092723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Sep 28 06:08:32 2023

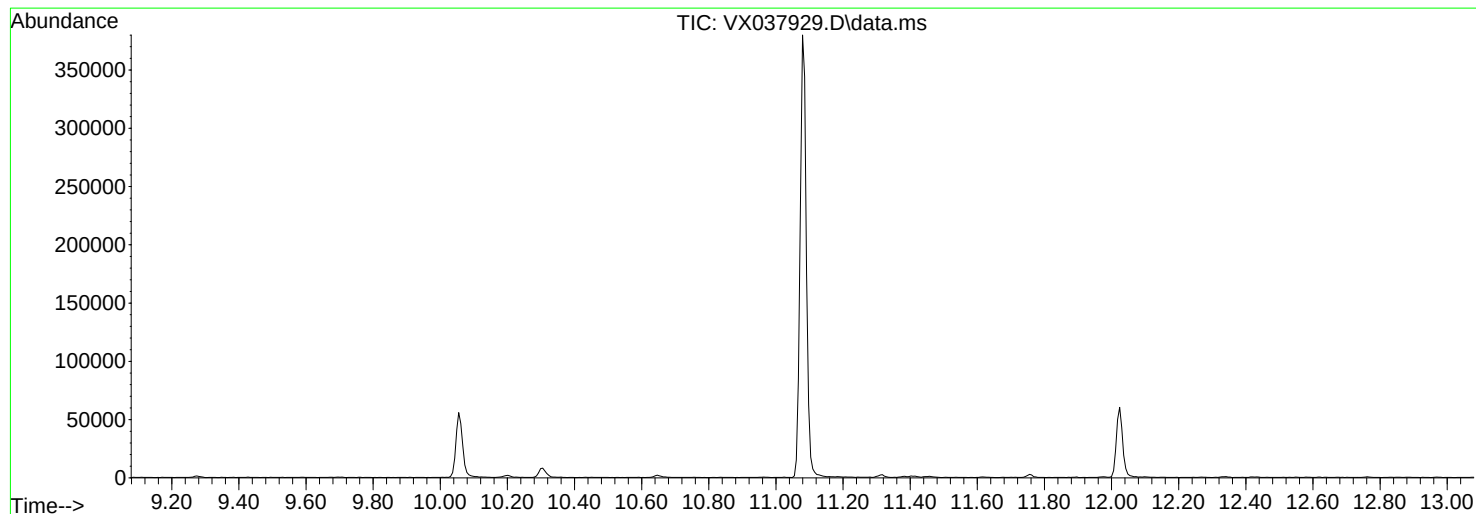

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	12138	PASS
75	95	30	60	50.8	33384	PASS
95	95	100	100	100.0	65704	PASS
96	95	5	9	6.9	4505	PASS
173	174	0.00	2	1.0	530	PASS
174	95	50	100	78.5	51597	PASS
175	174	5	9	6.9	3578	PASS
176	174	95	101	98.1	50600	PASS
177	176	5	9	6.8	3425	PASS