

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092818\
 Data File : VX004813.D
 Acq On : 28 Sep 2018 11:14
 Operator : JC/MD
 Sample : VX0928WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0928WBL01

Quant Time: Sep 29 06:35:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	236399	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	392183	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	391002	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	216005	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	186014	55.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.16%	
35) Dibromofluoromethane	5.50	113	155284	46.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.44%	
50) Toluene-d8	8.71	98	562335	50.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.78%	
62) 4-Bromofluorobenzene	11.14	95	203048	51.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.02%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092818\
Data File : VX004813.D
Acq On : 28 Sep 2018 11:14
Operator : JC/MD
Sample : VX0928WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0928WBL01

Quant Time: Sep 29 06:35:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 26 14:17:02 2018
Response via : Initial Calibration

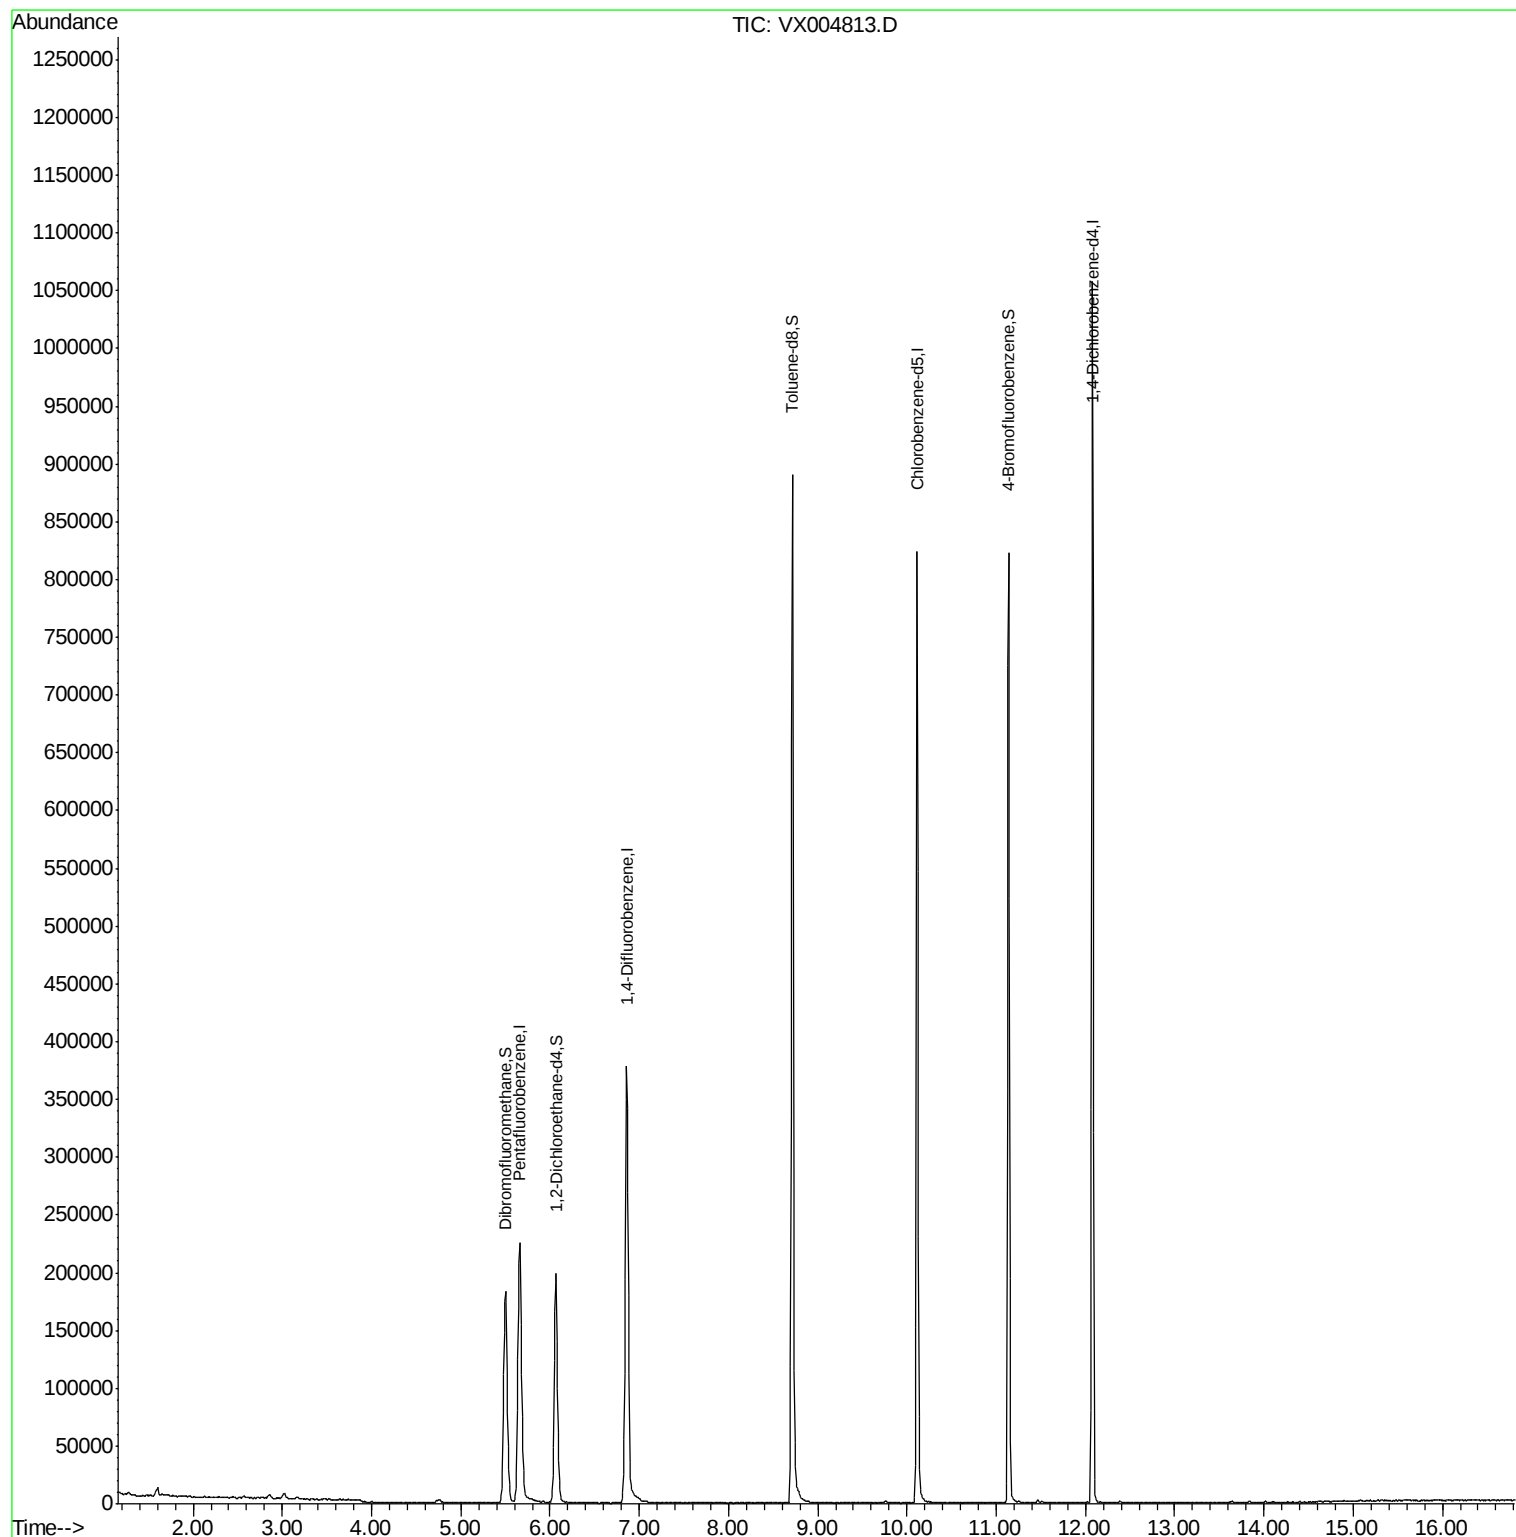

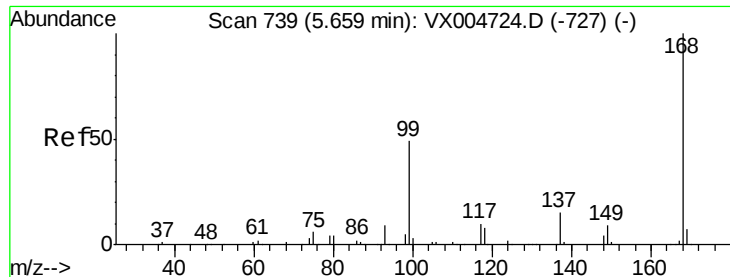

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX004813.D

Acq: 28 Sep 2018 11:14

Instrument :

MSVOA_X

ClientSampleId :


VX0928WBL01

Tot Ion:168 Resp: 236399

Ion Ratio Lower Upper




168 100

99 49.0 39.9 59.9

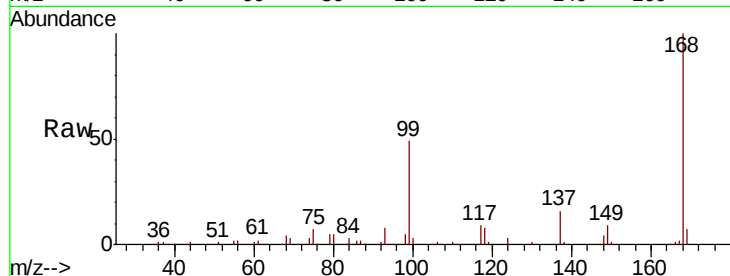

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

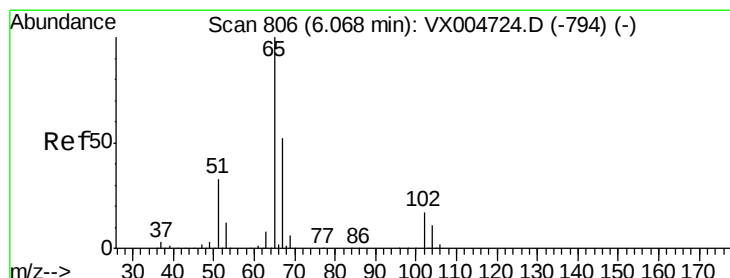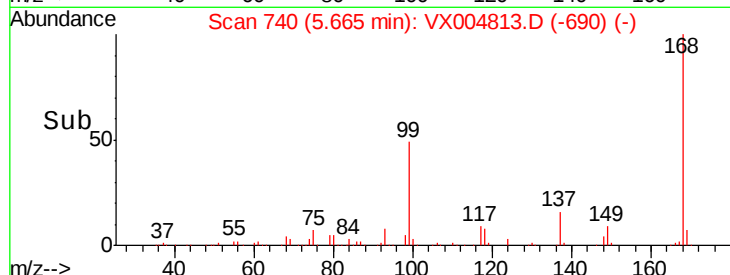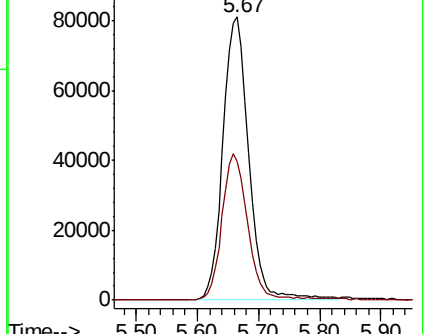

#33

1,2-Dichloroethane-d4

Concen: 55.083 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX004813.D


Acq: 28 Sep 2018 11:14

Tgt Ion: 65 Resp: 186014

Ion Ratio Lower Upper



65 100


67 53.7 0.0 106.8

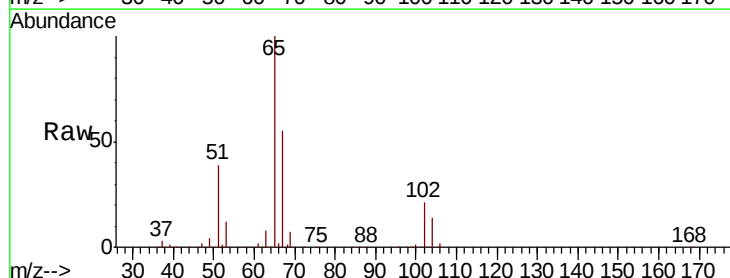

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0



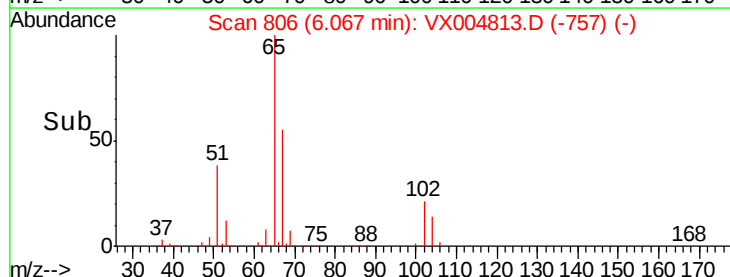
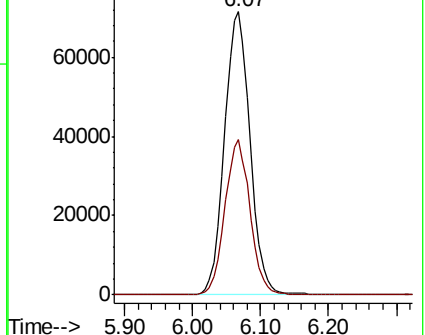


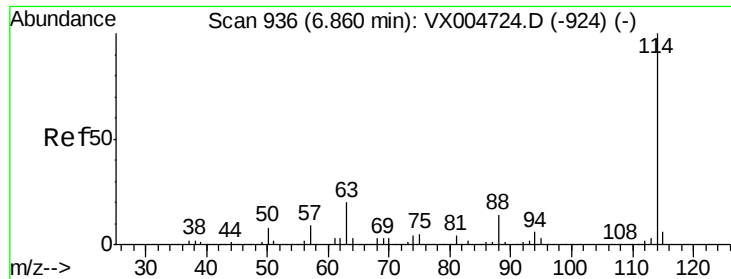

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX004813.D
 Acq: 28 Sep 2018 11:14




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0928WBL01


Tot Ion:114 Resp: 392183
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 39.0
 88 15.8 0.0 30.4

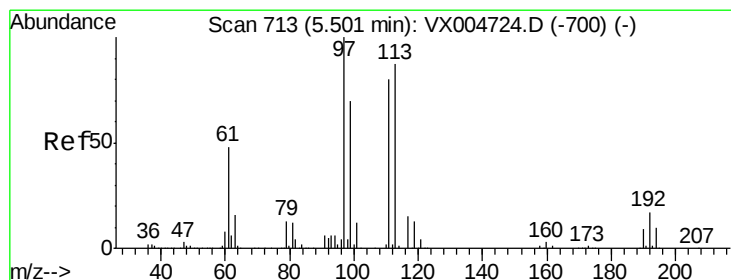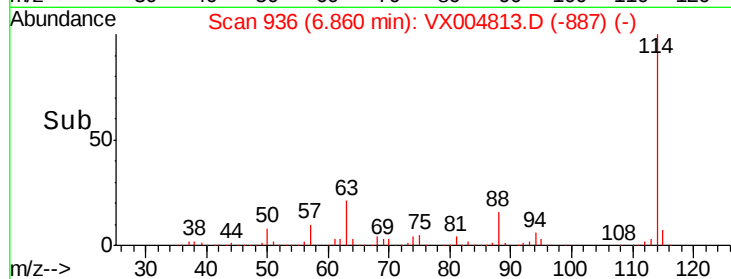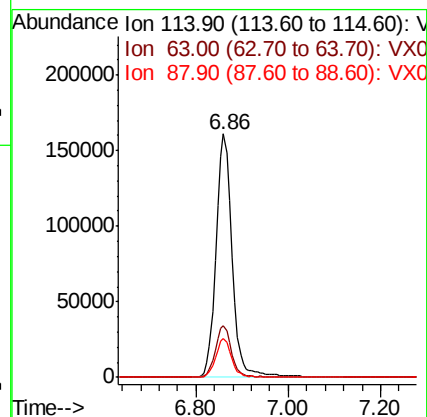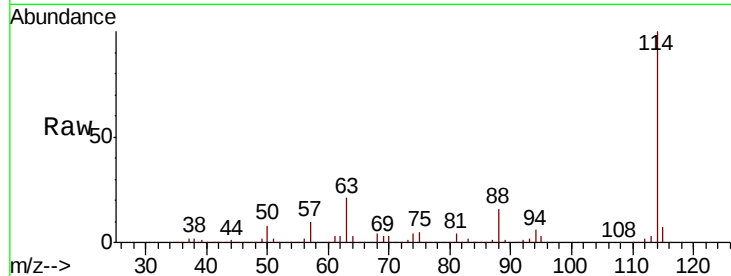

#35
 Dibromofluoromethane
 Concen: 46.719 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX004813.D
 Acq: 28 Sep 2018 11:14

Tgt Ion:113 Resp: 155284
 Ion Ratio Lower Upper
 113 100
 111 101.7 82.4 123.6
 192 22.9 19.4 29.2

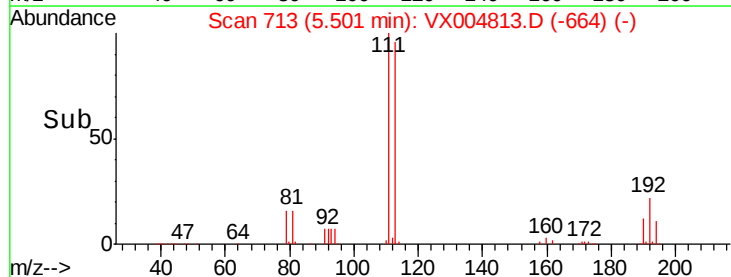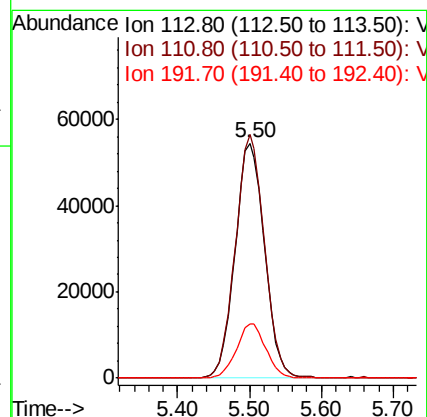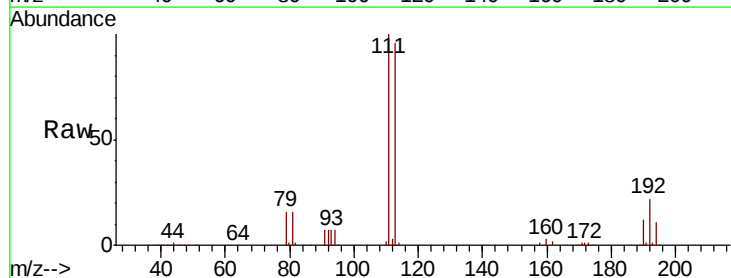

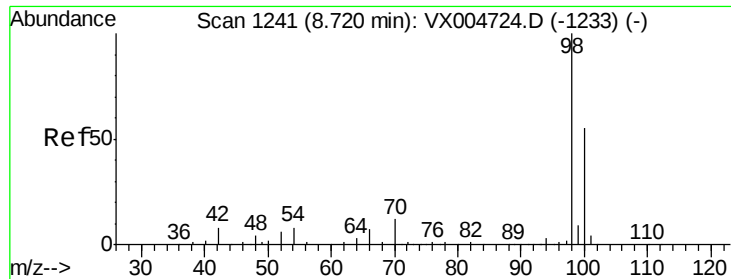

#50

Toluene-d8

Concen: 50.890 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.01 min

Lab File: VX004813.D

Acq: 28 Sep 2018 11:14

Instrument :

MSVOA_X

ClientSampleId :





VX0928WBL01

Tot Ion: 98 Resp: 562335

Ion Ratio Lower Upper

98 100

100 63.3 52.9 79.3

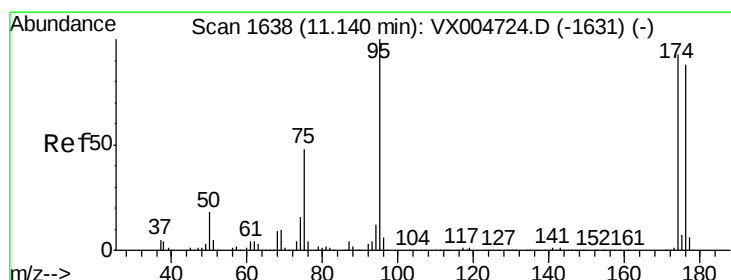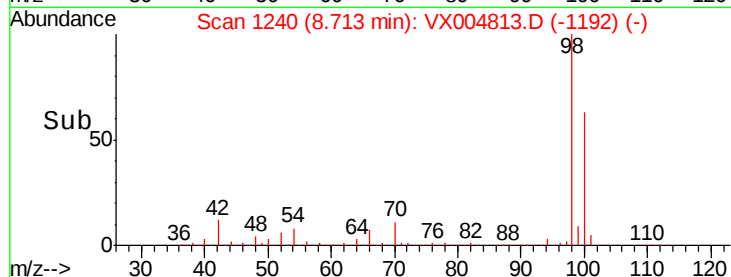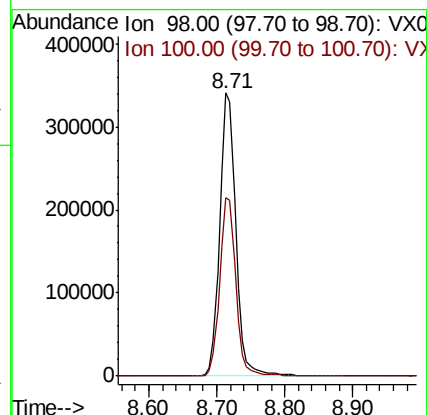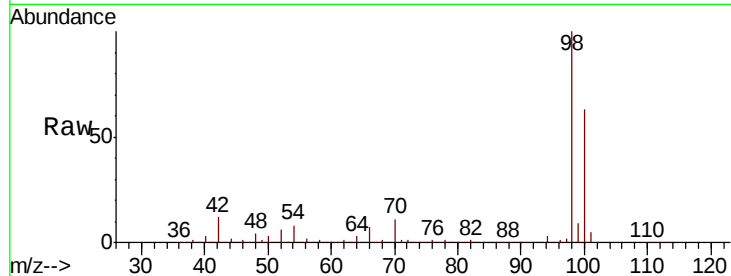

#62

4-Bromofluorobenzene

Concen: 51.007 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.00 min

Lab File: VX004813.D

Acq: 28 Sep 2018 11:14




Tgt Ion: 95 Resp: 203048


Ion Ratio Lower Upper

95 100

174 92.4 0.0 185.2

176 88.6 0.0 178.6

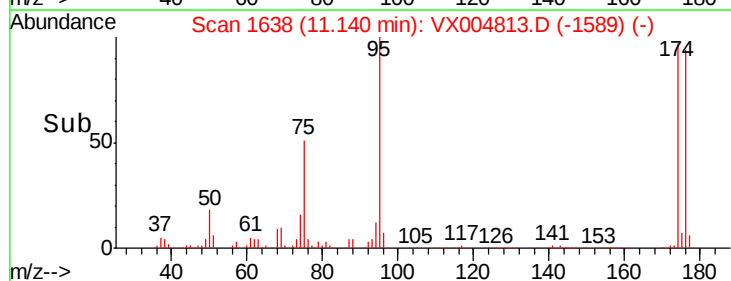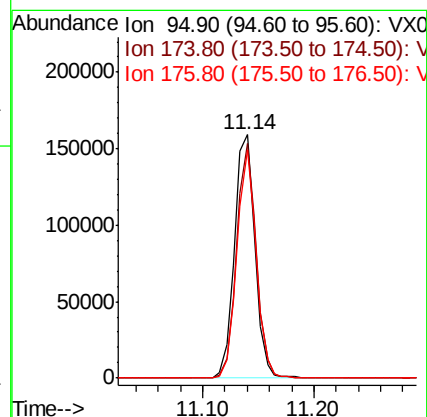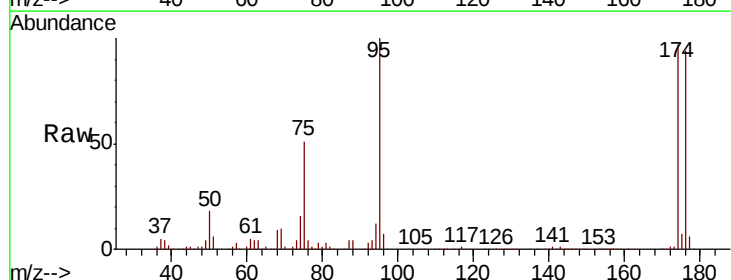


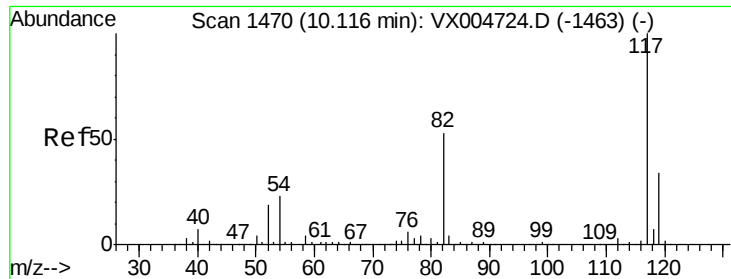




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX004813.D
Acq: 28 Sep 2018 11:14

Instrument :
MSVOA_X
ClientSampleId :
VX0928WBL01

Tot Ion:117 Resp: 391002
Ion Ratio Lower Upper
117 100
82 54.0 47.8 71.6
119 31.6 29.3 43.9

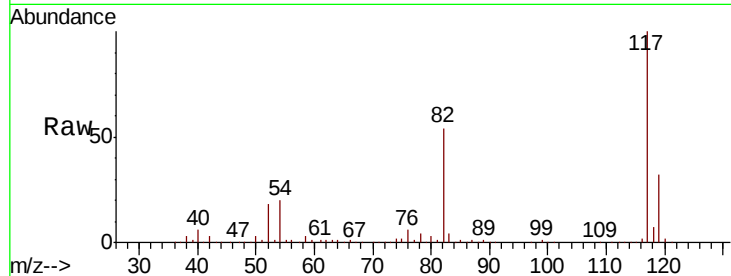


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

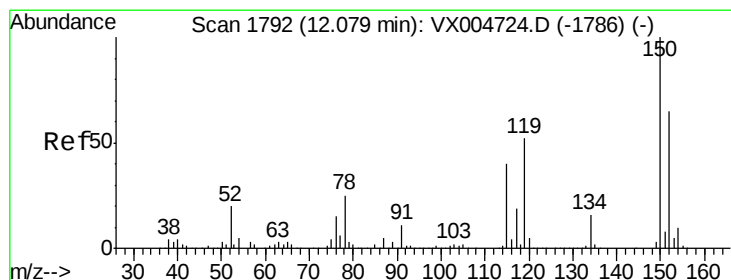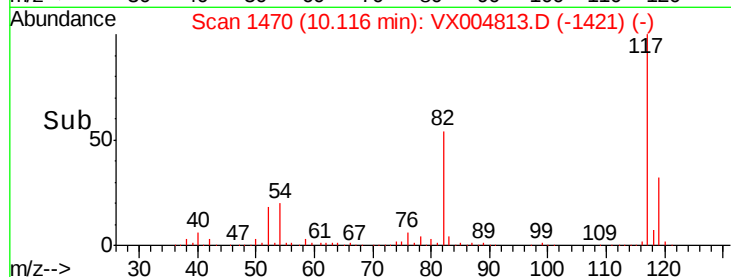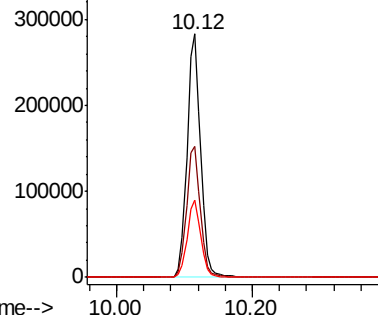

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX004813.D
Acq: 28 Sep 2018 11:14

Tgt Ion:152 Resp: 216005
Ion Ratio Lower Upper
152 100
115 55.1 39.0 117.0
150 156.4 0.0 351.0

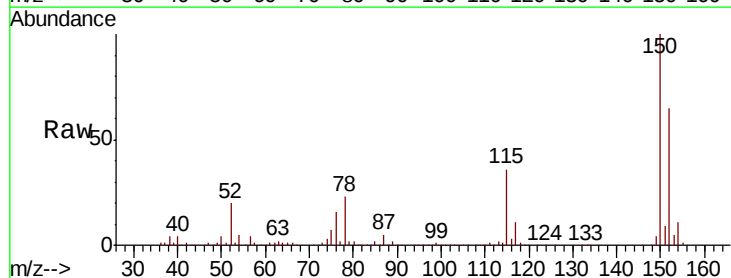

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

