


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092818\
Data File : VX004811.D
Acq On : 28 Sep 2018 09:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Title : VOC Analysis
Last Update : Mon Oct 01 05:52:45 2018

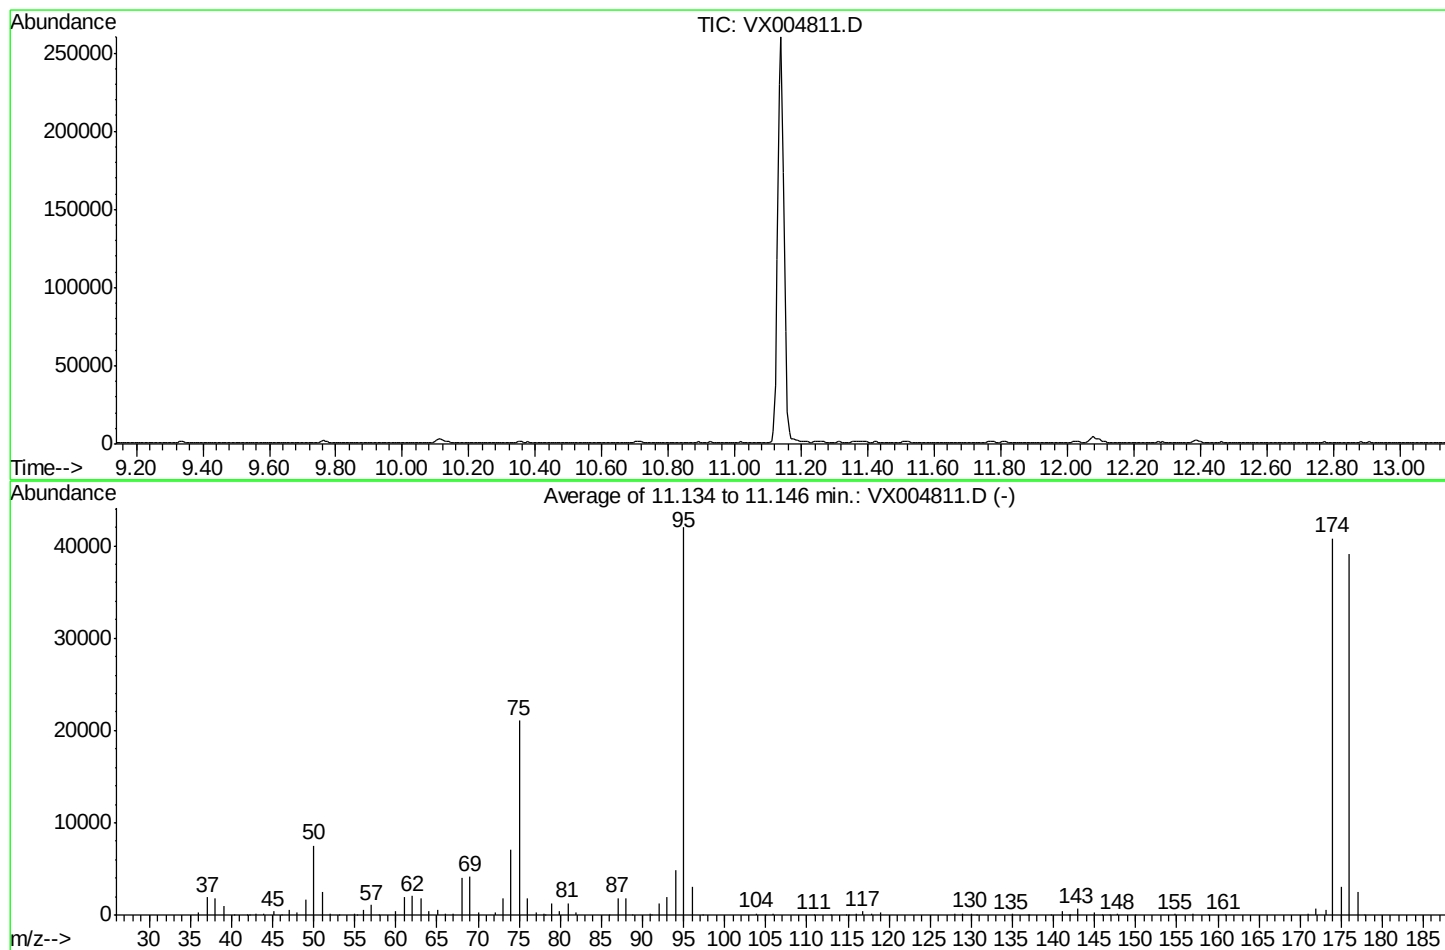

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7517	PASS
75	95	30	80	50.2	21079	PASS
95	95	100	100	100.0	42002	PASS
96	95	5	9	7.1	2998	PASS
173	174	0.00	2	1.3	523	PASS
174	95	50	120	97.2	40805	PASS
175	174	5	9	7.6	3100	PASS
176	174	95	101	95.9	39120	PASS
177	176	5	9	6.5	2542	PASS