


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092818\
Data File : VX004835.D
Acq On : 28 Sep 2018 21:26
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Title : VOC Analysis
Last Update : Mon Oct 01 05:52:45 2018

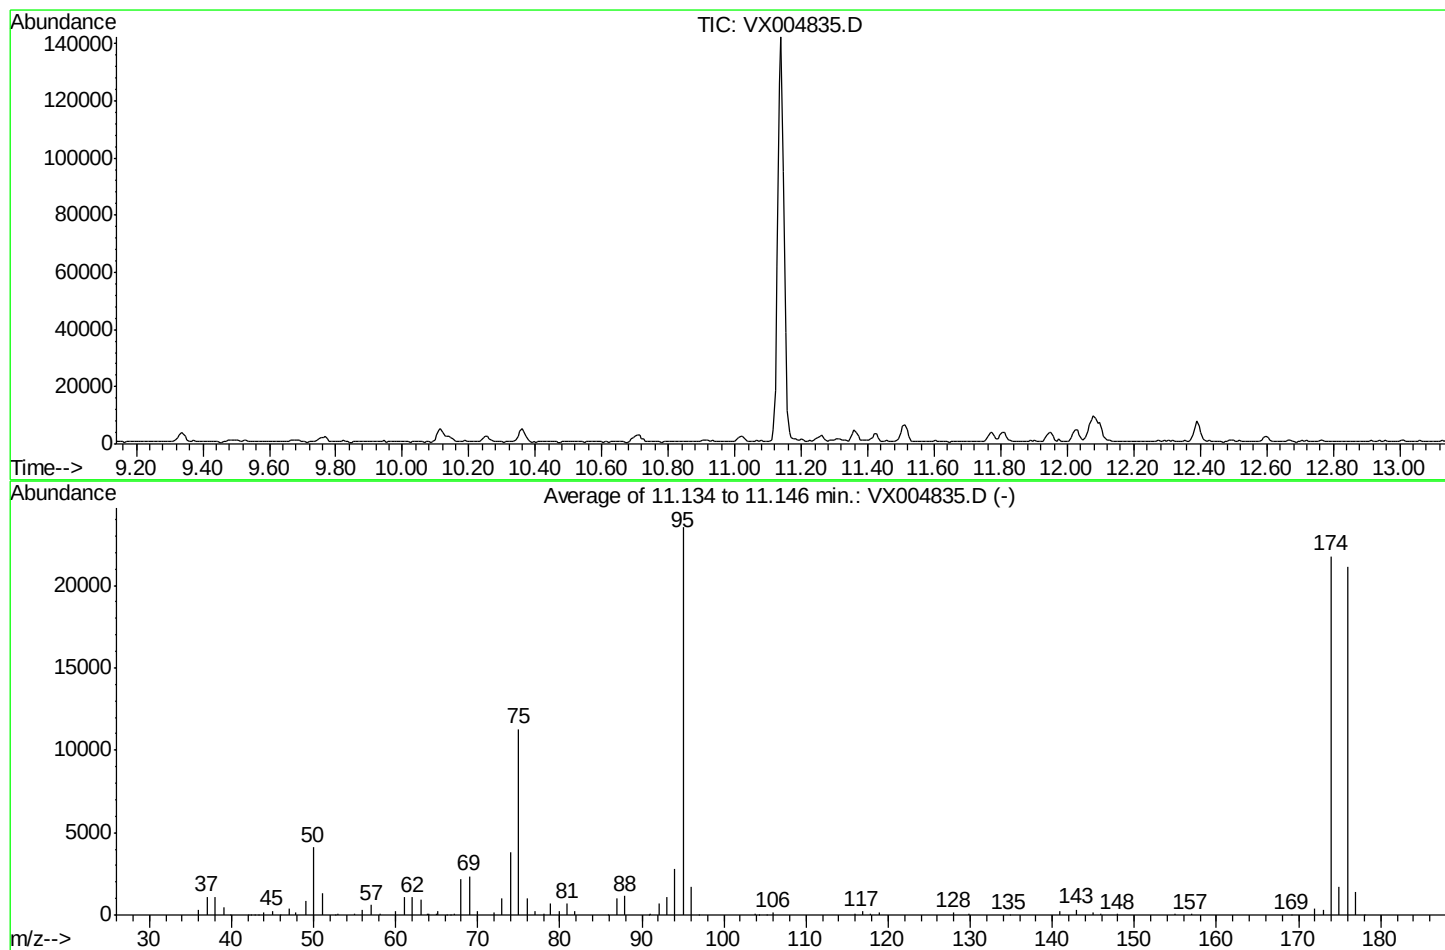

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4109	PASS
75	95	30	80	47.9	11273	PASS
95	95	100	100	100.0	23528	PASS
96	95	5	9	7.2	1686	PASS
173	174	0.00	2	1.3	292	PASS
174	95	50	120	92.5	21760	PASS
175	174	5	9	7.7	1674	PASS
176	174	95	101	97.3	21162	PASS
177	176	5	9	6.5	1384	PASS