
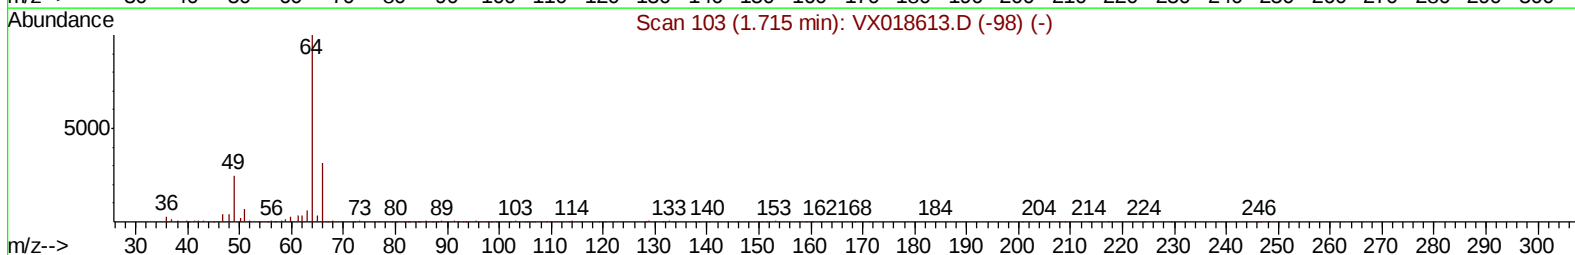
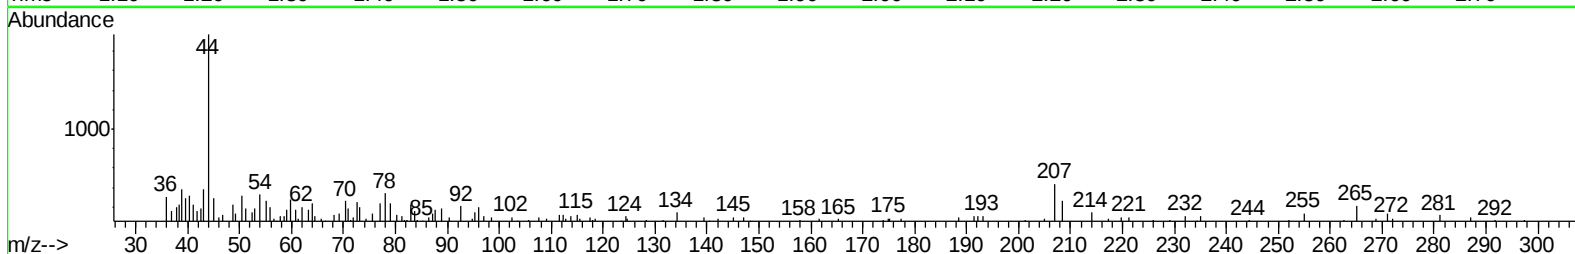


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092820\  
Data File : VX018617.D  
Acq On : 28 Sep 2020 13:28  
Operator : JC/SP  
Sample : VSTD0.563  
Misc : 25.0mL/MSVOA X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Sep 29 00:17:32 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\SOMXTR092820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Sep 29 00:09:07 2020  
Response via : Initial Calibration

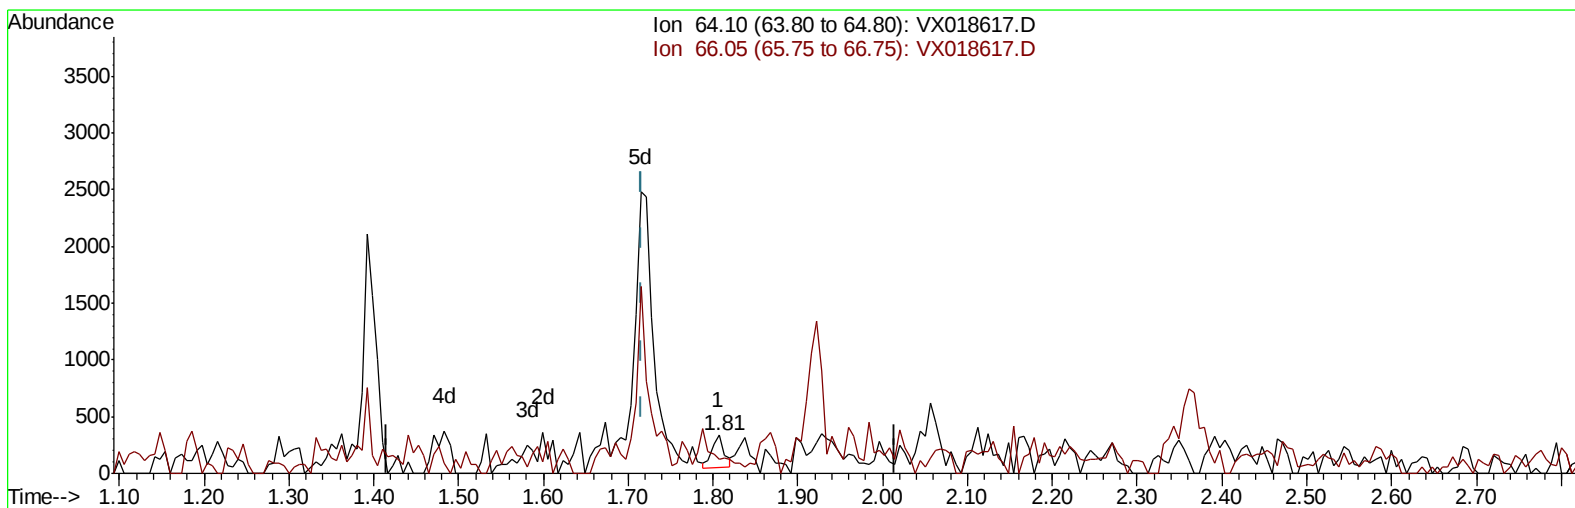

TIC: VX018617.D

(8) Chloroethane (T)

1.807min (+0.091) 0.04ug/L

response 270

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 64.10 | 100   | 100   |
| 66.05 | 31.80 | 38.32 |
| 0.00  | 0.00  | 0.00  |
| 0.00  | 0.00  | 0.00  |