
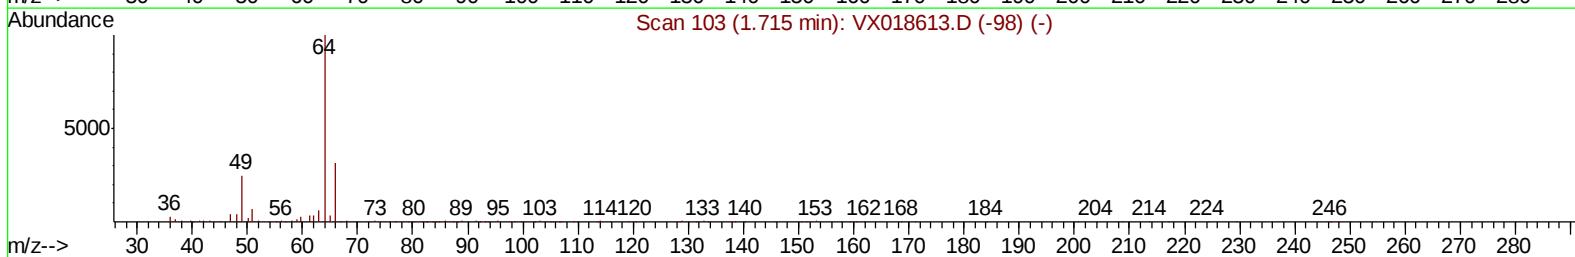
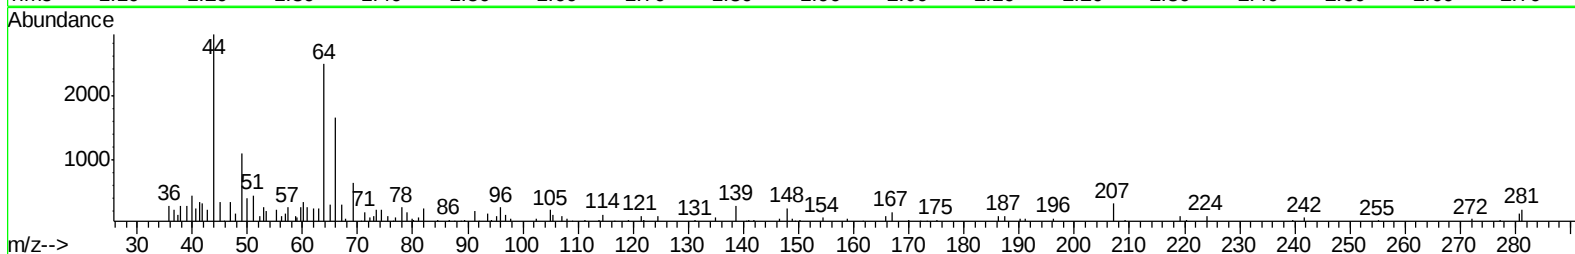


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092820\
Data File : VX018617.D
Acq On : 28 Sep 2020 13:28
Operator : JC/SP
Sample : VSTD0.563
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Sep 29 00:17:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 29 00:09:07 2020
Response via : Initial Calibration

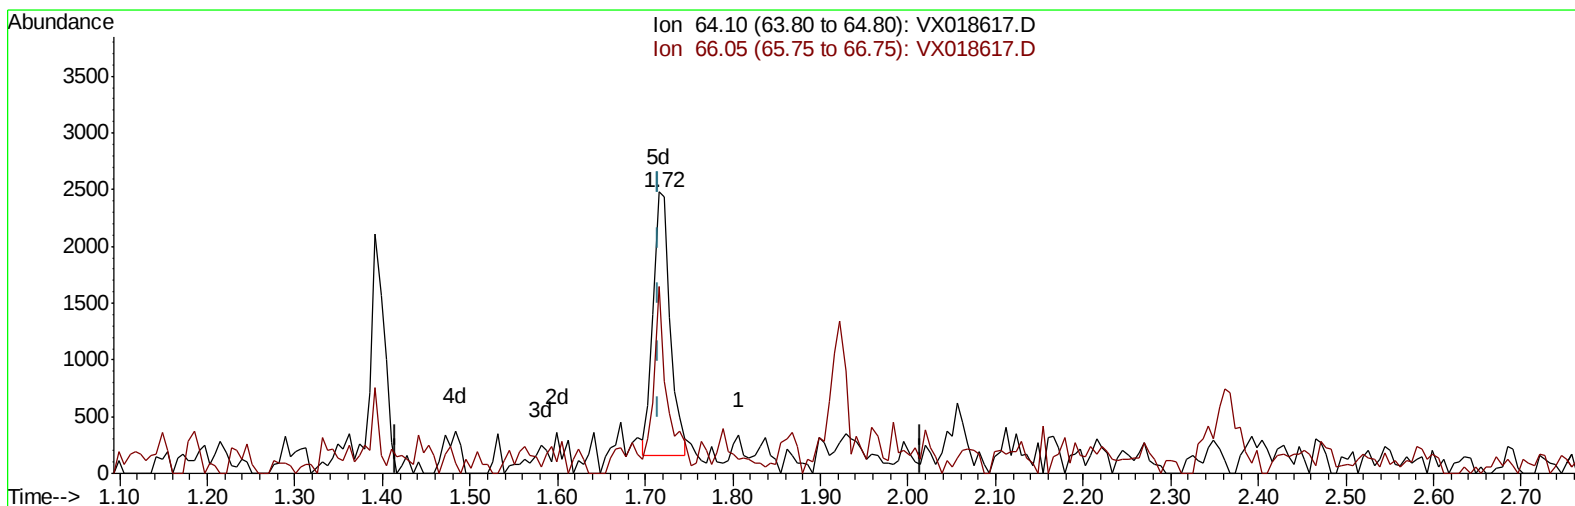

TIC: VX018617.D

(8) Chloroethane (T)

1.715min (-0.000) 0.41ug/L m

response 3124

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	66.30#
0.00	0.00	0.00
0.00	0.00	0.00