
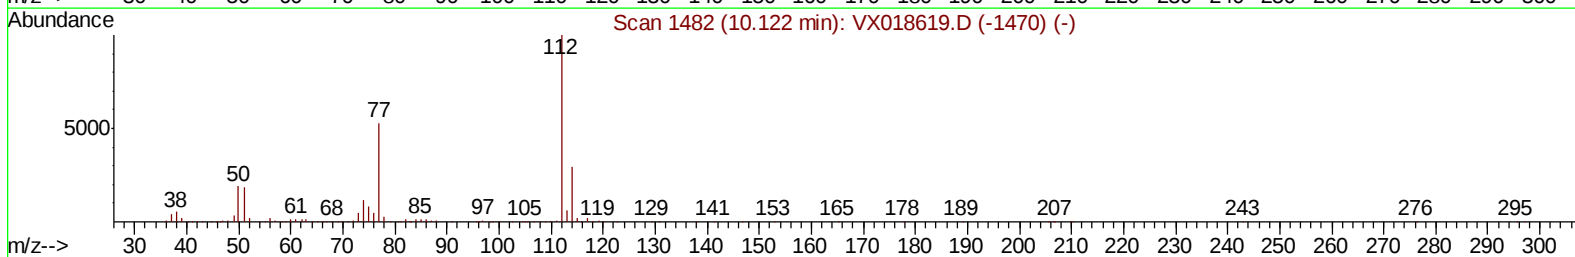
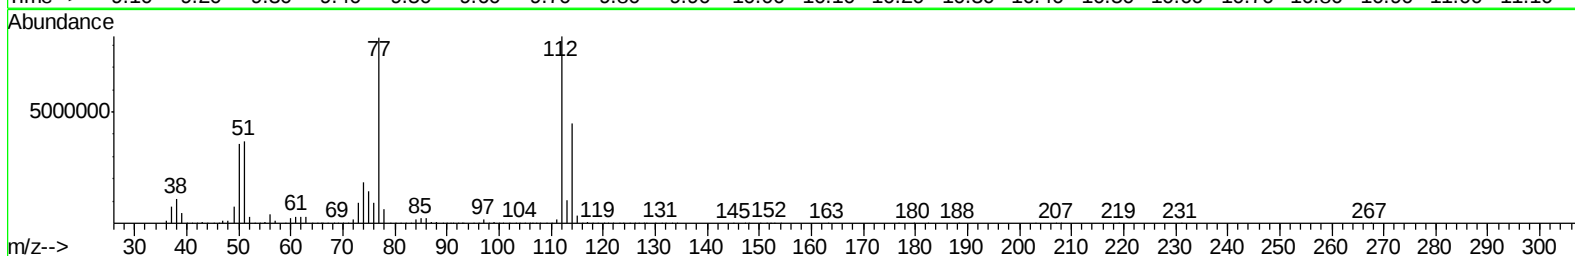


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092820\
 Data File : VX018621.D
 Acd On : 28 Sep 2020 17:42
 Operator : JC/SP
 Sample : L4135-01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 29 02:38:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 29 02:30:52 2020
 Response via : Initial Calibration

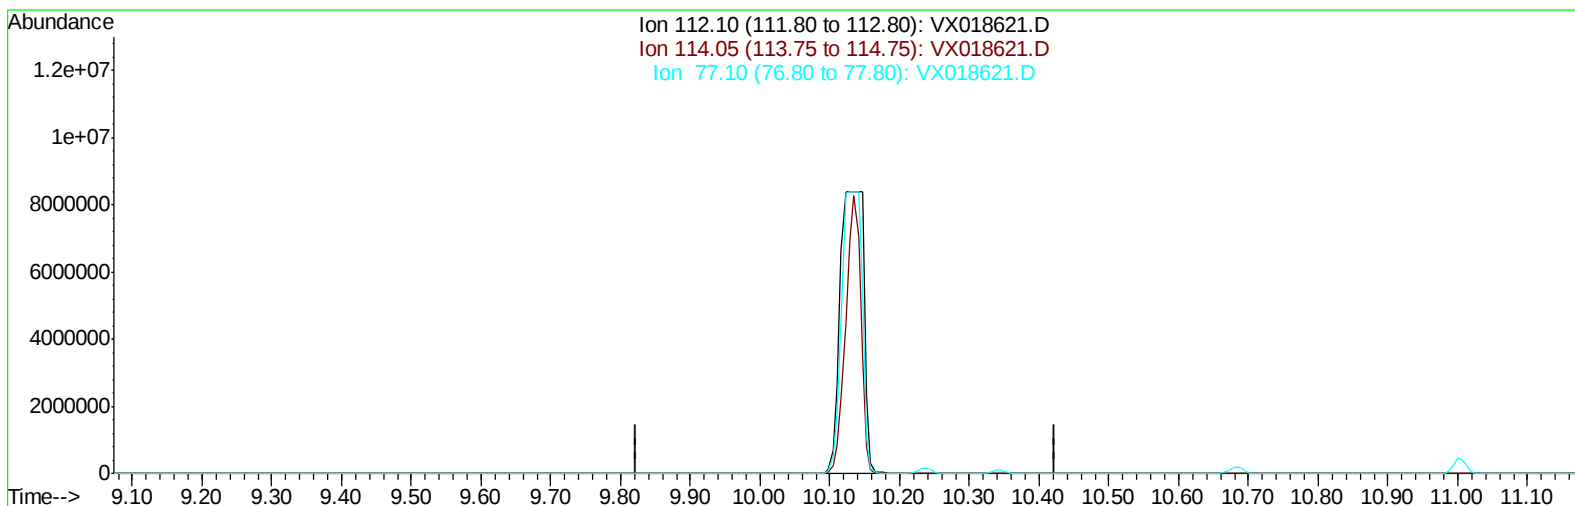

TIC: VX018621.D

(53) Chlorobenzene (T)

10.122min (-10.122) 0.00ug/L

response 0

Ion	Exp%	Act%
112.10	100	0.00
114.05	29.50	0.00#
77.10	58.20	0.00#
0.00	0.00	0.00