
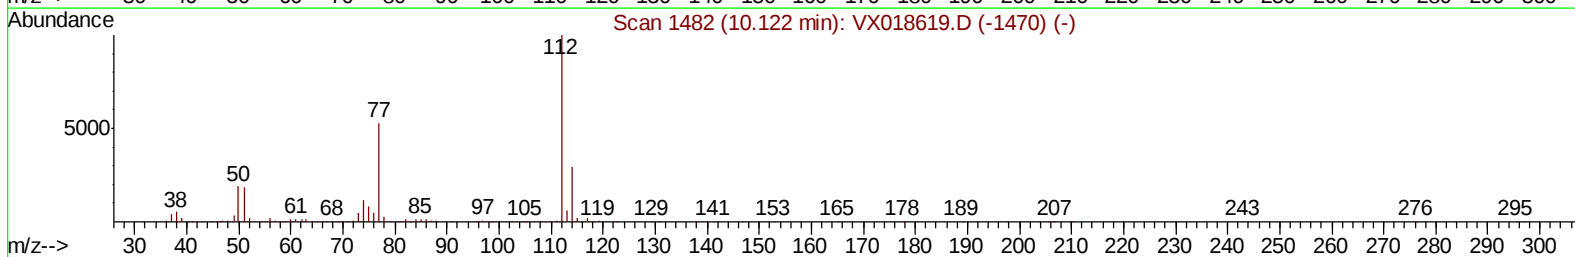
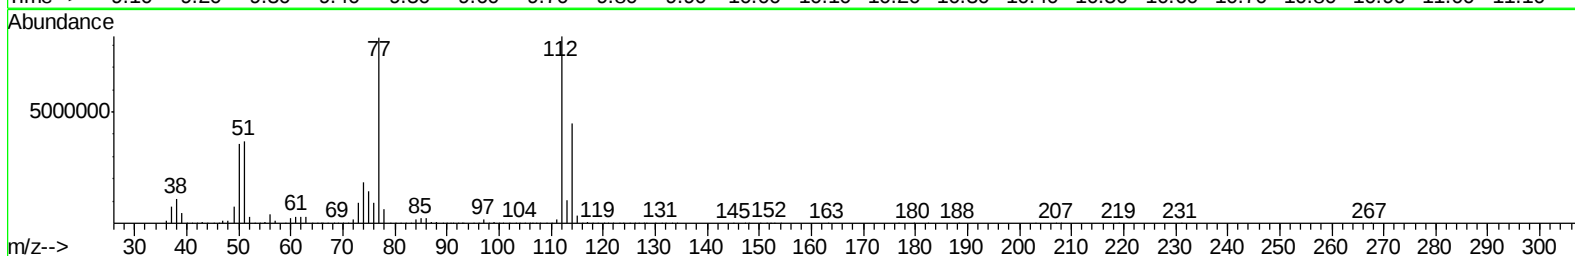


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092820\
Data File : VX018621.D
Acq On : 28 Sep 2020 17:42
Operator : JC/SP
Sample : L4135-01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 29 02:38:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 29 02:30:52 2020
Response via : Initial Calibration

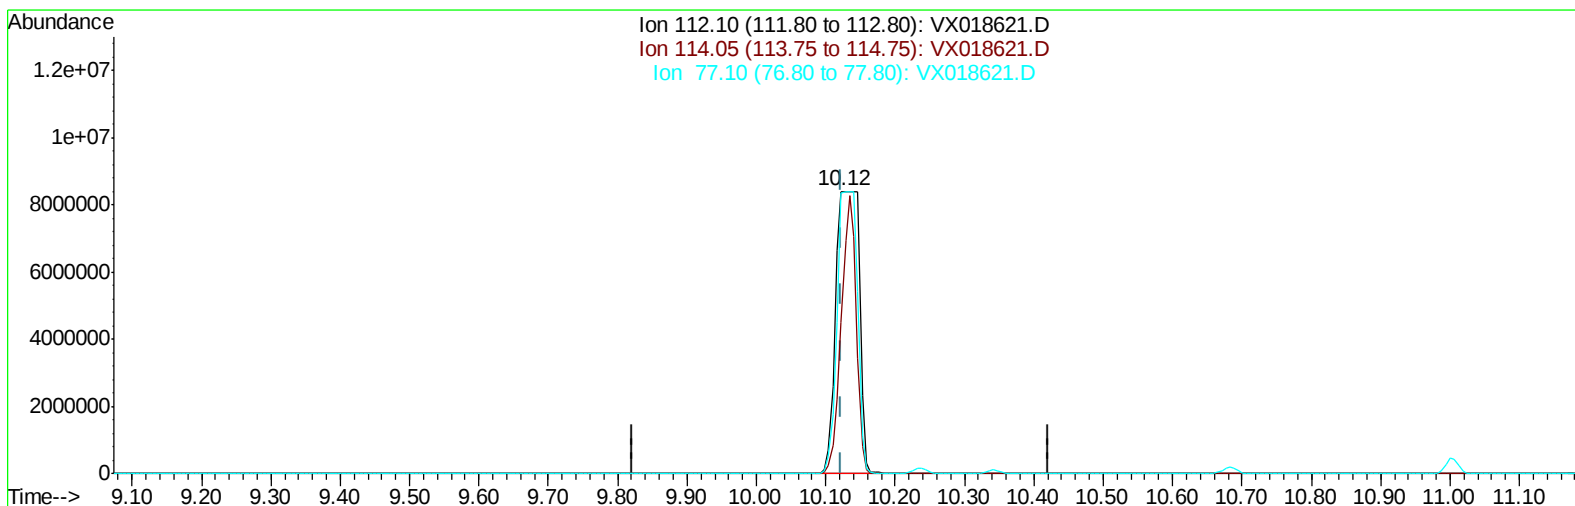

TIC: VX018621.D

(53) Chlorobenzene (T)

10.122min (0.000) 536.48ug/L m

response 20019967

Ion	Exp%	Act%
112.10	100	100
114.05	29.50	53.46#
77.10	58.20	99.41#
0.00	0.00	0.00