
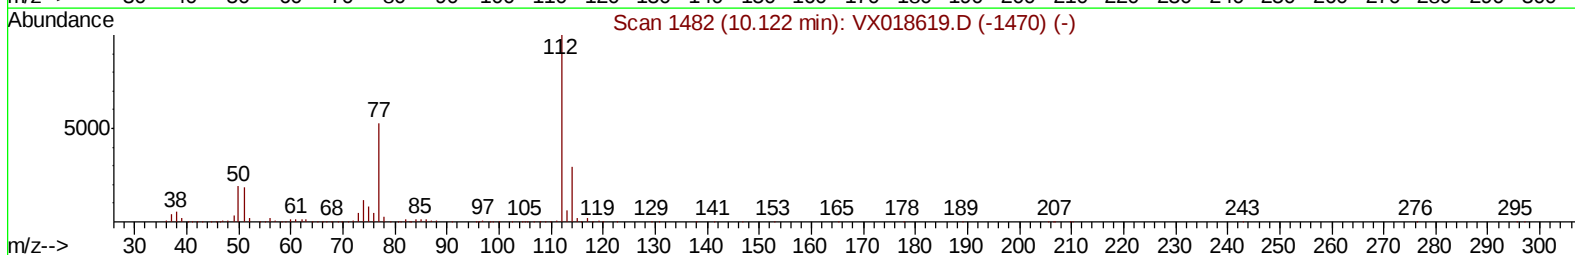
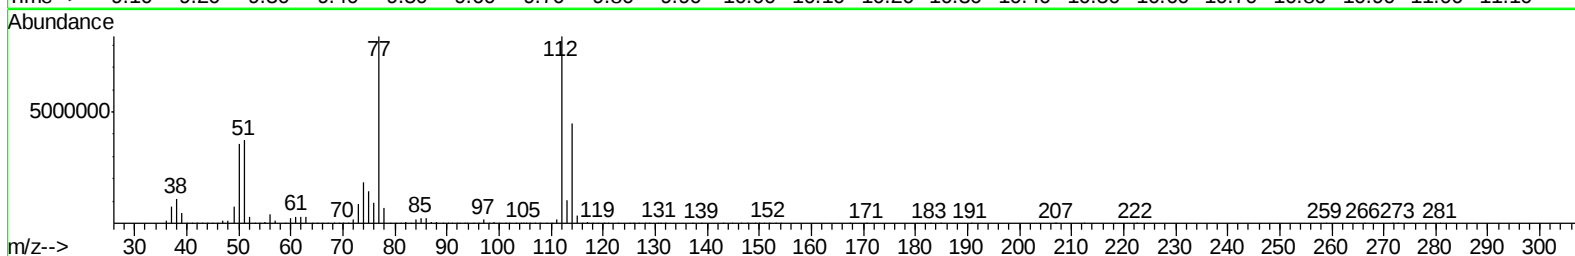


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092820\
 Data File : VX018627.D
 Acq On : 28 Sep 2020 20:07
 Operator : JC/SP
 Sample : L4135-07
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 29 02:39:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 29 02:30:52 2020
 Response via : Initial Calibration

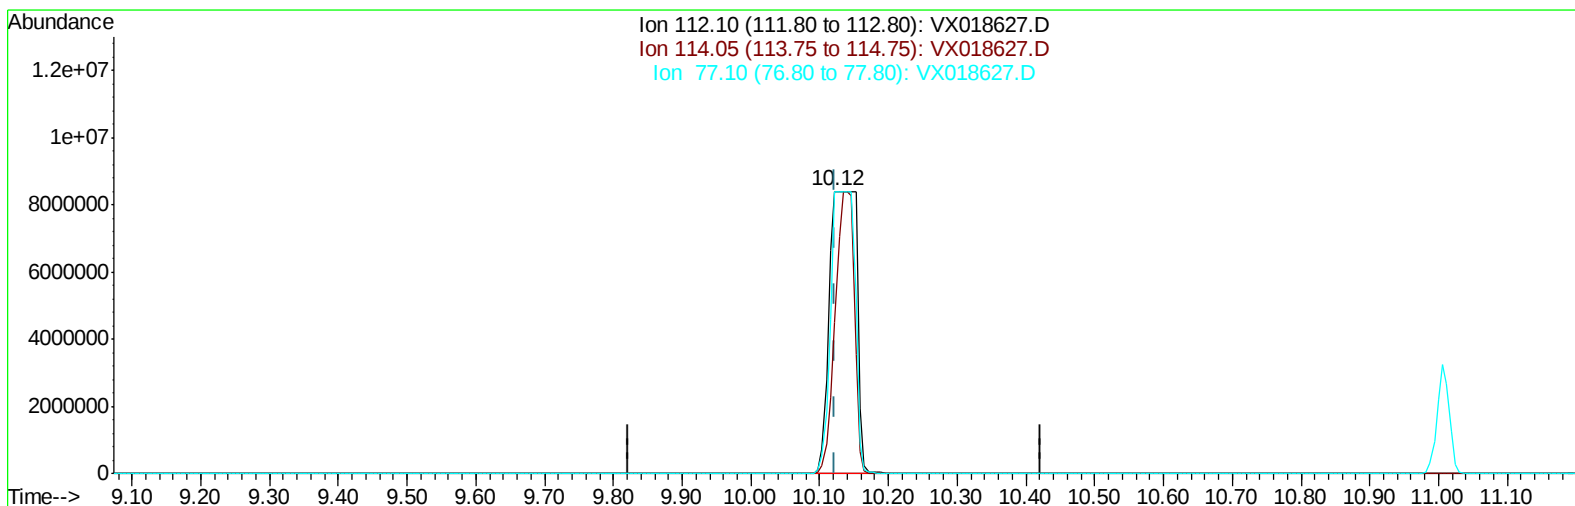

TIC: VX018627.D

(53) Chlorobenzene (T)

10.122min (-0.000) 627.42ug/L m

response 23033602

Ion	Exp%	Act%
112.10	100	100
114.05	29.50	53.67#
77.10	58.20	100.00#
0.00	0.00	0.00