

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX092820\
 Data File : VX018620.D
 Acq On : 28 Sep 2020 17:18
 Operator : JC/SP
 Sample : VX0928WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK71

Quant Time: Sep 29 02:52:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 29 02:30:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	249527	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	242142	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	107468	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	64085	4.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.20%
7) Chloroethane-d5	1.70	69	52734	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.34	63	117160	4.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.20%
20) 2-Butanone-d5	4.56	46	177324	53.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.52%
24) Chloroform-d	5.14	84	154322	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	6.03	65	85359	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	6.05	84	282270	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	7.37	67	85170	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	8.70	98	254525	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
45) trans-1,3-Dichloropropene-	8.99	79	35614	4.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.00%
48) 2-Hexanone-d5	9.43	63	140856	51.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.86%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	63623	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
65) 1,2-Dichlorobenzene-d4	12.36	152	92136	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%


Target Compounds					Ovalue
16) Methylene chloride	2.84	84	5556	0.334 ug/L	90




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092820\
Data File : VX018620.D
Acq On : 28 Sep 2020 17:18
Operator : JC/SP
Sample : VX0928WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK71

Quant Time: Sep 29 02:52:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 29 02:30:52 2020
Response via : Initial Calibration

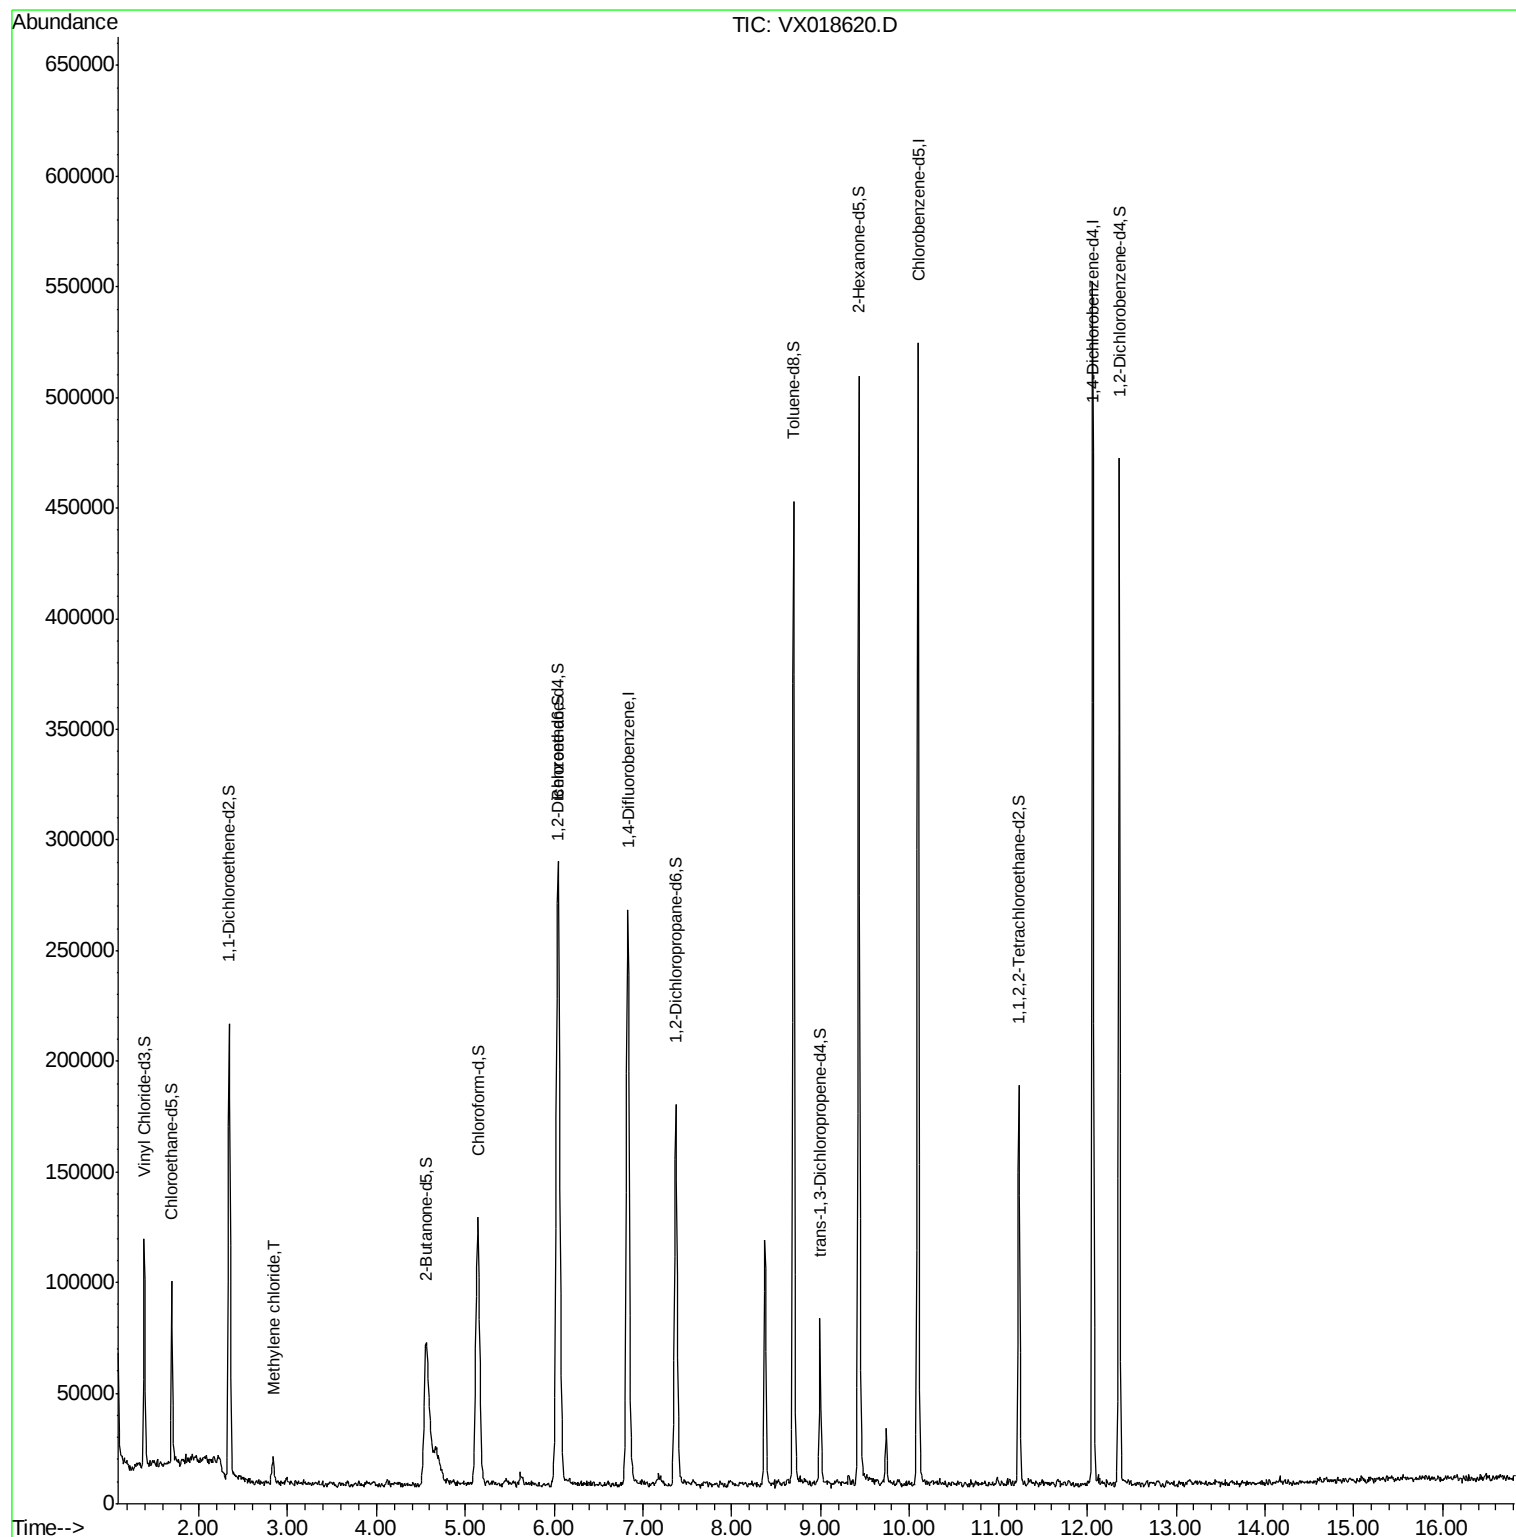

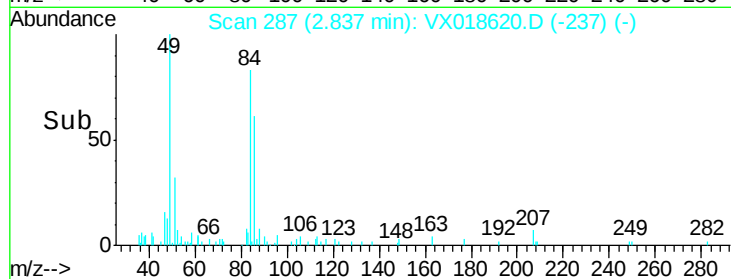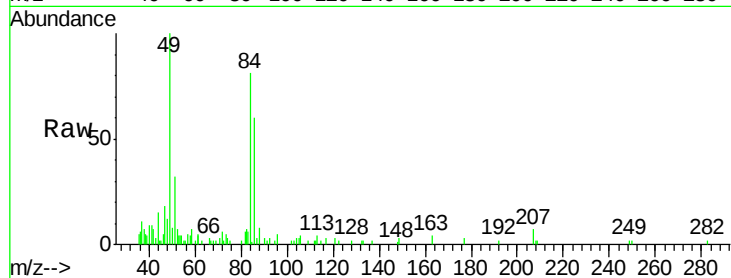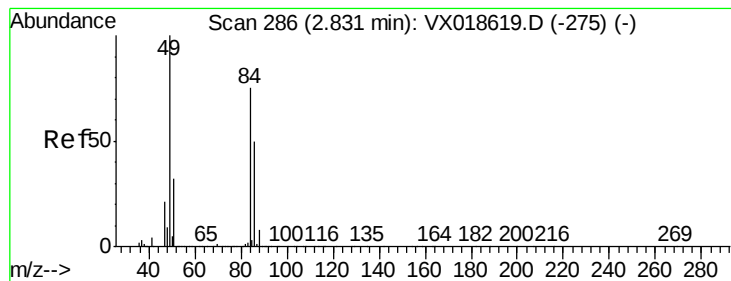

#16

Methylene chloride

Concen: 0.334 ug/L

RT: 2.84 min Scan# 287

Delta R.T. 0.01 min

Lab File: VX018620.D

Acq: 28 Sep 2020 17:18

Instrument :

MSVOA_X

ClientSampleId :

VBLK71

Tot Ion: 84 Resp: 5556

Ion Ratio Lower Upper

84 100

86 73.3 41.9 77.7

49 122.7 80.8 150.2

