

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
 Data File : VX031736.D
 Acq On : 28 Sep 2022 18:47
 Operator : JC/MD
 Sample : N4793-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 29 04:33:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 27 01:44:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	112992	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	182434	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	190332	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	102550	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	123891	51.661	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.320%
35) Dibromofluoromethane	5.385	113	102496	47.152	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.300%
50) Toluene-d8	8.653	98	395788	50.222	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.440%
62) 4-Bromofluorobenzene	11.079	95	130196	45.075	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031736.D
Acq On : 28 Sep 2022 18:47
Operator : JC/MD
Sample : N4793-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 29 04:33:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 27 01:44:18 2022
Response via : Initial Calibration




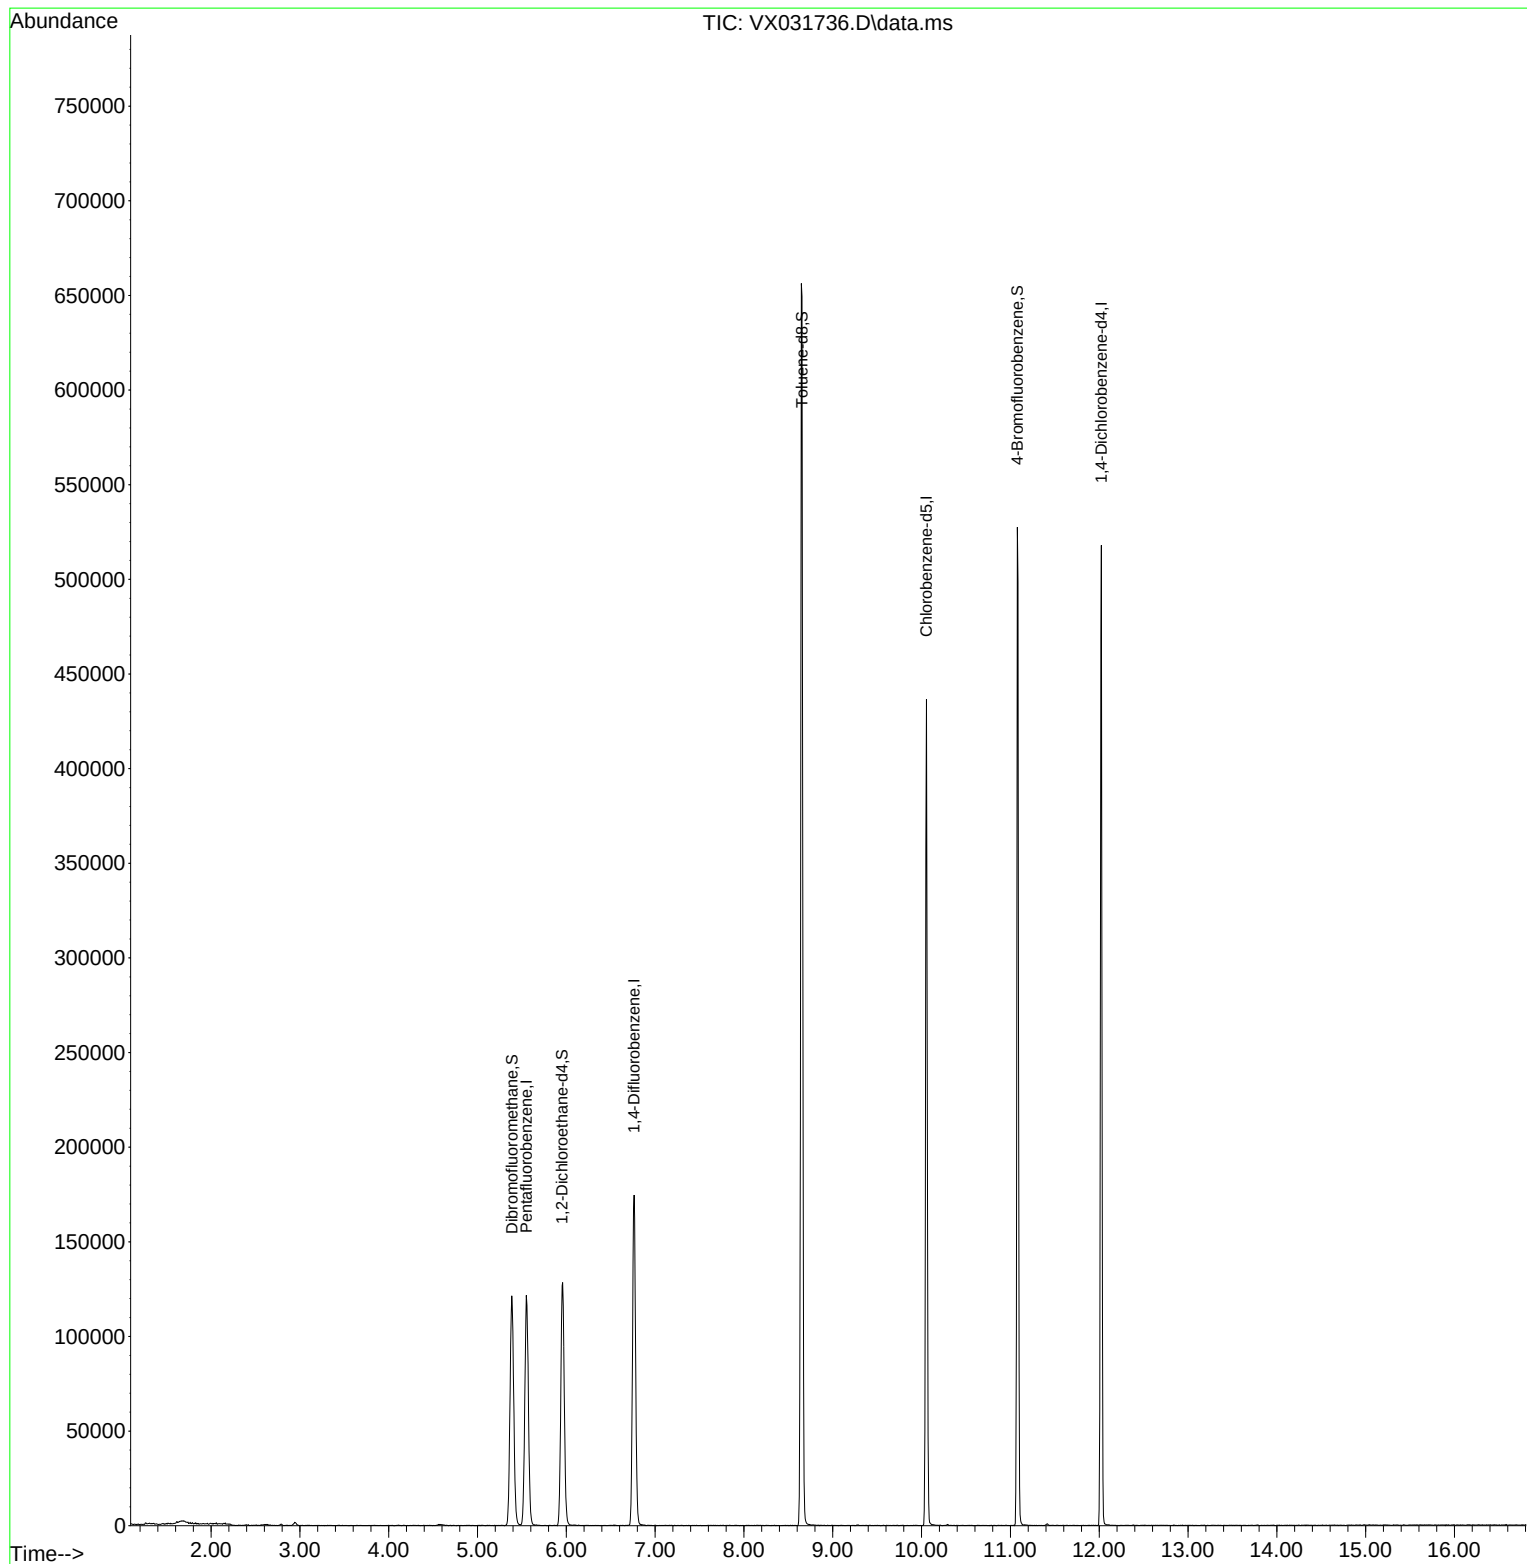


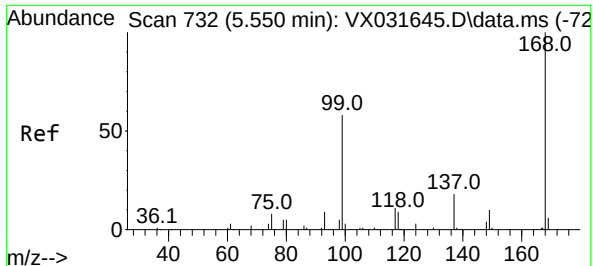

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.006 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 112992
Ion Ratio Lower Upper
168 100
99 59.1 48.8 73.2

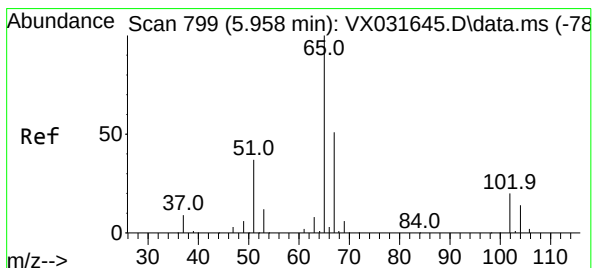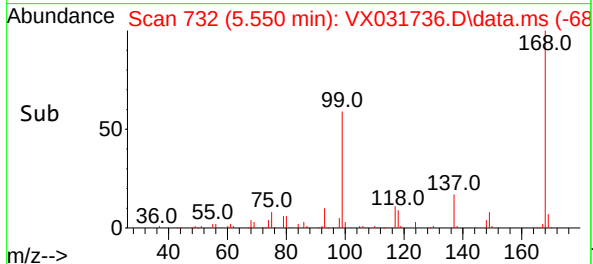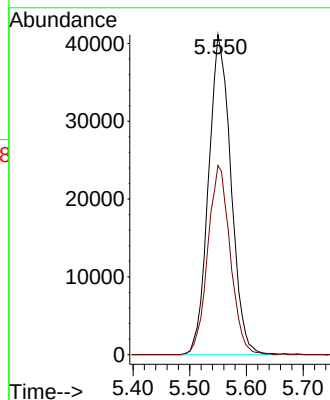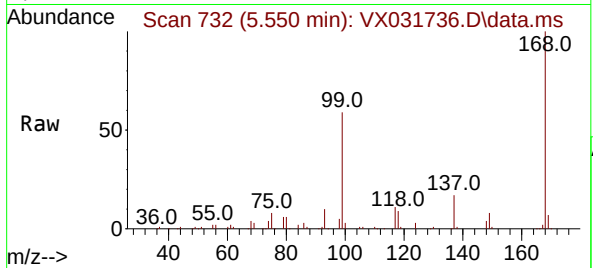

#33
1,2-Dichloroethane-d4
Concen: 51.661 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47

Tgt Ion: 65 Resp: 123891
Ion Ratio Lower Upper
65 100
67 50.7 0.0 102.4


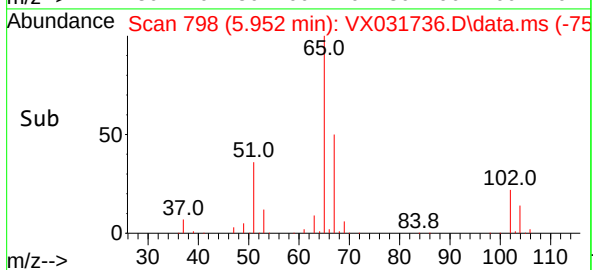
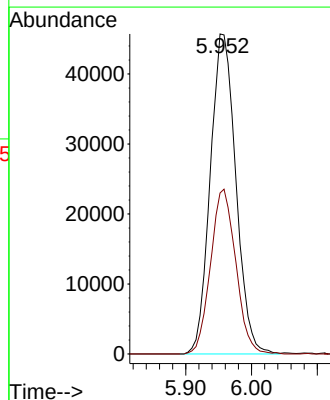
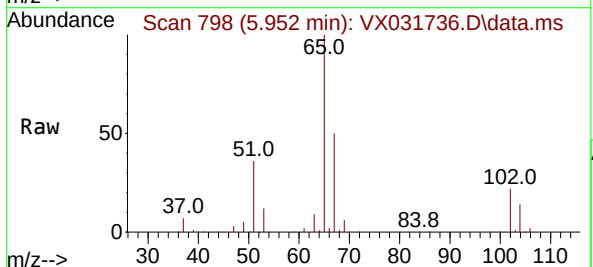


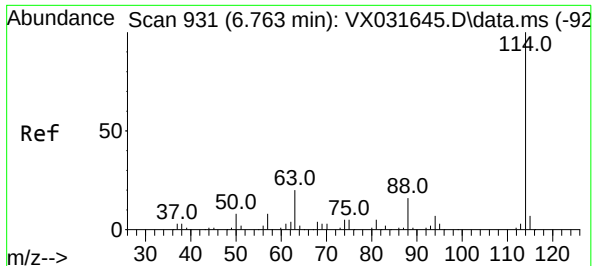

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 182434
Ion Ratio Lower Upper
114 100
63 18.9 0.0 42.6
88 14.9 0.0 33.0

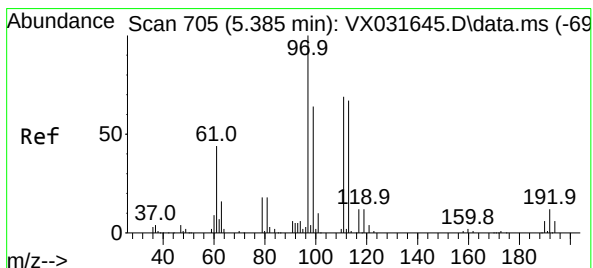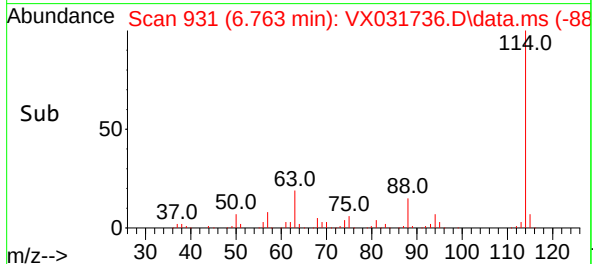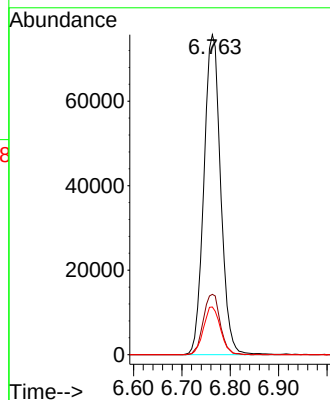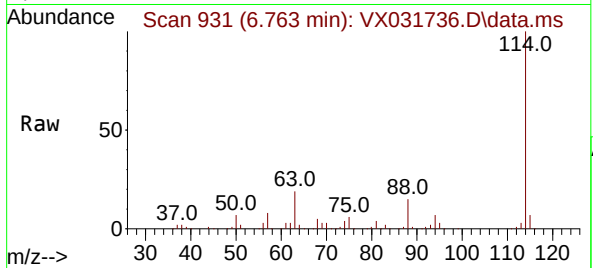

#35
Dibromofluoromethane
Concen: 47.152 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47

Tgt Ion:113 Resp: 102496
Ion Ratio Lower Upper
113 100
111 100.7 82.4 123.6
192 18.7 14.1 21.1


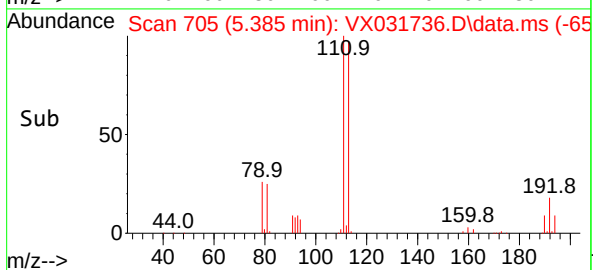
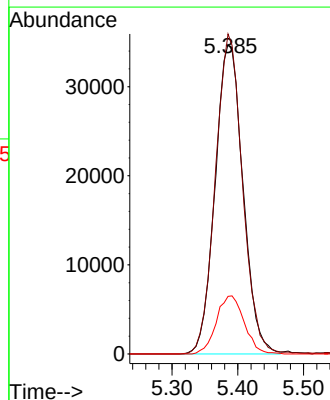
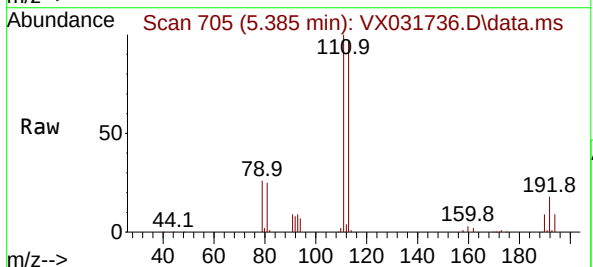


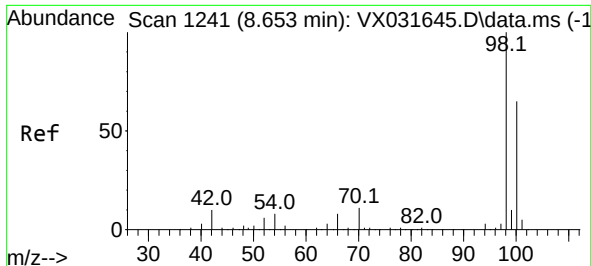

#50
Toluene-d8
Concen: 50.222 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 395788
Ion Ratio Lower Upper
98 100
100 66.1 52.5 78.7

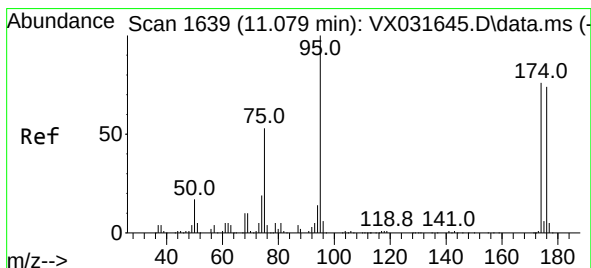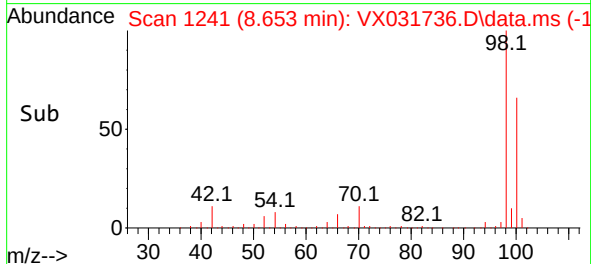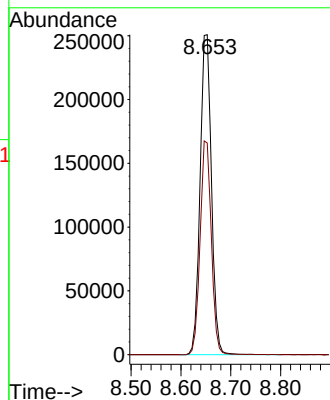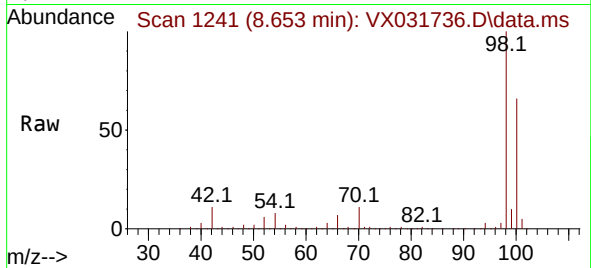

#62
4-Bromofluorobenzene
Concen: 45.075 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47

Tgt Ion: 95 Resp: 130196
Ion Ratio Lower Upper
95 100
174 81.1 0.0 153.2
176 80.8 0.0 144.0


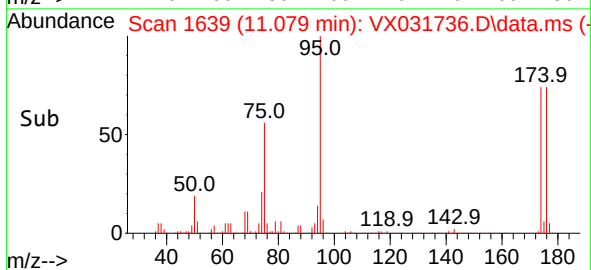
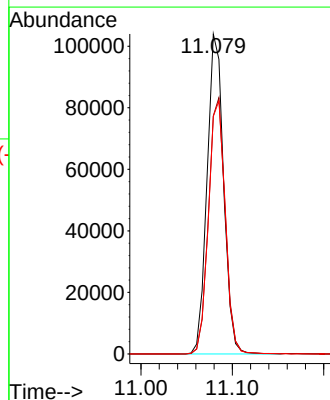
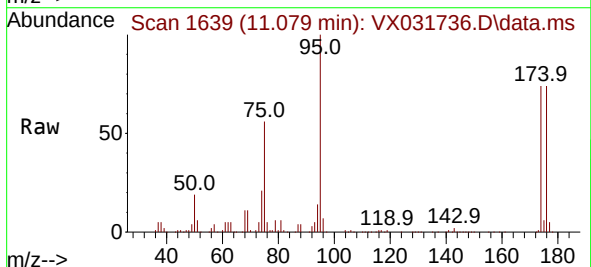


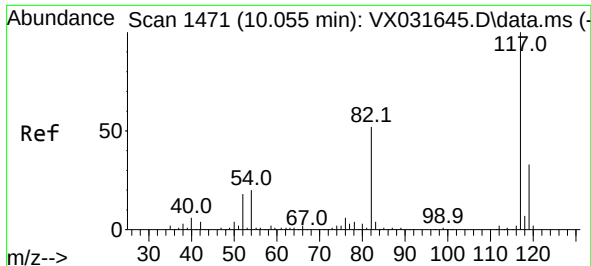

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 190332
Ion Ratio Lower Upper
117 100
82 52.4 46.8 70.2
119 31.3 26.4 39.6

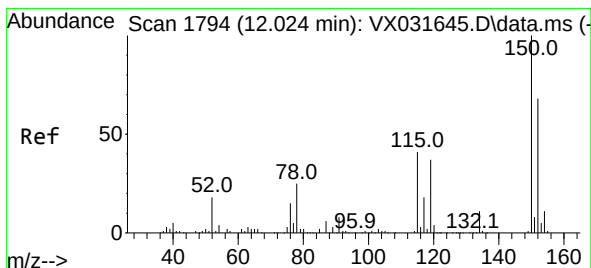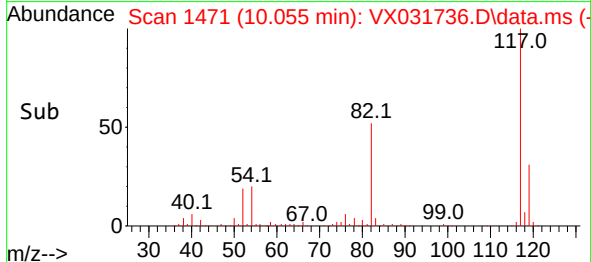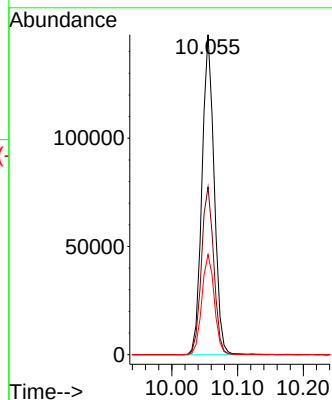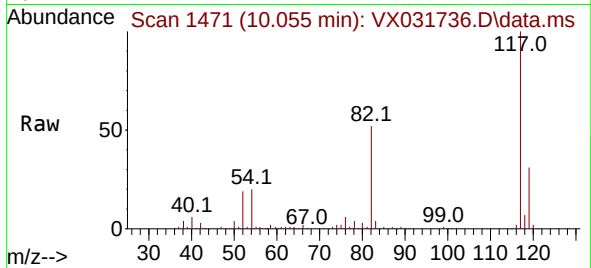

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031736.D
Acq: 28 Sep 2022 18:47

Tgt Ion:152 Resp: 102550
Ion Ratio Lower Upper
152 100
115 59.0 43.4 130.1
150 156.9 0.0 346.8

