

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
 Data File : VX031750.D
 Acq On : 29 Sep 2022 01:23
 Operator : JC/MD
 Sample : N4863-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M

Title : SW846 8260

Signal : TIC: VX031750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	5	9	15	rBV	21243	20592	1.82%	0.350%
2	1.270	26	30	49	rBV2	414245	866738	76.61%	14.725%
3	3.111	324	332	343	rVB	34246	82015	7.25%	1.393%
4	5.385	693	705	721	rBV2	134893	390251	34.49%	6.630%
5	5.549	721	732	746	rVB	133173	377303	33.35%	6.410%
6	5.958	787	799	811	rBV	142625	376922	33.32%	6.403%
7	6.763	919	931	946	rBV	199137	475399	42.02%	8.076%
8	8.646	1231	1240	1249	rBV	727550	1131352	100.00%	19.220%
9	10.055	1465	1471	1482	rBV	484079	651348	57.57%	11.066%
10	11.079	1634	1639	1653	rBV	599604	759860	67.16%	12.909%
11	12.024	1788	1794	1802	rBV	606828	754434	66.68%	12.817%




Sum of corrected areas: 5886214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031750.D
Acq On : 29 Sep 2022 01:23
Operator : JC/MD
Sample : N4863-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

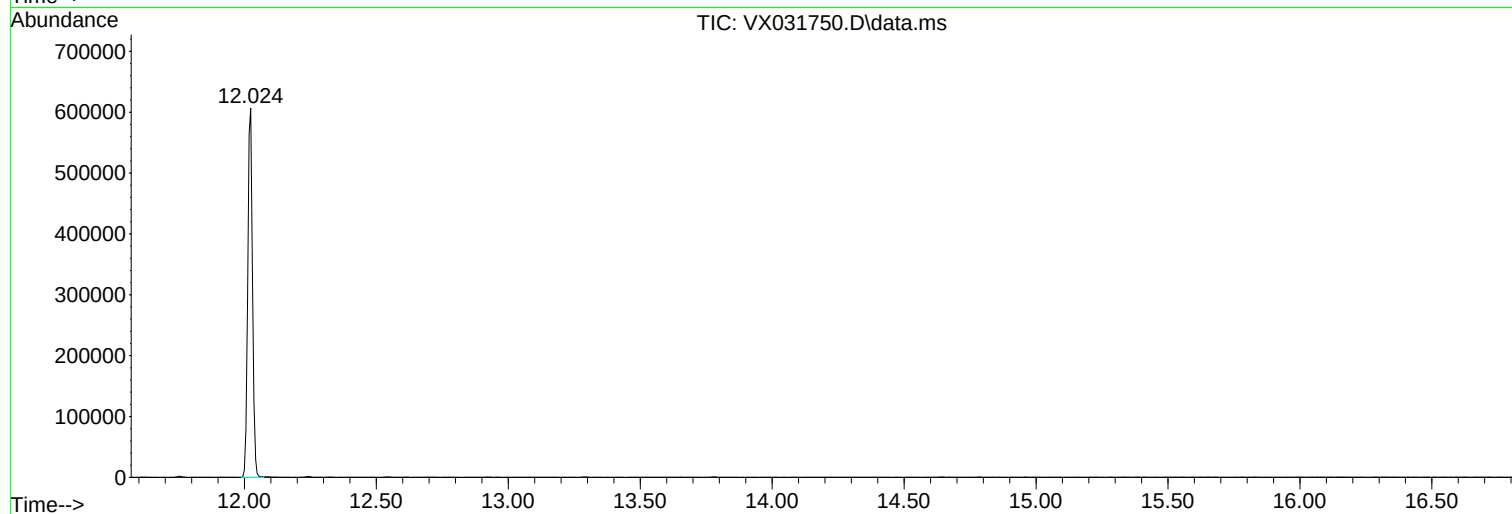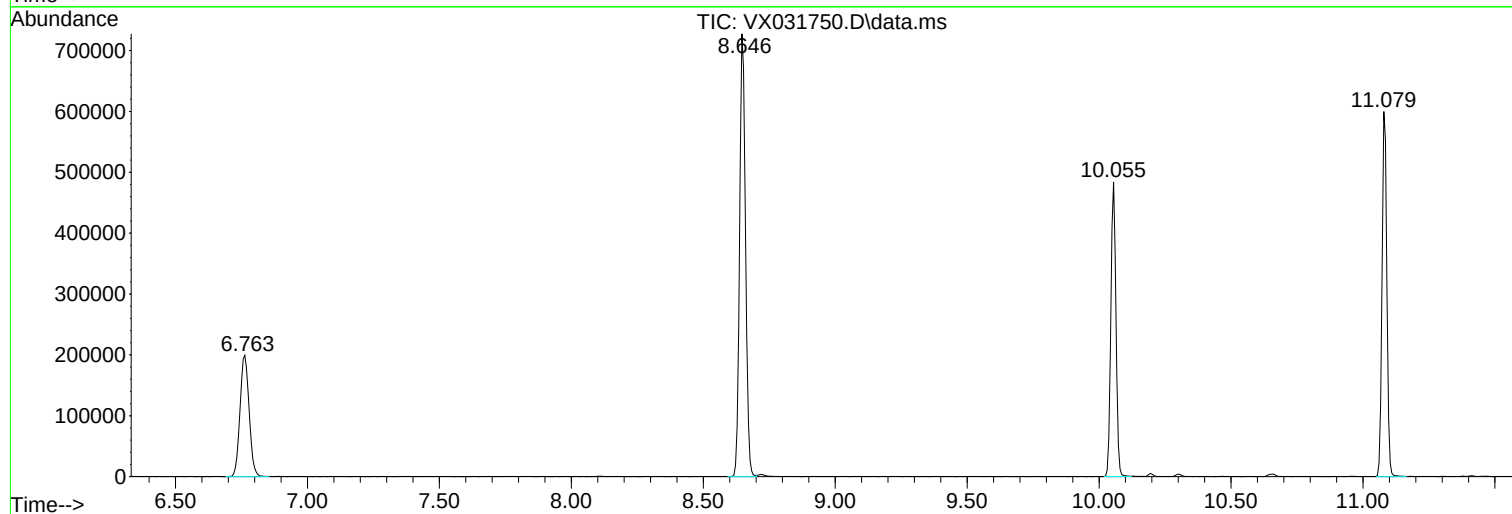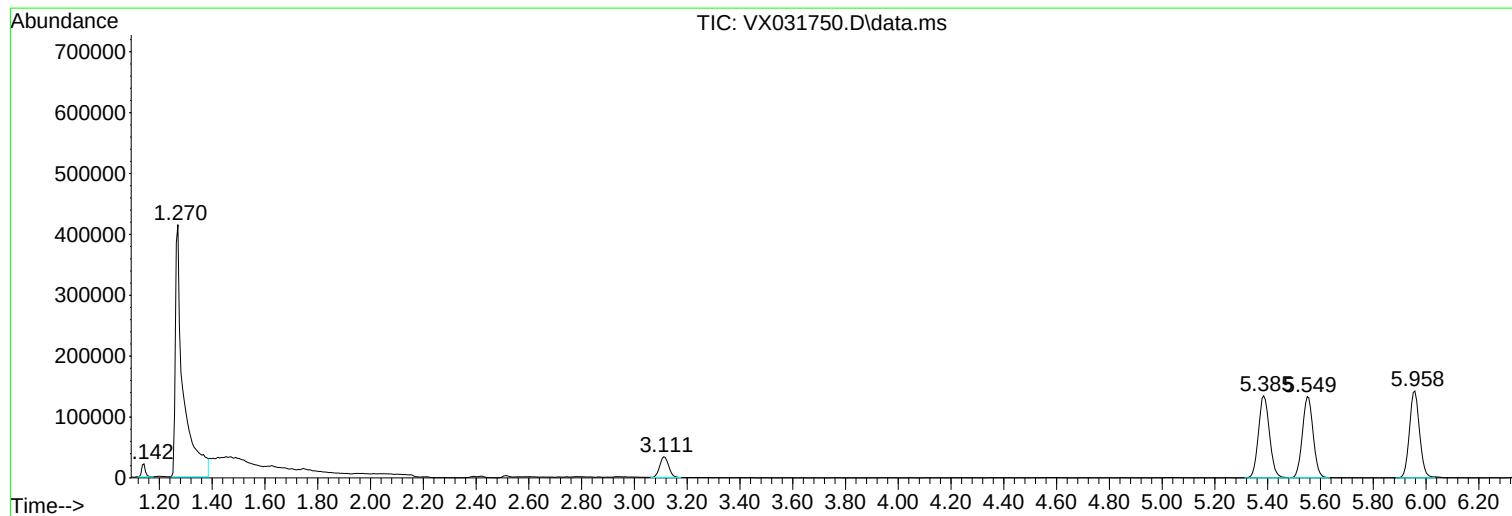

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031750.D
Acq On : 29 Sep 2022 01:23
Operator : JC/MD
Sample : N4863-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	114.86 ug/l	866738	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	78
2			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	4
3			2,2-Difluoropropionic acid	110	C3H4F2O2	000373-96-6	2
4			(S)-(-)-2-Chloropropionic acid	108	C3H5ClO2	029617-66-1	1
5			(S)-(+)-2-Chloro-1-propanol	94	C3H7ClO	019210-21-0	1

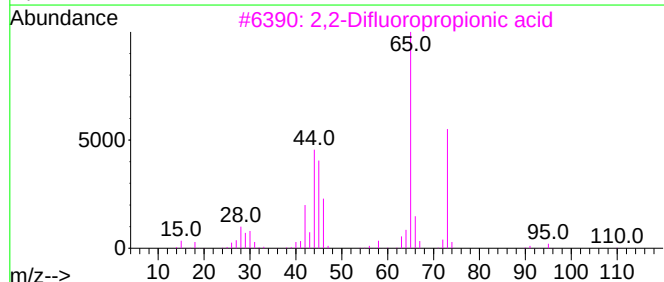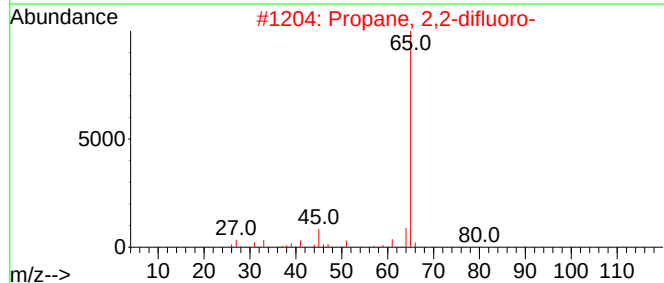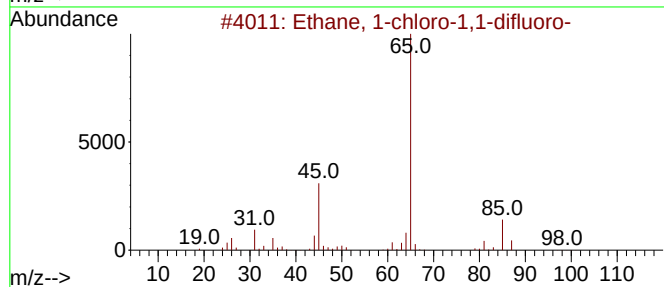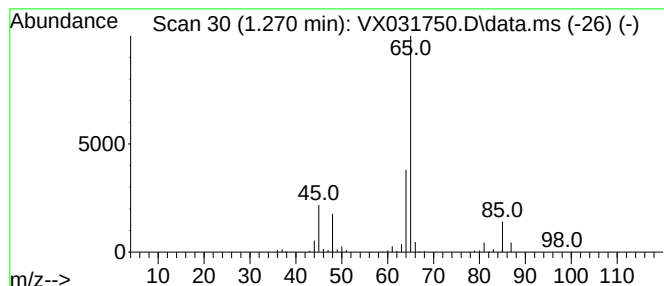

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031750.D
Acq On : 29 Sep 2022 01:23
Operator : JC/MD
Sample : N4863-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1-chlor...	1.270	114.9	ug/l	866738	1	5.556	377303	50.0