

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
 Data File : VX031754.D
 Acq On : 29 Sep 2022 02:56
 Operator : JC/MD
 Sample : PB147944ZHE#01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB147944ZHE#01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Title : SW846 8260

Signal : TIC: VX031754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	25	34	49	rBV2	7629	26843	2.21%	0.287%
2	2.392	207	214	226	rBV	10507	19823	1.63%	0.212%
3	2.788	271	279	288	rVB	22374	40462	3.33%	0.432%
4	4.721	588	596	608	rBV	6798	19371	1.60%	0.207%
5	5.385	693	705	721	rBV2	137996	396999	32.71%	4.241%
6	5.550	721	732	746	rVV2	135865	380651	31.36%	4.067%
7	5.958	787	799	813	rBV	142252	380355	31.34%	4.064%
8	6.342	848	862	875	rBV	42162	108072	8.90%	1.155%
9	6.763	920	931	943	rBV	209680	525265	43.28%	5.612%
10	7.641	1064	1075	1080	rBV	24959	45759	3.77%	0.489%
11	7.696	1080	1084	1091	rVB3	7995	15860	1.31%	0.169%
12	7.799	1094	1101	1114	rBV	632066	1064955	87.75%	11.377%
13	8.549	1215	1224	1234	rBV	147066	225983	18.62%	2.414%
14	8.653	1234	1241	1256	rVB	761272	1213631	100.00%	12.966%
15	8.952	1285	1290	1304	rBV	189581	281596	23.20%	3.008%
16	9.244	1330	1338	1345	rBV	203949	288885	23.80%	3.086%
17	9.311	1345	1349	1351	rVV2	17417	24783	2.04%	0.265%
18	9.348	1351	1355	1357	rVV	30561	48554	4.00%	0.519%
19	9.378	1357	1360	1368	rVV	82411	113850	9.38%	1.216%
20	9.482	1372	1377	1385	rVV	368059	473234	38.99%	5.056%
21	9.579	1388	1393	1409	rVB	237156	305364	25.16%	3.262%
22	9.915	1442	1448	1463	rBV	731084	883591	72.81%	9.440%
23	10.055	1464	1471	1478	rBV	569838	748768	61.70%	7.999%
24	10.281	1504	1508	1513	rBV	8579	12510	1.03%	0.134%
25	10.640	1562	1567	1580	rBV	59295	74482	6.14%	0.796%
26	11.079	1634	1639	1652	rBV	667170	827973	68.22%	8.846%
27	12.024	1788	1794	1802	rBV	673186	812602	66.96%	8.681%




Sum of corrected areas: 9360221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031754.D
Acq On : 29 Sep 2022 02:56
Operator : JC/MD
Sample : PB147944ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147944ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

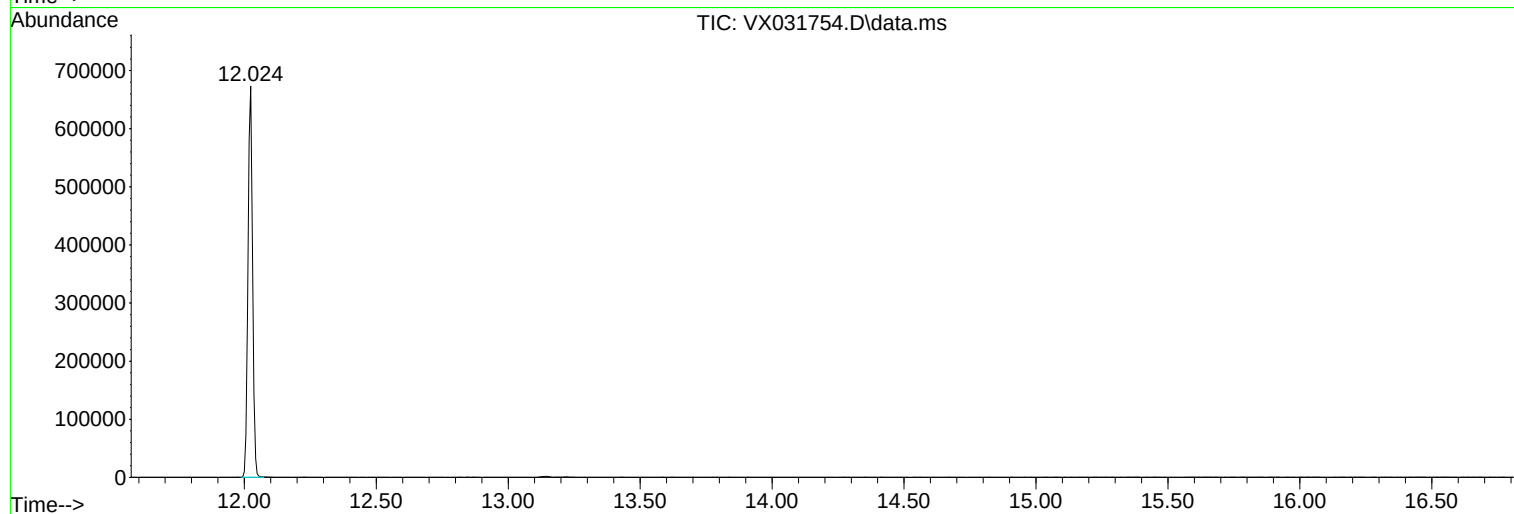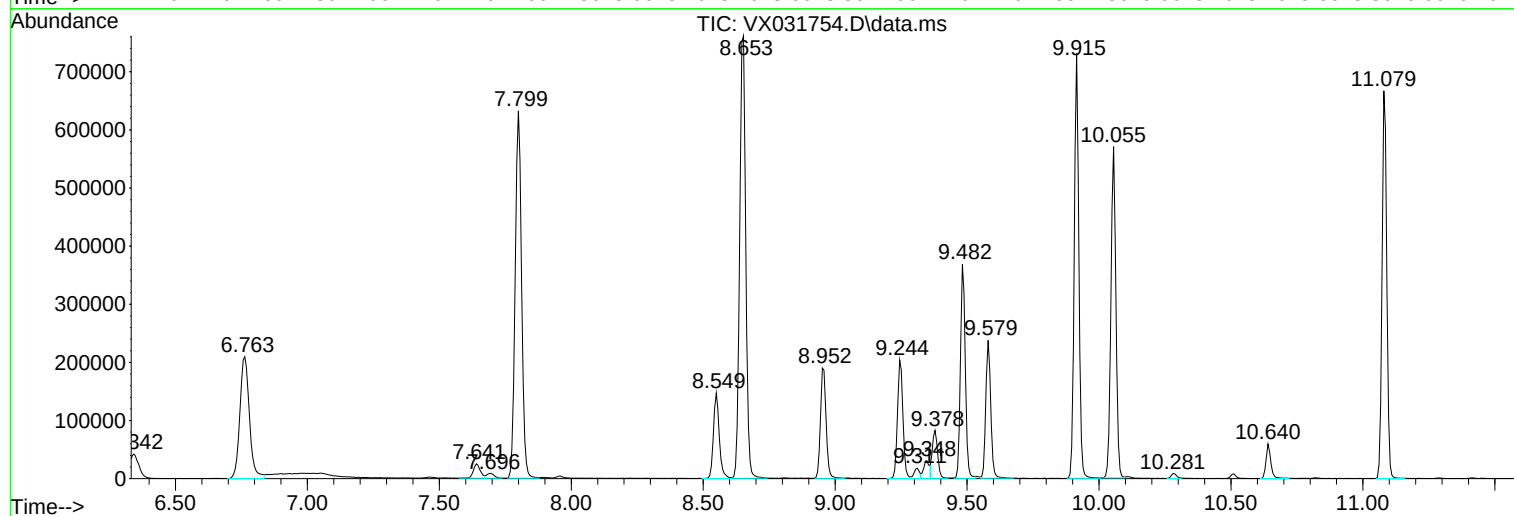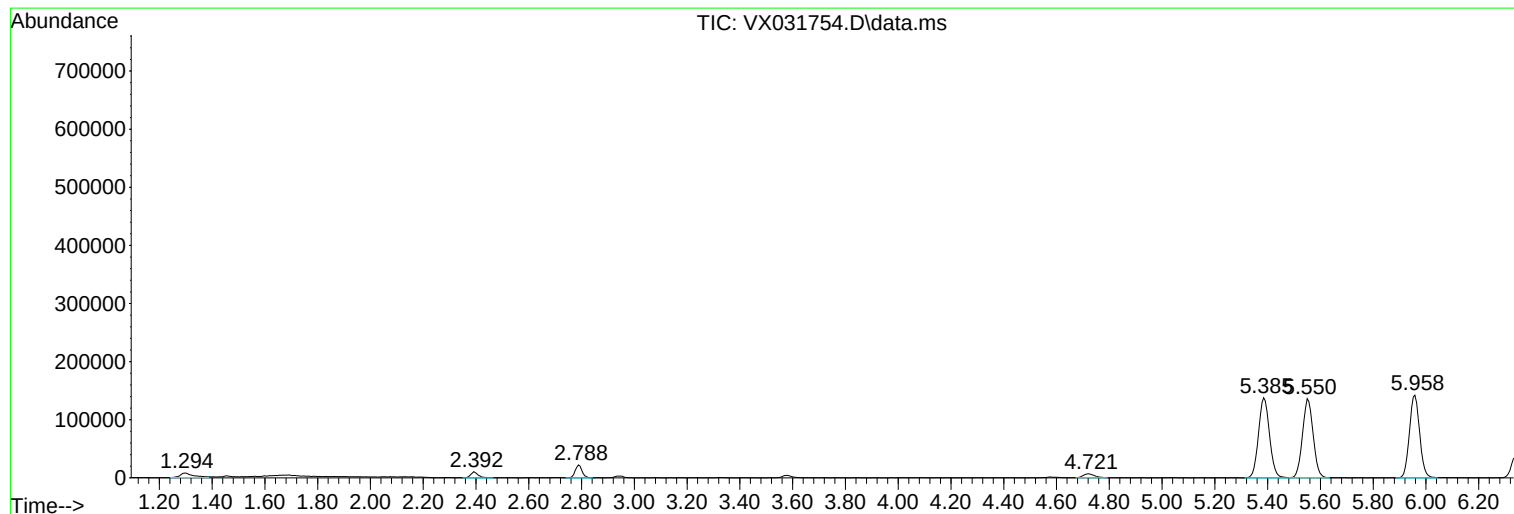

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031754.D
Acq On : 29 Sep 2022 02:56
Operator : JC/MD
Sample : PB147944ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147944ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031754.D
Acq On : 29 Sep 2022 02:56
Operator : JC/MD
Sample : PB147944ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147944ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------