
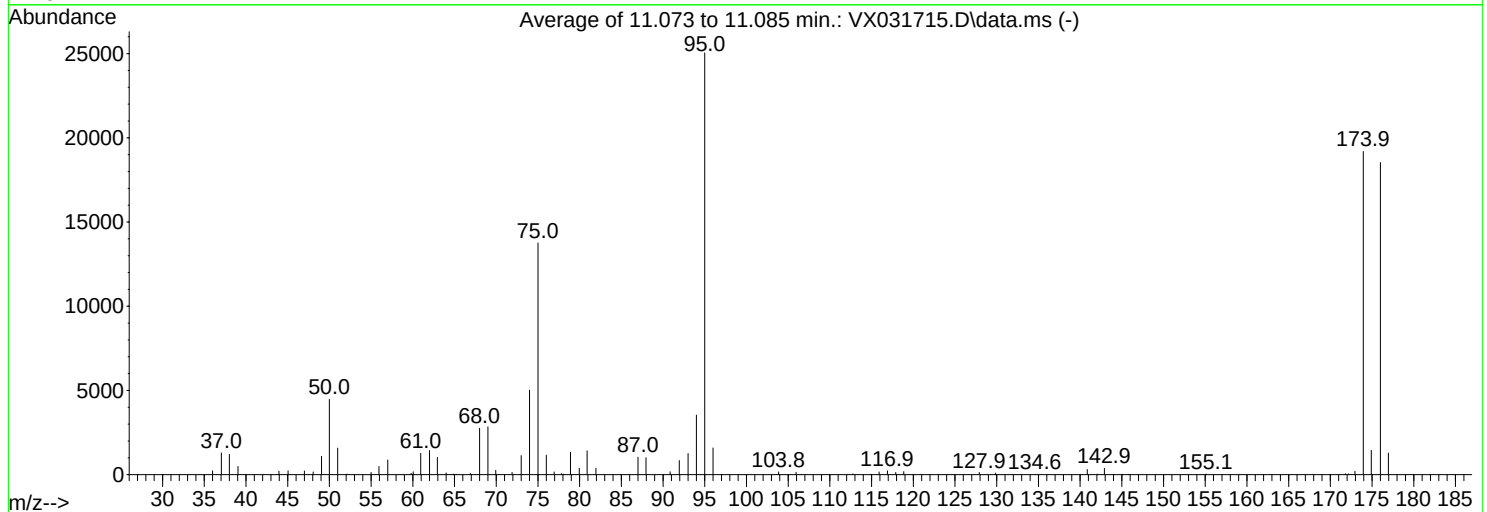


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031715.D
Acq On : 28 Sep 2022 08:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Title : SW846 8260
Last Update : Tue Sep 27 01:44:18 2022

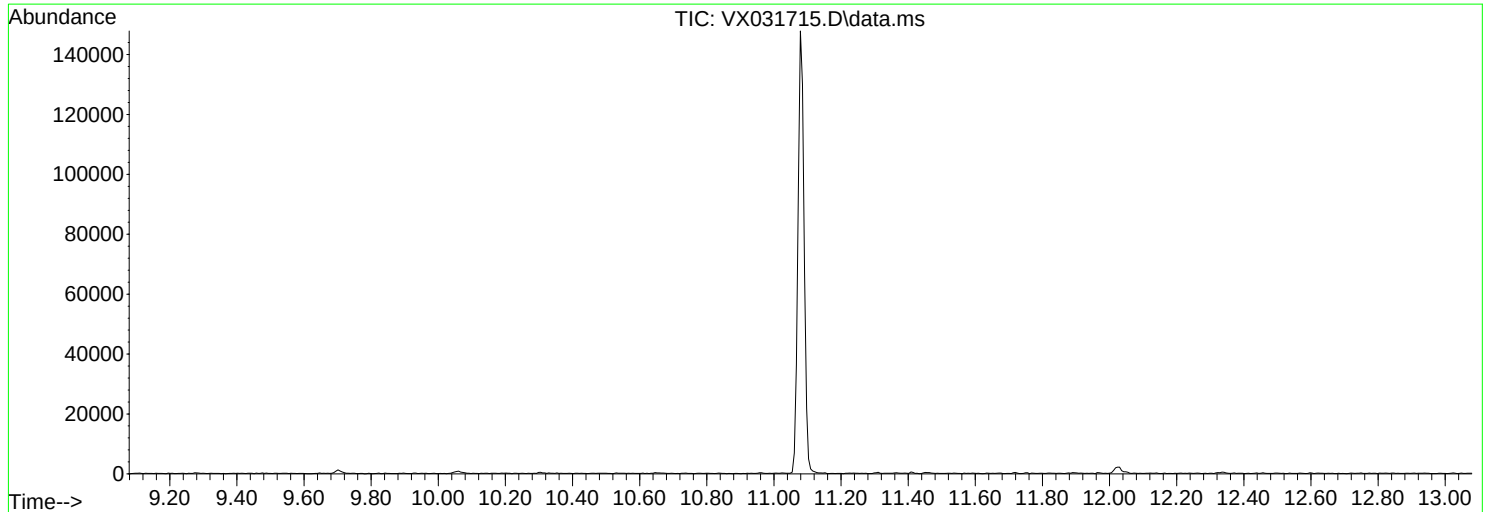

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	4478	PASS
75	95	30	60	54.9	13757	PASS
95	95	100	100	100.0	25045	PASS
96	95	5	9	6.3	1584	PASS
173	174	0.00	2	1.1	203	PASS
174	95	50	100	76.6	19191	PASS
175	174	5	9	7.5	1440	PASS
176	174	95	101	96.6	18537	PASS
177	176	5	9	6.9	1280	PASS