


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092822\
Data File : VX031740.D
Acq On : 28 Sep 2022 20:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Title : SW846 8260
Last Update : Tue Sep 27 01:44:18 2022

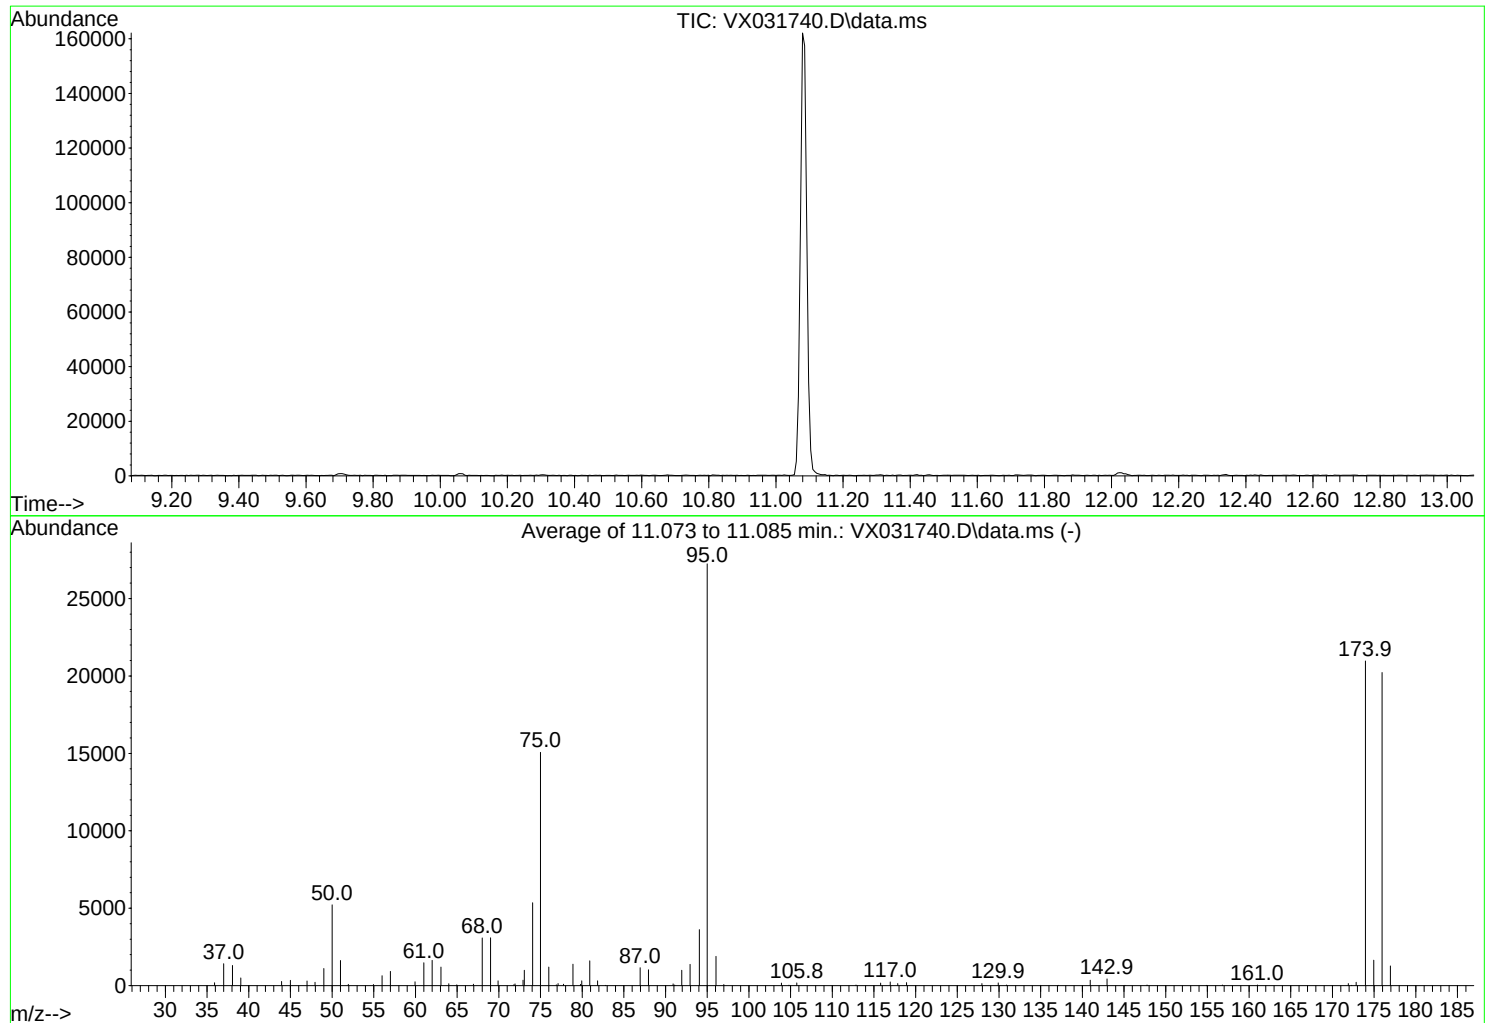

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	5218	PASS
75	95	30	60	55.3	15072	PASS
95	95	100	100	100.0	27243	PASS
96	95	5	9	6.9	1889	PASS
173	174	0.00	2	1.0	216	PASS
174	95	50	100	77.0	20971	PASS
175	174	5	9	7.8	1640	PASS
176	174	95	101	96.5	20227	PASS
177	176	5	9	6.3	1273	PASS