


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092823\
Data File : VX037937.D
Acq On : 28 Sep 2023 08:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X092723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Sep 28 06:08:32 2023

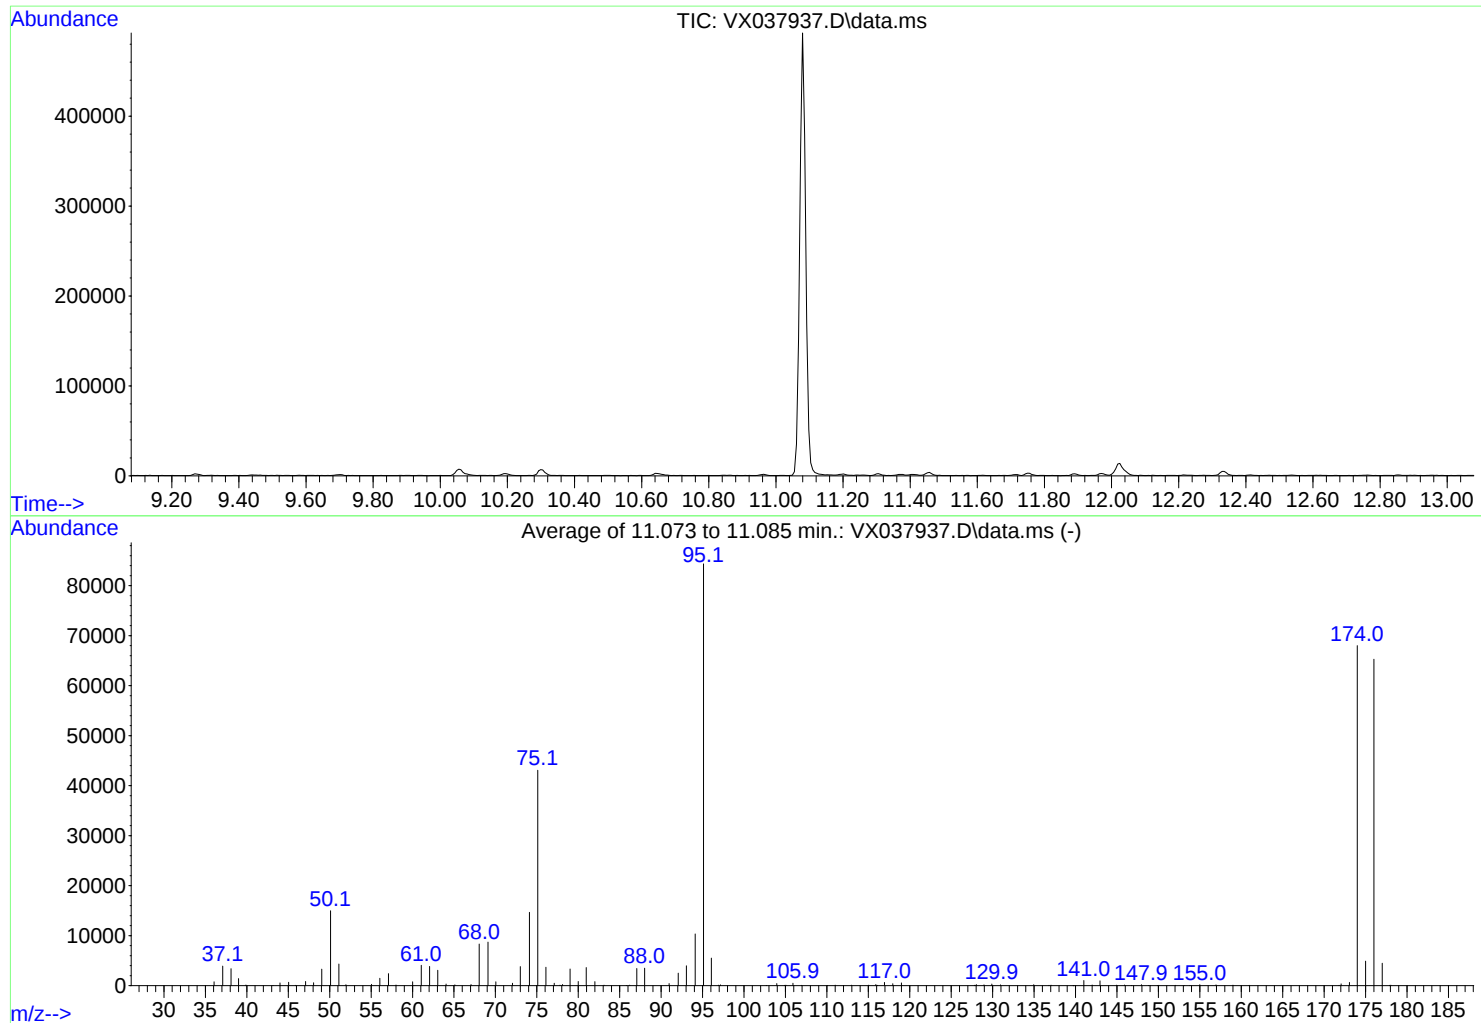

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	14989	PASS
75	95	30	60	51.1	43088	PASS
95	95	100	100	100.0	84368	PASS
96	95	5	9	6.5	5494	PASS
173	174	0.00	2	1.0	659	PASS
174	95	50	100	80.6	68005	PASS
175	174	5	9	7.2	4897	PASS
176	174	95	101	96.0	65288	PASS
177	176	5	9	6.9	4497	PASS