
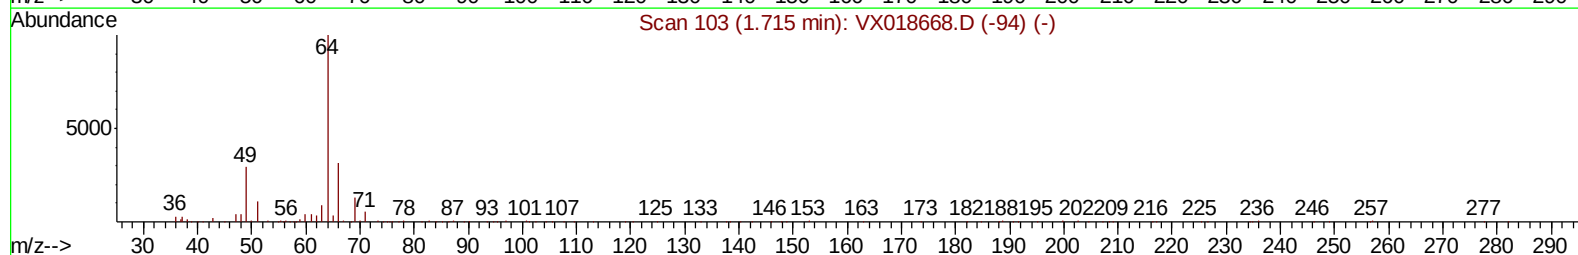
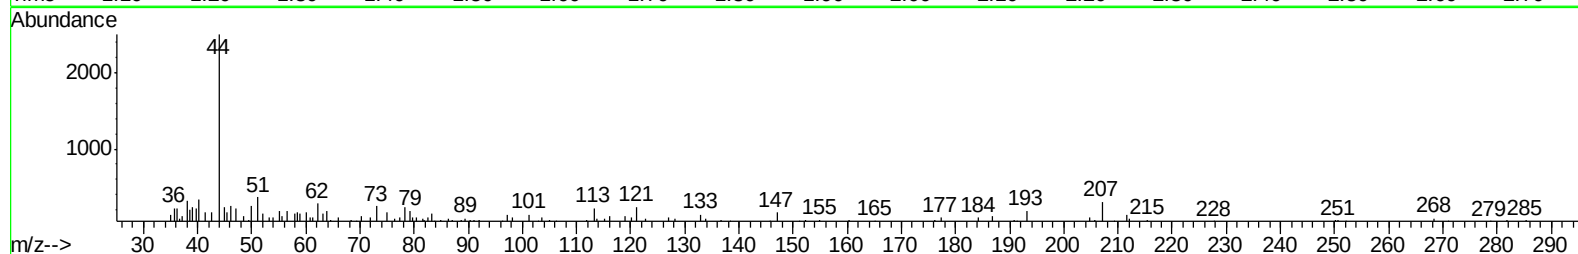


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
 Data File : VX018679.D
 Acq On : 30 Sep 2020 00:43
 Operator : JC/SP
 Sample : L4135-06DL 40X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Quant Time: Sep 30 08:31:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 07:04:14 2020
 Response via : Initial Calibration

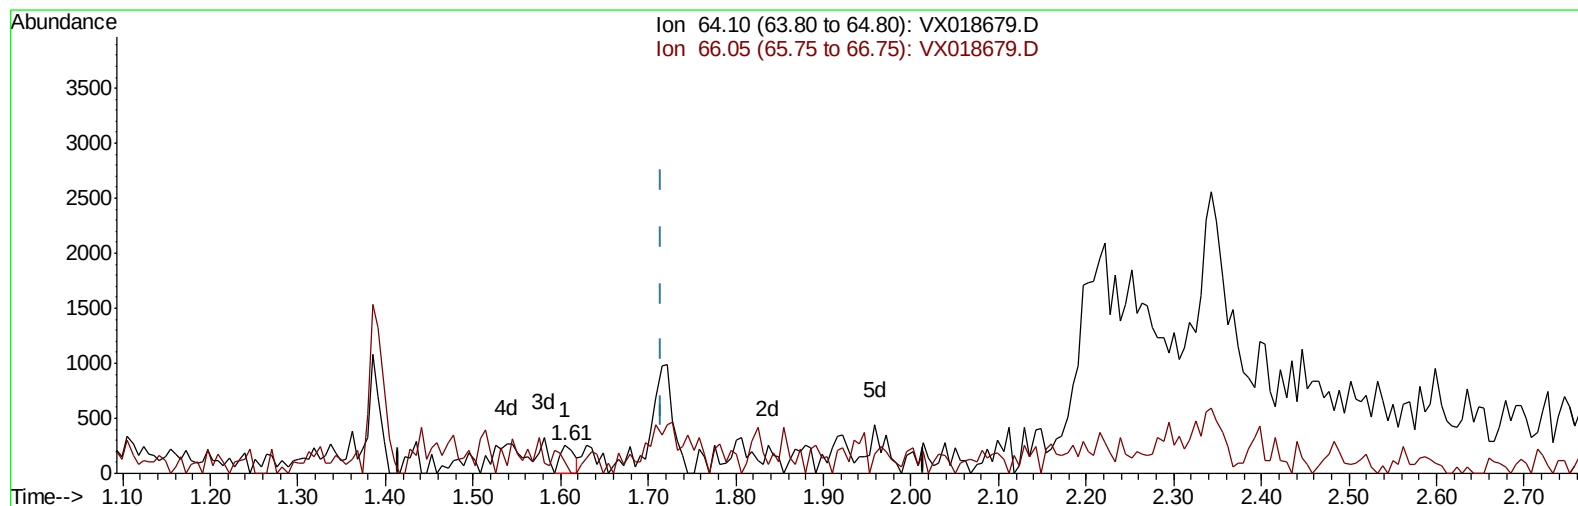

TIC: VX018679.D

(8) Chloroethane (T)

1.605min (-0.110) 0.04ug/L

response 279

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	39.37
0.00	0.00	0.00
0.00	0.00	0.00