
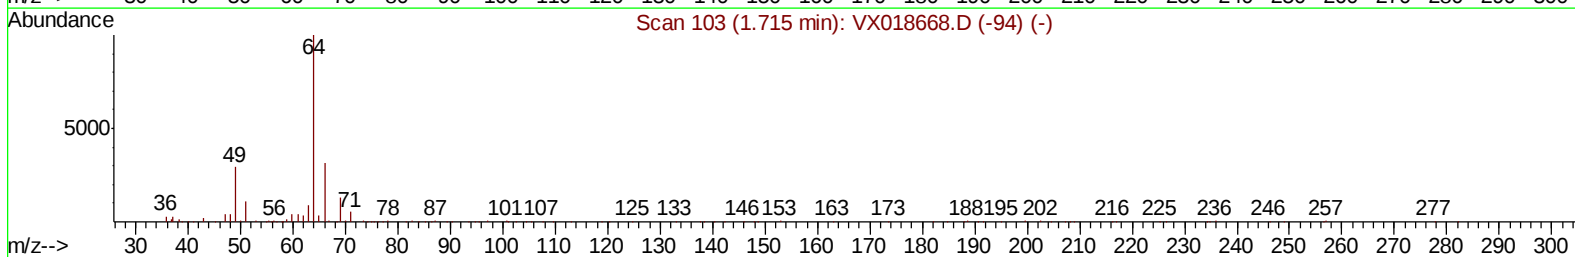
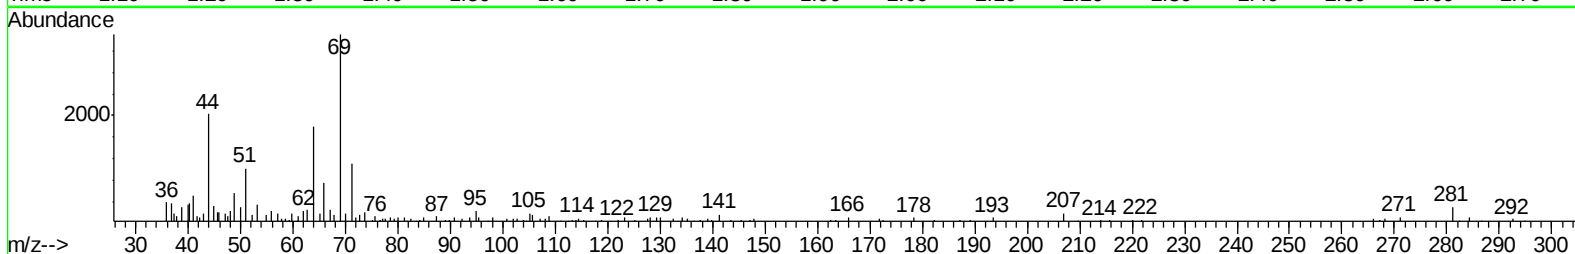


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
 Data File : VX018683.D
 Acq On : 30 Sep 2020 02:20
 Operator : JC/SP
 Sample : L4135-01DL 100X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Quant Time: Sep 30 07:14:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 07:04:14 2020
 Response via : Initial Calibration

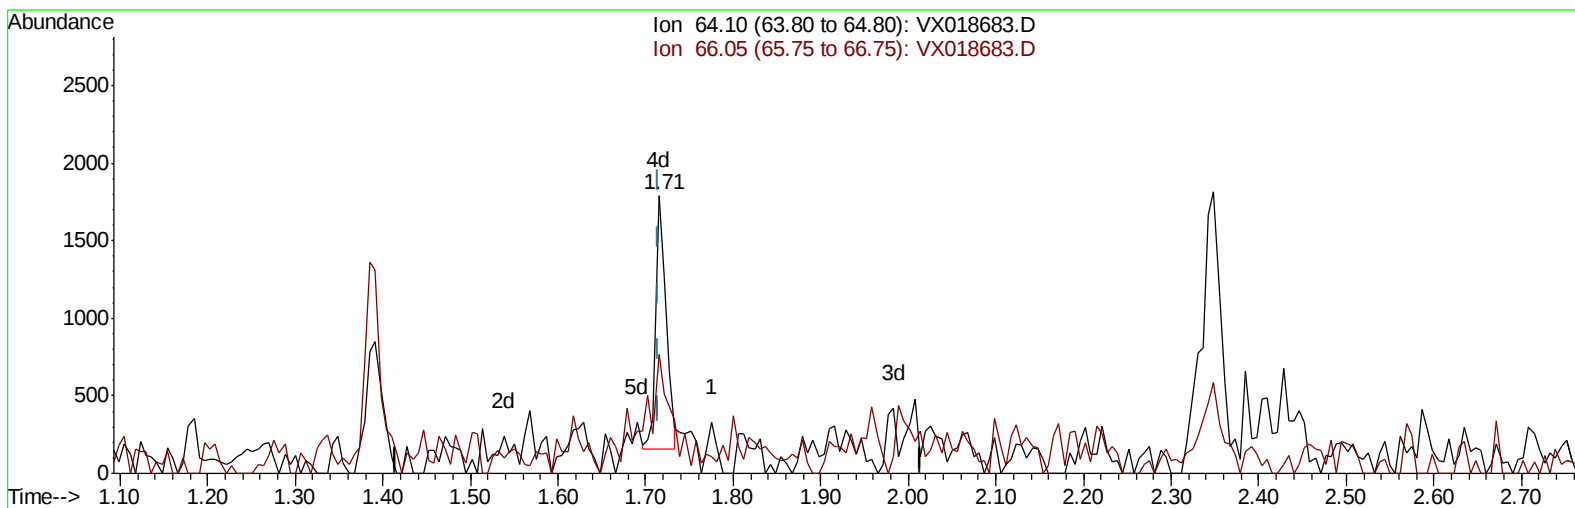

TIC: VX018683.D

(8) Chloroethane (T)

1.715min (-0.000) 0.20ug/L m

response 1327

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	42.75#
0.00	0.00	0.00
0.00	0.00	0.00