
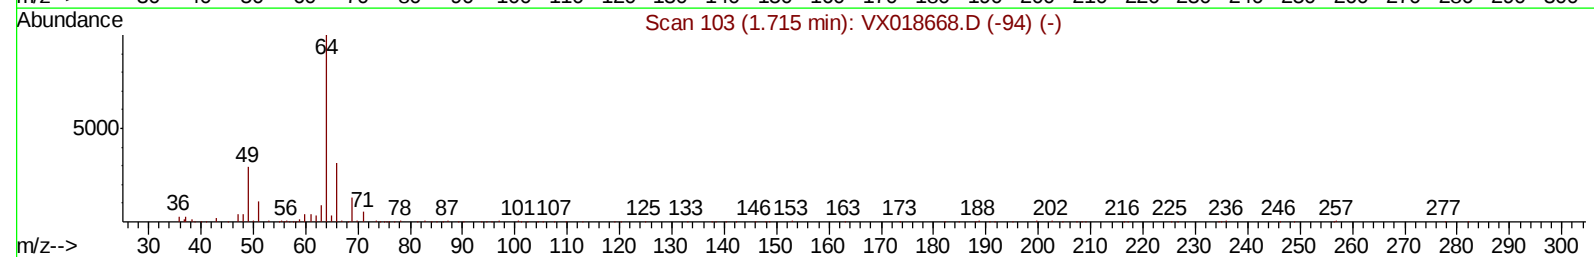
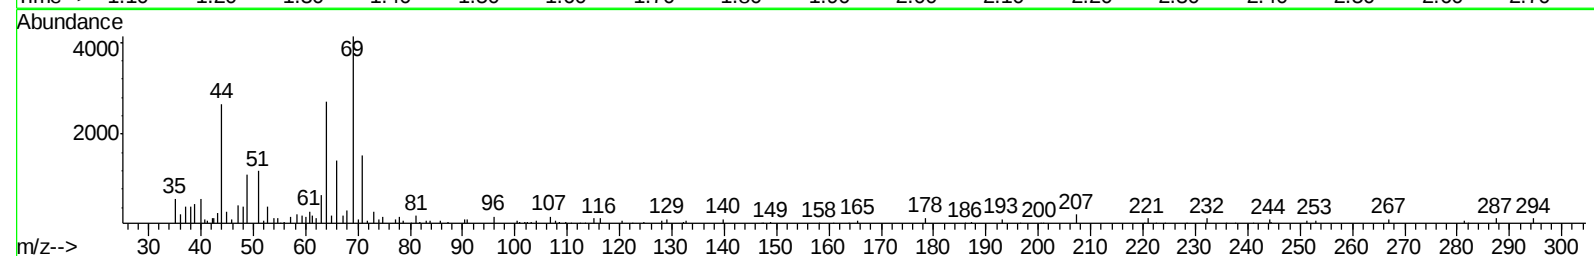


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
Data File : VX018684.D
Acq On : 30 Sep 2020 02:45
Operator : JC/SP
Sample : L4135-17DL 200X
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Sep 30 09:10:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 07:04:14 2020
Response via : Initial Calibration

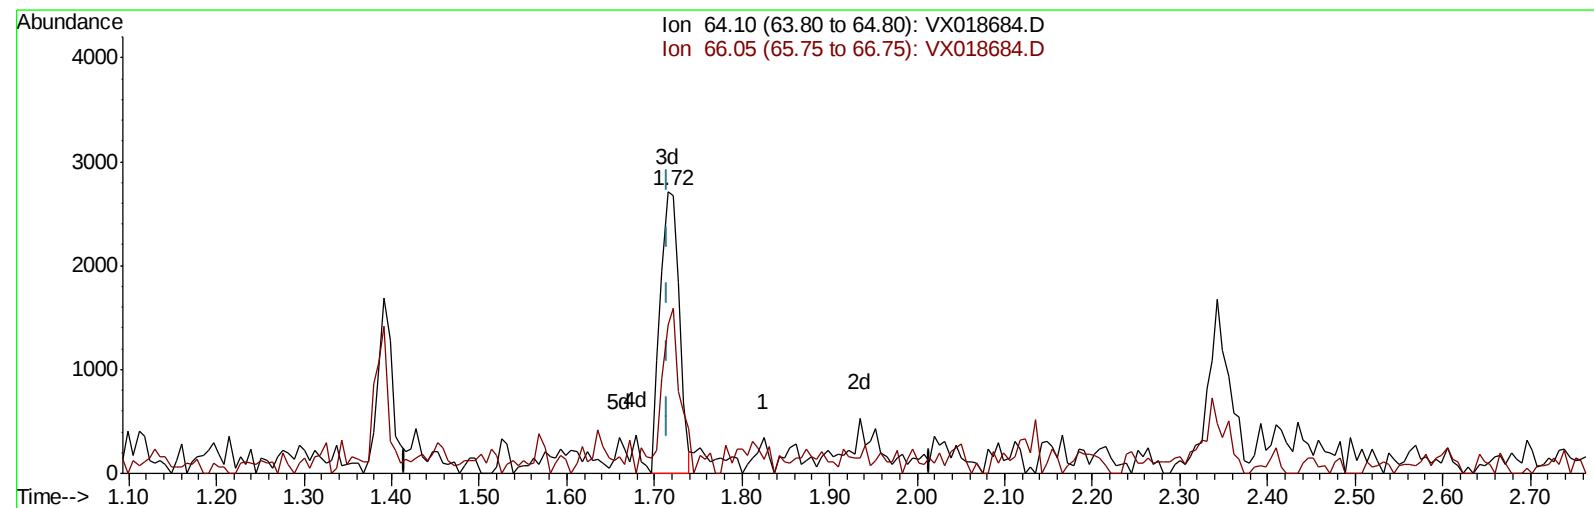

TIC: VX018684.D

(8) Chloroethane (T)

1.715min (+0.000) 0.59ug/L m

response 4079

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	52.86#
0.00	0.00	0.00
0.00	0.00	0.00