


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
Data File : VX018681.D
Acq On : 30 Sep 2020 01:32
Operator : JC/SP
Sample : L4135-13DL 40X
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG4A8DL

Manual Integrations
APPROVED

MMDadoda
10/1/2020 10:07:11 AM

Quant Time: Sep 30 08:43:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 07:04:14 2020
Response via : Initial Calibration

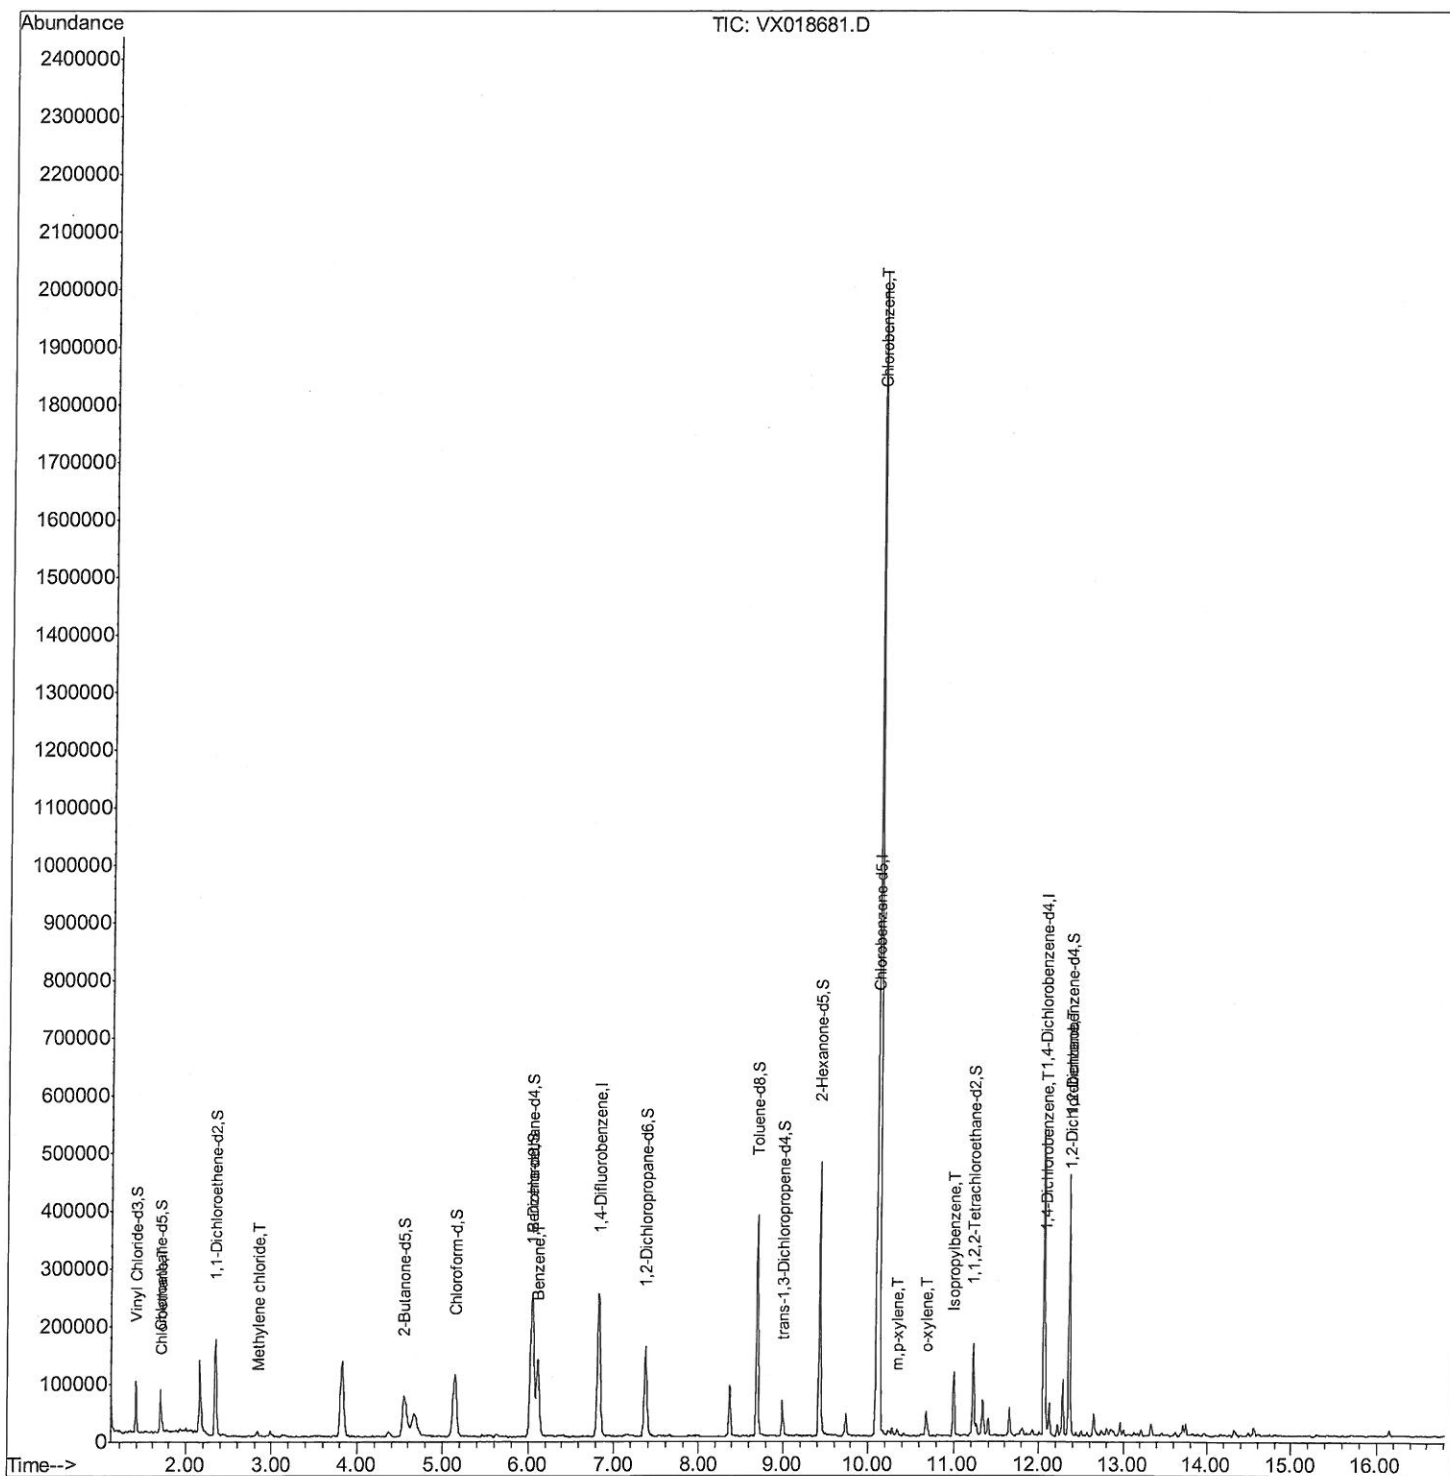

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
 Data File : VX018681.D
 Acq On : 30 Sep 2020 01:32
 Operator : JC/SP
 Sample : L4135-13DL 40X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 BG4A8DL

Manual Integrations
 APPROVED

MMDadoda
 10/1/2020 10:07:11 AM

Quant Time: Sep 30 07:13:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 07:04:14 2020
 Response via : Initial Calibration

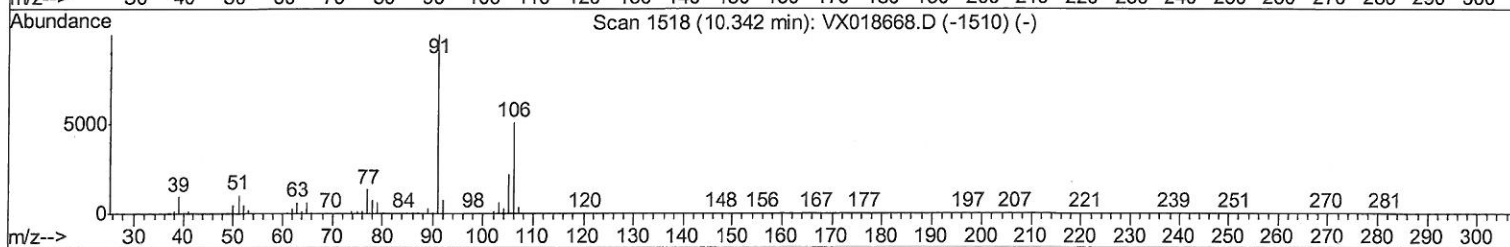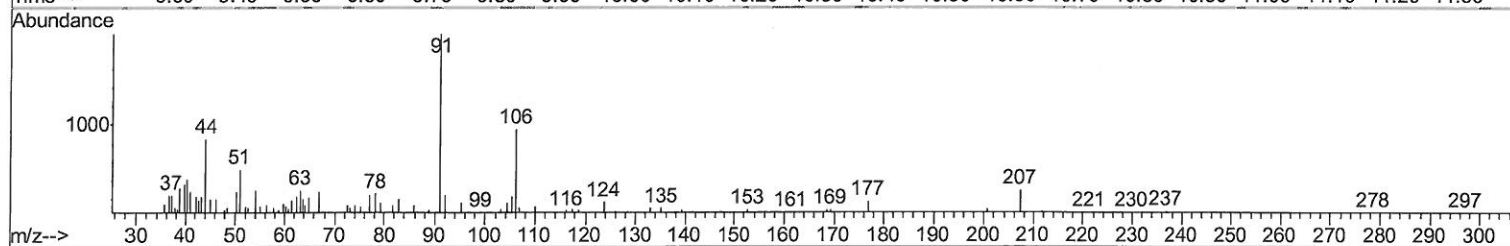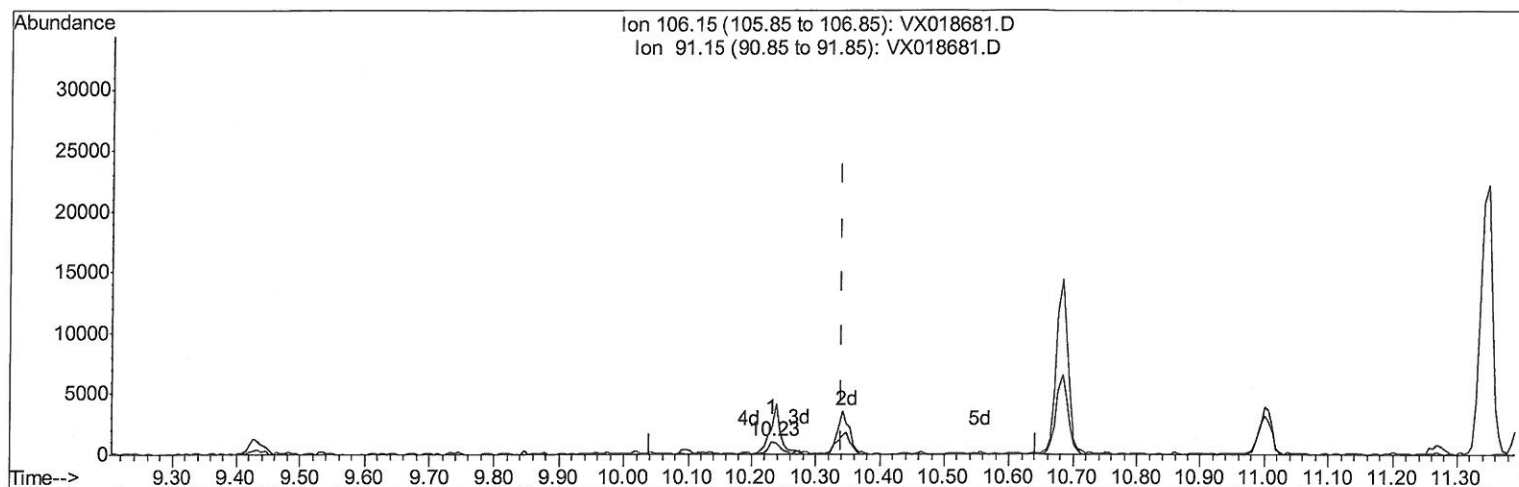

TIC: VX018681.D

(55) m,p-xylene (T)

10.232min (-0.110) 0.07ug/L

response 1380

Ion	Exp%	Act%
106.15	100	100
91.15	200.50	187.81
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092920\
 Data File : VX018681.D
 Acq On : 30 Sep 2020 01:32
 Operator : JC/SP
 Sample : L4135-13DL 40X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
ClientSampleId :
 BG4A8DL

Manual Integrations
APPROVED

MMDadoda
 10/1/2020 10:07:11 AM

Quant Time: Sep 30 07:13:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 07:04:14 2020
 Response via : Initial Calibration

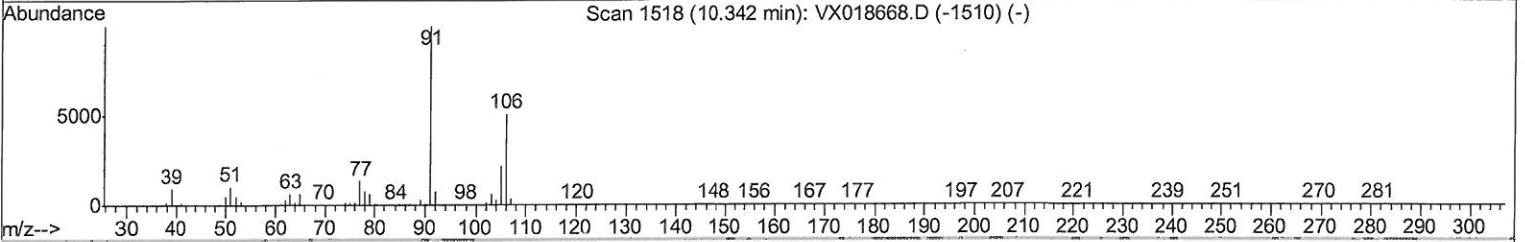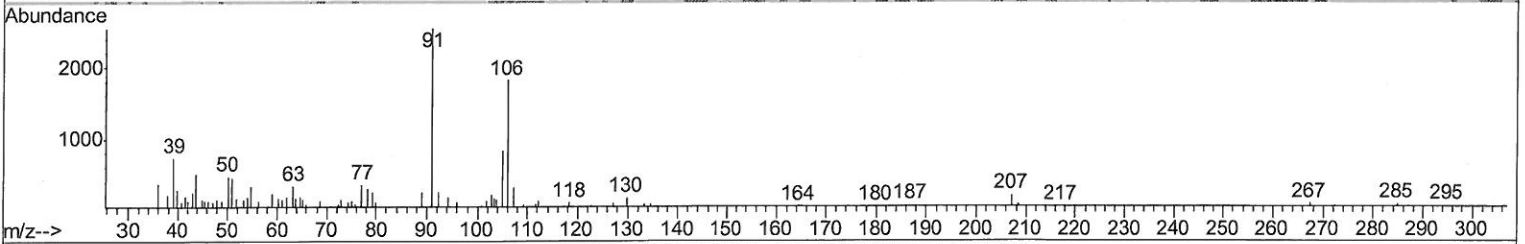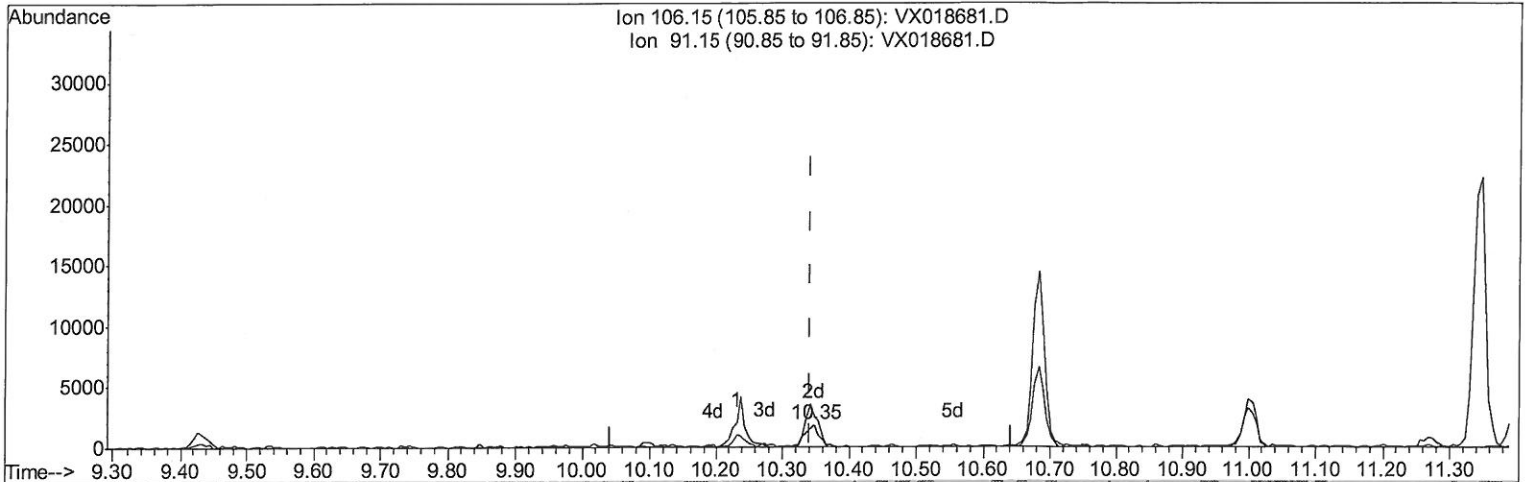

TIC: VX018681.D

(55) m,p-xylene (T)

10.347min (+0.006) 0.14ug/L m

response 2774

Ion	Exp%	Act%
106.15	100	100
91.15	200.50	139.75#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 7 mg
 10/06/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VO092920\
 Data File : VX018681.D
 Acq On : 30 Sep 2020 01:32
 Operator : JC/SP
 Sample : L4135-13DL 40X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 BG4A8DL

Manual Integrations
 APPROVED

MMDadoda
 10/1/2020 10:07:11 AM

Quant Time: Sep 30 08:43:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 07:04:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.83	114	239858	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	234230	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	105713	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	52015	4.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.80%
7) Chloroethane-d5	1.70	69	47883	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.34	63	98468	3.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.00%
20) 2-Butanone-d5	4.56	46	166868	52.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.28%
24) Chloroform-d	5.13	84	138074	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	6.03	65	78452	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
32) Benzene-d6	6.05	84	248304	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	7.37	67	74939	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	8.70	98	219999	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
45) trans-1,3-Dichloropropene-	8.99	79	31570	4.31	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.20%
48) 2-Hexanone-d5	9.43	63	127056	48.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.84%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	58653	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
65) 1,2-Dichlorobenzene-d4	12.36	152	85287	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Chloroethane	1.71	64	8068	1.130	ug/L	99
16) Methylene chloride	2.84	84	4478	0.280	ug/L	91
33) Benzene	6.12	78	157446	3.486	ug/L	100
53) Chlorobenzene	10.12	112	859767	26.681	ug/L	98
55) m,p-xylene	10.35	106	2774m	0.137	ug/L	99
56) o-xylene	10.68	106	8636	0.450	ug/L	88
58) Isopropylbenzene	11.01	105	56293	1.094	ug/L	99
64) 1,4-Dichlorobenzene	12.08	146	8275	0.356	ug/L	92
66) 1,2-Dichlorobenzene	12.37	146	4345	0.203	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed