

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VO092920\
 Data File : VX018647.D
 Acq On : 29 Sep 2020 11:00
 Operator : JC/SP
 Sample : L4135-05
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG4A9

Quant Time: Oct 05 02:04:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 04:47:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	305233	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	280903	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	130526	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	69716	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.70	69	59665	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.35	63	122280	3.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.40%
20) 2-Butanone-d5	4.55	46	209563	51.45	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.90%
24) Chloroform-d	5.14	84	168307	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	6.04	65	93465	4.24	ug/L	0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
32) Benzene-d6	6.05	84	319430	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	7.37	67	96642	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	8.70	98	299364	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
45) trans-1,3-Dichloropropene-	8.99	79	42179	4.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.00%
48) 2-Hexanone-d5	9.43	63	166864	53.03	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.06%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	72287	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
65) 1,2-Dichlorobenzene-d4	12.36	152	113007	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.45	43	17253	7.653 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092920\
Data File : VX018647.D
Acq On : 29 Sep 2020 11:00
Operator : JC/SP
Sample : L4135-05
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG4A9

Quant Time: Oct 05 02:04:09 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 04:47:32 2020
Response via : Initial Calibration

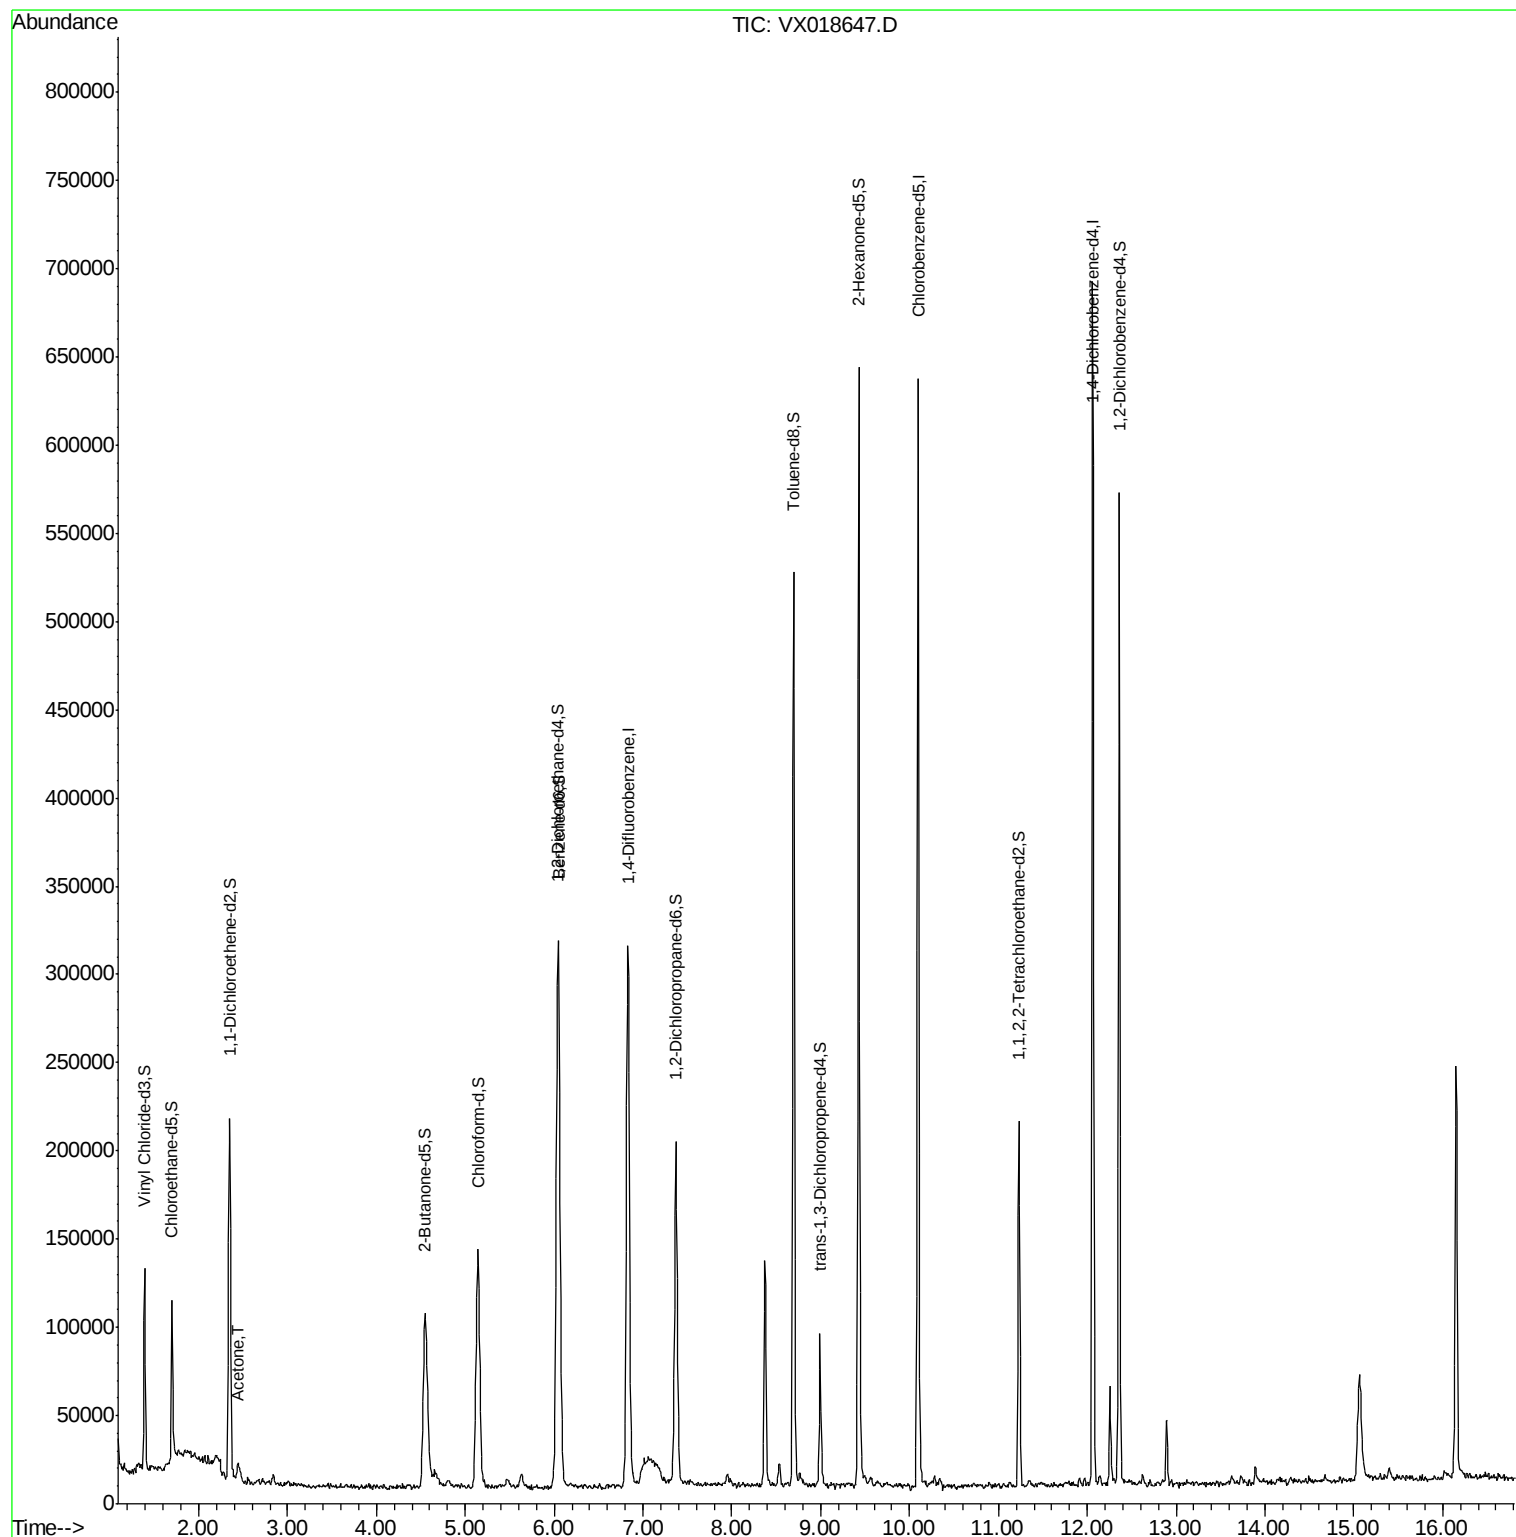

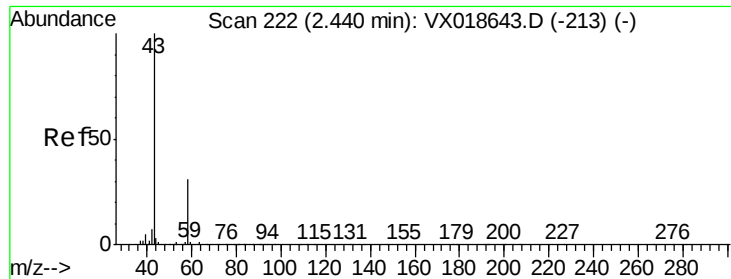

#13
 Acetone
 Concen: 7.653 ug/L
 RT: 2.45 min Scan# 223
 Delta R.T. 0.01 min
 Lab File: VX018647.D
 Acq: 29 Sep 2020 11:00

Instrument :
 MSVOA_X
 ClientSampleId :
 BG4A9

Tot Ion: 43 Resp: 17253
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 61.6

