

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
 Data File : VX031782.D
 Acq On : 29 Sep 2022 18:38
 Operator : JC/MD
 Sample : N4850-05RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14B-SP-2-GRRE

Quant Time: Sep 30 04:37:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 27 01:44:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	68110	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	109408	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	127009	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	80120	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	71005	49.119	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.240%		
35) Dibromofluoromethane	5.385	113	60201	46.180	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.360%		
50) Toluene-d8	8.647	98	219106	46.360	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	92.720%		
62) 4-Bromofluorobenzene	11.079	95	79504	45.897	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	91.800%		
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	697	Below Cal	#	41
5) Bromomethane	1.617	94	386	Below Cal	#	33
6) Chloroethane	1.764	64	127	Below Cal	#	49
8) Diethyl Ether	2.002	74	19	Below Cal	#	1
11) Tert butyl alcohol	2.940	59	3327	Below Cal	#	73
12) 1,1-Dichloroethene	2.099	96	20	Below Cal	#	1
13) Acrolein	2.117	56	19	Below Cal	#	15
16) Acetone	2.392	43	13838	24.170	ug/l	99
17) Carbon Disulfide	2.508	76	5459	2.144	ug/l	99
18) Methyl Acetate	2.703	43	2013	1.550	ug/l	99
20) Methylene Chloride	2.788	84	6968	6.138	ug/l	87
25) 2-Butanone	4.586	43	1476	2.139	ug/l	99
29) Tetrahydrofuran	5.019	42	306	0.706	ug/l #	83
31) Cyclohexane	5.550	56	1373	0.999	ug/l #	40
36) 1,1-Dichloropropene	5.550	75	5060	3.380	ug/l #	50
37) Ethyl Acetate	4.721	43	13679	9.058	ug/l #	93
38) Carbon Tetrachloride	5.550	117	6968	4.130	ug/l #	18
40) Benzene	6.031	78	1416	0.308	ug/l	95
41) Methacrylonitrile	5.032	41	254	0.331	ug/l #	32
43) Isopropyl Acetate	6.342	43	58760	24.723	ug/l #	94
48) Methyl methacrylate	7.799	41	43085	41.220	ug/l #	46
51) 4-Methyl-2-Pentanone	8.549	43	44554	29.616	ug/l #	52
52) Toluene	8.720	92	686	0.224	ug/l	82
53) t-1,3-Dichloropropene	8.958	75	132	1.953	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	23420	13.935	ug/l #	59
56) Ethyl methacrylate	9.250	69	565	0.335	ug/l #	1
57) 1,3-Dichloropropane	9.488	76	2031	0.972	ug/l #	43
59) 2-Hexanone	9.482	43	21698	19.331	ug/l #	55
76) 1,2,3-Trichloropropane	11.079	75	40201	27.677	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	40201	91.463	ug/l #	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031782.D
Acq On : 29 Sep 2022 18:38
Operator : JC/MD
Sample : N4850-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE

Quant Time: Sep 30 04:37:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 27 01:44:18 2022
Response via : Initial Calibration




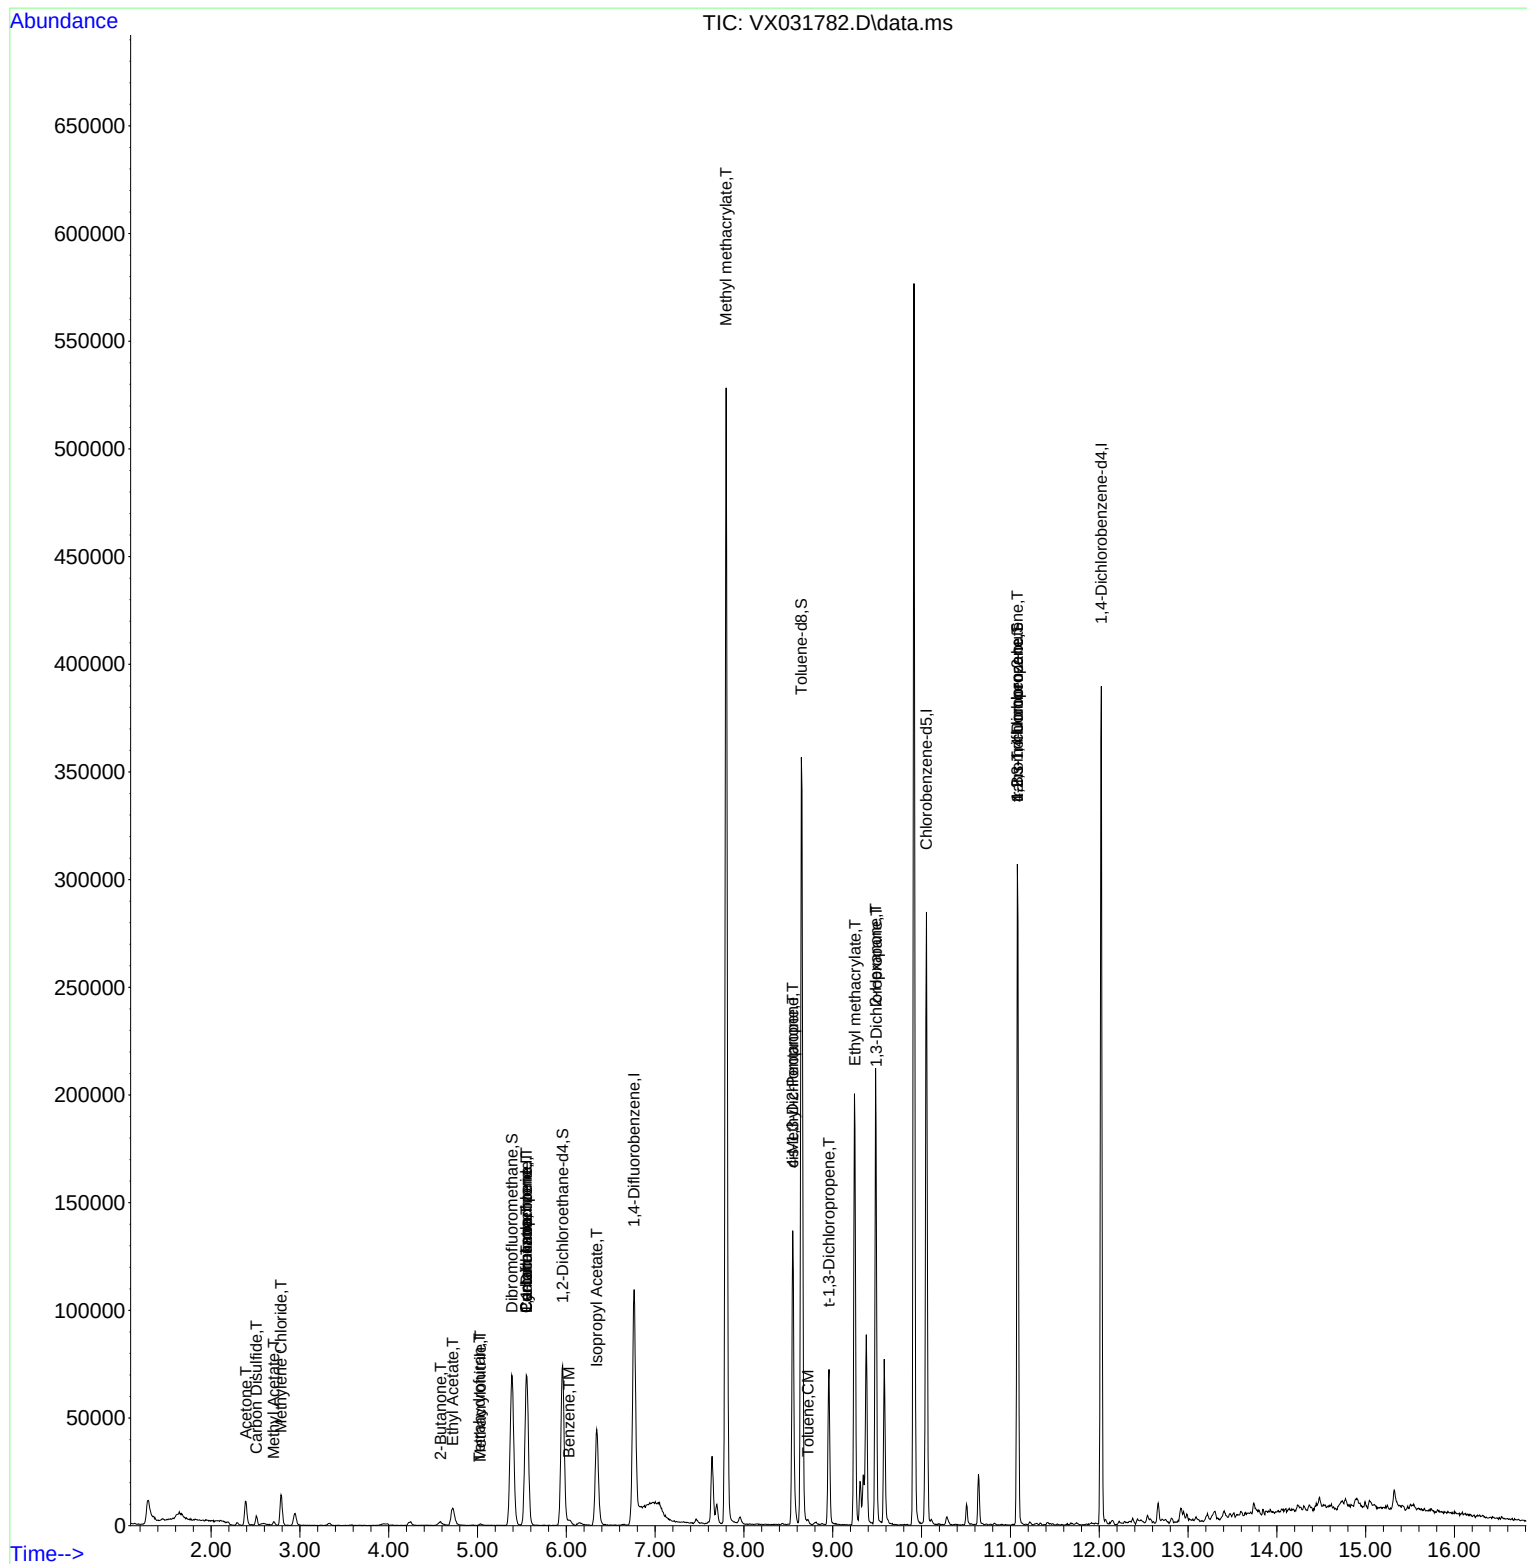


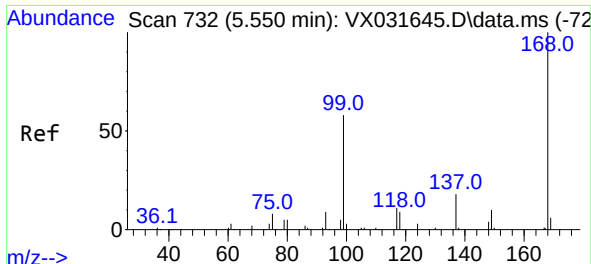

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion:168 Resp: 68110
Ion Ratio Lower Upper
168 100
99 58.1 48.8 73.2

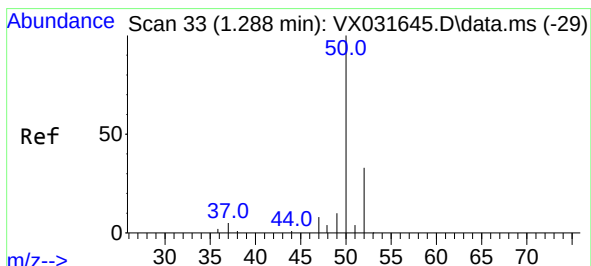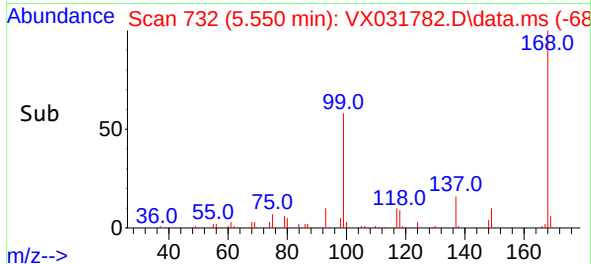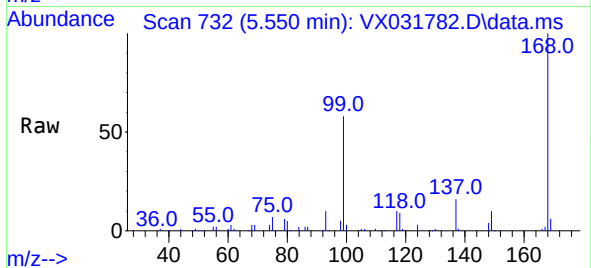

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 50 Resp: 697
Ion Ratio Lower Upper
50 100
52 0.0 26.9 40.3#


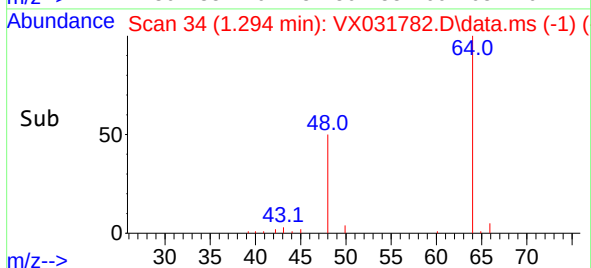
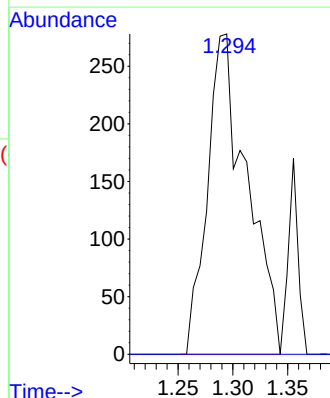
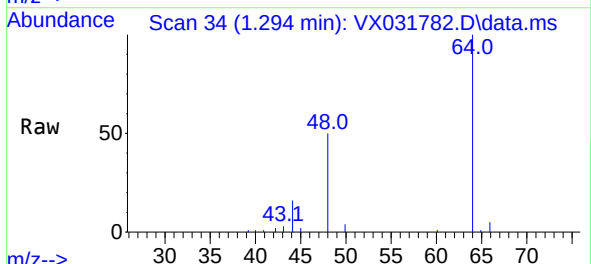


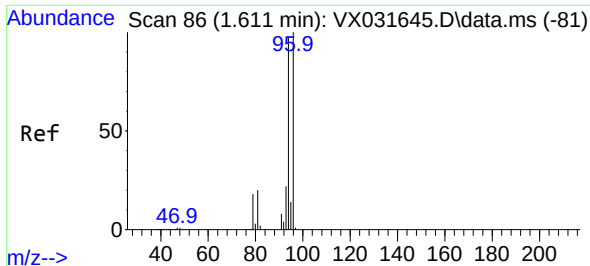

#5
Bromomethane
Concen: Below Cal
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 94 Resp: 386
Ion Ratio Lower Upper
94 100
96 156.9 74.4 111.6#

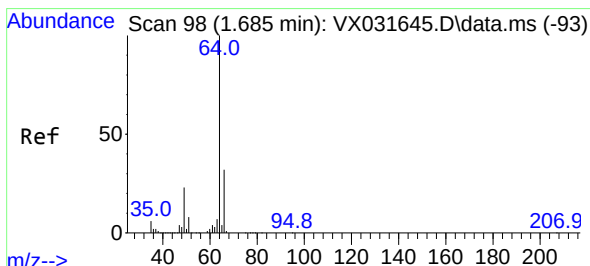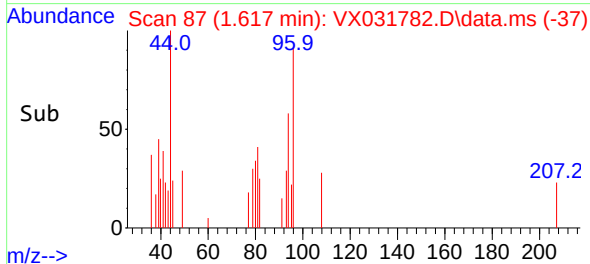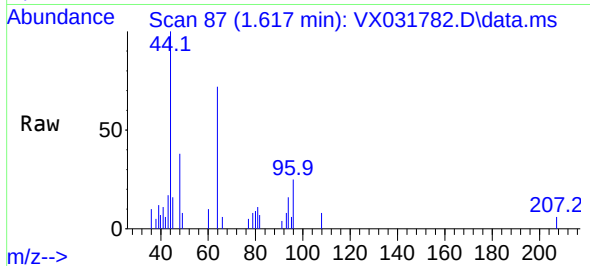

#6
Chloroethane
Concen: Below Cal
RT: 1.764 min Scan# 111
Delta R.T. 0.079 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 64 Resp: 127
Ion Ratio Lower Upper
64 100
66 2.9 25.0 37.4#


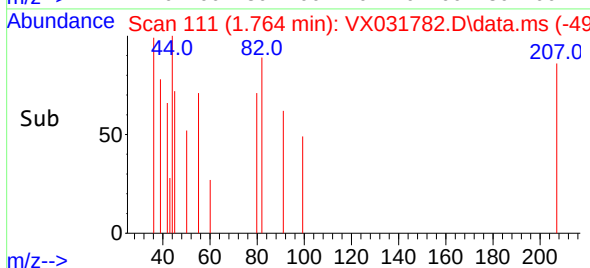
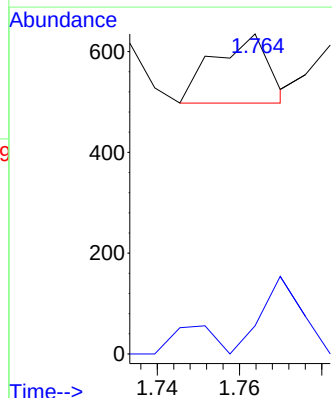
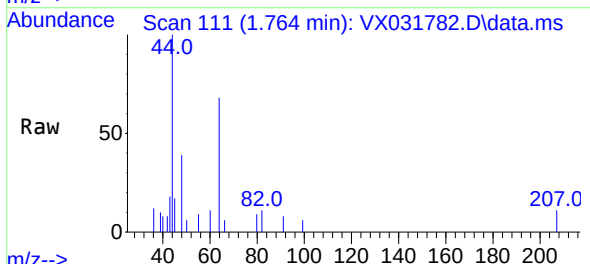




#8
Diethyl Ether
Concen: Below Cal
RT: 2.002 min Scan# 11
Delta R.T. -0.134 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 74 Resp: 19
Ion Ratio Lower Upper
74 100
45 1263.2 48.5 145.6#



#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.940 min Scan# 304
Delta R.T. -0.049 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 59 Resp: 3327
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#



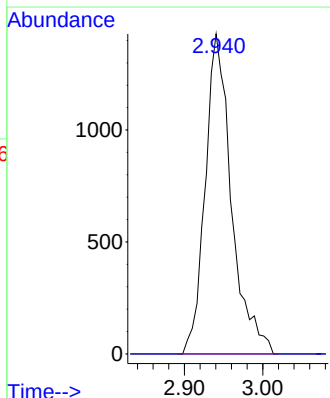





#12
1,1-Dichloroethene
Concen: Below Cal
RT: 2.099 min Scan# 1
Delta R.T. -0.220 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 96 Resp: 20
Ion Ratio Lower Upper
96 100
61 0.0 135.3 202.9#
98 0.0 49.4 74.2#



#13
Acrolein
Concen: Below Cal
RT: 2.117 min Scan# 169
Delta R.T. -0.122 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 56 Resp: 19
Ion Ratio Lower Upper
56 100
55 0.0 56.0 84.0#



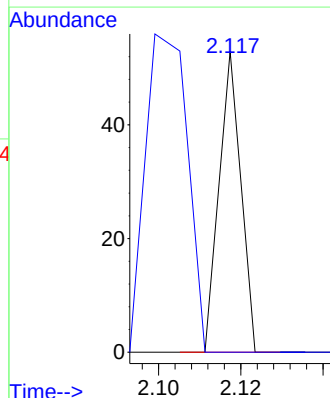



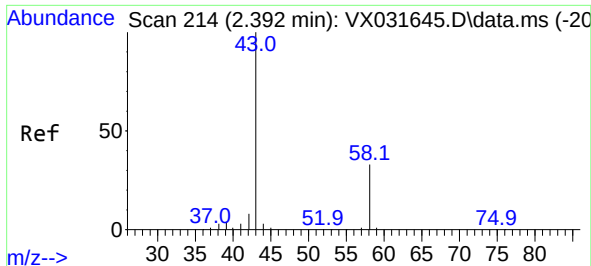

#16
Acetone
Concen: 24.170 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 43 Resp: 13838
Ion Ratio Lower Upper
43 100
58 29.5 23.8 35.8

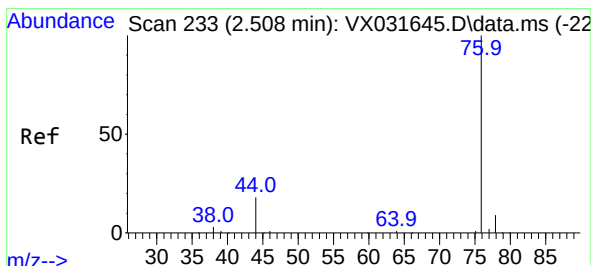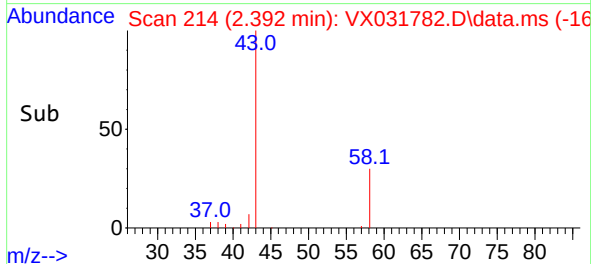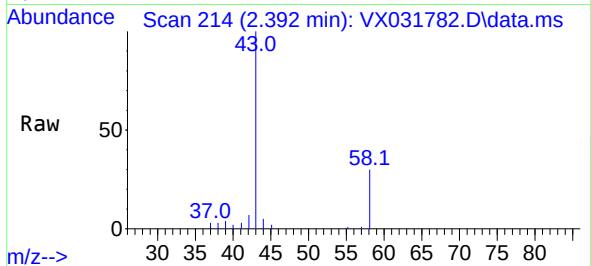

#17
Carbon Disulfide
Concen: 2.144 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 76 Resp: 5459
Ion Ratio Lower Upper
76 100
78 9.5 7.2 10.8


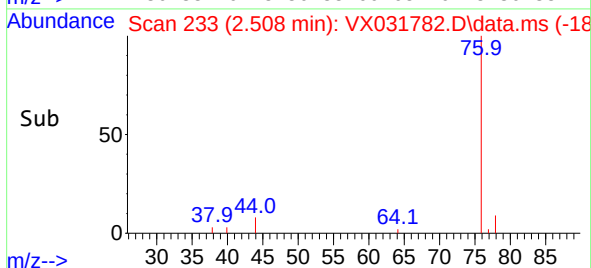
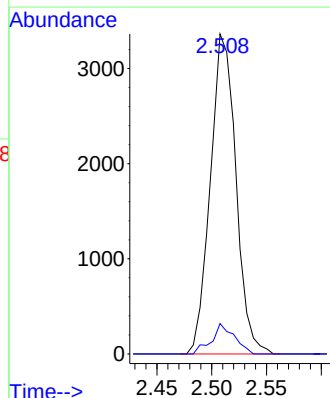
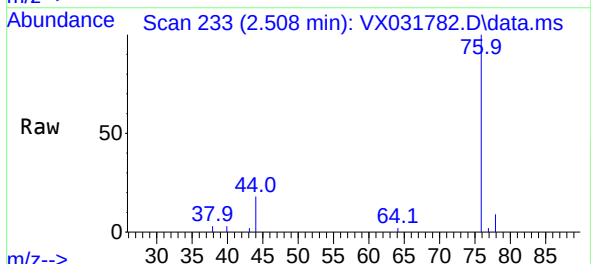


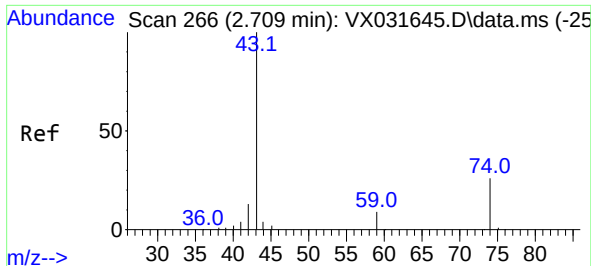

#18
Methyl Acetate
Concen: 1.550 ug/l
RT: 2.703 min Scan# 2013
Delta R.T. -0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 43 Resp: 2013
Ion Ratio Lower Upper
43 100
74 23.5 18.6 27.8

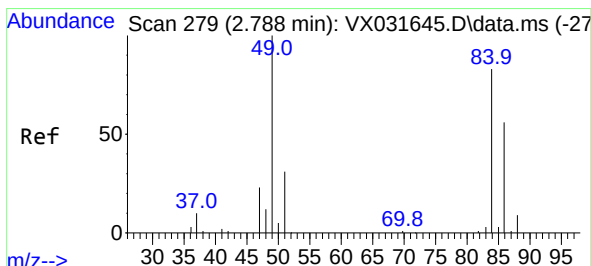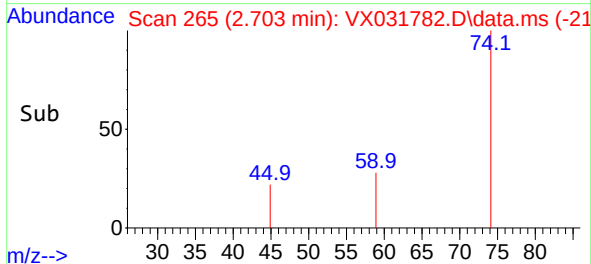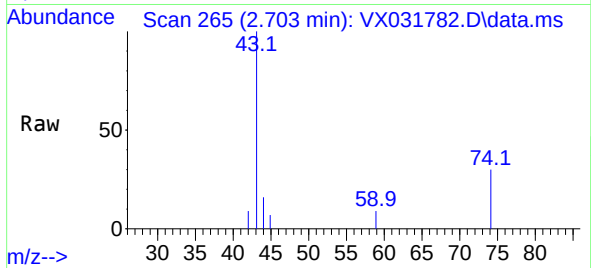

#20
Methylene Chloride
Concen: 6.138 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 84 Resp: 6968
Ion Ratio Lower Upper
84 100
49 107.2 105.9 158.9
51 36.9 32.2 48.2
86 64.9 50.8 76.2

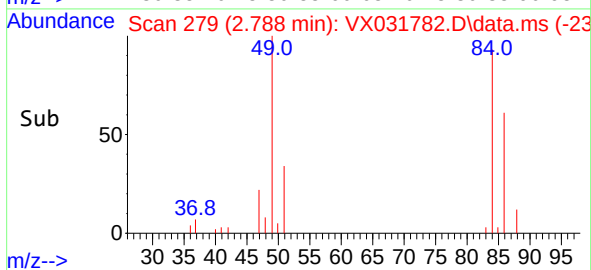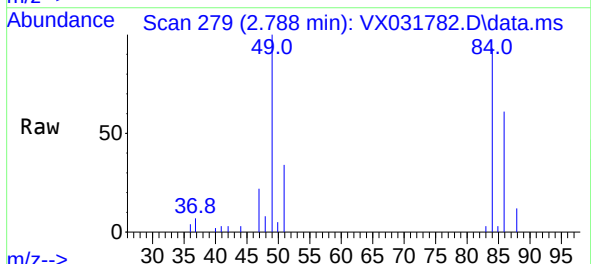



#25

2-Butanone

Concen: 2.139 ug/l

RT: 4.586 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Instrument :

MSVOA_X

ClientSampleId :





WC-14B-SP-2-GRRE

Tgt Ion: 43 Resp: 1476

Ion Ratio Lower Upper

43 100

72 26.7 21.1 31.7

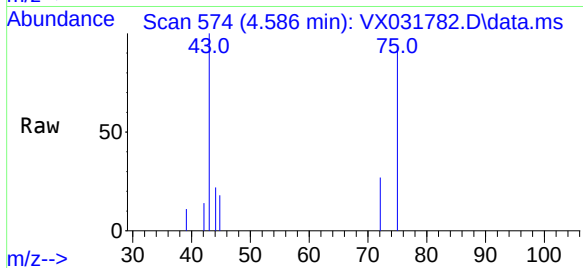

#29

Tetrahydrofuran

Concen: 0.706 ug/l

RT: 5.019 min Scan# 645

Delta R.T. 0.006 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38




Tgt Ion: 42 Resp: 306


Ion Ratio Lower Upper

42 100

72 58.8 36.4 54.6#


71 50.7 33.5 50.3#

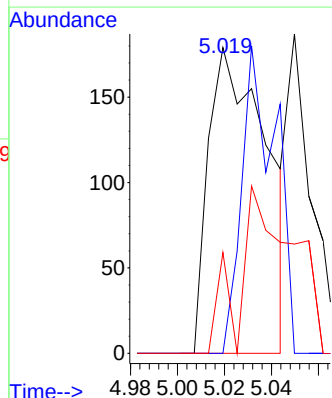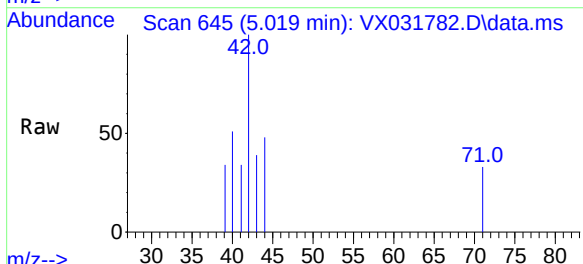



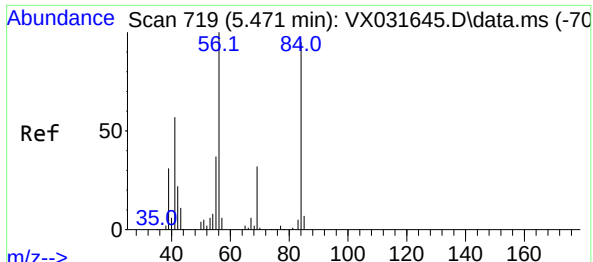


#31
Cyclohexane
Concen: 0.999 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE



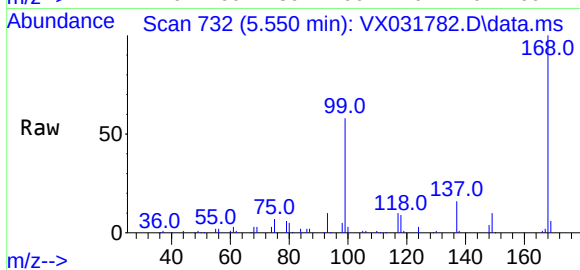



Tgt Ion: 56 Resp: 1373
Ion Ratio Lower Upper
56 100
69 153.6 25.1 37.7#
84 90.3 70.2 105.4



#33
1,2-Dichloroethane-d4
Concen: 49.119 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 65 Resp: 71005
Ion Ratio Lower Upper
65 100
67 50.5 0.0 102.4


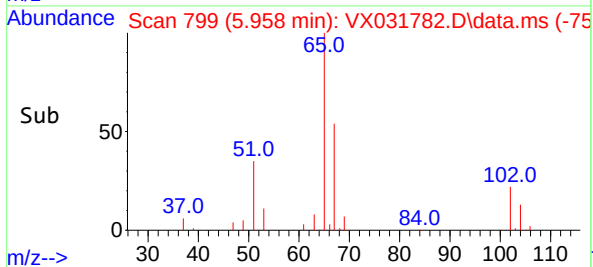

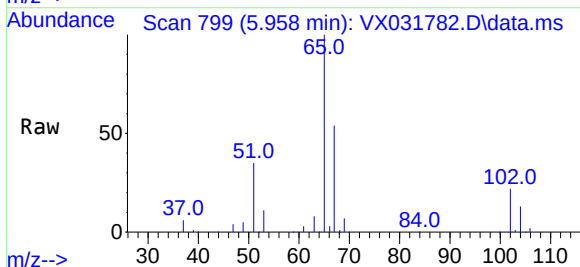


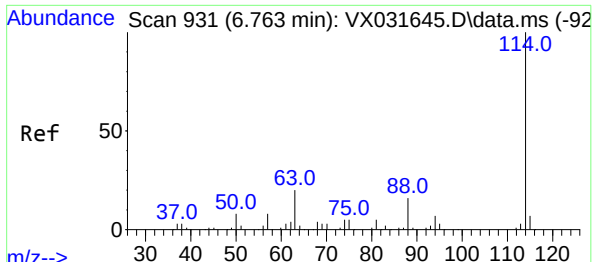

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion:114 Resp: 109408
Ion Ratio Lower Upper
114 100
63 15.7 0.0 42.6
88 15.3 0.0 33.0

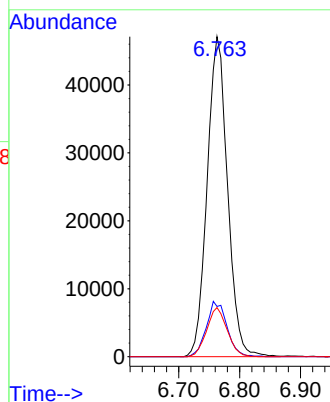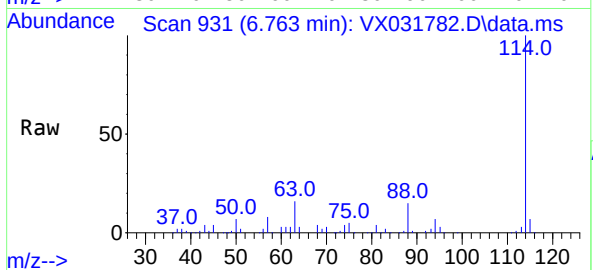

#35
Dibromofluoromethane
Concen: 46.180 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion:113 Resp: 60201
Ion Ratio Lower Upper
113 100
111 102.6 82.4 123.6
192 18.6 14.1 21.1


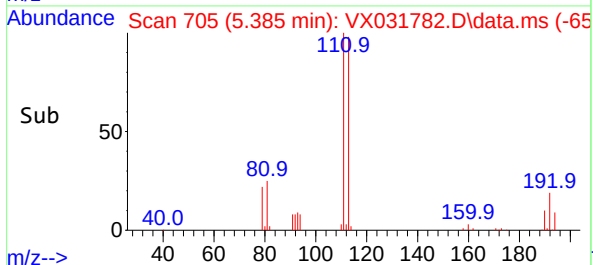

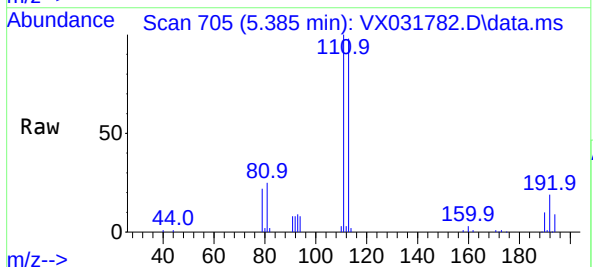




#36
1,1-Dichloropropene
Concen: 3.380 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion: 75 Resp: 5060
Ion Ratio Lower Upper
75 100
110 8.8 17.5 52.5#
77 0.0 24.9 37.3#

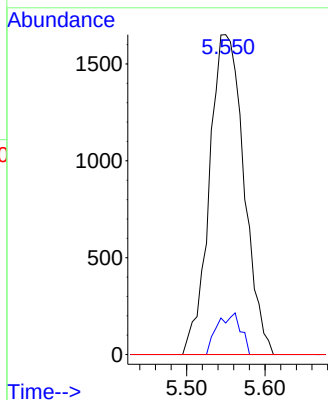

#37
Ethyl Acetate
Concen: 9.058 ug/l
RT: 4.721 min Scan# 596
Delta R.T. -0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38


Tgt Ion: 43 Resp: 13679
Ion Ratio Lower Upper
43 100
61 16.7 11.1 16.7
70 13.9 8.6 13.0#

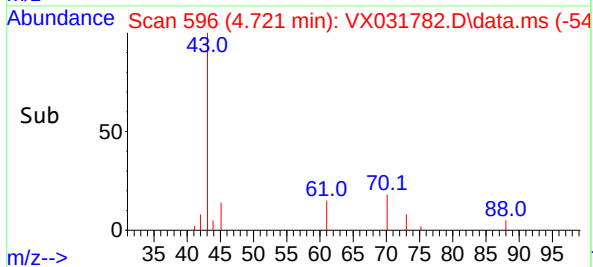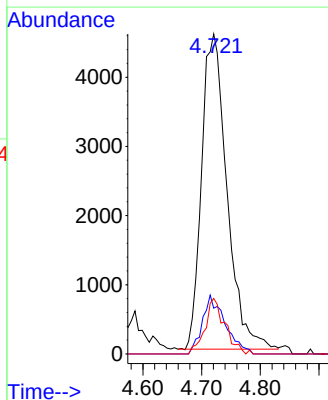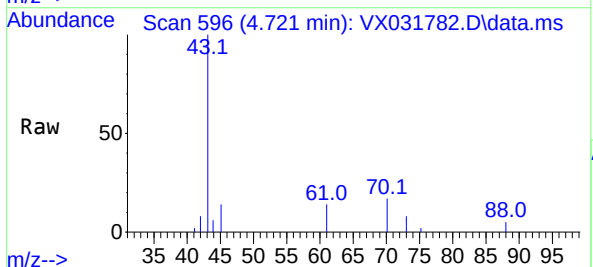






#38
Carbon Tetrachloride
Concen: 4.130 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE







Tgt Ion:117 Resp: 6968
Ion Ratio Lower Upper
117 100
119 6.6 74.6 112.0#
121 0.0 25.3 37.9#



#40
Benzene
Concen: 0.308 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.013 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 78 Resp: 1416
Ion Ratio Lower Upper
78 100
77 21.1 18.7 28.1

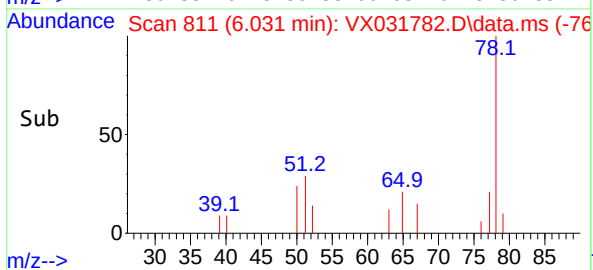




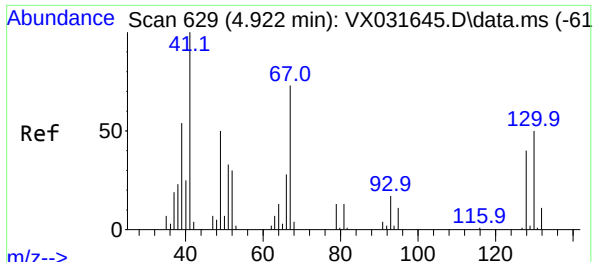


#41
Methacrylonitrile
Concen: 0.331 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.104 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE

Tgt Ion: 41 Resp: 254




Ion	Ratio	Lower	Upper
41	100		
39	19.7	45.0	67.6#
67	0.0	58.2	87.4#
52	0.0	25.0	37.6#

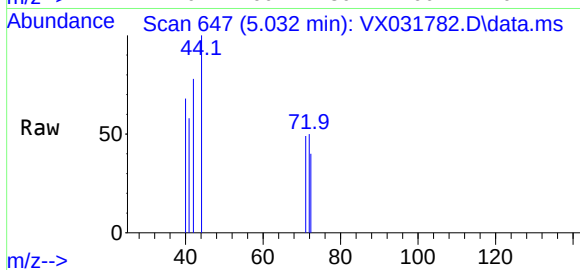


#43
Isopropyl Acetate
Concen: 24.723 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 43 Resp: 58760

Ion	Ratio	Lower	Upper
43	100		
61	21.4	15.3	22.9
87	16.3	10.6	15.8#

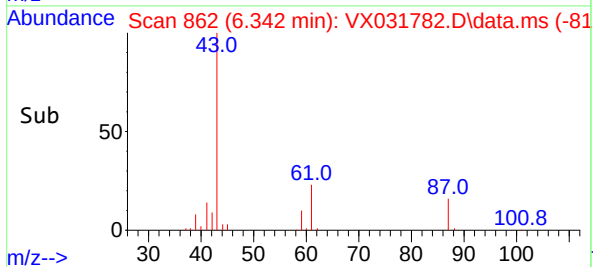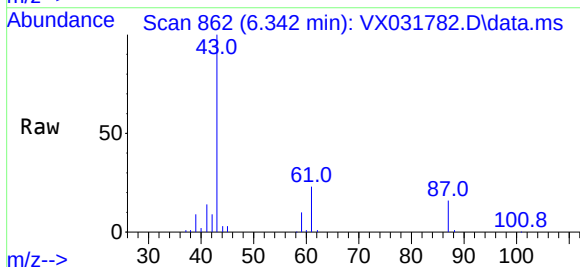



#48

Methyl methacrylate

Concen: 41.220 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.103 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Instrument :

MSVOA_X

ClientSampleId :

WC-14B-SP-2-GRRE





Tgt Ion: 41 Resp: 43085

Ion Ratio Lower Upper

41 100

69 0.1 64.6 96.8#

39 58.1 51.4 77.0

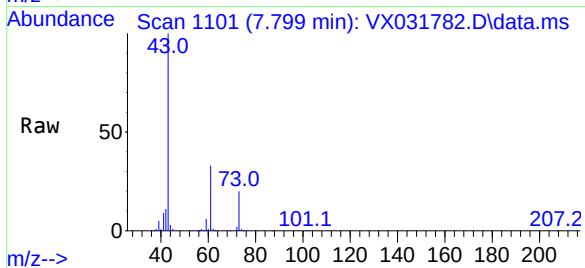

#50

Toluene-d8

Concen: 46.360 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX031782.D




Acq: 29 Sep 2022 18:38


Tgt Ion: 98 Resp: 219106

Ion Ratio Lower Upper

98 100

100 65.7 52.5 78.7

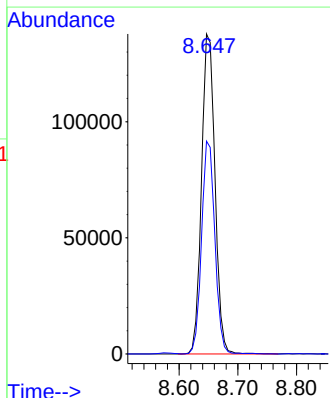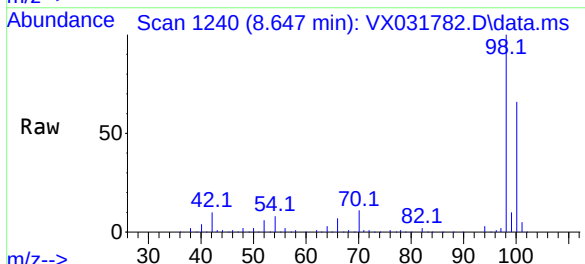



#51

4-Methyl-2-Pentanone

Concen: 29.616 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.031 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Instrument :

MSVOA_X

ClientSampleId :





WC-14B-SP-2-GRRE

Tgt Ion: 43 Resp: 44554

Ion Ratio Lower Upper

43 100

58 9.0 30.6 46.0#

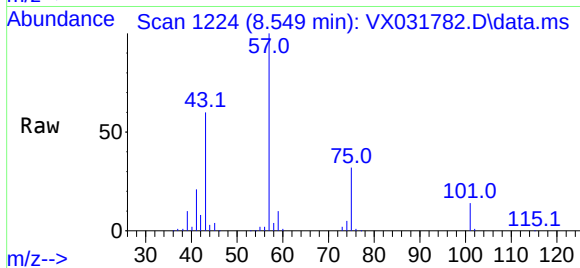

#52

Toluene

Concen: 0.224 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031782.D




Acq: 29 Sep 2022 18:38


Tgt Ion: 92 Resp: 686

Ion Ratio Lower Upper

92 100

91 146.9 137.1 205.7

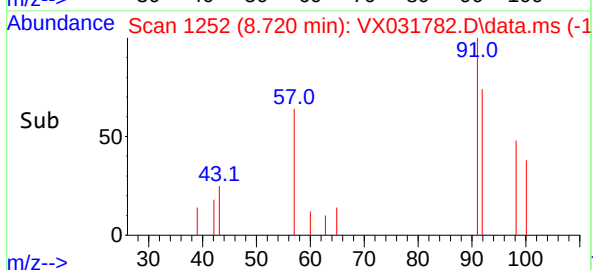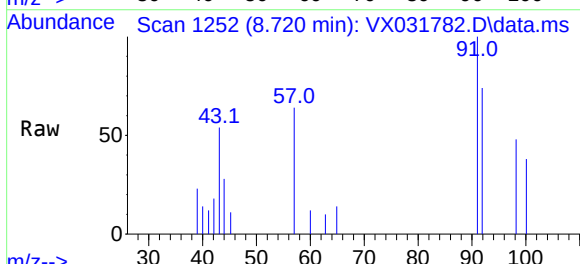



#53

t-1,3-Dichloropropene

Concen: 1.953 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Instrument :

MSVOA_X

ClientSampleId :





WC-14B-SP-2-GRRE

Tgt Ion: 75 Resp: 132

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

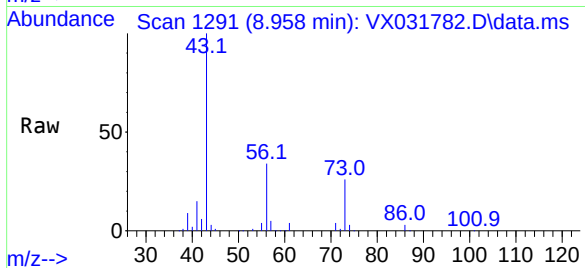

#54

cis-1,3-Dichloropropene

Concen: 13.935 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38




Tgt Ion: 75 Resp: 23420


Ion Ratio Lower Upper

75 100

77 0.6 24.4 36.6#

39 30.4 43.7 65.5#

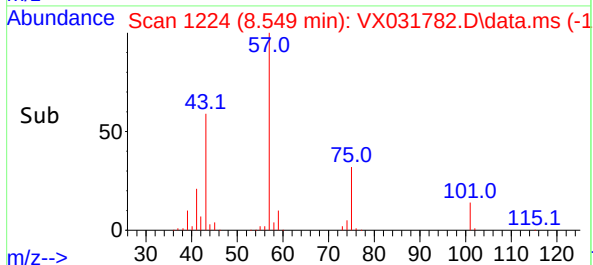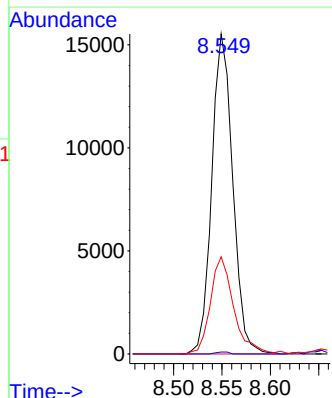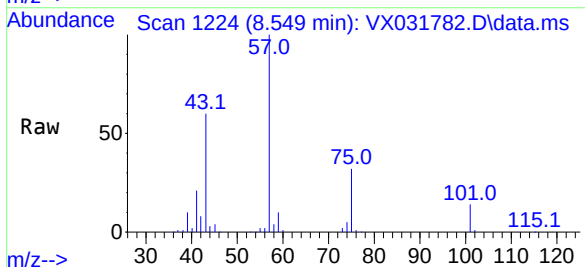



#56

Ethyl methacrylate

Concen: 0.335 ug/l

RT: 9.250 min Scan# 11

Delta R.T. 0.134 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38





Instrument :

MSVOA_X

ClientSampleId :

WC-14B-SP-2-GRRE

Tgt Ion:	69	Resp:	565
Ion	Ratio	Lower	Upper
69	100		
41	5561.8	54.2	81.4#
39	2458.4	34.2	51.2#



#57

1,3-Dichloropropane

Concen: 0.972 ug/l




RT: 9.488 min Scan# 1378


Delta R.T. 0.177 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Tgt Ion:	76	Resp:	2031
Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.5	38.3#

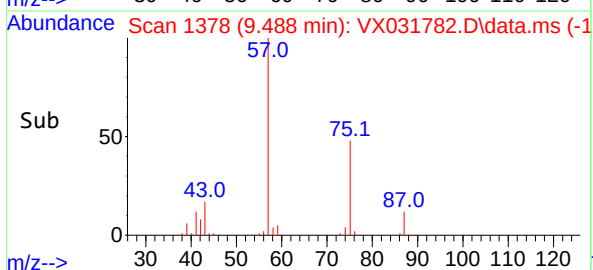



#59

2-Hexanone

Concen: 19.331 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.049 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38

Instrument :

MSVOA_X

ClientSampleId :





WC-14B-SP-2-GRRE

Tgt Ion: 43 Resp: 21698

Ion Ratio Lower Upper

43 100

58 21.5 26.7 80.0#

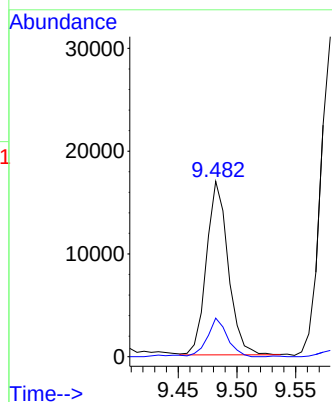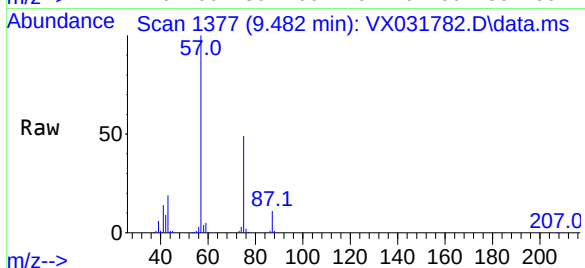

#62

4-Bromofluorobenzene

Concen: 45.897 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX031782.D

Acq: 29 Sep 2022 18:38




Tgt Ion: 95 Resp: 79504


Ion Ratio Lower Upper

95 100

174 82.3 0.0 153.2

176 79.8 0.0 144.0


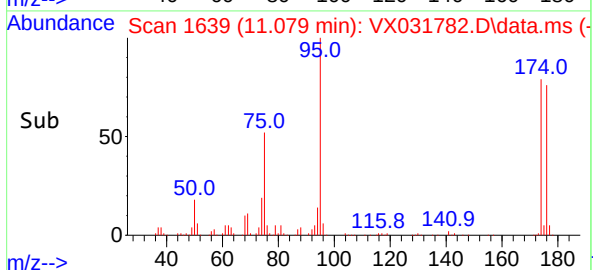

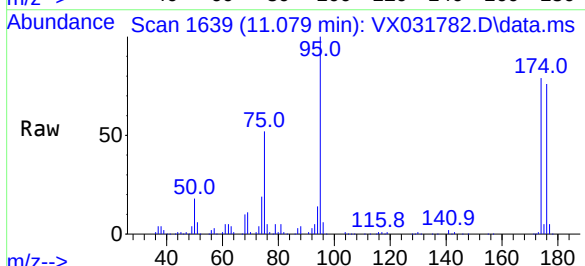


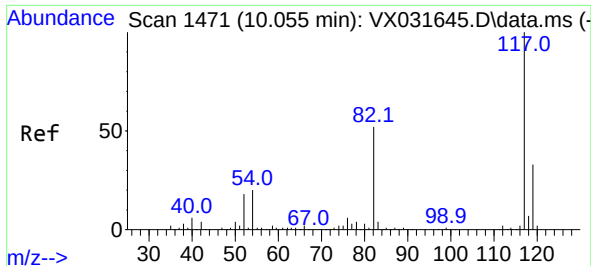

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38




Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE


Tgt Ion:117 Resp: 127009
Ion Ratio Lower Upper
117 100
82 50.9 46.8 70.2
119 32.1 26.4 39.6

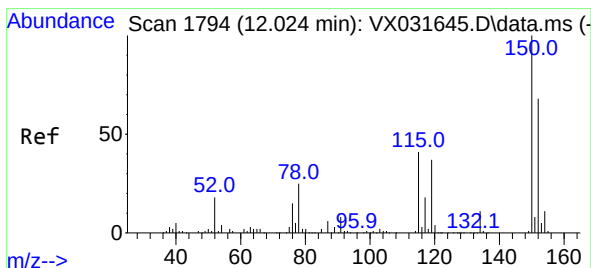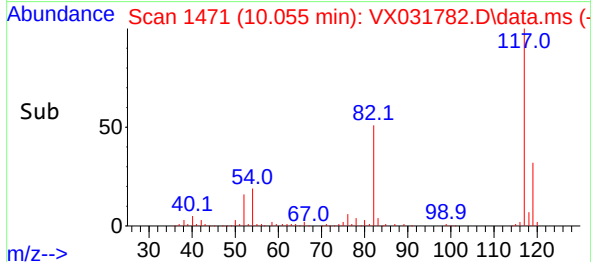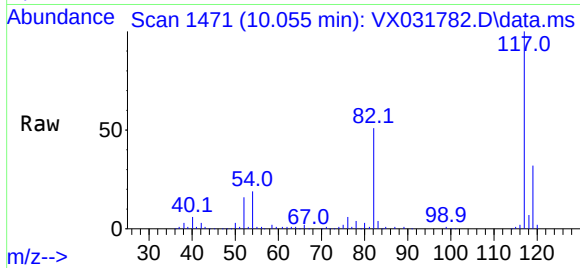

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion:152 Resp: 80120
Ion Ratio Lower Upper
152 100
115 59.7 43.4 130.1
150 159.5 0.0 346.8


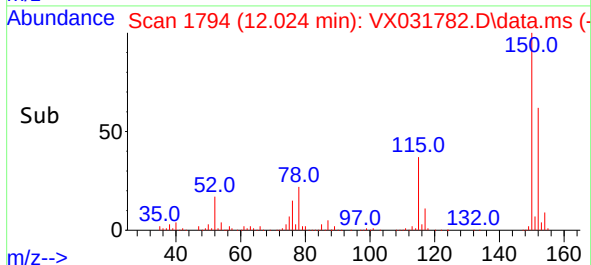
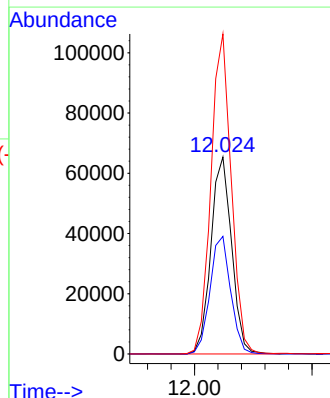
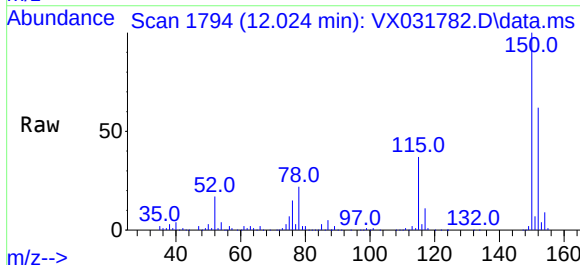


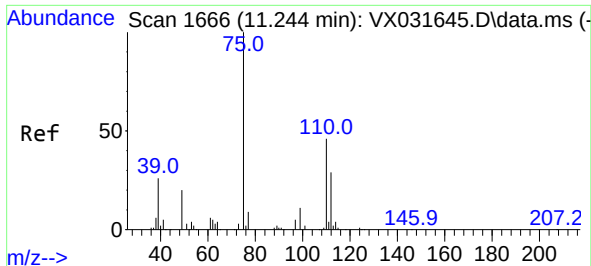

#76
1,2,3-Trichloropropane
Concen: 27.677 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Instrument :
MSVOA_X
ClientSampleId :
WC-14B-SP-2-GRRE

Tgt Ion: 75 Resp: 40201
Ion Ratio Lower Upper
75 100
77 1.1 20.3 60.9#

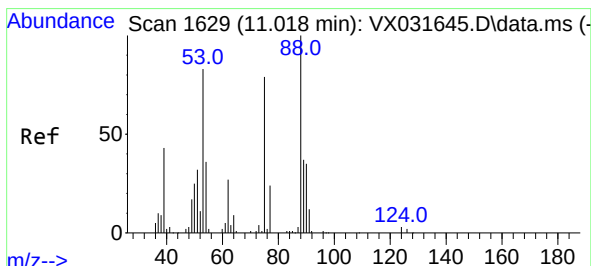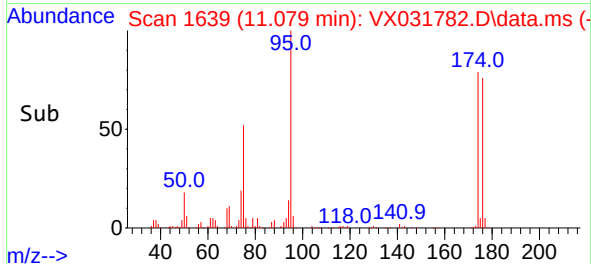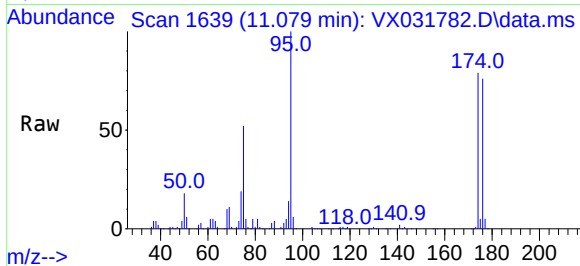

#81
trans-1,4-Dichloro-2-butene
Concen: 91.463 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031782.D
Acq: 29 Sep 2022 18:38

Tgt Ion: 75 Resp: 40201
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

