

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
 Data File : VX031798.D
 Acq On : 30 Sep 2022 04:34
 Operator : JC/MD
 Sample : N4864-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-7

Quant Time: Sep 30 06:26:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 27 01:44:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	68508	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	108461	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	116918	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	76924	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	70665	48.600	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.200%
35) Dibromofluoromethane	5.385	113	61422	47.528	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.060%
50) Toluene-d8	8.647	98	217175	46.353	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.700%
62) 4-Bromofluorobenzene	11.079	95	77739	45.270	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.540%
Target Compounds						
					Qvalue	
3) Chloromethane	1.294	50	88	Below Cal	#	41
5) Bromomethane	1.618	94	731	Below Cal		97
6) Chloroethane	1.654	64	102	Below Cal	#	43
11) Tert butyl alcohol	2.941	59	3285	Below Cal	#	73
13) Acrolein	2.337	56	240	Below Cal	#	36
14) Allyl chloride	2.776	41	1485	1.239 ug/l	#	70
16) Acetone	2.392	43	1837	Below Cal	#	85
17) Carbon Disulfide	2.508	76	356	Below Cal	#	75
18) Methyl Acetate	2.782	43	3295	2.522 ug/l	#	52
20) Methylene Chloride	2.788	84	184	Below Cal	#	74
25) 2-Butanone	4.574	43	473	0.682 ug/l	#	49
36) 1,1-Dichloropropene	5.550	75	5265	3.547 ug/l	#	49
38) Carbon Tetrachloride	5.550	117	7165	4.284 ug/l	#	18
39) Methylcyclohexane	7.379	83	663	0.392 ug/l		90
51) 4-Methyl-2-Pentanone	8.641	43	831	0.557 ug/l	#	1
55) 1,1,2-Trichloroethane	9.104	97	590	0.451 ug/l	#	15
67) Ethyl Benzene	10.195	91	15748	2.842 ug/l		95
68) m/p-Xylenes	10.305	106	484	0.217 ug/l		90
73) Isopropylbenzene	10.963	105	11151	2.242 ug/l		97
76) 1,2,3-Trichloropropane	11.079	75	39901	28.612 ug/l	#	37
78) n-propylbenzene	11.305	91	13179	2.381 ug/l		100
79) 2-Chlorotoluene	11.305	91	13179	3.855 ug/l	#	40
80) 1,3,5-Trimethylbenzene	11.616	105	3097	0.734 ug/l		77
81) trans-1,4-Dichloro-2-b...	11.079	75	39901	94.450 ug/l	#	11
82) 4-Chlorotoluene	11.305	91	13179	3.337 ug/l	#	44
85) sec-Butylbenzene	11.890	105	3311	0.641 ug/l	#	65
86) p-Isopropyltoluene	12.177	119	1270	0.285 ug/l		95
89) n-Butylbenzene	12.335	91	2219	0.610 ug/l	#	47
90) Hexachloroethane	12.616	117	1198	1.676 ug/l	#	15
95) Naphthalene	13.774	128	84870	17.696 ug/l		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031798.D
Acq On : 30 Sep 2022 04:34
Operator : JC/MD
Sample : N4864-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Quant Time: Sep 30 06:26:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 27 01:44:18 2022
Response via : Initial Calibration




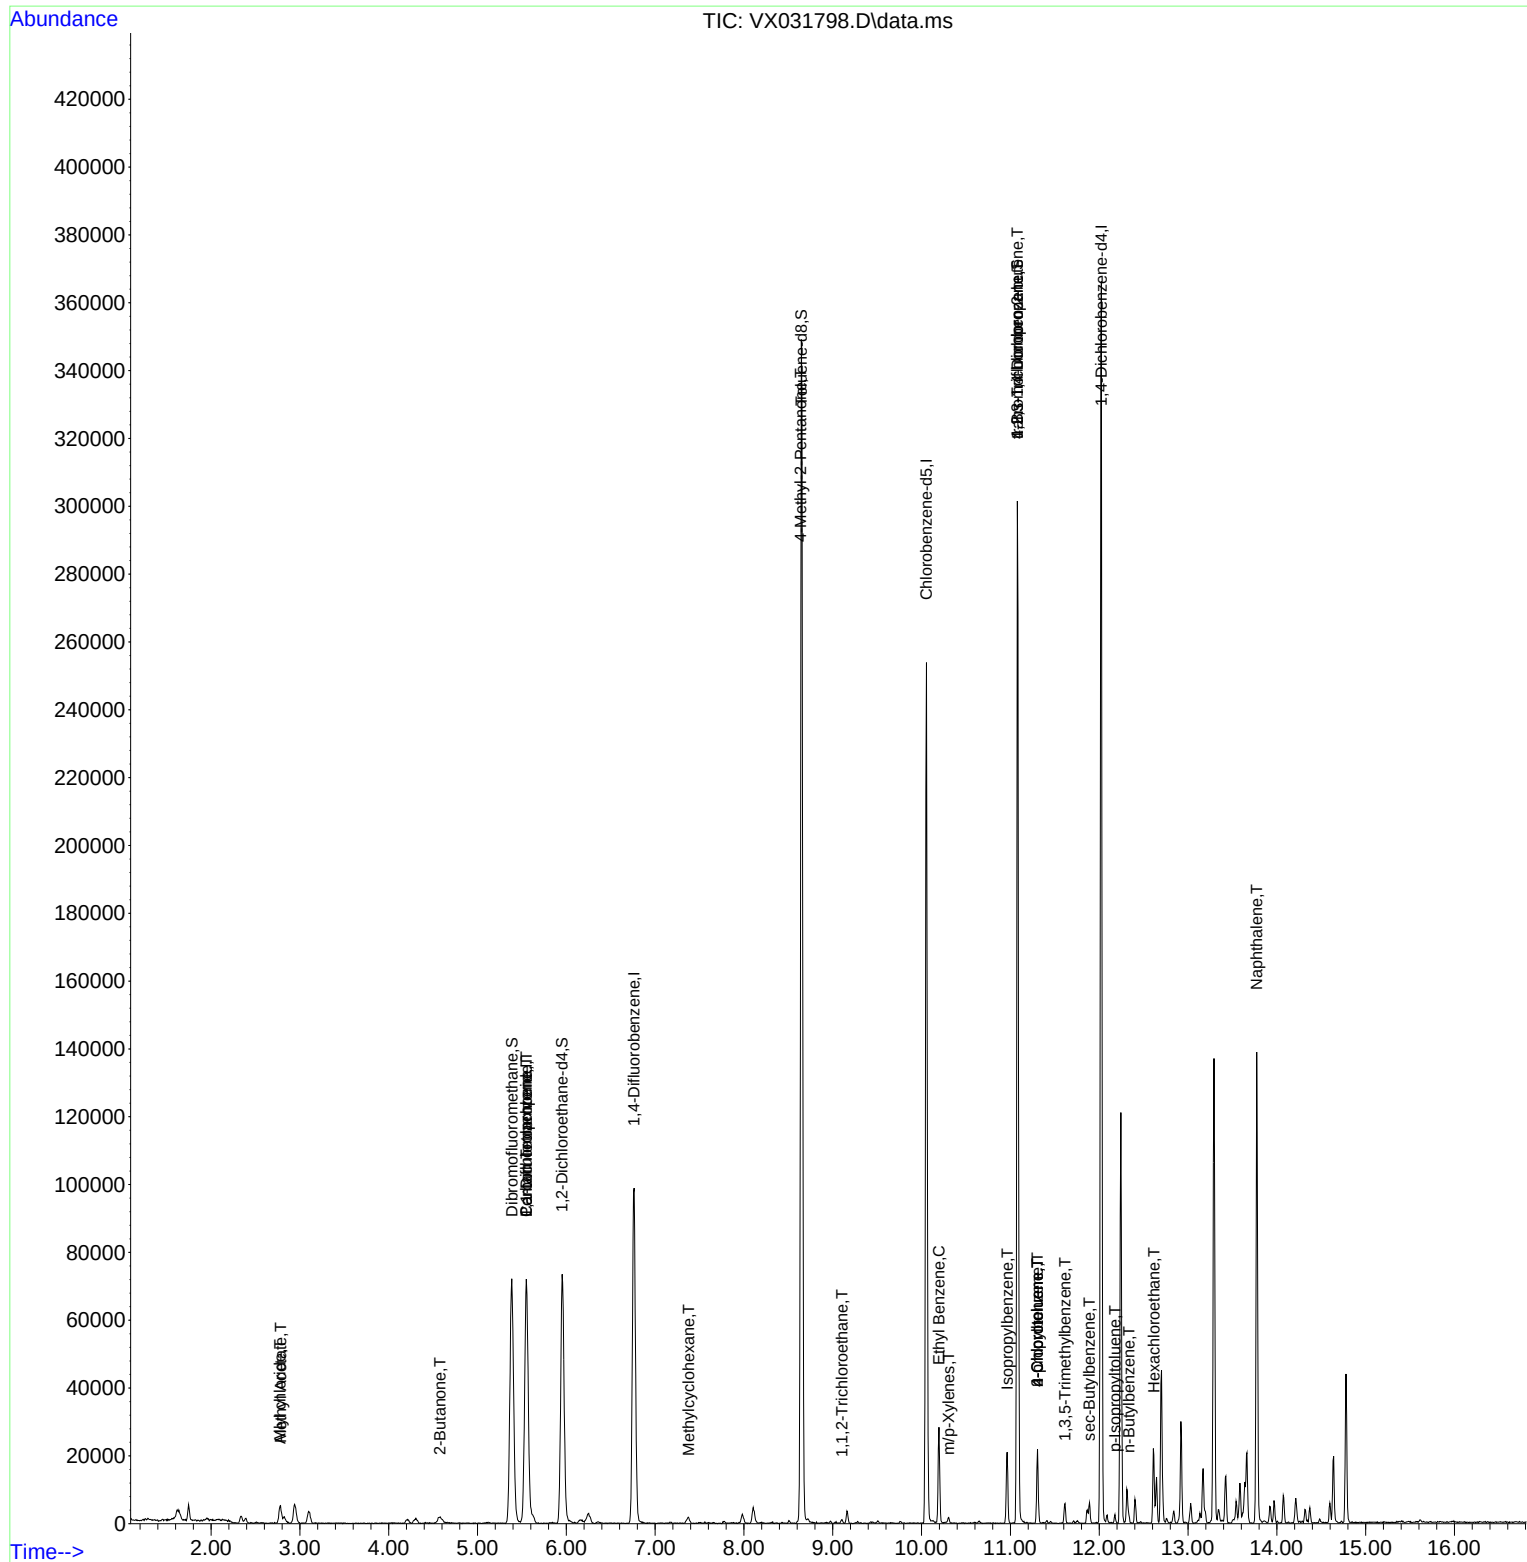


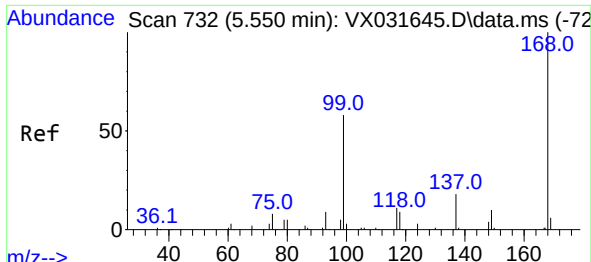

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:168 Resp: 68508
Ion Ratio Lower Upper
168 100
99 64.2 48.8 73.2

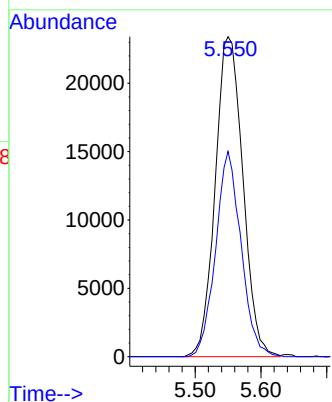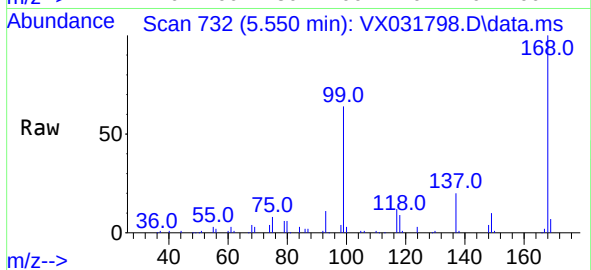

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 50 Resp: 88
Ion Ratio Lower Upper
50 100
52 0.0 26.9 40.3#


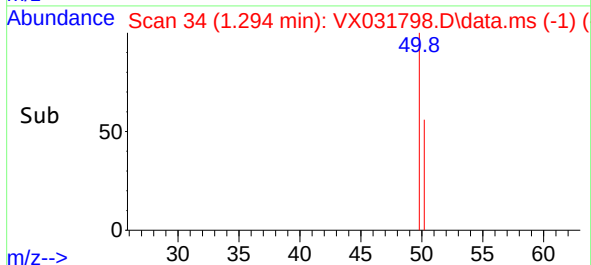

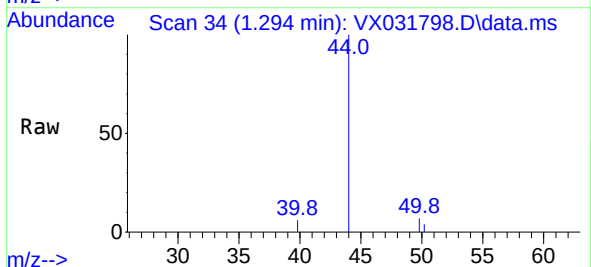


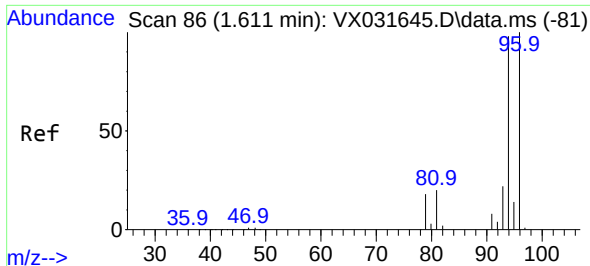

#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 81
Delta R.T. 0.007 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion: 94 Resp: 731
Ion Ratio Lower Upper
94 100
96 95.9 74.4 111.6

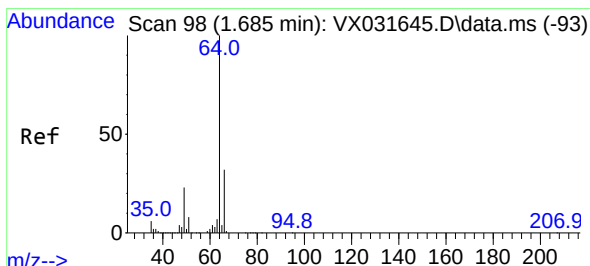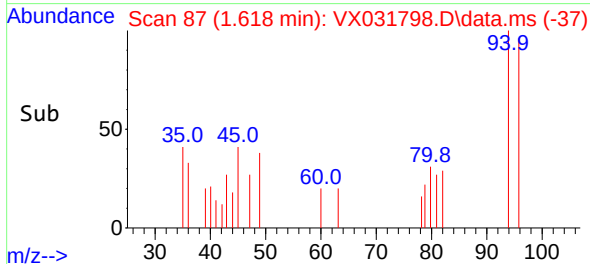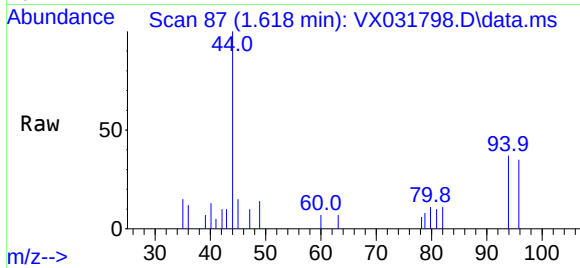

#6
Chloroethane
Concen: Below Cal
RT: 1.654 min Scan# 93
Delta R.T. -0.031 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 64 Resp: 102
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

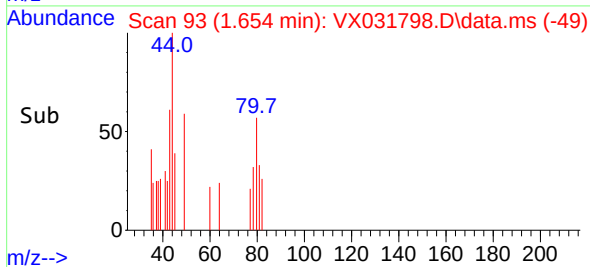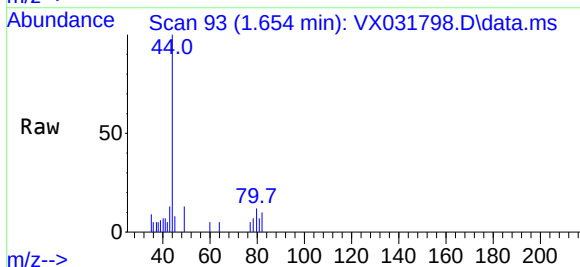



#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.941 min Scan# 30

Delta R.T. -0.048 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34

Instrument :

MSVOA_X

ClientSampleId :





MW-7

Tgt Ion: 59 Resp: 3285

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

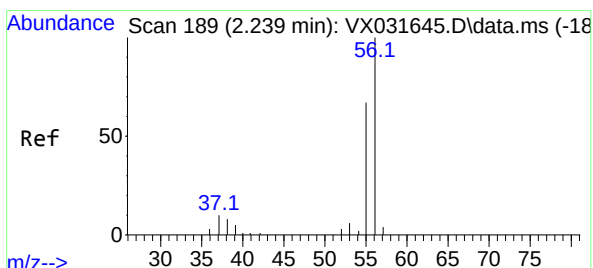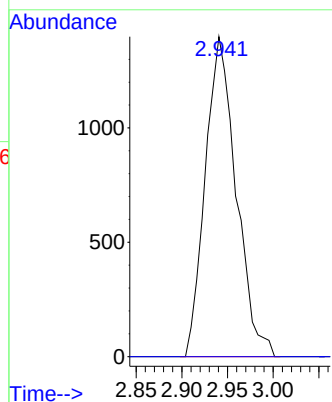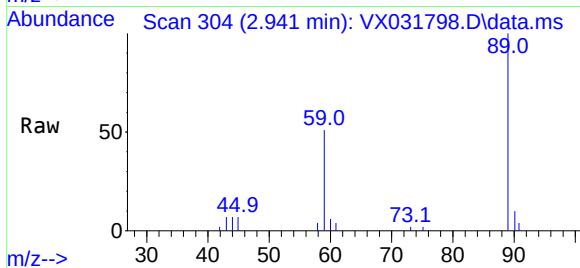

#13

Acrolein

Concen: Below Cal

RT: 2.337 min Scan# 205

Delta R.T. 0.098 min

Lab File: VX031798.D




Acq: 30 Sep 2022 04:34


Tgt Ion: 56 Resp: 240

Ion Ratio Lower Upper

56 100

55 17.5 56.0 84.0#


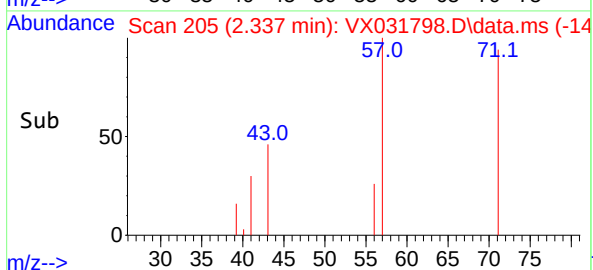

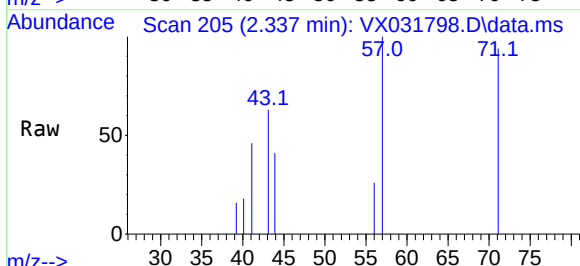




#14
 Allyl chloride
 Concen: 1.239 ug/l
 RT: 2.776 min Scan# 214
 Delta R.T. 0.110 min
 Lab File: VX031798.D
 Acq: 30 Sep 2022 04:34




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-7


Tgt Ion: 41 Resp: 1485
 Ion Ratio Lower Upper
 41 100
 39 58.9 58.2 87.4
 76 0.0 26.9 40.3#

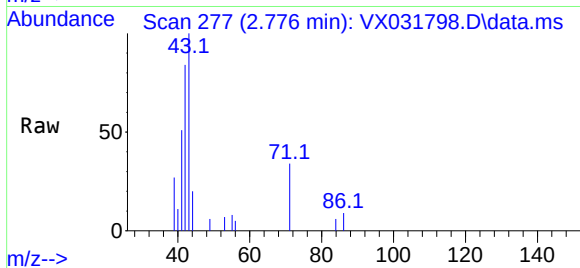

#16
 Acetone
 Concen: Below Cal
 RT: 2.392 min Scan# 214
 Delta R.T. 0.006 min
 Lab File: VX031798.D
 Acq: 30 Sep 2022 04:34

Tgt Ion: 43 Resp: 1837
 Ion Ratio Lower Upper
 43 100
 58 22.0 23.8 35.8#


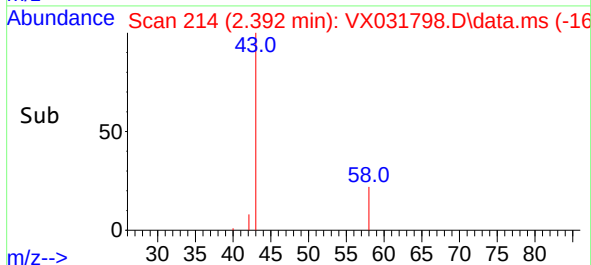

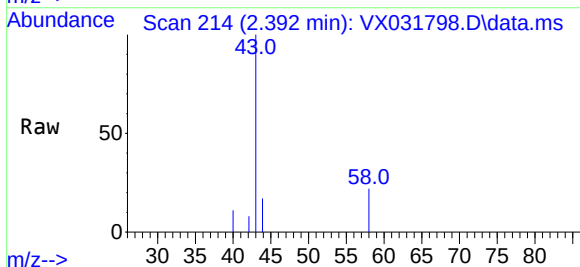


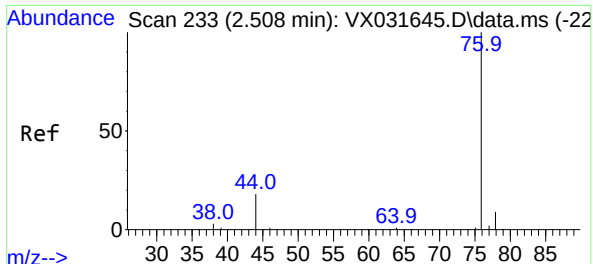

#17
Carbon Disulfide
Concen: Below Cal
RT: 2.508 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion: 76 Resp: 356
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#



#18
Methyl Acetate
Concen: 2.522 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.073 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 43 Resp: 3295
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#

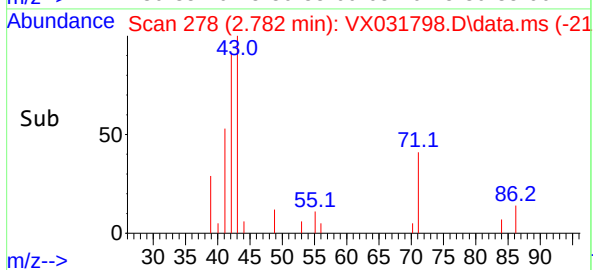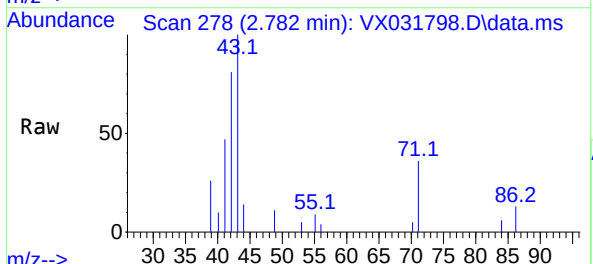

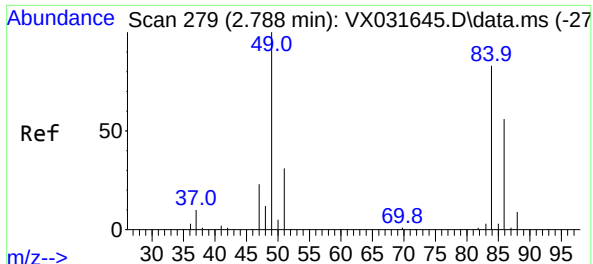

#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34

Instrument :

MSVOA_X

ClientSampleId :

MW-7

Tgt Ion: 84 Resp: 184





Ion Ratio Lower Upper

84 100

49 136.5 105.9 158.9

51 0.0 32.2 48.2#

86 100.0 50.8 76.2#

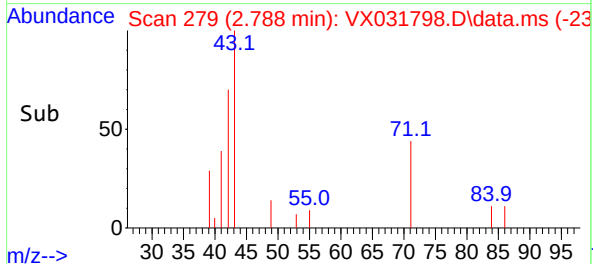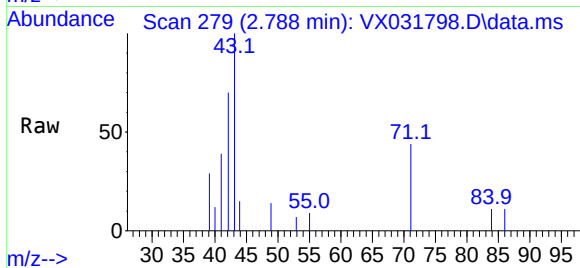

#25

2-Butanone

Concen: 0.682 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.012 min

Lab File: VX031798.D




Acq: 30 Sep 2022 04:34


Tgt Ion: 43 Resp: 473

Ion Ratio Lower Upper

43 100

72 0.0 21.1 31.7#

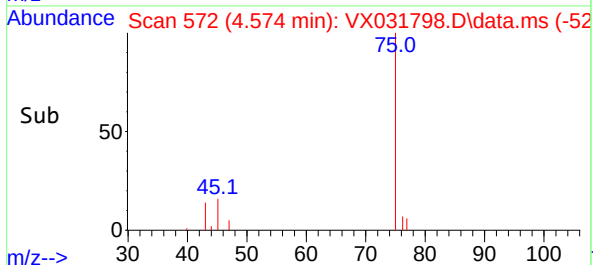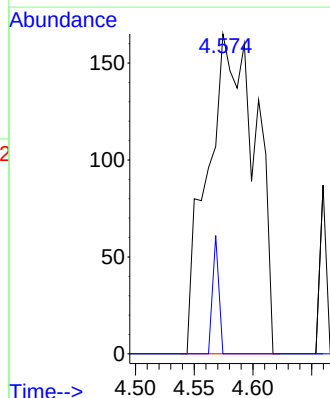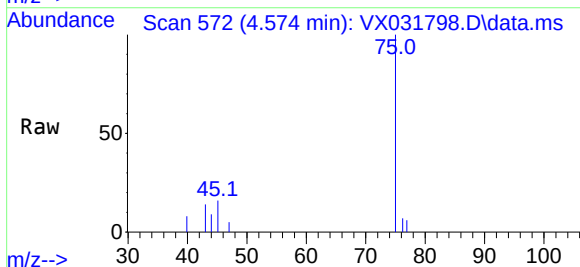



#33

1,2-Dichloroethane-d4

Concen: 48.600 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34

Instrument :

MSVOA_X

ClientSampleId :





MW-7

Tgt Ion: 65 Resp: 70665

Ion Ratio Lower Upper

65 100

67 50.3 0.0 102.4

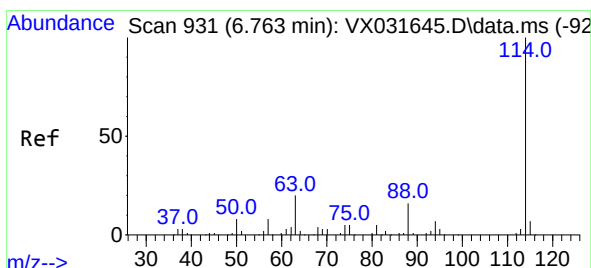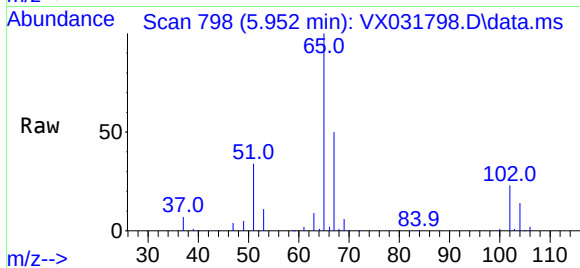

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34




Tgt Ion: 114 Resp: 108461


Ion Ratio Lower Upper

114 100

63 18.0 0.0 42.6

88 14.2 0.0 33.0


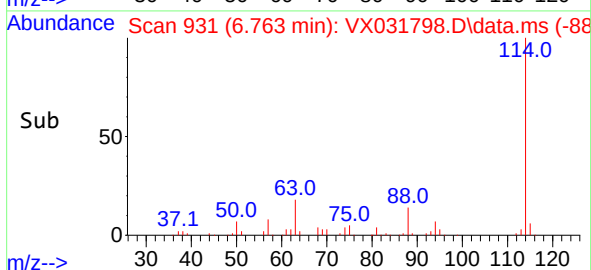

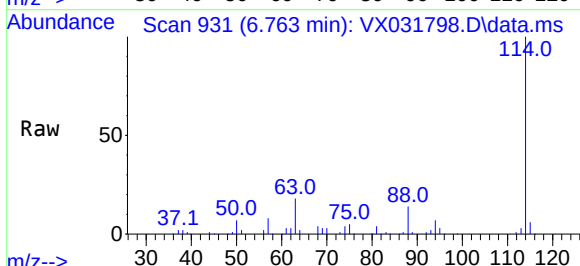


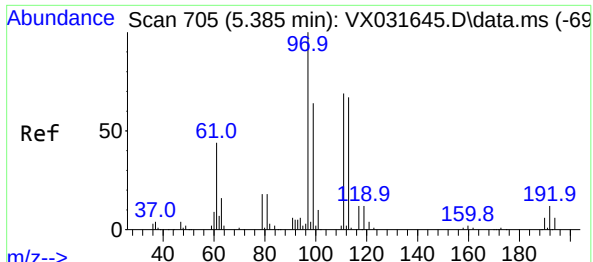

#35
Dibromofluoromethane
Concen: 47.528 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:113 Resp: 61422
Ion Ratio Lower Upper
113 100
111 103.4 82.4 123.6
192 19.4 14.1 21.1

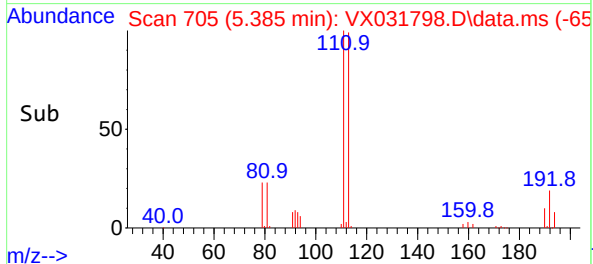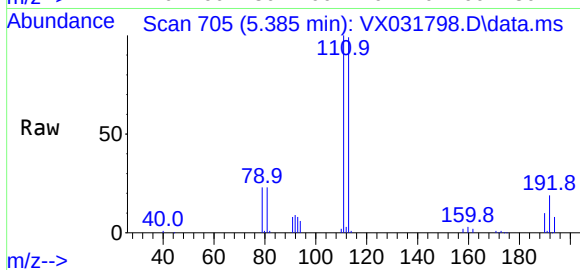

#36
1,1-Dichloropropene
Concen: 3.547 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 75 Resp: 5265
Ion Ratio Lower Upper
75 100
110 8.4 17.5 52.5#
77 0.0 24.9 37.3#


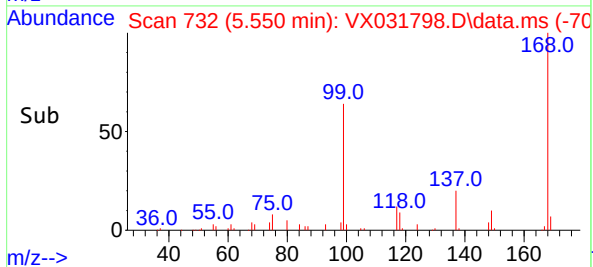

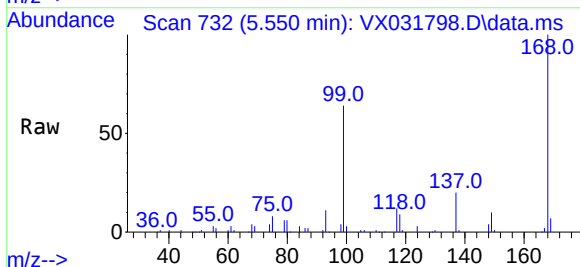




#38
Carbon Tetrachloride
Concen: 4.284 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:117 Resp: 7165
Ion Ratio Lower Upper
117 100
119 6.0 74.6 112.0#
121 0.0 25.3 37.9#

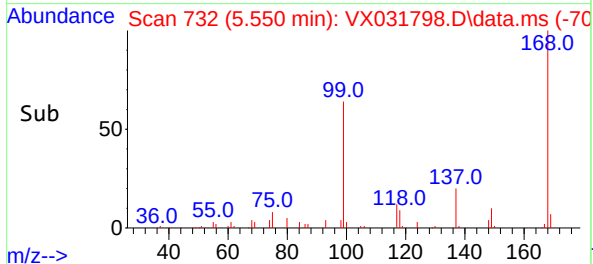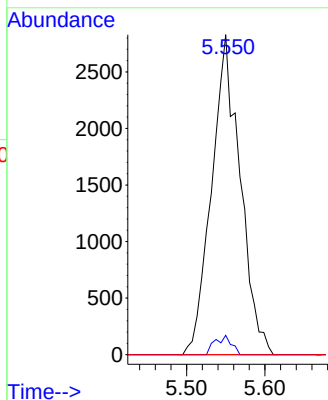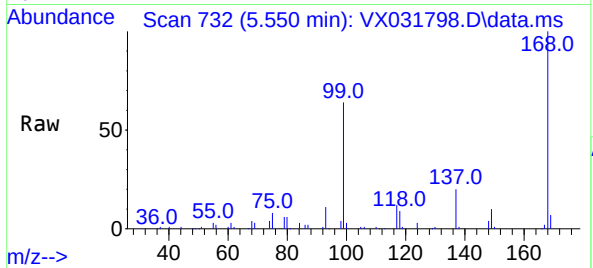

#39
Methylcyclohexane
Concen: 0.392 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 83 Resp: 663
Ion Ratio Lower Upper
83 100
55 86.0 61.0 91.4
98 52.7 37.7 56.5

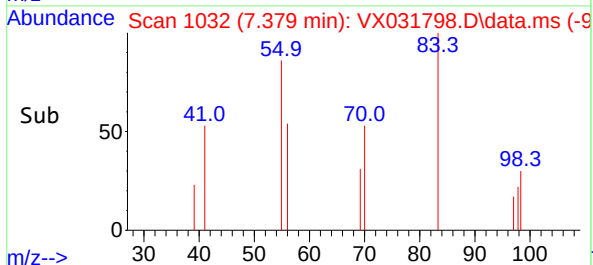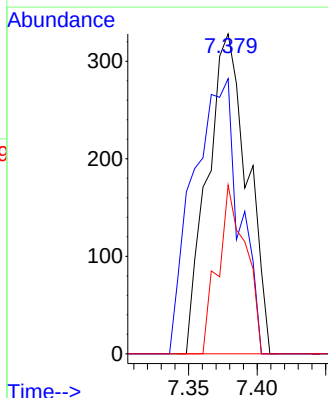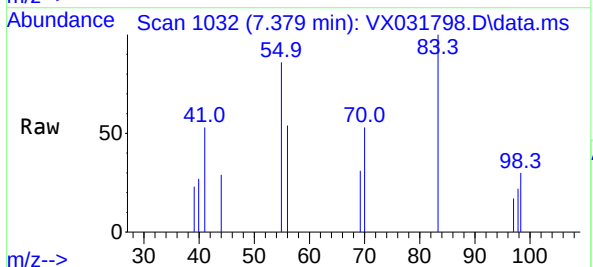



#50

Toluene-d8

Concen: 46.353 ug/l

RT: 8.647 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34

Instrument :

MSVOA_X

ClientSampleId :





MW-7

Tgt Ion: 98 Resp: 217175

Ion Ratio Lower Upper

98 100

100 66.7 52.5 78.7

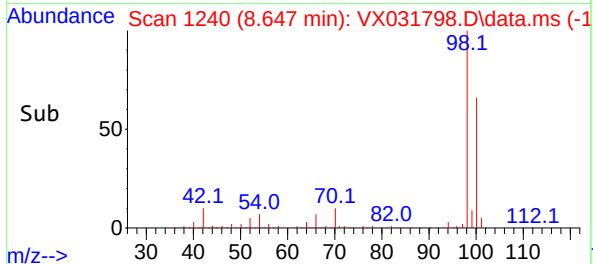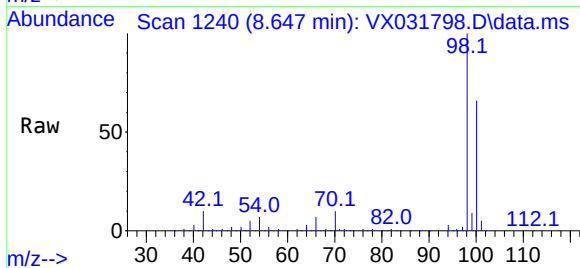

#51

4-Methyl-2-Pentanone

Concen: 0.557 ug/l

RT: 8.641 min Scan# 1239

Delta R.T. 0.061 min

Lab File: VX031798.D




Acq: 30 Sep 2022 04:34


Tgt Ion: 43 Resp: 831

Ion Ratio Lower Upper

43 100

58 189.3 30.6 46.0#

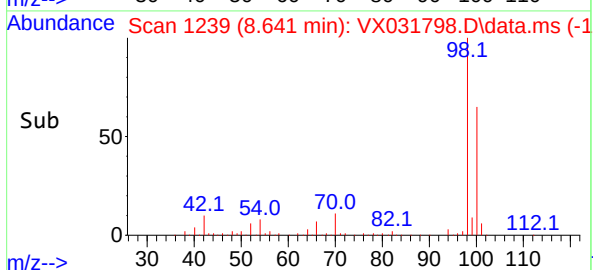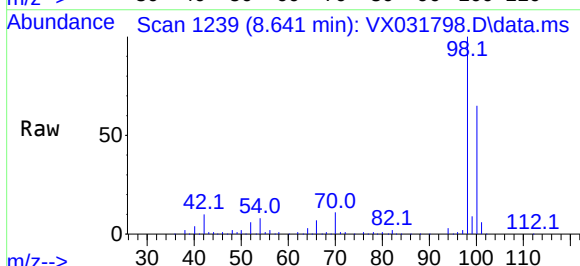







#55
1,1,2-Trichloroethane
Concen: 0.451 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Tgt Ion: 97 Resp: 590




Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.0	103.6#
85	0.0	44.1	66.1#
99	0.0	51.3	76.9#

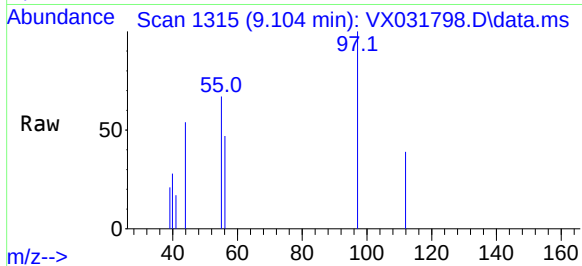


#62
4-Bromofluorobenzene
Concen: 45.270 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 95 Resp: 77739

Ion	Ratio	Lower	Upper
95	100		
174	81.2	0.0	153.2
176	79.0	0.0	144.0


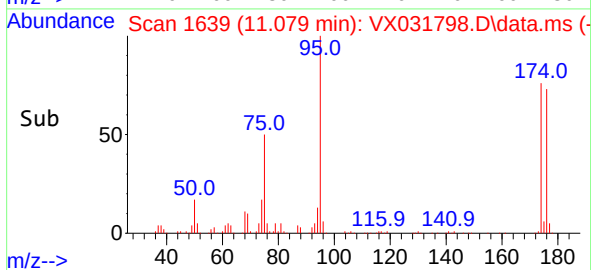

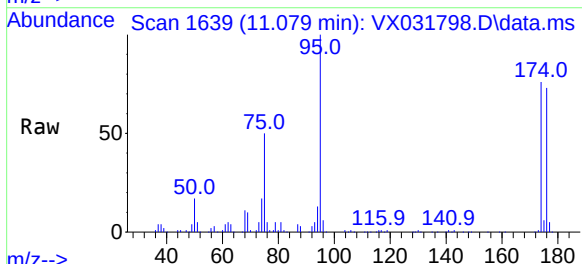




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:117 Resp: 116918
Ion Ratio Lower Upper
117 100
82 49.6 46.8 70.2
119 30.5 26.4 39.6

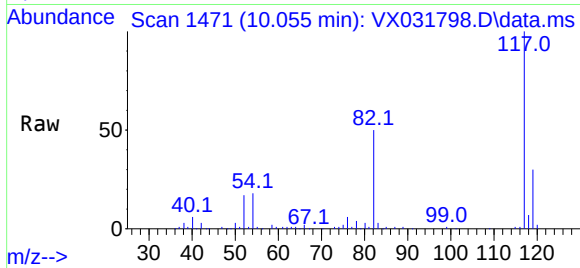

#67
Ethyl Benzene
Concen: 2.842 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 91 Resp: 15748
Ion Ratio Lower Upper
91 100
106 34.1 25.2 37.8


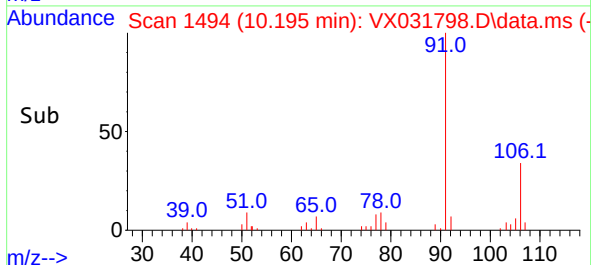
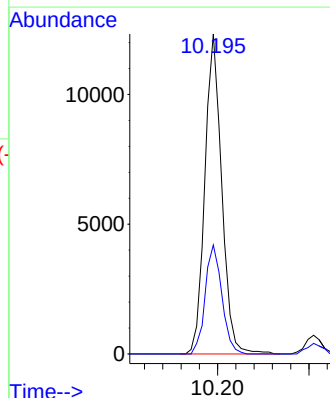
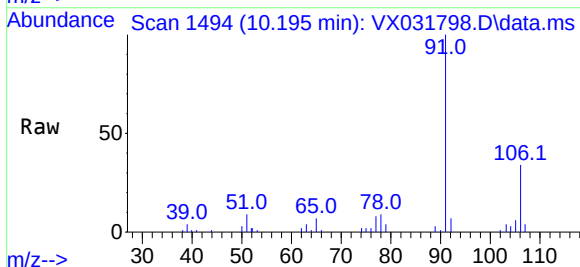




#68
m/p-Xylenes
Concen: 0.217 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:106 Resp: 484
Ion Ratio Lower Upper
106 100
91 185.5 161.0 241.4

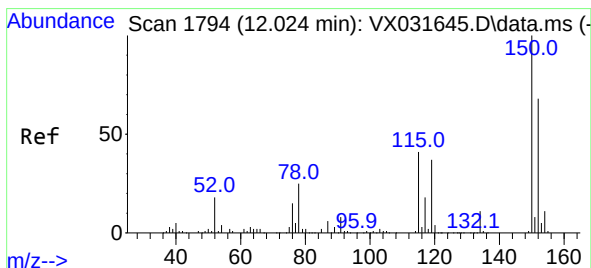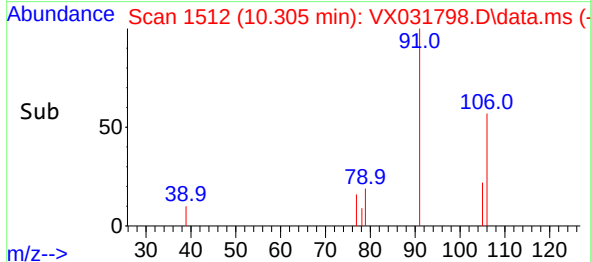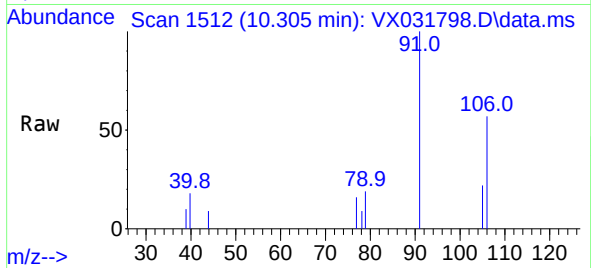

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion:152 Resp: 76924
Ion Ratio Lower Upper
152 100
115 58.9 43.4 130.1
150 157.1 0.0 346.8


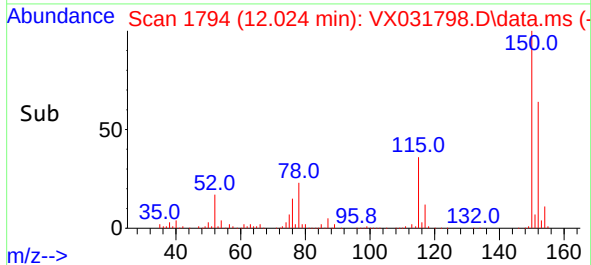

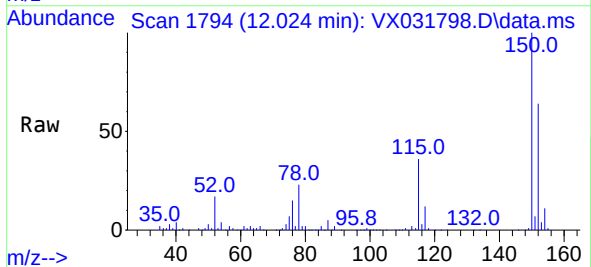




#73
Isopropylbenzene
Concen: 2.242 ug/l
RT: 10.963 min Scan# 11151
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:105 Resp: 11151
Ion Ratio Lower Upper
105 100
120 28.8 13.7 41.0

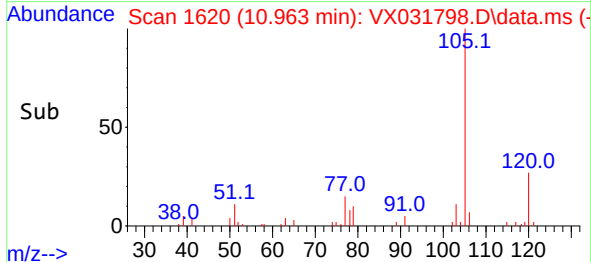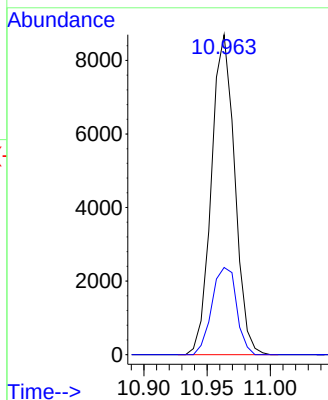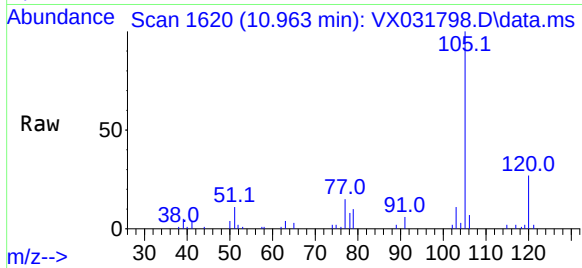

#76
1,2,3-Trichloropropane
Concen: 28.612 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 75 Resp: 39901
Ion Ratio Lower Upper
75 100
77 1.4 20.3 60.9#


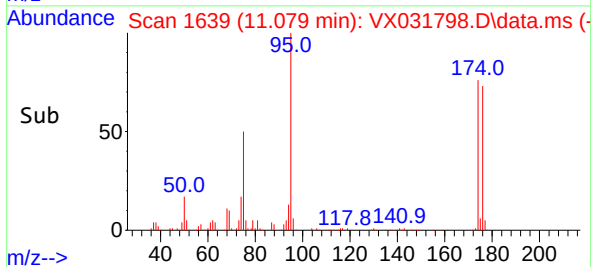
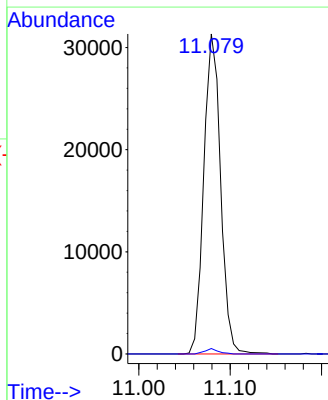
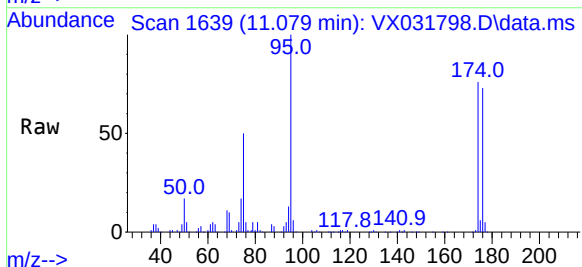




#78
n-propylbenzene
Concen: 2.381 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion: 91 Resp: 13179
Ion Ratio Lower Upper
91 100
120 23.5 11.8 35.4



#79
2-Chlorotoluene
Concen: 3.855 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 91 Resp: 13179
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


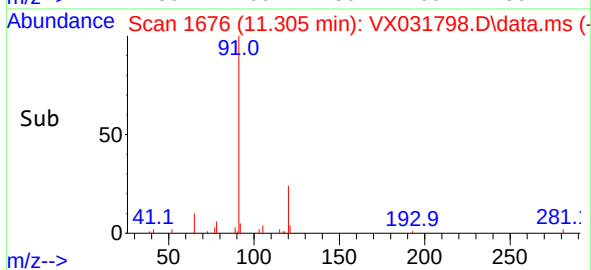






#80
1,3,5-Trimethylbenzene
Concen: 0.734 ug/l
RT: 11.616 min Scan# 11
Delta R.T. 0.165 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion:105 Resp: 3097
Ion Ratio Lower Upper
105 100
120 33.0 24.5 73.5

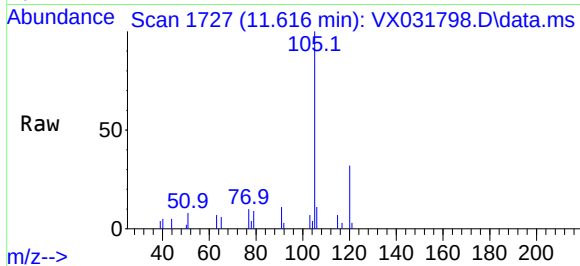

#81
trans-1,4-Dichloro-2-butene
Concen: 94.450 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 75 Resp: 39901
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.1 37.4 56.0#


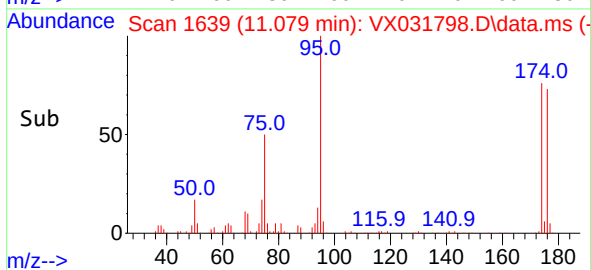

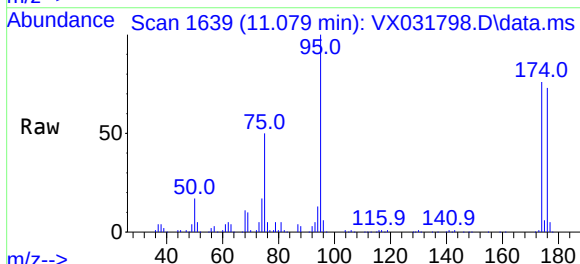




#82
4-Chlorotoluene
Concen: 3.337 ug/l
RT: 11.305 min Scan# 1701
Delta R.T. -0.152 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34




Instrument :
MSVOA_X
ClientSampleId :
MW-7


Tgt Ion: 91 Resp: 13179
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#



#85
sec-Butylbenzene
Concen: 0.641 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion: 105 Resp: 3311
Ion Ratio Lower Upper
105 100
134 37.1 10.4 31.1#

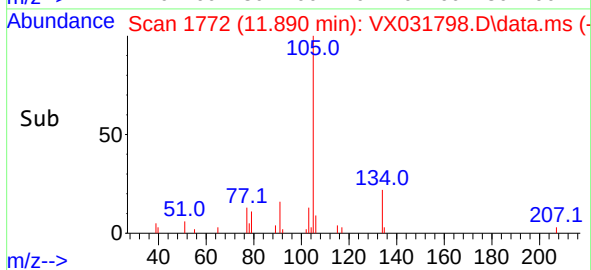



#86

p-Isopropyltoluene

Concen: 0.285 ug/l

RT: 12.177 min Scan# 119

Delta R.T. 0.165 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34

Instrument :

MSVOA_X

ClientSampleId :

MW-7





Tgt Ion:119 Resp: 1270

Ion Ratio Lower Upper

119 100

134 30.9 13.4 40.2

91 25.5 12.4 37.2

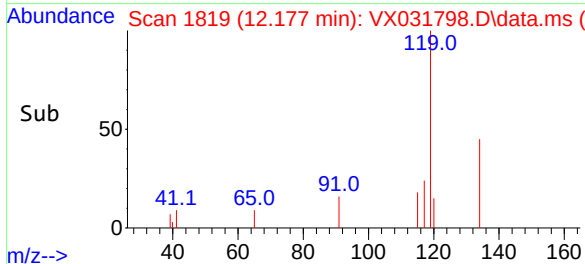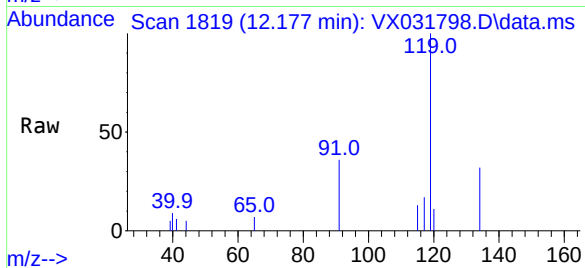

#89

n-Butylbenzene

Concen: 0.610 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX031798.D

Acq: 30 Sep 2022 04:34




Tgt Ion: 91 Resp: 2219


Ion Ratio Lower Upper

91 100

92 31.5 27.0 81.0

134 76.1 13.3 39.9#


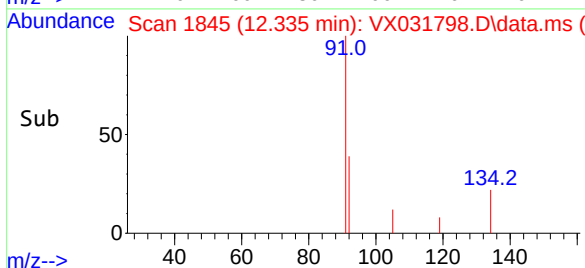
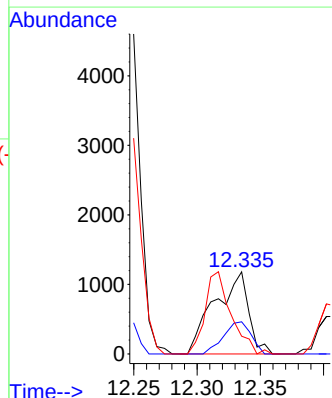
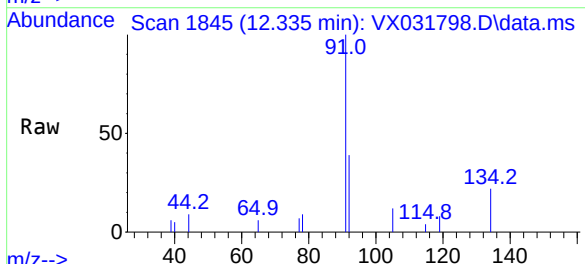




#90
Hexachloroethane
Concen: 1.676 ug/l
RT: 12.616 min Scan# 1879
Delta R.T. 0.074 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Tgt Ion:117 Resp: 1198
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

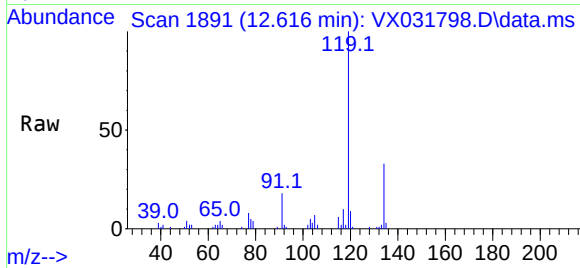

#95
Naphthalene
Concen: 17.696 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX031798.D
Acq: 30 Sep 2022 04:34

Tgt Ion:128 Resp: 84870
Ion Ratio Lower Upper
128 100
127 12.8 10.4 15.6
129 11.4 8.8 13.2

