

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
 Data File : VX031775.D
 Acq On : 29 Sep 2022 15:56
 Operator : JC/MD
 Sample : N4860-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-06

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Title : SW846 8260

Signal : TIC: VX031775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	50	rBV2	7331	24121	4.55%	0.908%
2	3.111	324	332	344	rBV	24558	57690	10.88%	2.171%
3	5.385	694	705	719	rBV2	68379	197339	37.23%	7.426%
4	5.550	722	732	747	rVB	68609	194791	36.75%	7.330%
5	5.958	789	799	814	rBV	72266	191333	36.09%	7.200%
6	6.763	921	931	945	rBV	95990	231785	43.73%	8.722%
7	8.647	1233	1240	1251	rBV	331601	530083	100.00%	19.947%
8	10.055	1465	1471	1481	rBV	249096	329344	62.13%	12.393%
9	11.079	1634	1639	1652	rBV	281013	364892	68.84%	13.731%
10	12.024	1788	1794	1802	rBV	356372	446046	84.15%	16.784%
11	12.244	1824	1830	1837	rBV2	23466	30314	5.72%	1.141%
12	12.646	1892	1896	1901	rVV2	5576	6949	1.31%	0.261%
13	12.695	1901	1904	1911	rVB	3681	5381	1.02%	0.202%
14	12.841	1920	1928	1934	rBV2	5423	8731	1.65%	0.329%
15	13.140	1969	1977	1980	rVV3	3427	6895	1.30%	0.259%
16	13.640	2053	2059	2061	rBV4	4938	9332	1.76%	0.351%
17	13.664	2061	2063	2071	rVB4	6702	9941	1.88%	0.374%
18	13.926	2101	2106	2110	rBV2	5974	7182	1.35%	0.270%
19	14.792	2241	2248	2251	rBV3	2923	5345	1.01%	0.201%




Sum of corrected areas: 2657494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031775.D
Acq On : 29 Sep 2022 15:56
Operator : JC/MD
Sample : N4860-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

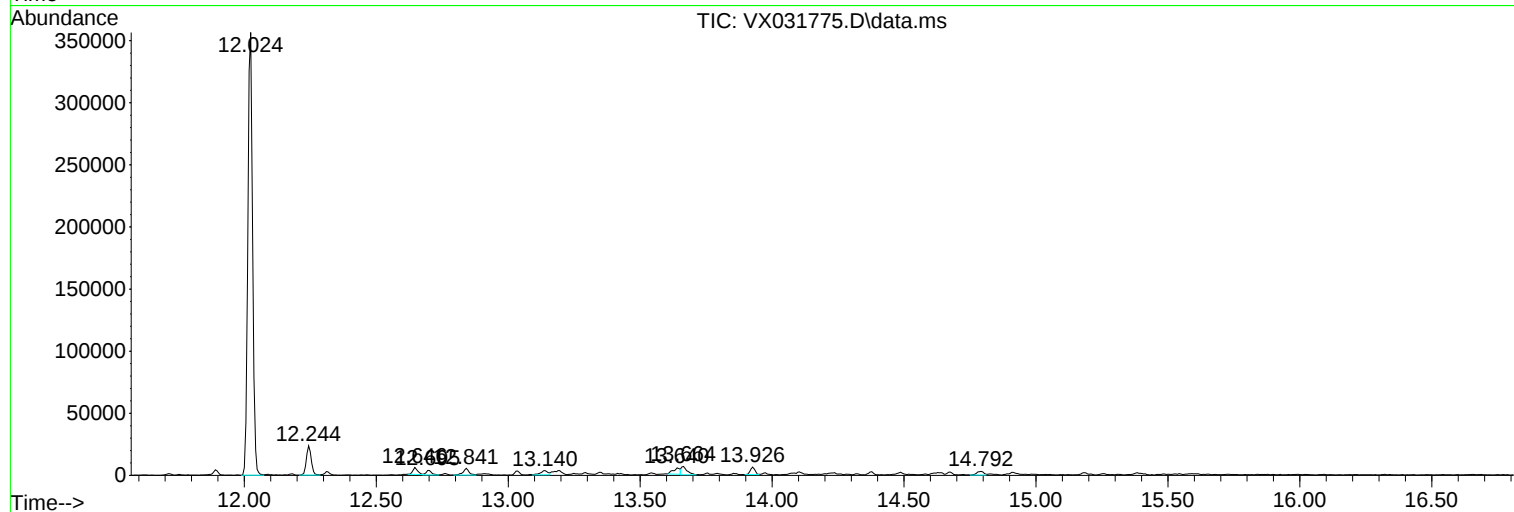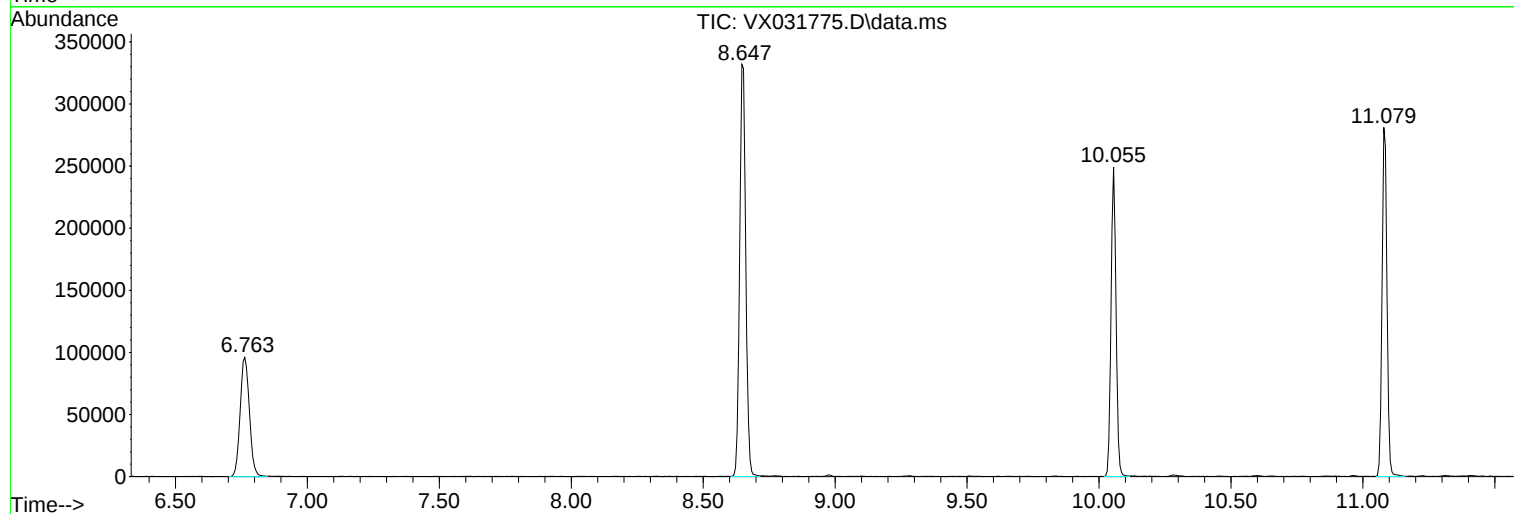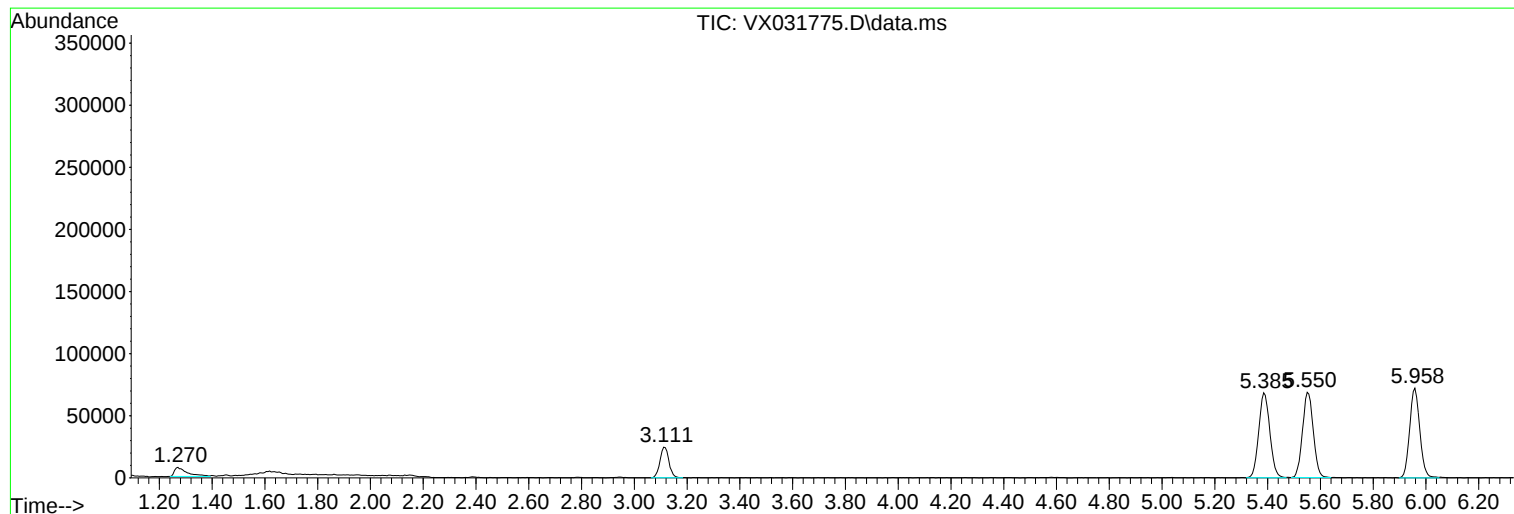

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031775.D
Acq On : 29 Sep 2022 15:56
Operator : JC/MD
Sample : N4860-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	6.19 ug/l	24121	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	4
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

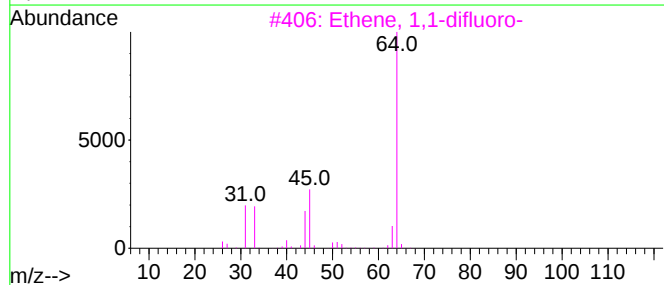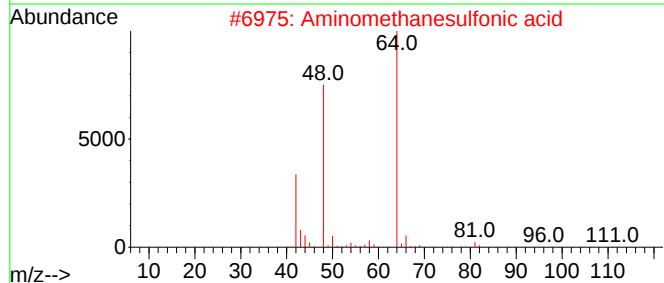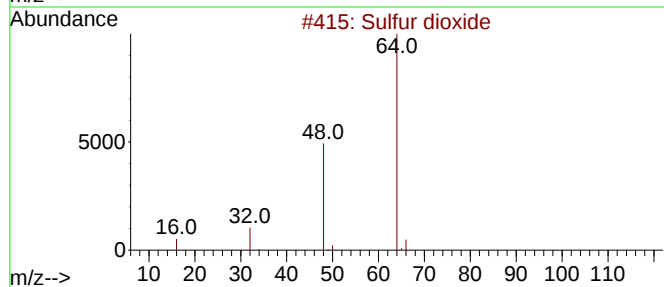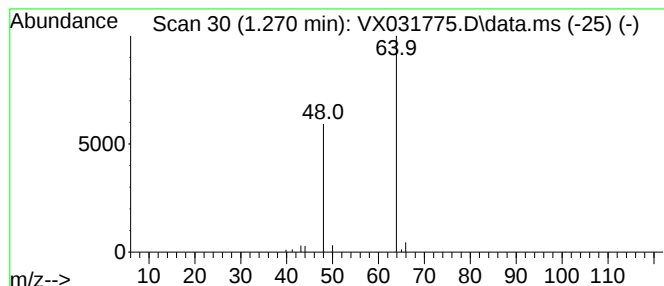

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031775.D
Acq On : 29 Sep 2022 15:56
Operator : JC/MD
Sample : N4860-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.270	6.2	ug/l	24121	1	5.550	194791	50.0