

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
 Data File : VX031776.D
 Acq On : 29 Sep 2022 16:19
 Operator : JC/MD
 Sample : N4860-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Title : SW846 8260

Signal : TIC: VX031776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	26	33	50	rBV	82061	353972	54.86%	3.742%
2	5.385	695	705	719	rBV2	67112	193888	30.05%	2.049%
3	5.550	722	732	746	rVB	57994	161794	25.08%	1.710%
4	5.958	789	799	815	rBV	69759	184534	28.60%	1.951%
5	6.763	922	931	942	rBV2	90040	212205	32.89%	2.243%
6	8.647	1234	1240	1251	rBV	258425	414052	64.17%	4.377%
7	10.055	1465	1471	1477	rBV	190370	250787	38.87%	2.651%
8	10.281	1503	1508	1517	rBV6	4377	9317	1.44%	0.098%
9	10.591	1556	1559	1565	rVB4	3814	6733	1.04%	0.071%
10	10.963	1614	1620	1624	rBV	4558	6547	1.01%	0.069%
11	11.079	1634	1639	1645	rBV	181001	235443	36.49%	2.489%
12	11.219	1658	1662	1667	rVB4	7975	12185	1.89%	0.129%
13	11.616	1721	1727	1734	rBV6	7050	14067	2.18%	0.149%
14	11.713	1740	1743	1746	rBV2	8442	9444	1.46%	0.100%
15	11.853	1759	1766	1768	rBV6	4768	9454	1.47%	0.100%
16	11.890	1768	1772	1776	rVB	10490	14476	2.24%	0.153%
17	12.024	1789	1794	1800	rBV	186445	232903	36.10%	2.462%
18	12.177	1813	1819	1825	rVB	20890	31540	4.89%	0.333%
19	12.244	1825	1830	1837	rBV	523603	645208	100.00%	6.820%
20	12.311	1837	1841	1848	rVB2	34297	53157	8.24%	0.562%
21	12.408	1848	1857	1861	rBV3	22690	37881	5.87%	0.400%
22	12.469	1864	1867	1872	rVB6	5884	10841	1.68%	0.115%
23	12.542	1872	1879	1880	rBV6	3449	6746	1.05%	0.071%
24	12.585	1883	1886	1887	rVV3	8841	11506	1.78%	0.122%
25	12.616	1887	1891	1893	rVV	26254	38001	5.89%	0.402%
26	12.646	1893	1896	1900	rVV	83891	102749	15.92%	1.086%
27	12.701	1900	1905	1912	rVV	228442	326527	50.61%	3.452%
28	12.762	1912	1915	1919	rVV2	12649	17425	2.70%	0.184%
29	12.817	1919	1924	1926	rVV3	22754	33883	5.25%	0.358%
30	12.841	1926	1928	1931	rVB	28518	27267	4.23%	0.288%
31	12.920	1939	1941	1947	rVB	30253	33162	5.14%	0.351%
32	12.981	1947	1951	1955	rBV3	17227	22047	3.42%	0.233%
33	13.030	1955	1959	1965	rVB2	51131	75305	11.67%	0.796%
34	13.097	1965	1970	1973	rBV	21839	35848	5.56%	0.379%
35	13.134	1973	1976	1980	rVV	46705	54134	8.39%	0.572%
36	13.170	1980	1982	1983	rVV	12620	10333	1.60%	0.109%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
 Data File : VX031776.D
 Acq On : 29 Sep 2022 16:19
 Operator : JC/MD
 Sample : N4860-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
 Title : SW846 8260

37	13.195	1983	1986	1991	rVB	34505	46908	7.27%	0.496%
38	13.256	1991	1996	1998	rBV2	16847	25664	3.98%	0.271%
39	13.292	1998	2002	2008	rVB	449795	532623	82.55%	5.630%
40	13.347	2008	2011	2014	rBV3	29003	36552	5.67%	0.386%
41	13.390	2014	2018	2020	rVV3	22877	33996	5.27%	0.359%
42	13.420	2020	2023	2032	rVB4	55631	100959	15.65%	1.067%
43	13.506	2032	2037	2040	rBV4	22851	40344	6.25%	0.426%
44	13.542	2040	2043	2046	rBV	61580	72829	11.29%	0.770%
45	13.585	2046	2050	2053	rVV2	122882	149053	23.10%	1.576%
46	13.640	2053	2059	2060	rVV2	105304	138224	21.42%	1.461%
47	13.664	2060	2063	2068	rVB	193140	241743	37.47%	2.555%
48	13.749	2072	2077	2081	rBV3	26537	39030	6.05%	0.413%
49	13.798	2081	2085	2089	rBV4	32508	50174	7.78%	0.530%
50	13.853	2089	2094	2099	rVB3	137725	195388	30.28%	2.065%
51	13.926	2099	2106	2110	rBV2	215030	293785	45.53%	3.105%
52	13.969	2110	2113	2117	rBV	93677	125503	19.45%	1.327%
53	14.005	2117	2119	2125	rVB3	28980	36244	5.62%	0.383%
54	14.073	2125	2130	2133	rBV2	86375	117594	18.23%	1.243%
55	14.103	2133	2135	2137	rVB2	14480	11199	1.74%	0.118%
56	14.134	2138	2140	2143	rBV4	10535	9963	1.54%	0.105%
57	14.164	2143	2145	2147	rVB	14085	11679	1.81%	0.123%
58	14.213	2148	2153	2158	rBV	189031	250690	38.85%	2.650%
59	14.286	2163	2165	2167	rVB	14072	12434	1.93%	0.131%
60	14.323	2167	2171	2175	rBV	123955	144593	22.41%	1.528%
61	14.371	2175	2179	2184	rVB	162762	209764	32.51%	2.217%
62	14.420	2184	2187	2192	rVB	48220	64493	10.00%	0.682%
63	14.481	2192	2197	2202	rBV2	266138	368850	57.17%	3.899%
64	14.615	2210	2219	2225	rBV4	194144	372029	57.66%	3.932%
65	14.670	2225	2228	2233	rVB	99803	141934	22.00%	1.500%
66	14.725	2233	2237	2241	rBV	52101	79584	12.33%	0.841%
67	14.786	2243	2247	2250	rVV2	81022	149797	23.22%	1.583%
68	14.816	2250	2252	2255	rVV2	82865	112556	17.44%	1.190%
69	14.847	2255	2257	2261	rVV2	70223	86093	13.34%	0.910%
70	14.908	2263	2267	2273	rVV3	57582	133986	20.77%	1.416%
71	14.963	2273	2276	2283	rVB5	45245	98682	15.29%	1.043%
72	15.048	2284	2290	2294	rBV2	35116	62138	9.63%	0.657%
73	15.182	2307	2312	2315	rBV2	153007	238465	36.96%	2.521%
74	15.213	2315	2317	2320	rVB	88845	88798	13.76%	0.939%
75	15.249	2320	2323	2326	rBV4	17975	21843	3.39%	0.231%
76	15.377	2340	2344	2346	rBV2	31940	46632	7.23%	0.493%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031776.D
Acq On : 29 Sep 2022 16:19
Operator : JC/MD
Sample : N4860-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M

Title : SW846 8260

77	15.408	2347	2349	2354	rVV3	32632	49254	7.63%	0.521%
78	15.481	2357	2361	2364	rBV2	27886	42599	6.60%	0.450%
79	15.524	2365	2368	2373	rVV5	25756	52934	8.20%	0.560%
80	15.572	2373	2376	2378	rVV4	12282	15987	2.48%	0.169%
81	15.615	2379	2383	2388	rVB3	34447	56373	8.74%	0.596%
82	15.810	2411	2415	2418	rBV	43134	64186	9.95%	0.678%
83	15.847	2418	2421	2430	rVB4	44504	81017	12.56%	0.856%
84	15.987	2441	2444	2447	rVB2	15314	20519	3.18%	0.217%
85	16.267	2486	2490	2492	rBV2	15661	25118	3.89%	0.266%
86	16.426	2512	2516	2519	rVB3	11526	16246	2.52%	0.172%
87	16.529	2529	2533	2539	rBV3	17849	39645	6.14%	0.419%
88	16.596	2541	2544	2549	rVV2	30687	52853	8.19%	0.559%
89	16.657	2550	2554	2559	rVB2	33806	55506	8.60%	0.587%


Sum of corrected areas: 9460413

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031776.D
Acq On : 29 Sep 2022 16:19
Operator : JC/MD
Sample : N4860-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

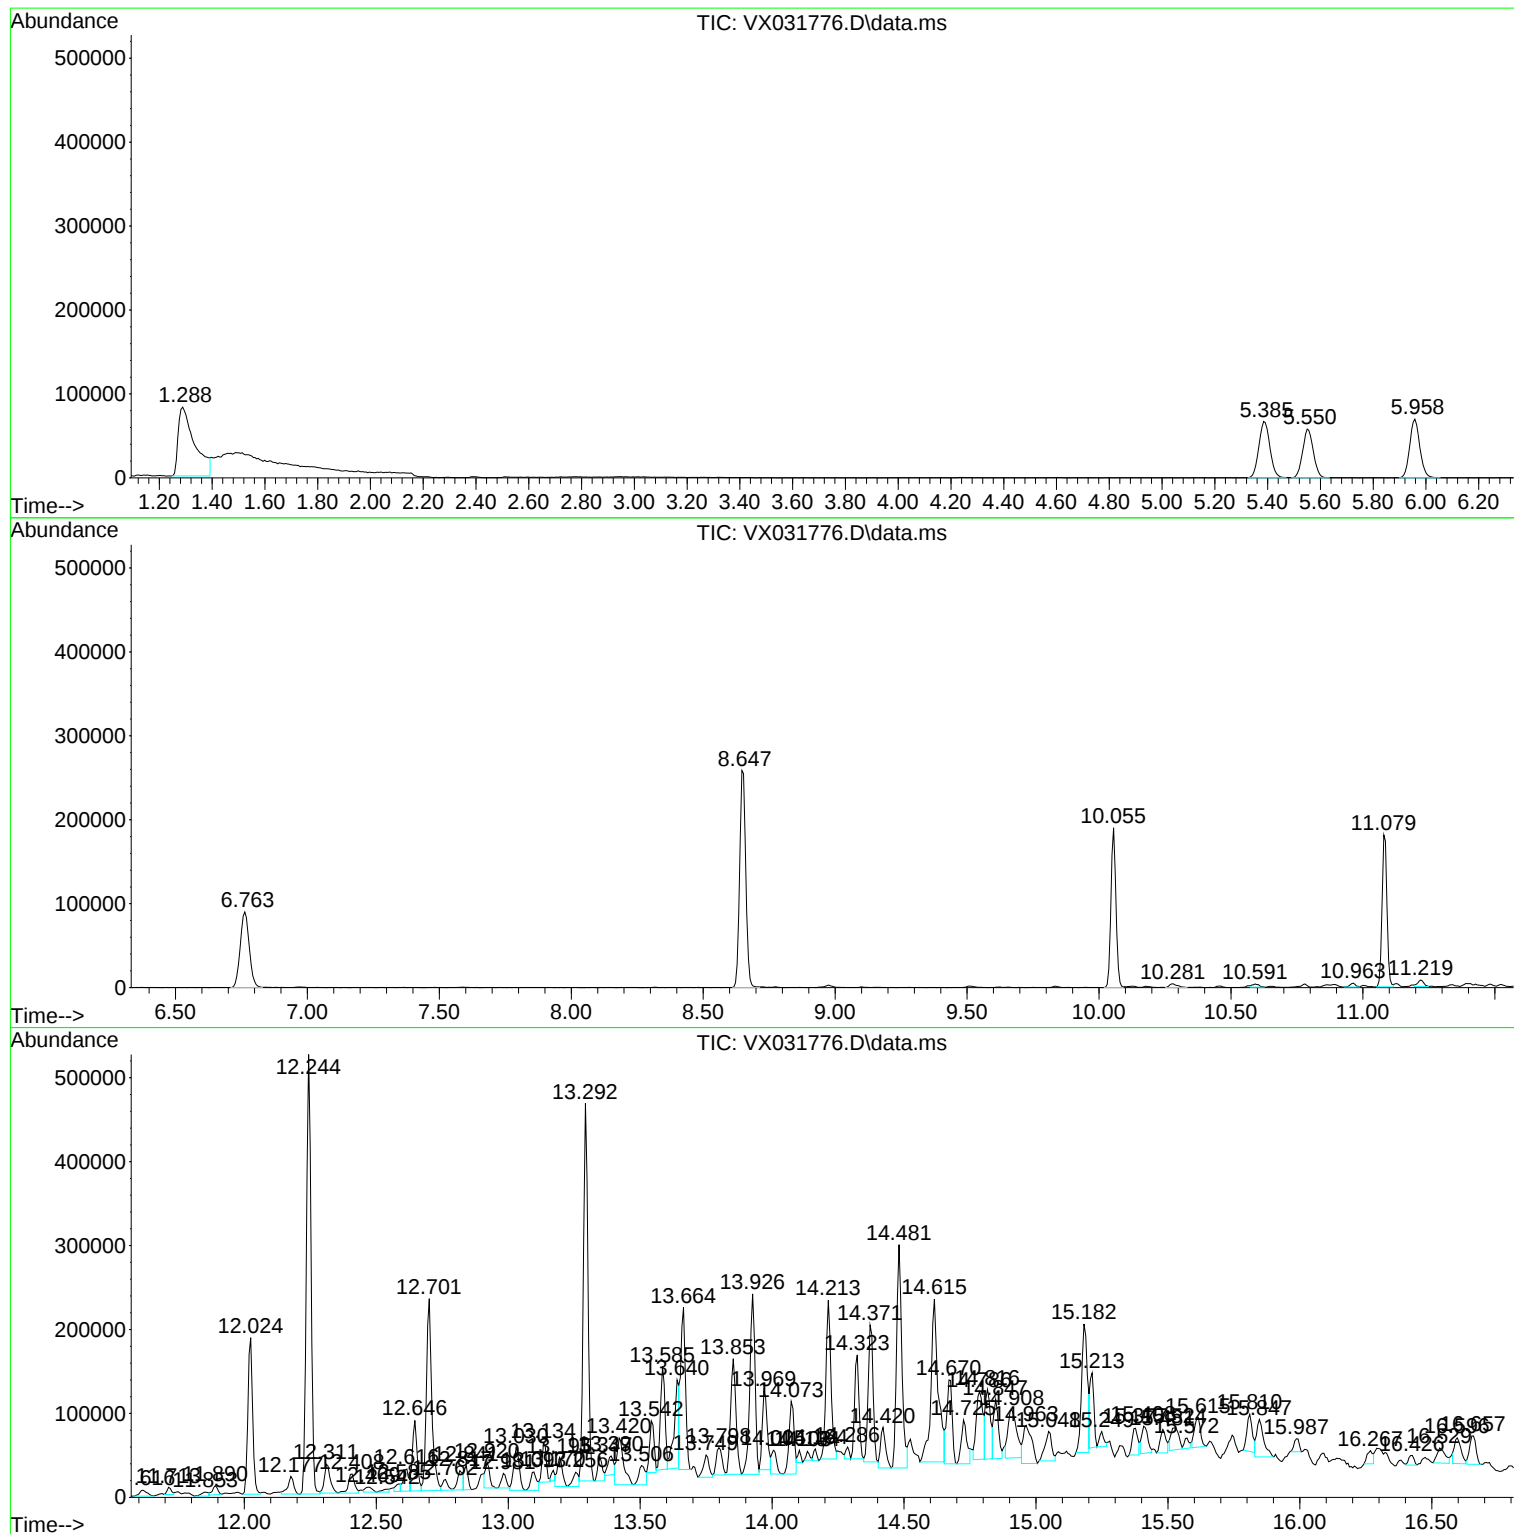

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031776.D
Acq On : 29 Sep 2022 16:19
Operator : JC/MD
Sample : N4860-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092922\
Data File : VX031776.D
Acq On : 29 Sep 2022 16:19
Operator : JC/MD
Sample : N4860-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc