

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
 Data File : VX037965.D
 Acq On : 29 Sep 2023 11:04
 Operator : JC/MD
 Sample : VX0929WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0929WBL01

Quant Time: Sep 29 23:00:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	253829	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	436524	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	428630	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	230941	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	161004	48.278	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.560%
35) Dibromofluoromethane	5.385	113	139007	47.592	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.180%
50) Toluene-d8	8.647	98	526952	48.555	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.120%
62) 4-Bromofluorobenzene	11.079	95	206715	52.417	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037965.D
Acq On : 29 Sep 2023 11:04
Operator : JC/MD
Sample : VX0929WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01

Quant Time: Sep 29 23:00:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




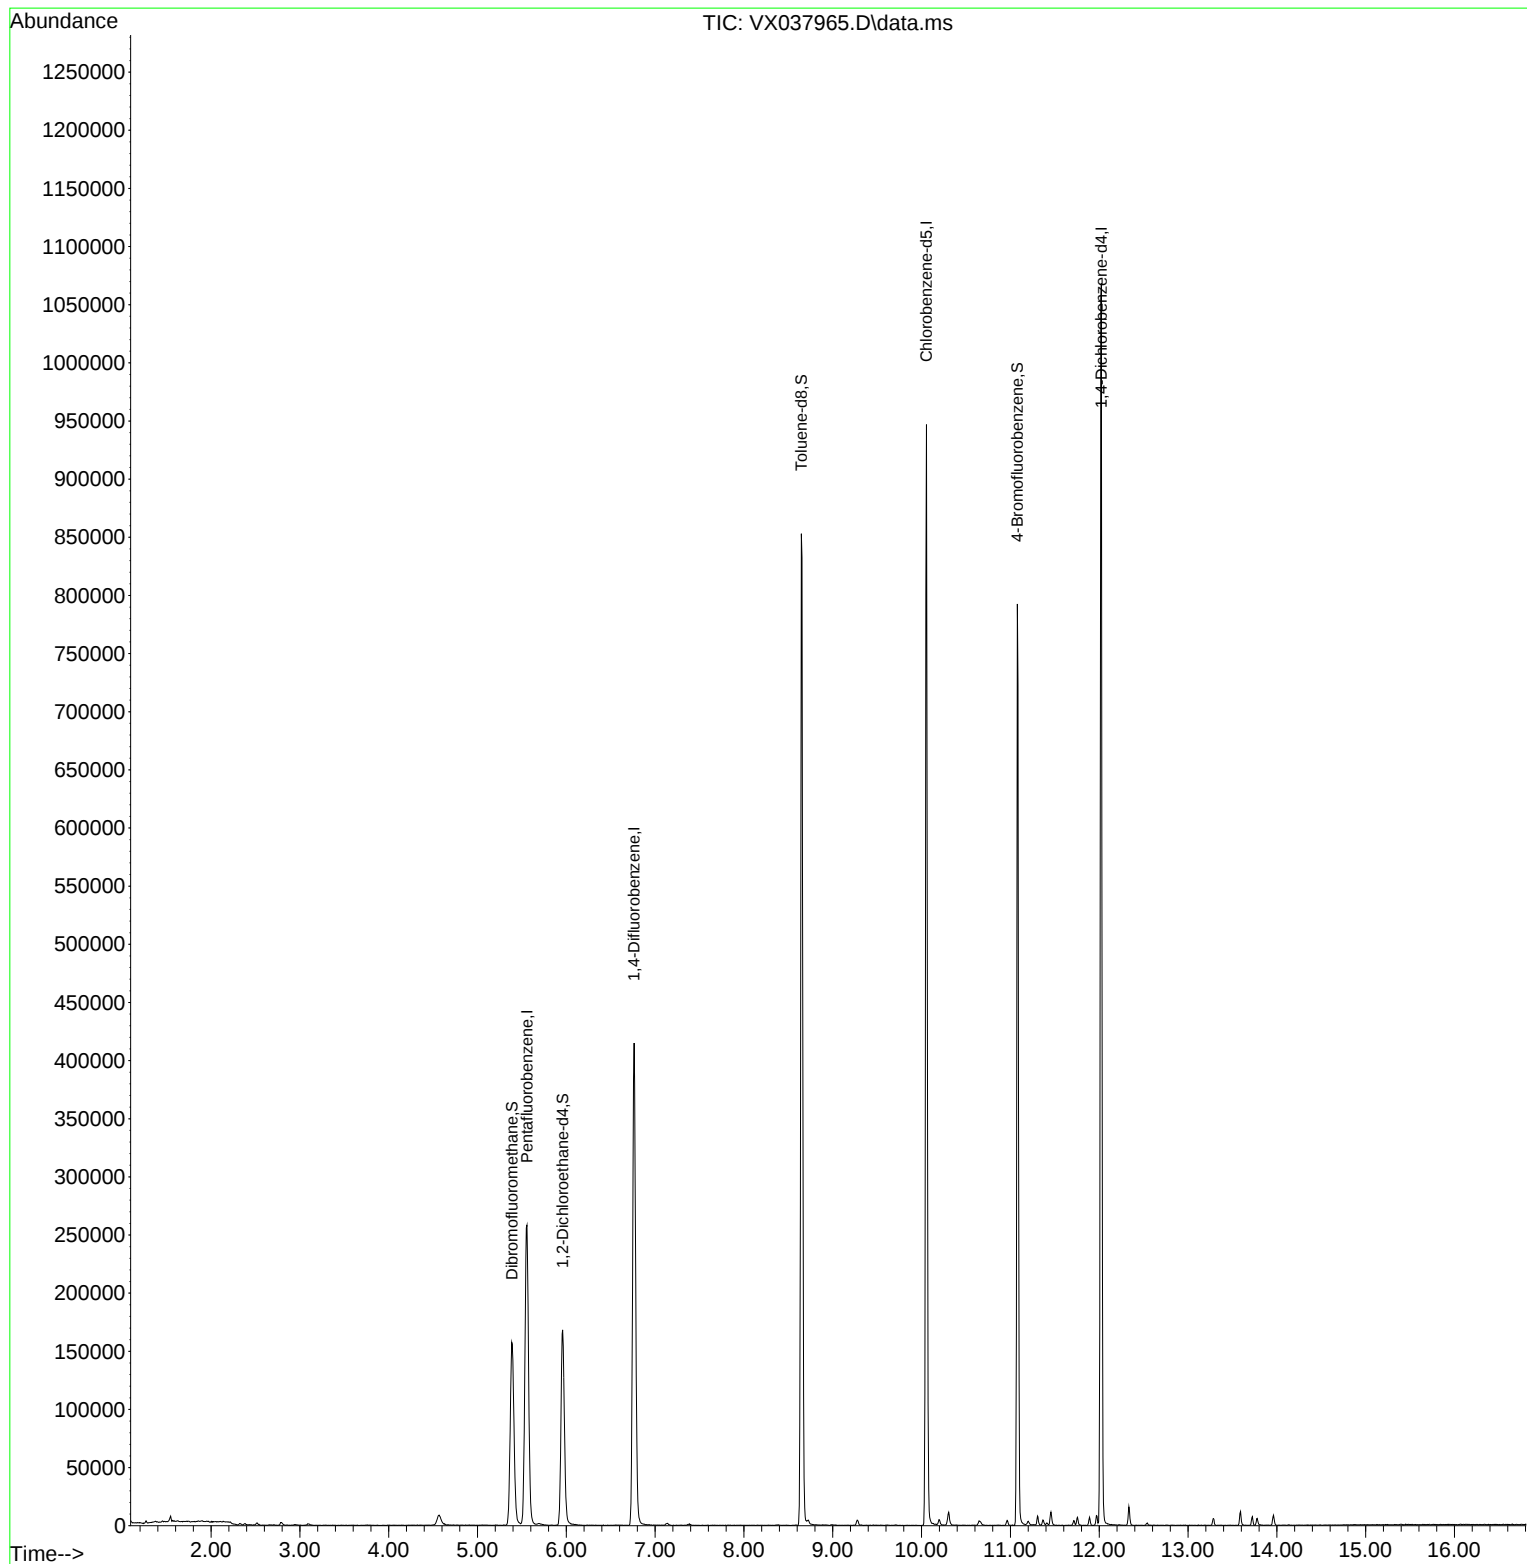


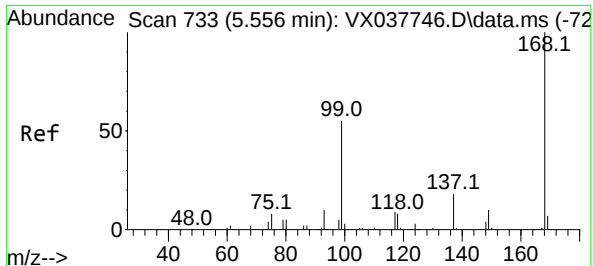

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04




Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Tgt Ion:168 Resp: 253829
Ion Ratio Lower Upper
168 100
99 54.7 56.6 85.0#

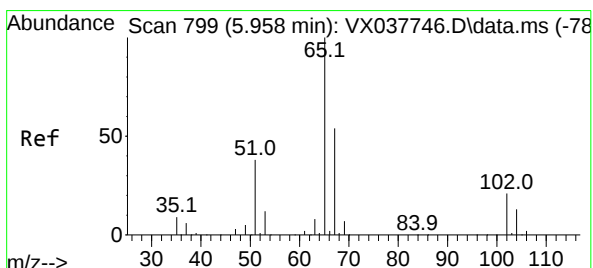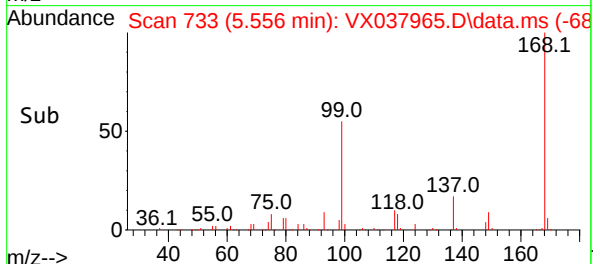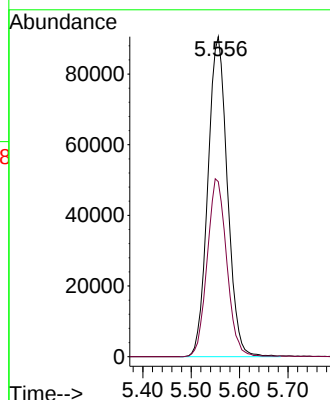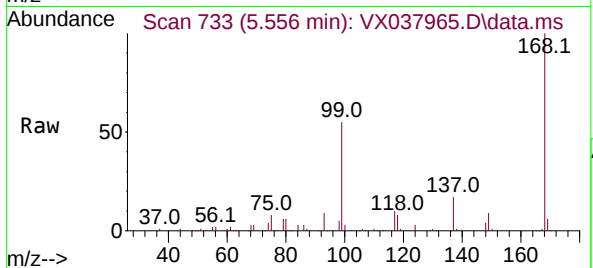

#33
1,2-Dichloroethane-d4
Concen: 48.278 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04

Tgt Ion: 65 Resp: 161004
Ion Ratio Lower Upper
65 100
67 53.2 0.0 100.2


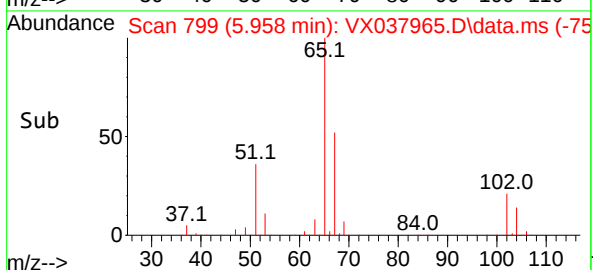
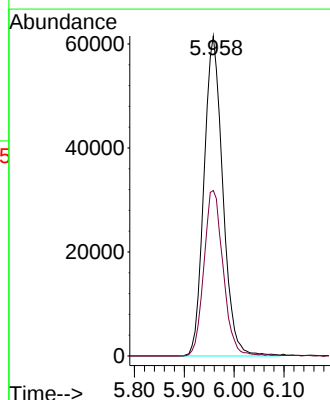
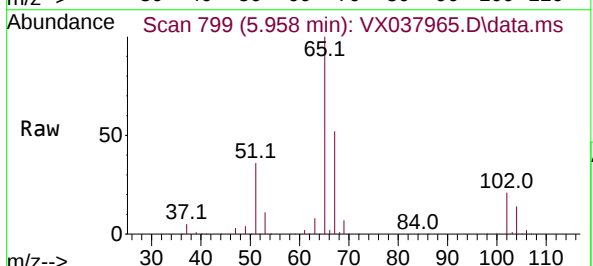


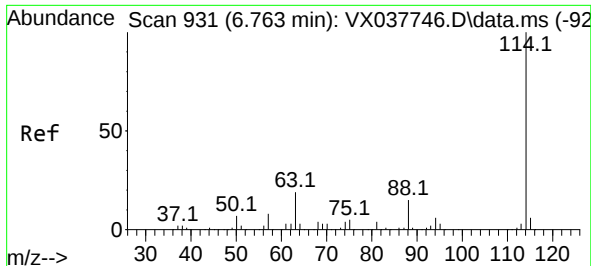

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04




Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Tgt Ion:114 Resp: 436524
Ion Ratio Lower Upper
114 100
63 18.5 0.0 45.0
88 15.5 0.0 36.6

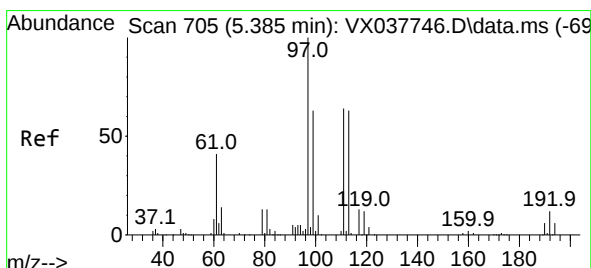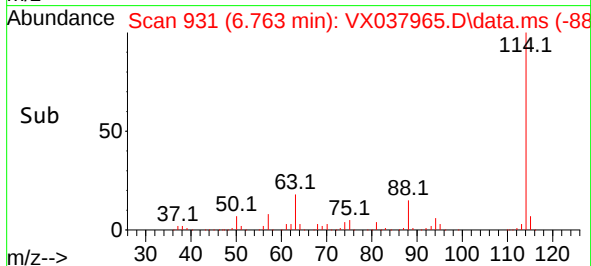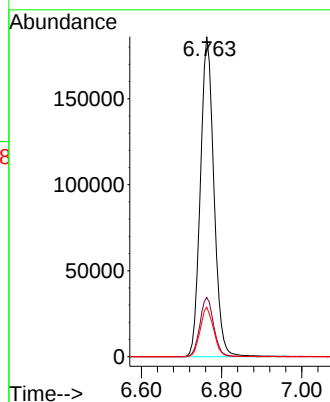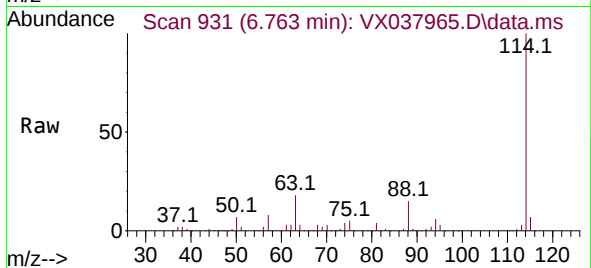

#35
Dibromofluoromethane
Concen: 47.592 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04

Tgt Ion:113 Resp: 139007
Ion Ratio Lower Upper
113 100
111 103.9 82.9 124.3
192 18.8 13.3 19.9


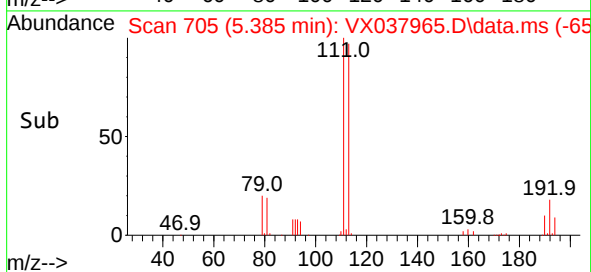
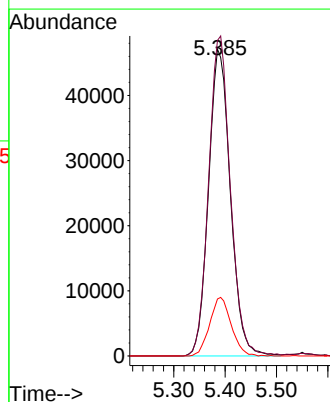
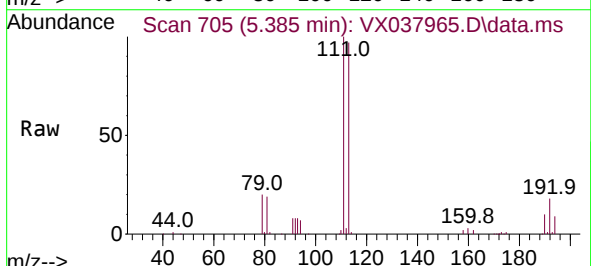


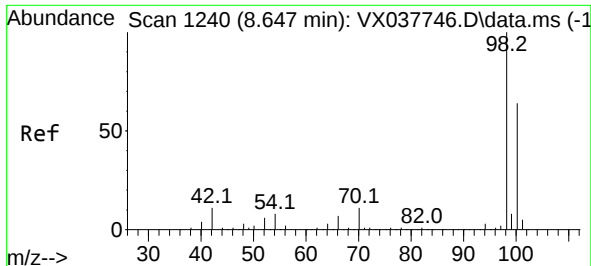

#50
Toluene-d8
Concen: 48.555 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04




Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Tgt Ion: 98 Resp: 526952
Ion Ratio Lower Upper
98 100
100 63.9 53.1 79.7

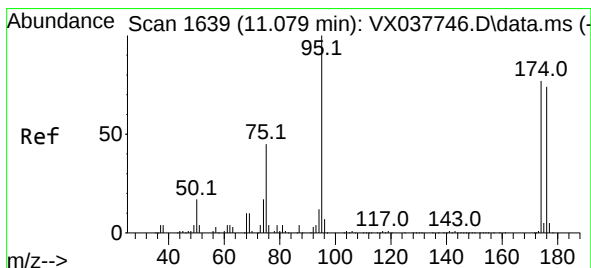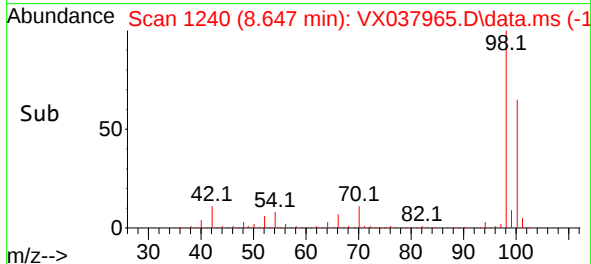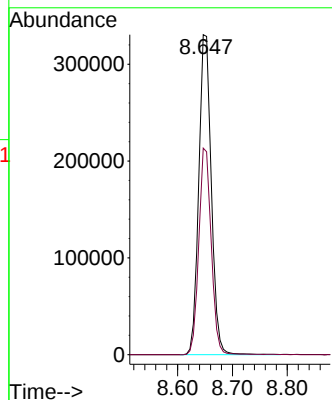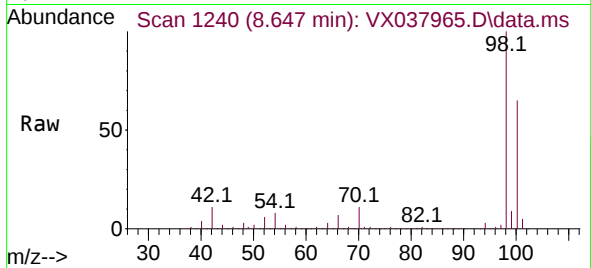

#62
4-Bromofluorobenzene
Concen: 52.417 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04

Tgt Ion: 95 Resp: 206715
Ion Ratio Lower Upper
95 100
174 83.0 0.0 135.6
176 80.4 0.0 131.0


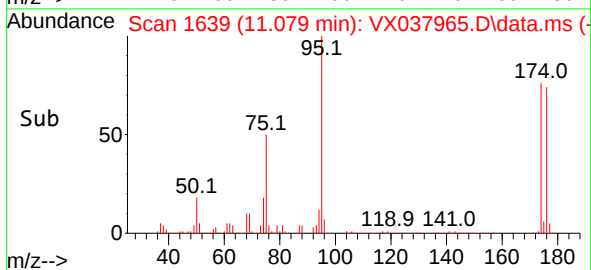
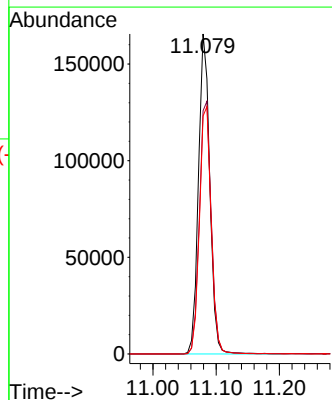
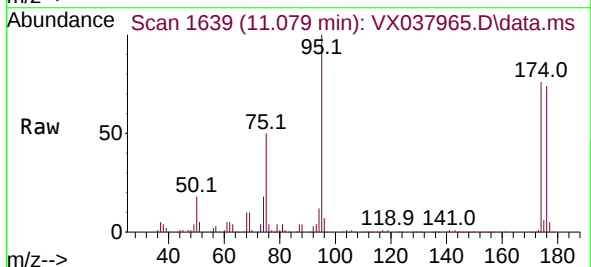


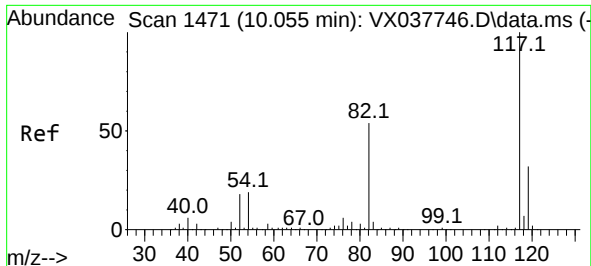

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04

Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01

Tgt Ion:117 Resp: 428630
Ion Ratio Lower Upper
117 100
82 53.5 46.2 69.4
119 31.8 25.5 38.3

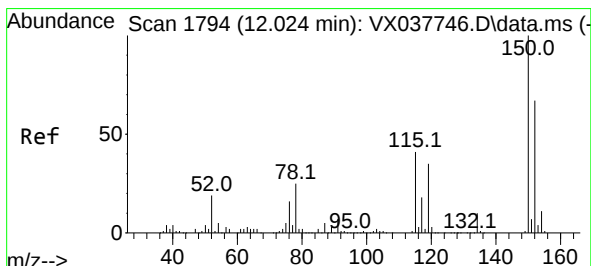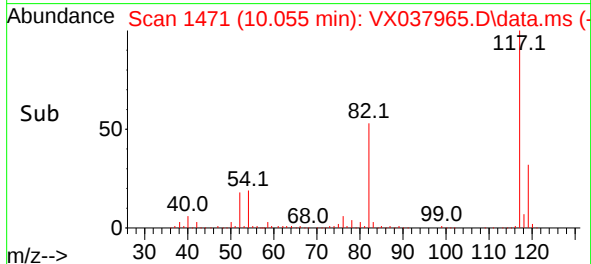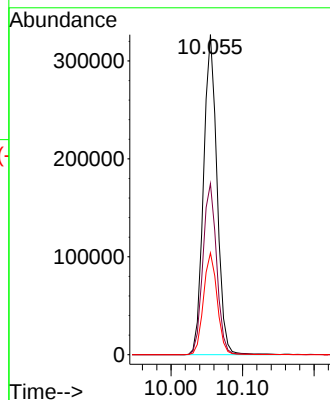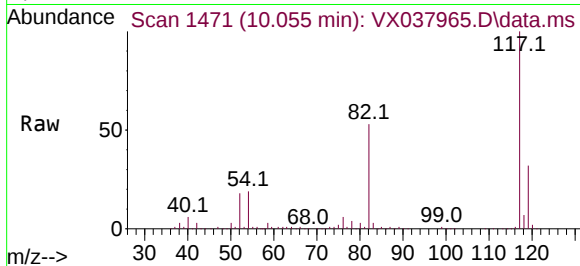

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037965.D
Acq: 29 Sep 2023 11:04

Tgt Ion:152 Resp: 230941
Ion Ratio Lower Upper
152 100
115 59.8 43.3 129.9
150 156.3 0.0 345.0

