

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
 Data File : VX037979.D
 Acq On : 29 Sep 2023 16:33
 Operator : JC/MD
 Sample : 04656-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-104D

Quant Time: Sep 29 23:07:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	217918	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	367013	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	351141	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	182260	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	135694	47.394	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.780%
35) Dibromofluoromethane	5.391	113	114894	46.787	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.580%
50) Toluene-d8	8.647	98	448965	49.205	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.400%
62) 4-Bromofluorobenzene	11.079	95	163055	49.177	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.360%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037979.D
Acq On : 29 Sep 2023 16:33
Operator : JC/MD
Sample : 04656-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-104D

Quant Time: Sep 29 23:07:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




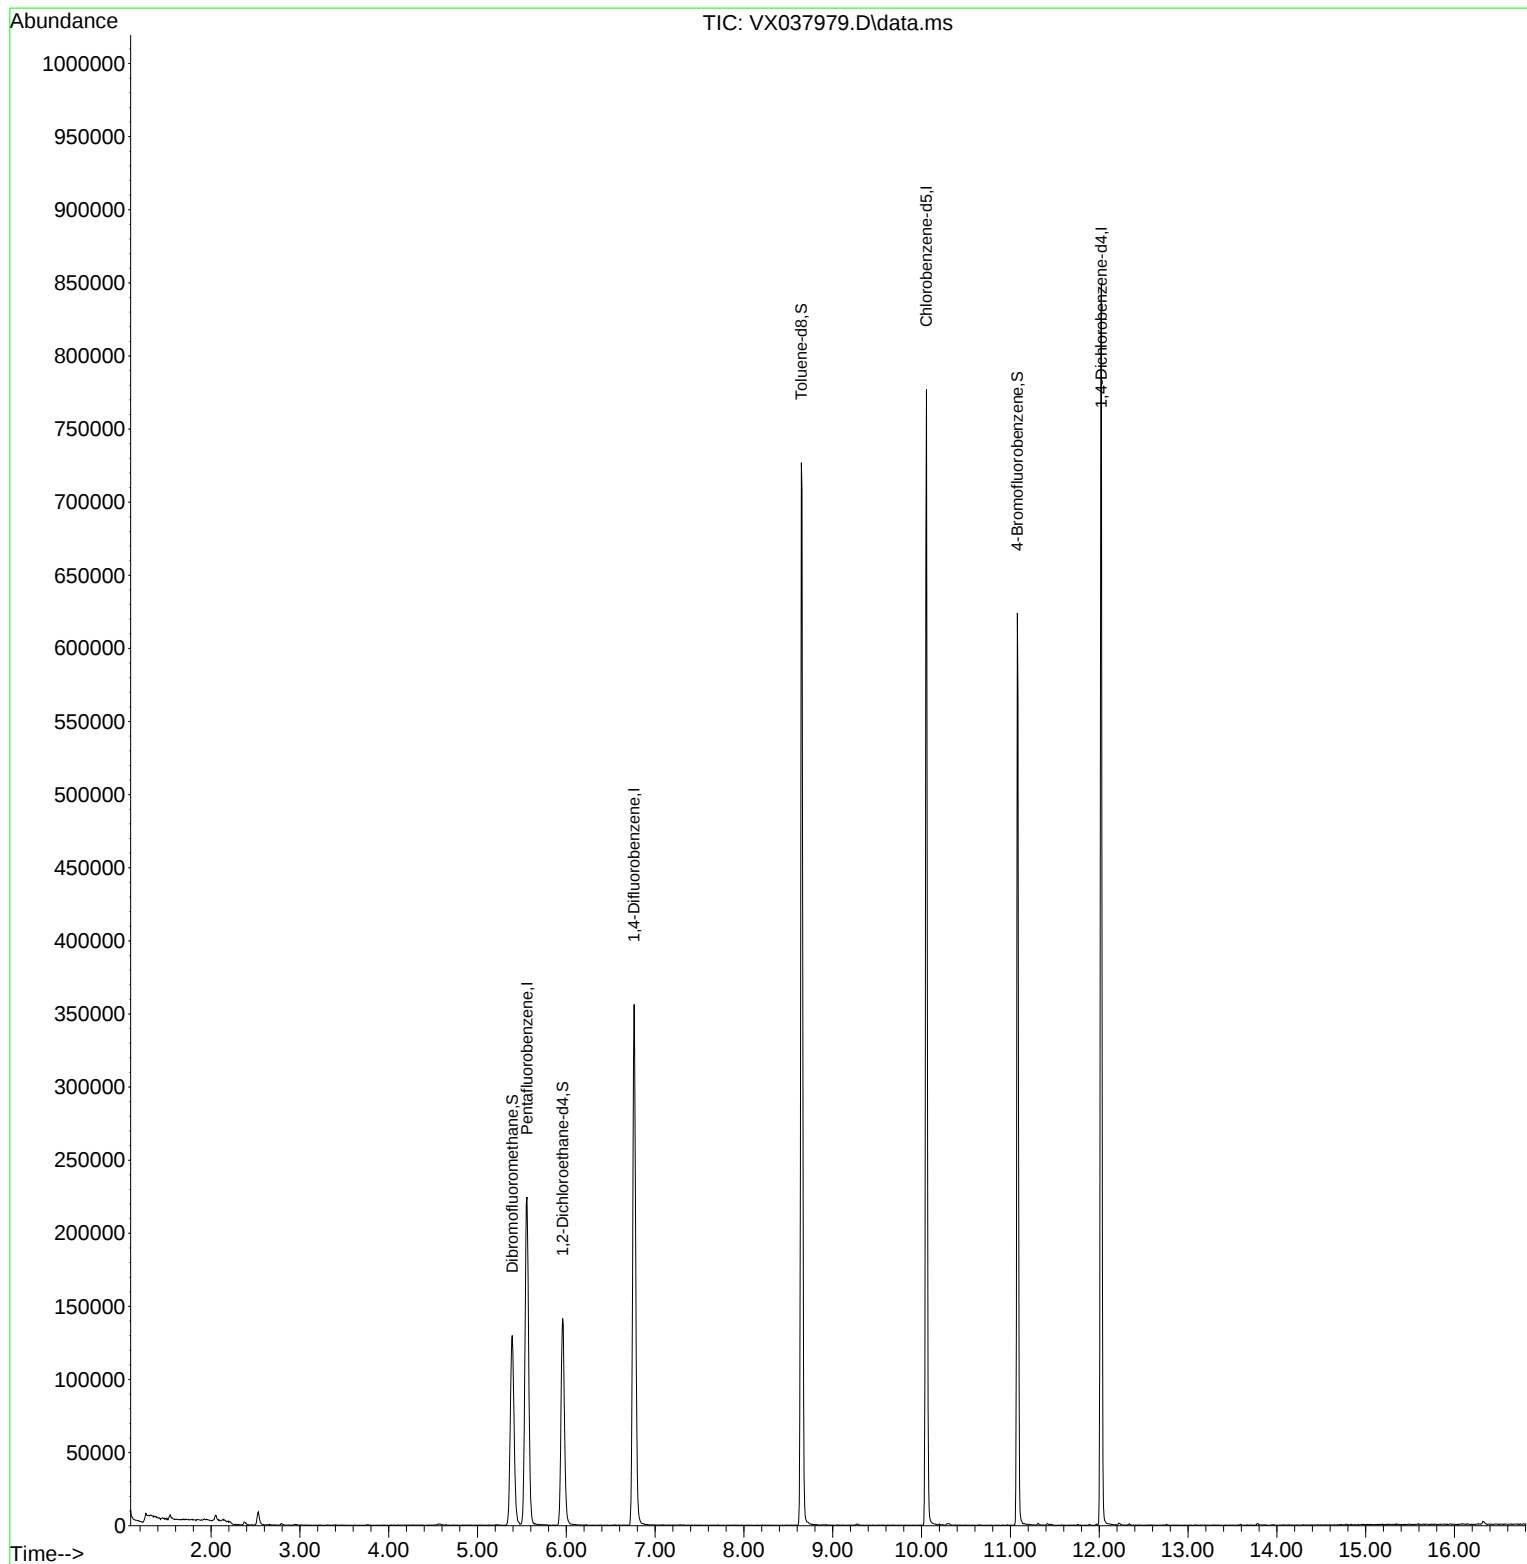




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33




Instrument :
MSVOA_X
ClientSampleId :
MW-104D

Tgt Ion:168 Resp: 217918
Ion Ratio Lower Upper
168 100
99 53.7 56.6 85.0#

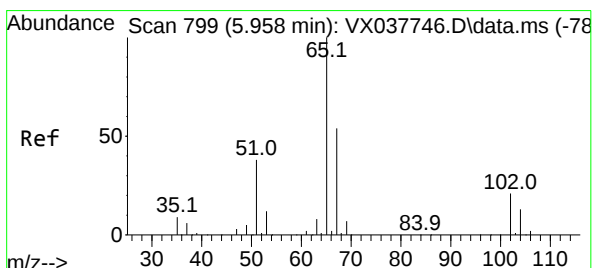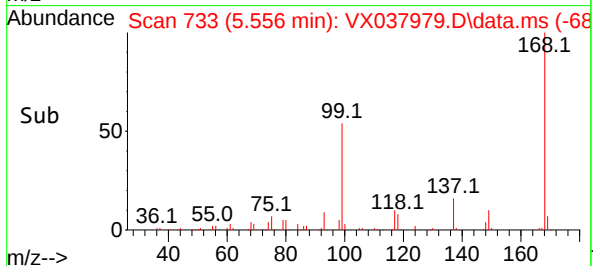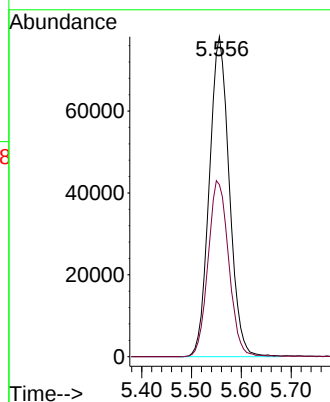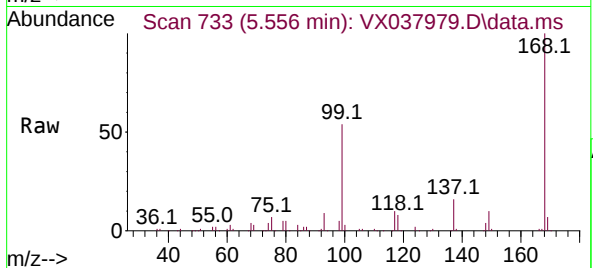

#33
1,2-Dichloroethane-d4
Concen: 47.394 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33

Tgt Ion: 65 Resp: 135694
Ion Ratio Lower Upper
65 100
67 53.0 0.0 100.2

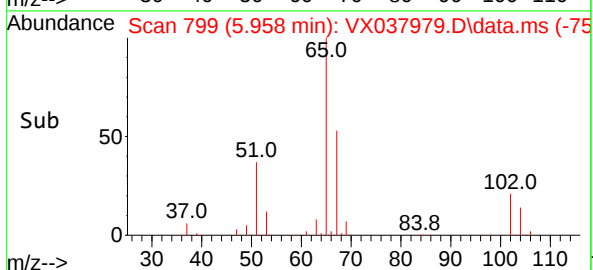
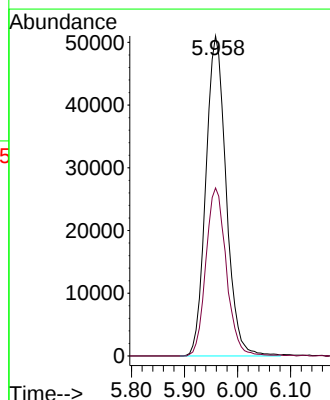
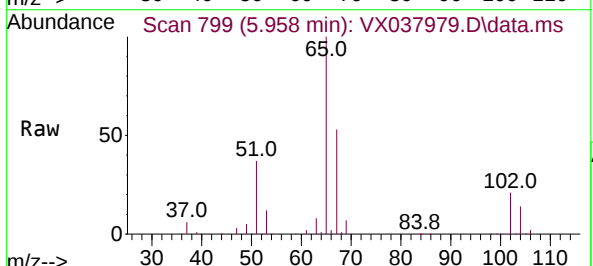




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33




Instrument :
MSVOA_X
ClientSampleId :
MW-104D


Tgt Ion:114 Resp: 367013
Ion Ratio Lower Upper
114 100
63 19.0 0.0 45.0
88 14.9 0.0 36.6

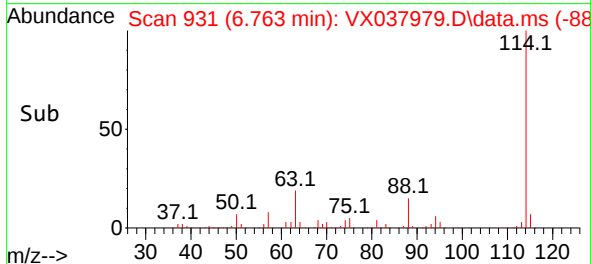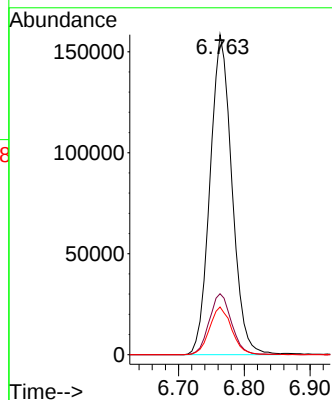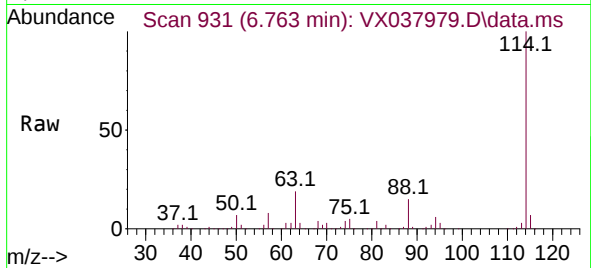

#35
Dibromofluoromethane
Concen: 46.787 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33

Tgt Ion:113 Resp: 114894
Ion Ratio Lower Upper
113 100
111 103.5 82.9 124.3
192 19.3 13.3 19.9

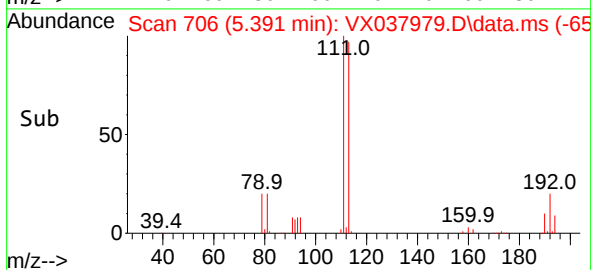
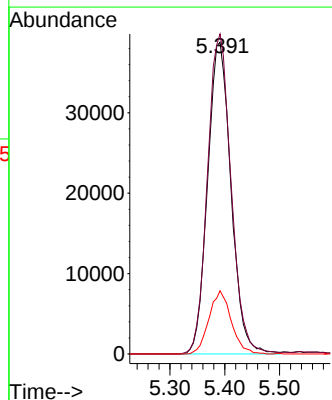
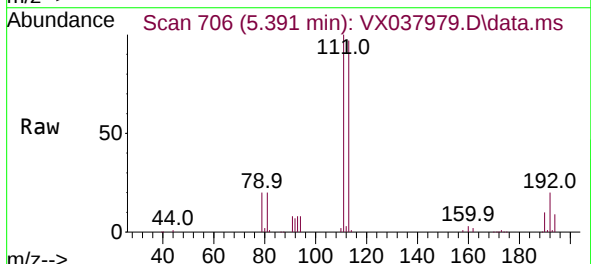


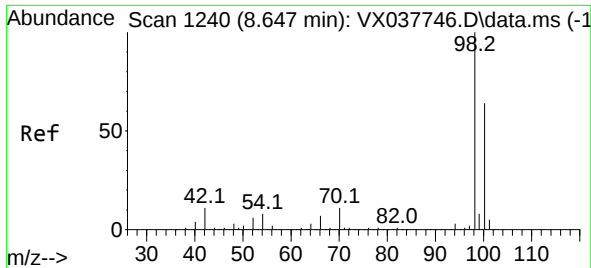

#50
Toluene-d8
Concen: 49.205 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33




Instrument :
MSVOA_X
ClientSampleId :
MW-104D


Tgt Ion: 98 Resp: 448965
Ion Ratio Lower Upper
98 100
100 63.8 53.1 79.7

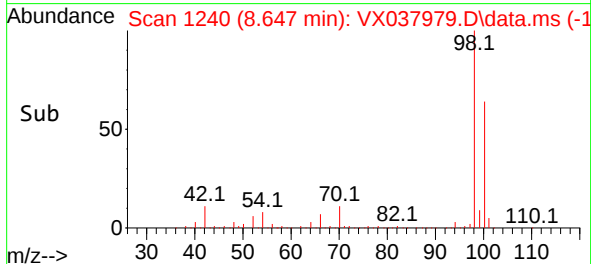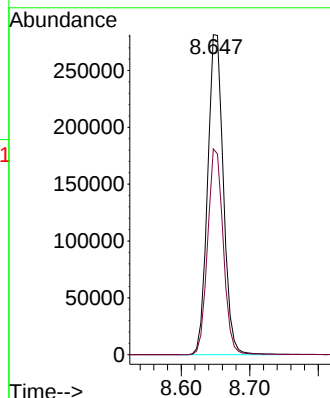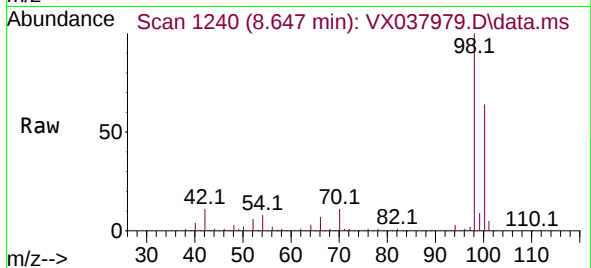

#62
4-Bromofluorobenzene
Concen: 49.177 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33

Tgt Ion: 95 Resp: 163055
Ion Ratio Lower Upper
95 100
174 82.8 0.0 135.6
176 80.3 0.0 131.0


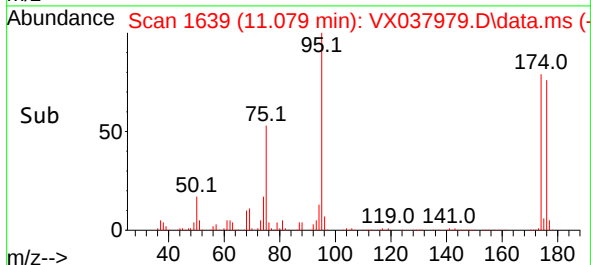
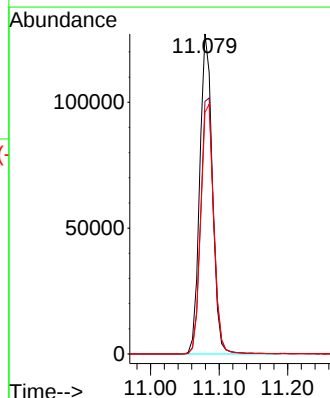
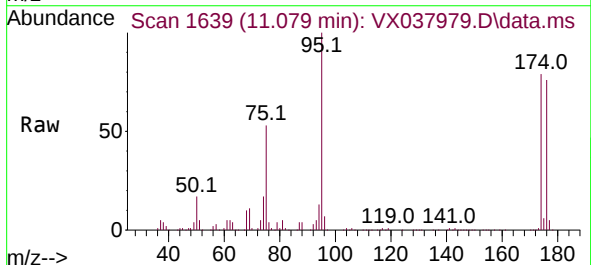


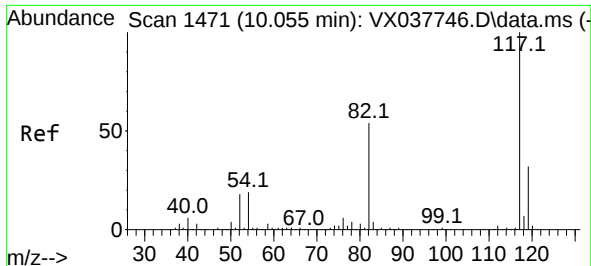

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33

Instrument :
MSVOA_X
ClientSampleId :
MW-104D

Tgt Ion:117 Resp: 351141
Ion Ratio Lower Upper
117 100
82 54.2 46.2 69.4
119 32.1 25.5 38.3

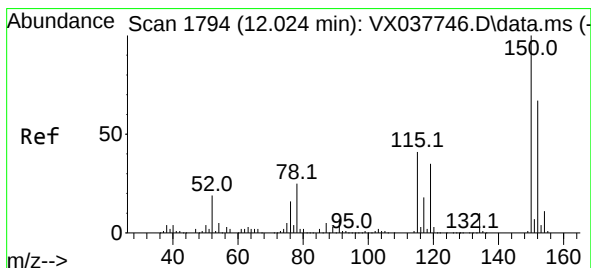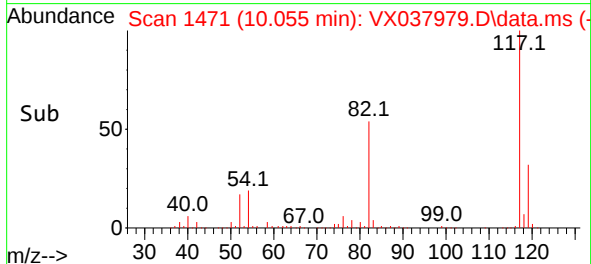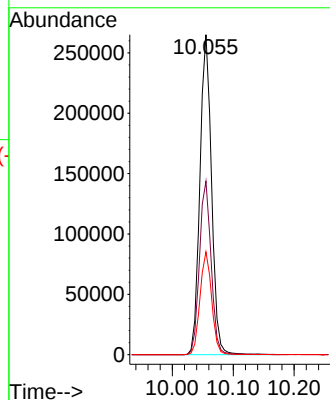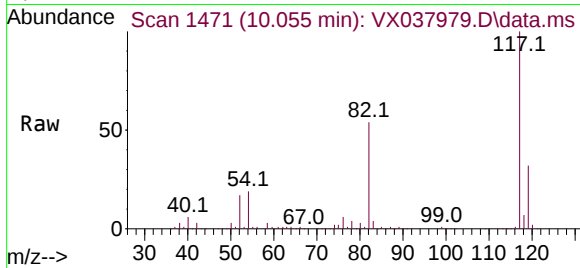

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037979.D
Acq: 29 Sep 2023 16:33

Tgt Ion:152 Resp: 182260
Ion Ratio Lower Upper
152 100
115 59.3 43.3 129.9
150 155.2 0.0 345.0

