

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
 Data File : VX037986.D
 Acq On : 29 Sep 2023 19:15
 Operator : JC/MD
 Sample : 04688-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 29 23:09:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	232715	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	397652	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	389596	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	206301	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	145684	47.648	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.300%
35) Dibromofluoromethane	5.385	113	125626	47.215	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.440%
50) Toluene-d8	8.647	98	486279	49.188	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.380%
62) 4-Bromofluorobenzene	11.079	95	185837	51.730	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.460%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037986.D
Acq On : 29 Sep 2023 19:15
Operator : JC/MD
Sample : 04688-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 29 23:09:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




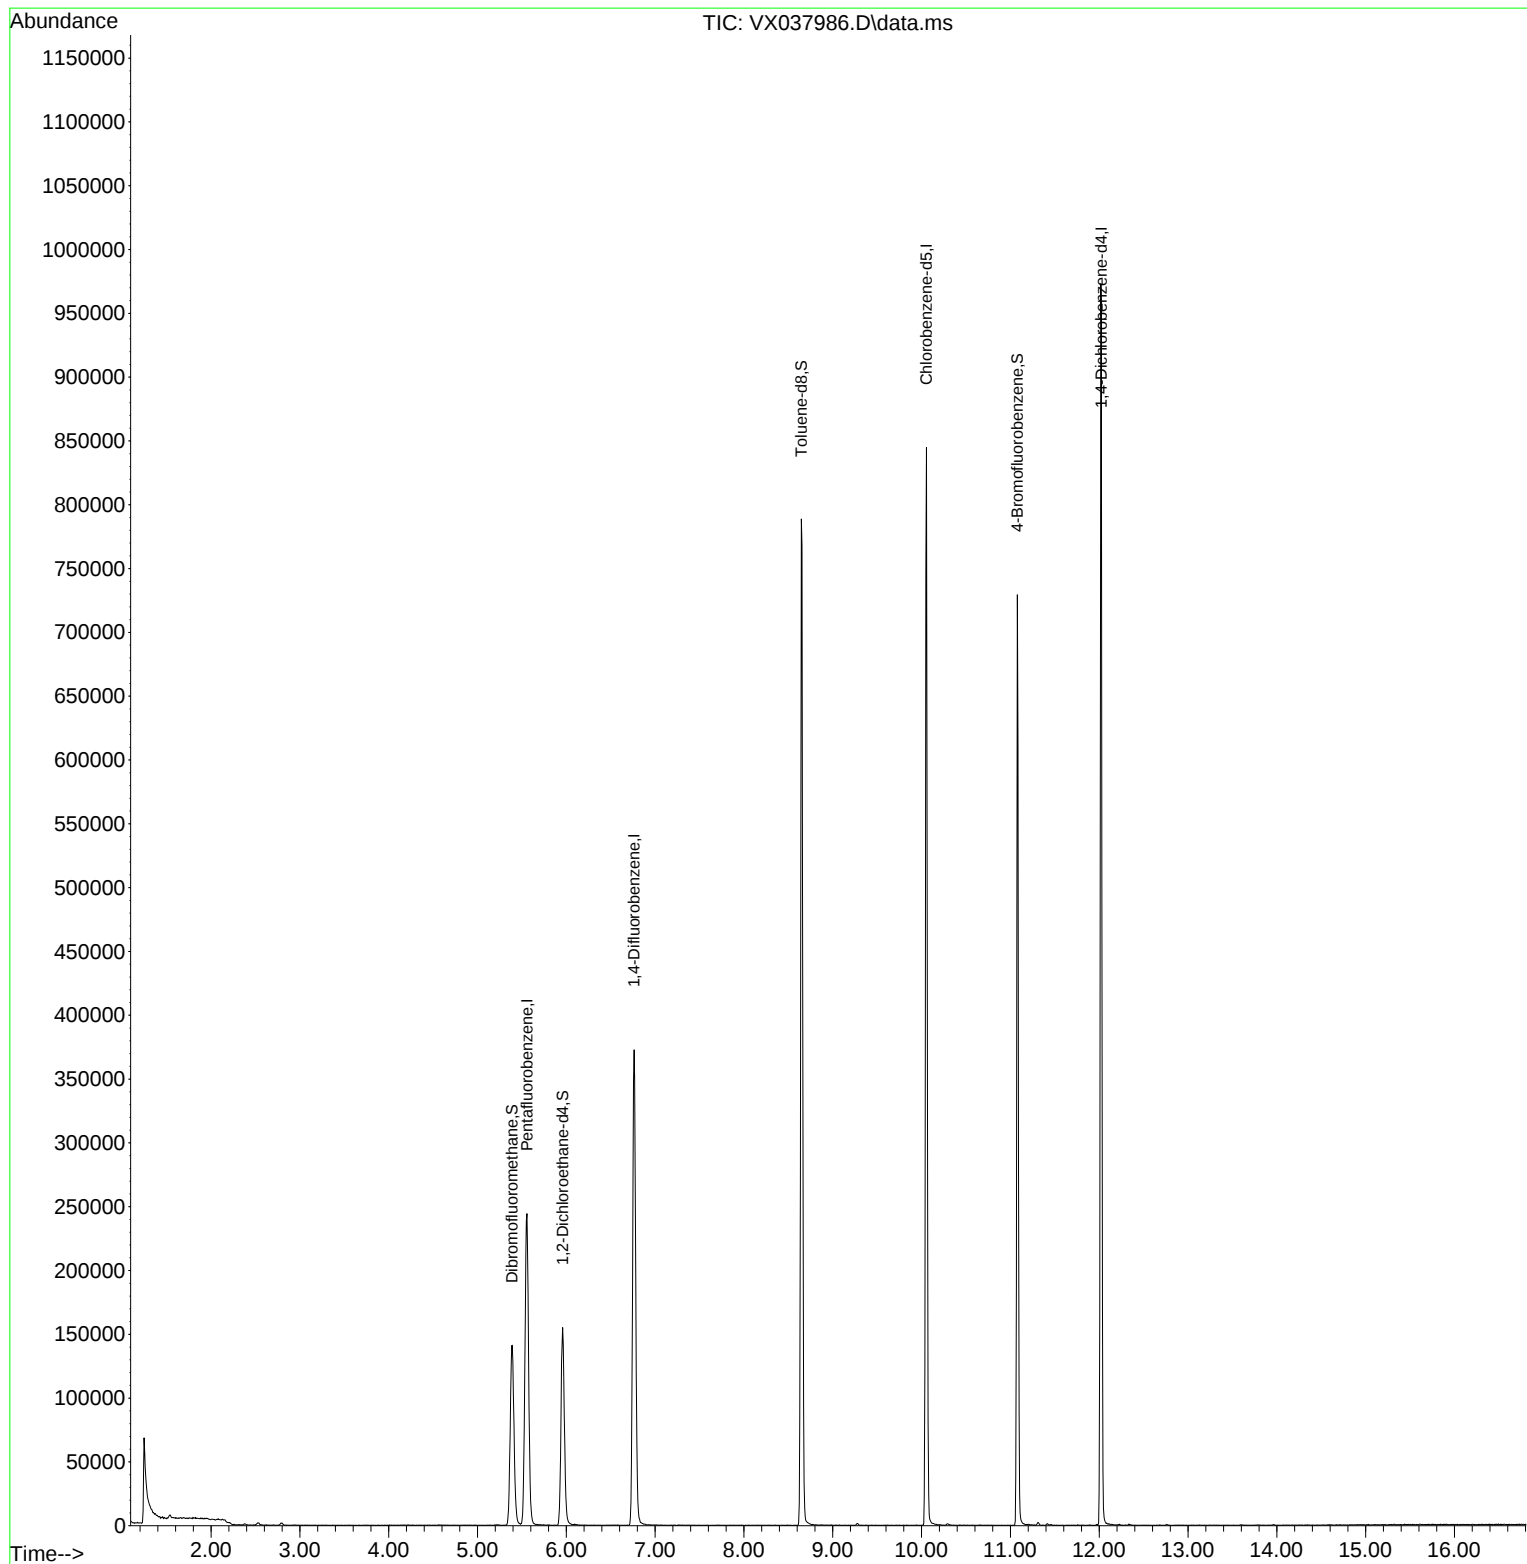




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:168 Resp: 232715
Ion Ratio Lower Upper
168 100
99 58.2 56.6 85.0

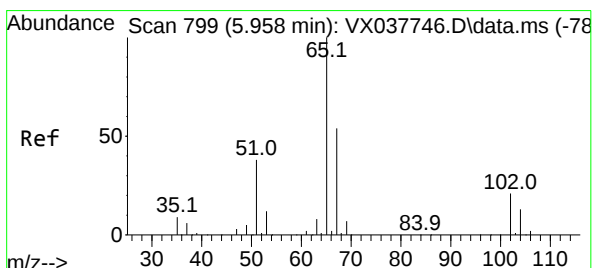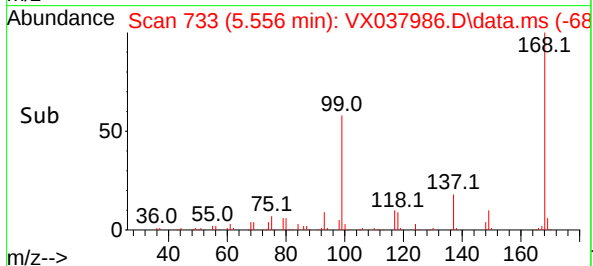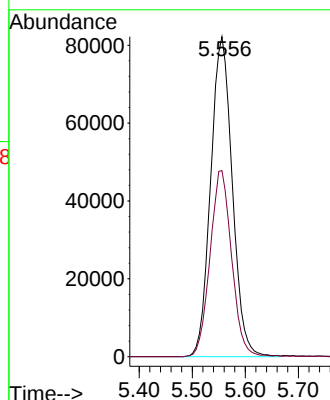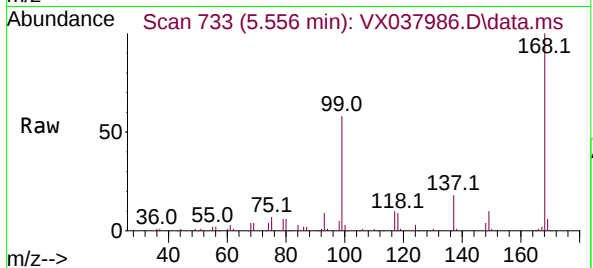

#33
1,2-Dichloroethane-d4
Concen: 47.648 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15

Tgt Ion: 65 Resp: 145684
Ion Ratio Lower Upper
65 100
67 53.0 0.0 100.2


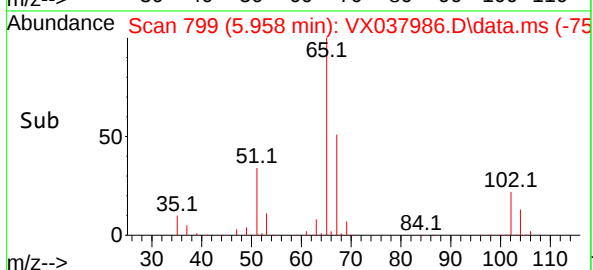
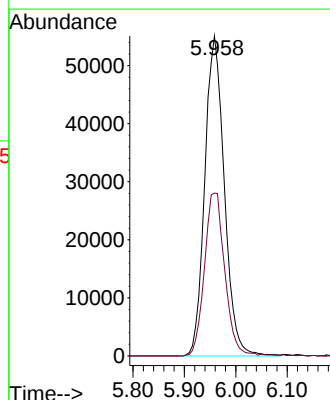
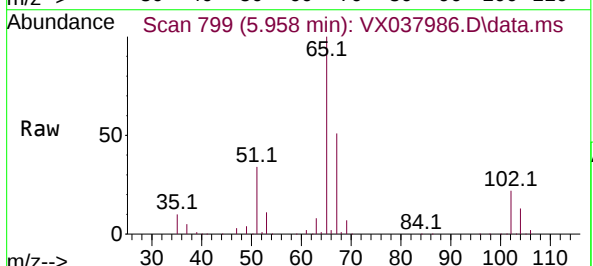




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 397652
Ion Ratio Lower Upper
114 100
63 18.8 0.0 45.0
88 15.0 0.0 36.6

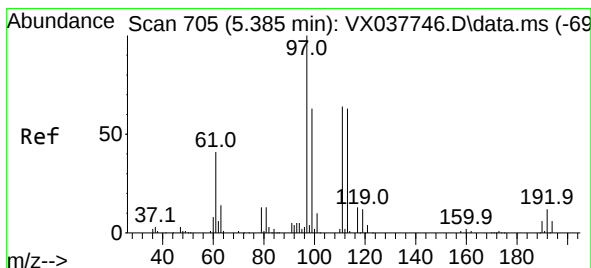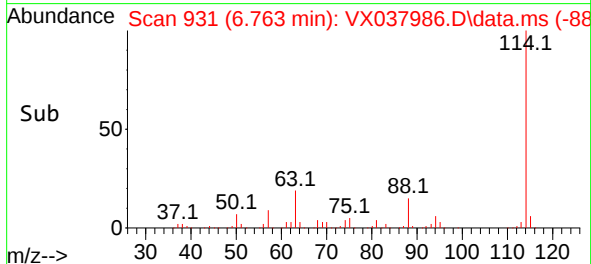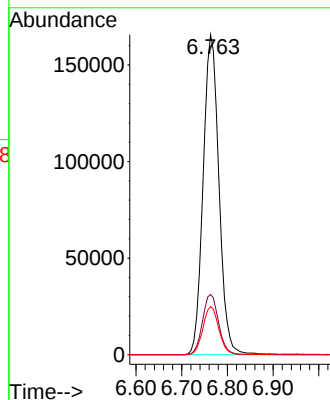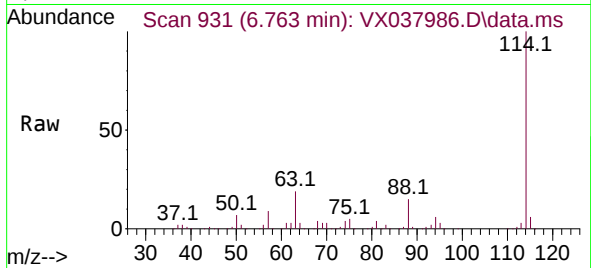

#35
Dibromofluoromethane
Concen: 47.215 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15

Tgt Ion:113 Resp: 125626
Ion Ratio Lower Upper
113 100
111 102.6 82.9 124.3
192 18.7 13.3 19.9

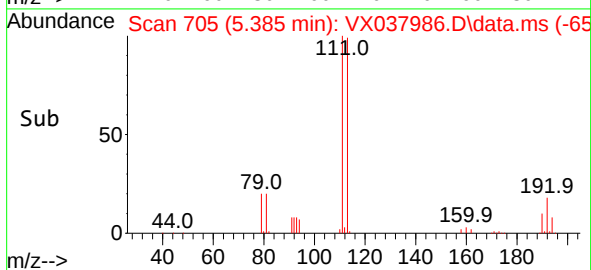
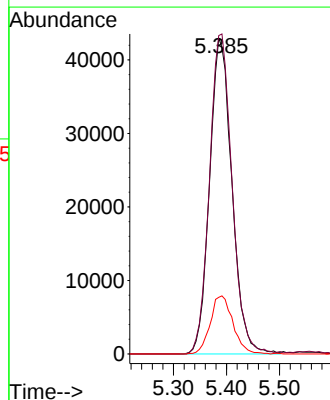
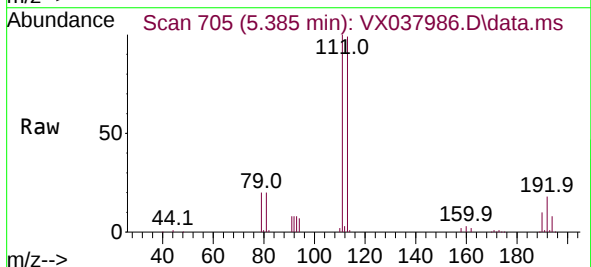


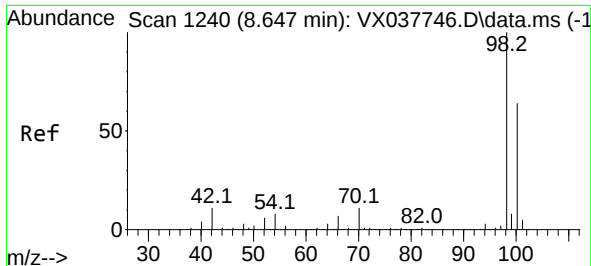

#50
Toluene-d8
Concen: 49.188 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 486279
Ion Ratio Lower Upper
98 100
100 63.8 53.1 79.7

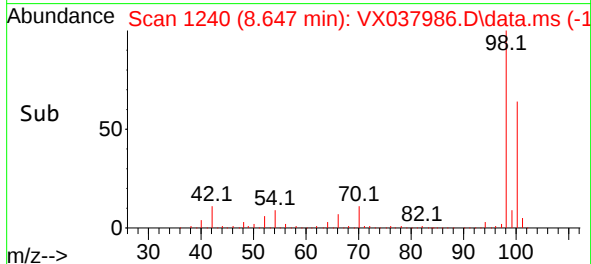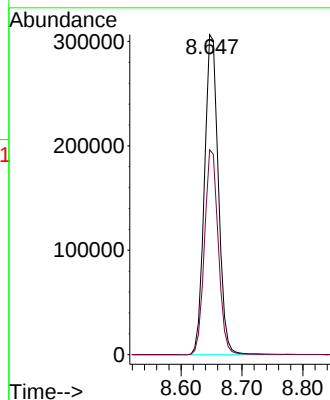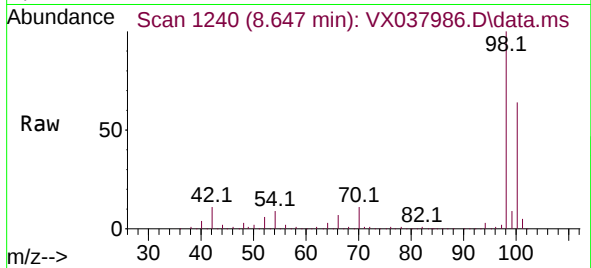

#62
4-Bromofluorobenzene
Concen: 51.730 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15

Tgt Ion: 95 Resp: 185837
Ion Ratio Lower Upper
95 100
174 80.7 0.0 135.6
176 78.9 0.0 131.0


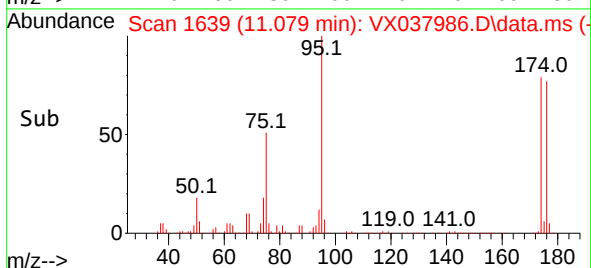
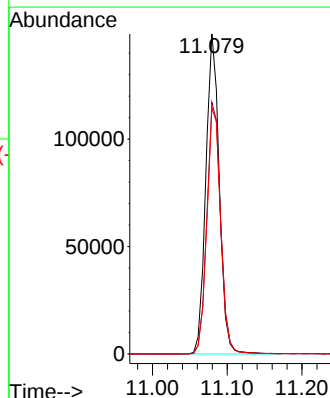
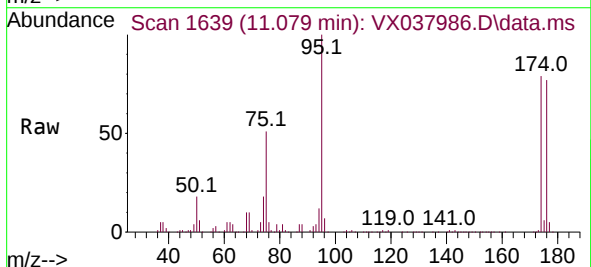


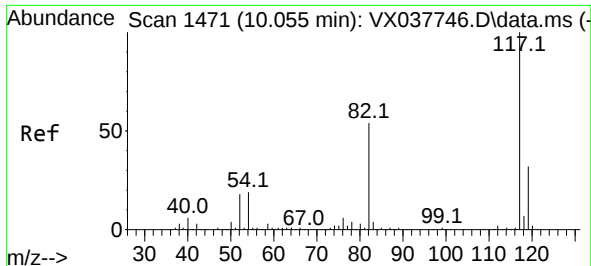

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 389596
Ion Ratio Lower Upper
117 100
82 54.4 46.2 69.4
119 32.2 25.5 38.3

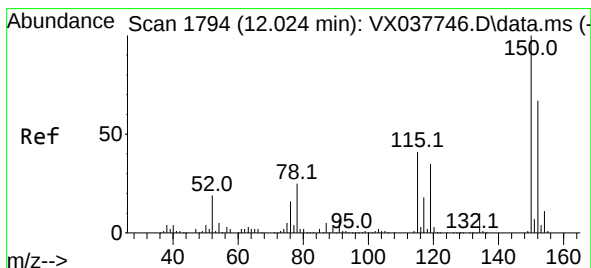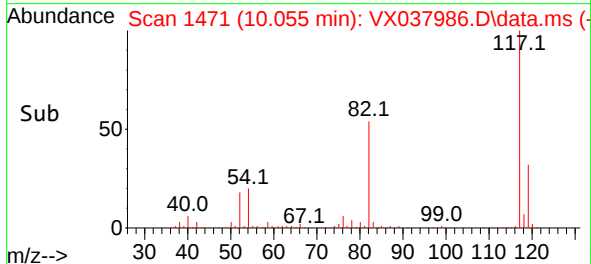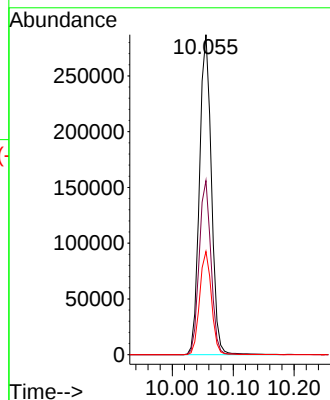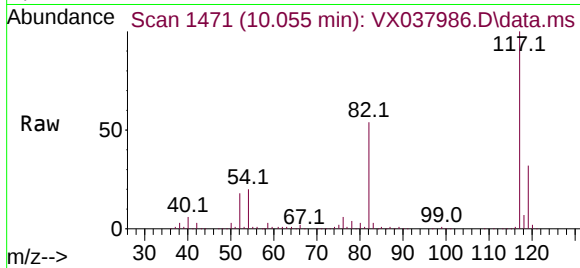

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037986.D
Acq: 29 Sep 2023 19:15

Tgt Ion:152 Resp: 206301
Ion Ratio Lower Upper
152 100
115 59.7 43.3 129.9
150 155.9 0.0 345.0

