

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
 Data File : VX037978.D
 Acq On : 29 Sep 2023 16:10
 Operator : JC/MD
 Sample : 04656-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-103S

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Title : SW846 8260

Signal : TIC: VX037978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	23	30	34	rBV3	9230	20411	1.77%	0.301%
2	2.532	229	237	245	rBV	10387	19204	1.67%	0.283%
3	4.562	559	570	584	rBV	6019	19435	1.69%	0.287%
4	5.391	693	706	721	rBV	129518	381491	33.12%	5.624%
5	5.556	721	733	749	rVB	222528	620189	53.85%	9.143%
6	5.958	789	799	808	rBV	138680	370860	32.20%	5.467%
7	6.038	809	812	826	rVB2	14810	38685	3.36%	0.570%
8	6.763	921	931	947	rBV	342799	822288	71.39%	12.123%
9	8.647	1234	1240	1250	rBV	724083	1148288	99.70%	16.929%
10	10.055	1465	1471	1485	rBV	776731	1058295	91.88%	15.602%
11	11.079	1634	1639	1650	rBV	671343	840553	72.98%	12.392%
12	12.018	1788	1793	1803	rBV	907853	1151788	100.00%	16.980%
13	12.244	1823	1830	1836	rBV	26354	34366	2.98%	0.507%
14	12.908	1933	1939	1945	rBV3	16088	27044	2.35%	0.399%
15	13.286	1997	2001	2006	rVB2	9309	12145	1.05%	0.179%
16	13.506	2034	2037	2042	rBV3	10273	14069	1.22%	0.207%
17	13.774	2072	2081	2090	rBV	91296	120710	10.48%	1.780%
18	14.640	2214	2223	2226	rBV2	7510	11818	1.03%	0.174%
19	14.780	2241	2246	2256	rBV2	28478	41303	3.59%	0.609%
20	16.322	2494	2499	2508	rBV	16246	30171	2.62%	0.445%




Sum of corrected areas: 6783113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037978.D
Acq On : 29 Sep 2023 16:10
Operator : JC/MD
Sample : 04656-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

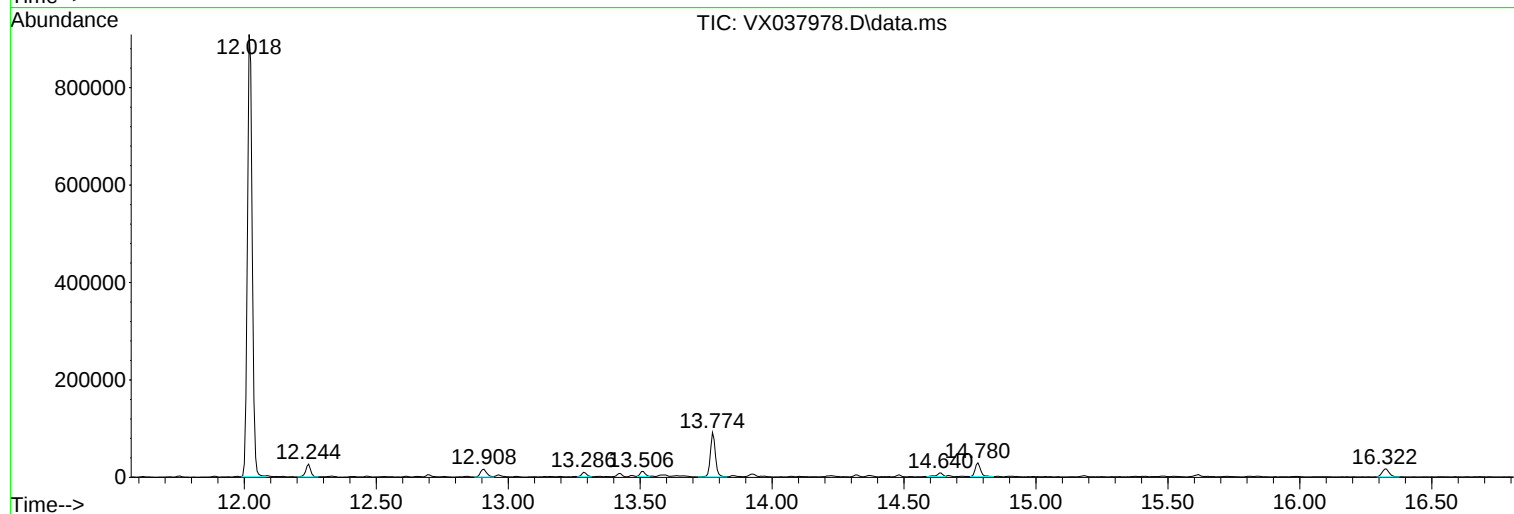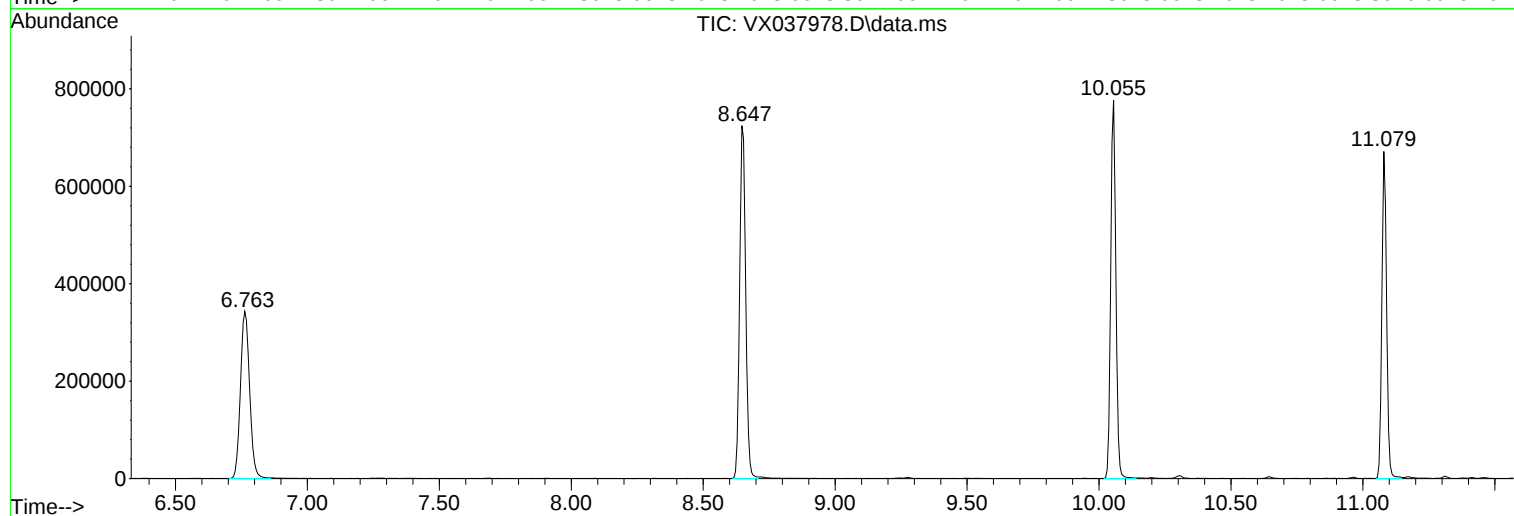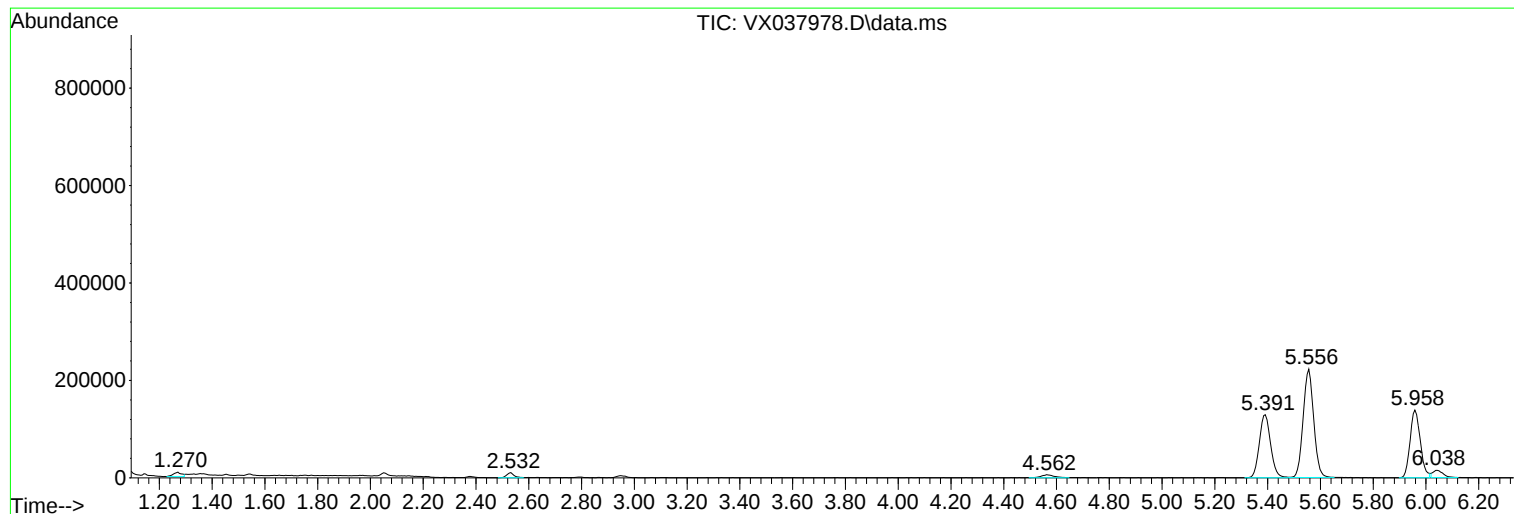

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037978.D
Acq On : 29 Sep 2023 16:10
Operator : JC/MD
Sample : 04656-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092923\
Data File : VX037978.D
Acq On : 29 Sep 2023 16:10
Operator : JC/MD
Sample : 04656-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------