

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
 Data File : VX012719.D
 Acq On : 30 Sep 2019 20:36
 Operator : JC/SP
 Sample : K5081-22
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-MW126S-20190926

Quant Time: Oct 01 04:54:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 23 12:27:01 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	166191	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	287781	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	240093	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	89516	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	117223	48.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.88%	
35) Dibromofluoromethane	5.49	113	87025	50.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.56%	
50) Toluene-d8	8.71	98	336186	50.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.88%	
62) 4-Bromofluorobenzene	11.14	95	112376	43.30	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.60%	
Target Compounds						
16) Acetone	2.44	43	7097	5.536	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012719.D
Acq On : 30 Sep 2019 20:36
Operator : JC/SP
Sample : K5081-22
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
SA-MW126S-20190926

Quant Time: Oct 01 04:54:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260
QLast Update : Mon Sep 23 12:27:01 2019
Response via : Initial Calibration




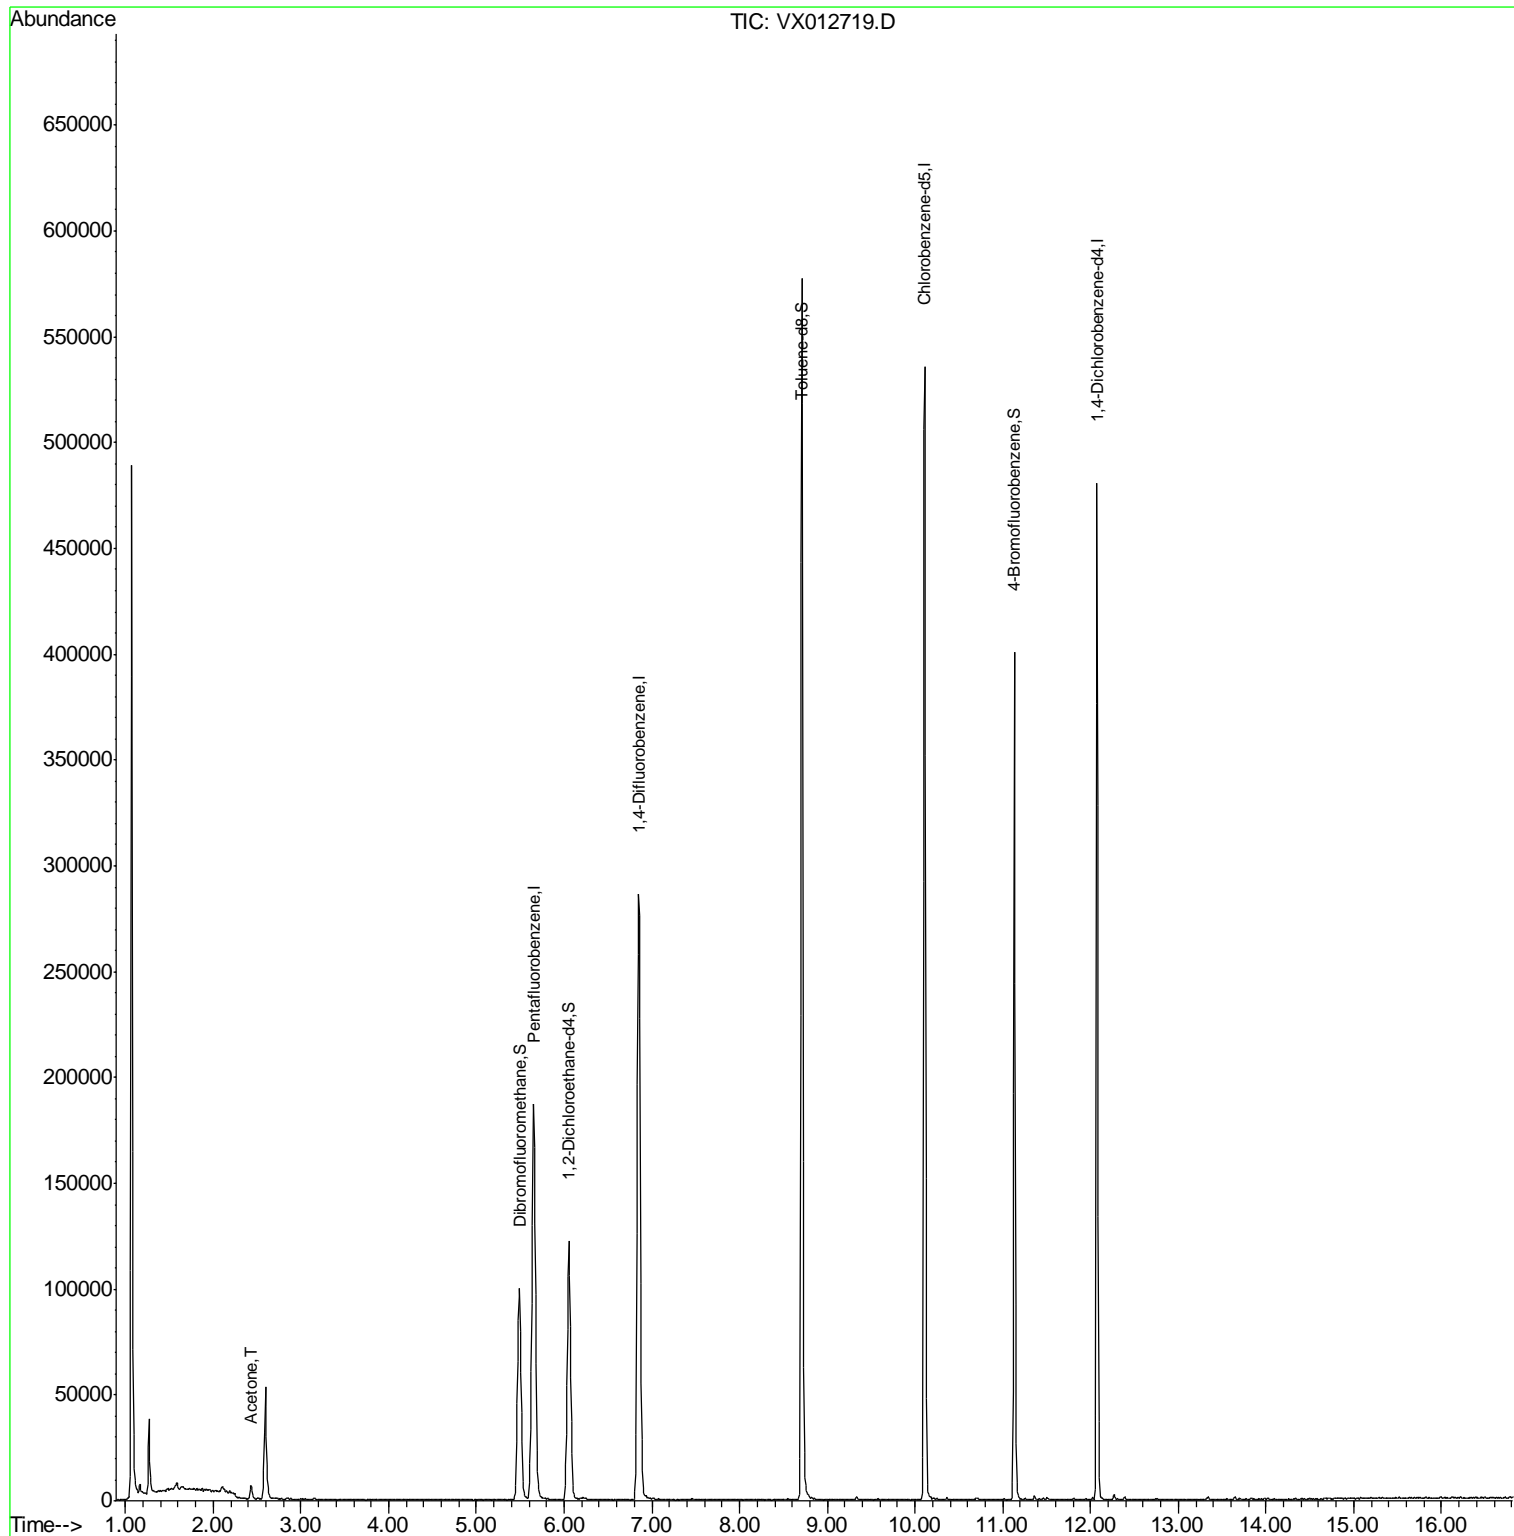


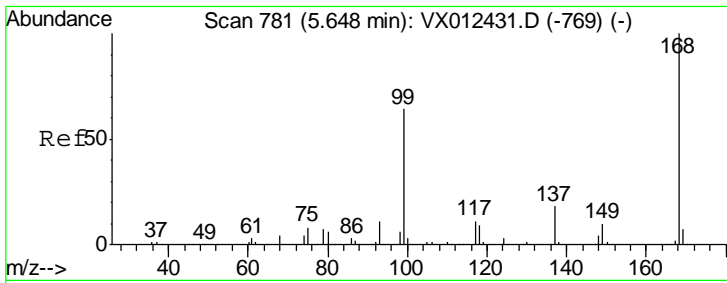

#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.65 min Scan# 782
 Delta R.T. 0.01 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36




Instrument :
 MSVOA_X
 ClientSampled :
 SA-MW126S-20190926


Tgt Ion: 168 Resp: 166191
 Ion Ratio Lower Upper
 168 100
 99 63.9 51.4 77.2

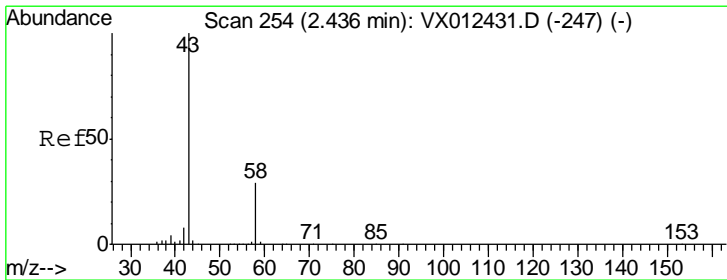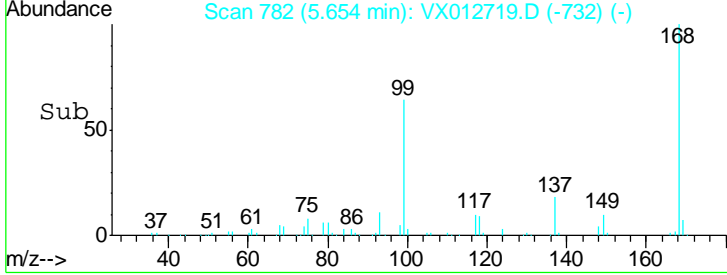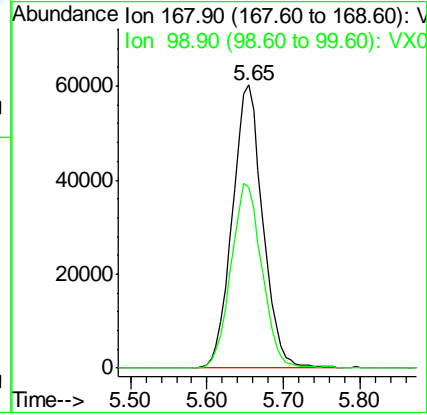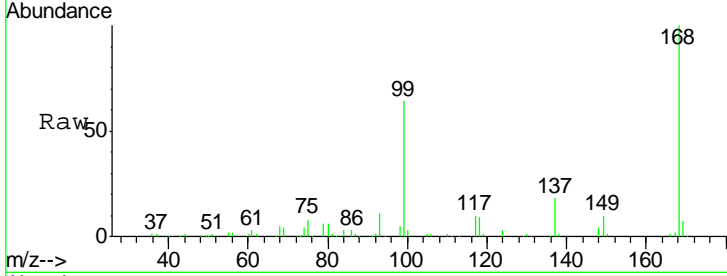

#16
 Acetone
 Concen: 5.536 ug/l
 RT: 2.44 min Scan# 254
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36

Tgt Ion: 43 Resp: 7097
 Ion Ratio Lower Upper
 43 100
 58 26.0 23.3 34.9


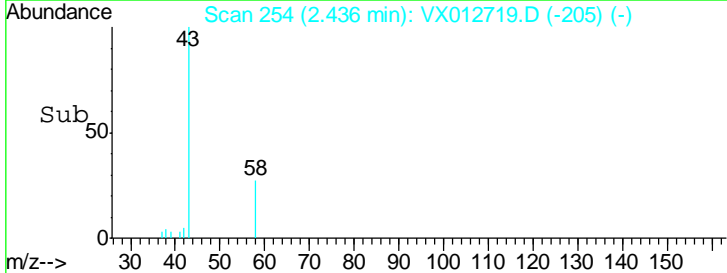
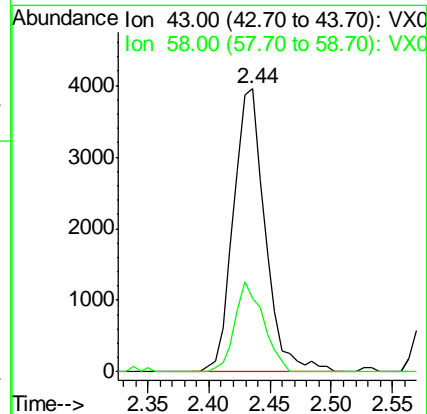
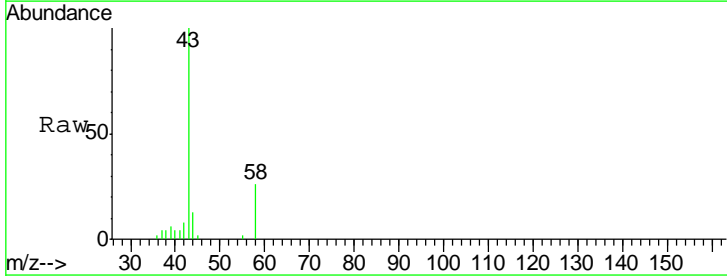


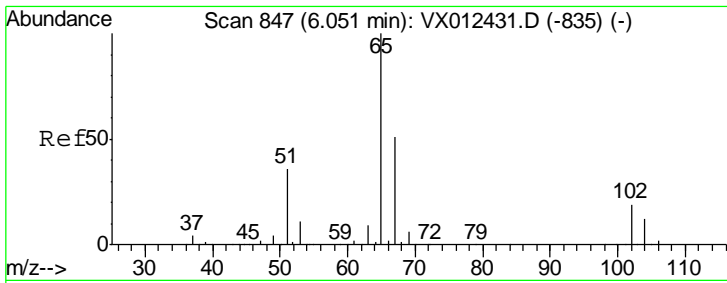

#33
 1,2-Dichloroethane-d4
 Concen: 48.438 ug/l
 RT: 6.05 min Scan# 847
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36




Instrument :
 MSVOA_X
ClientSampled :
 SA-MW126S-20190926


Tgt Ion	Resp	Lower	Upper
65	117223		
67	50.9	0.0	101.2

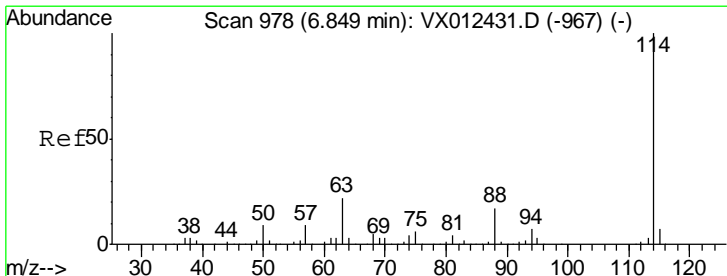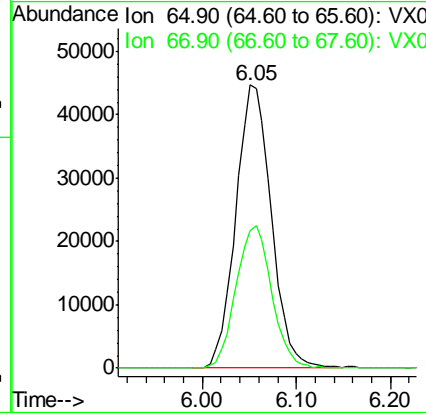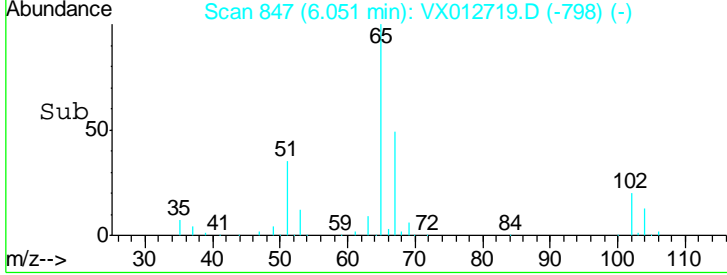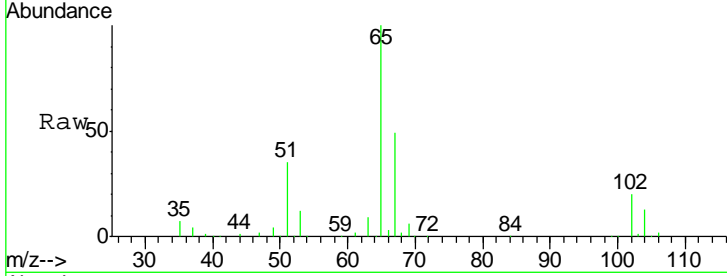

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 978
 Delta R.T. 0.01 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36

Tgt Ion	Resp	Lower	Upper
114	287781		
63	20.9	0.0	43.2
88	15.4	0.0	33.2


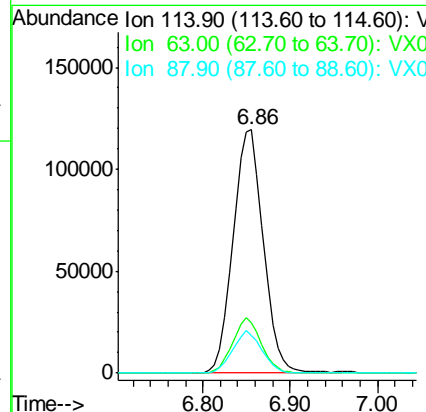
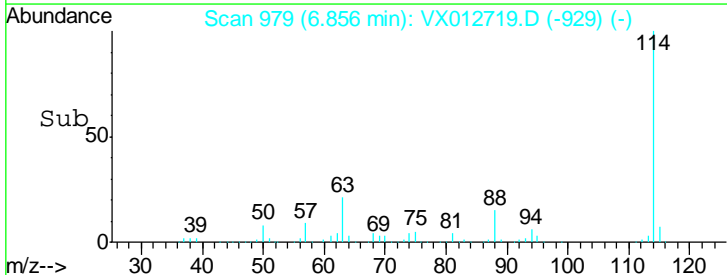
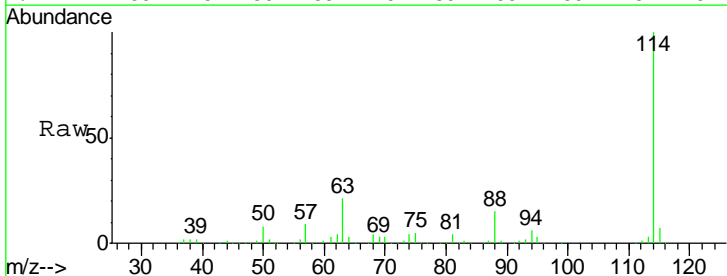


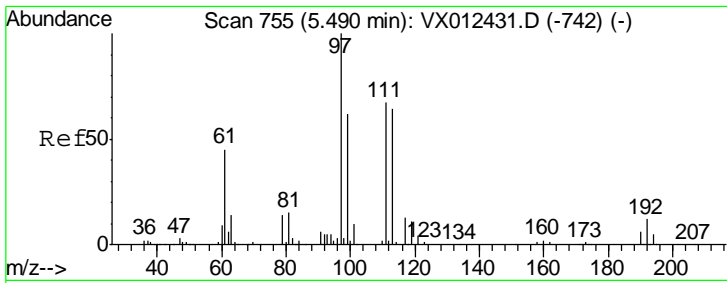

#35
 Dibromofluoromethane
 Concen: 50.777 ug/l
 RT: 5.49 min Scan# 755
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36




Instrument :
 MSVOA_X
ClientSampled :
 SA-MW126S-20190926


Tgt Ion	Resp	Lower	Upper
113	87025		
111	103.3	83.4	125.2
192	17.9	14.4	21.6

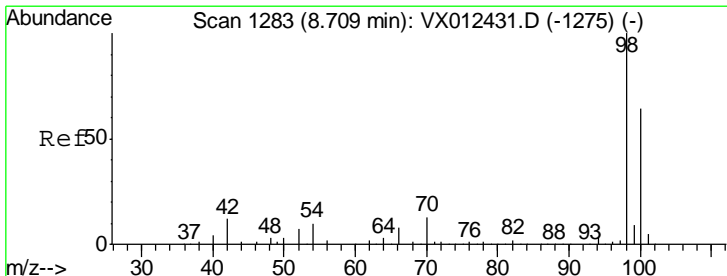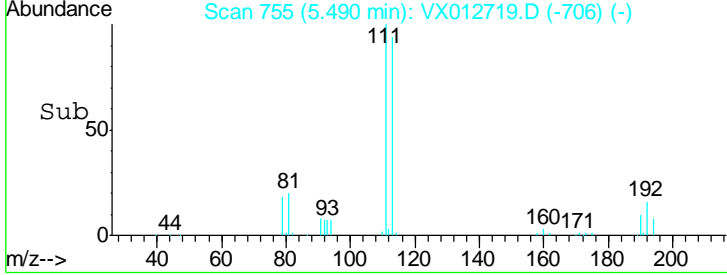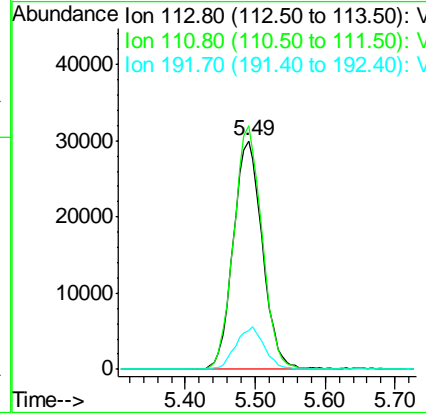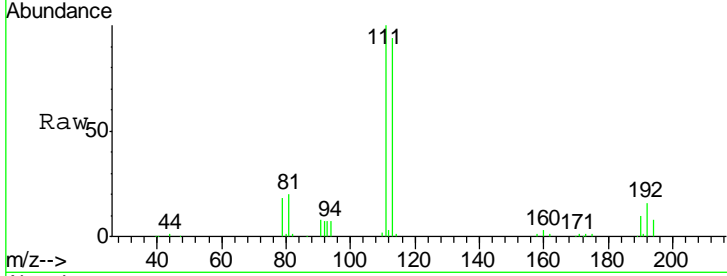

#50
 Toluene-d8
 Concen: 50.936 ug/l
 RT: 8.71 min Scan# 1283
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36

Tgt Ion	Resp	Lower	Upper
98	336186		
100	67.5	53.4	80.2


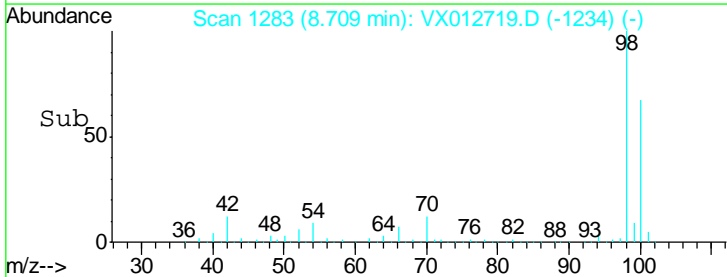
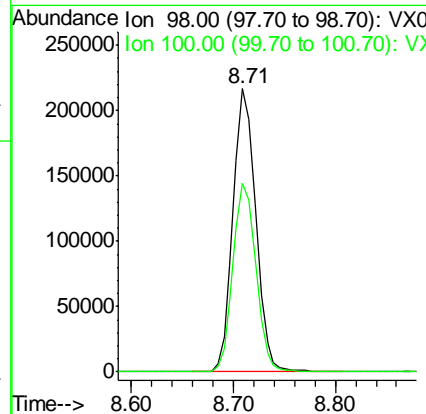
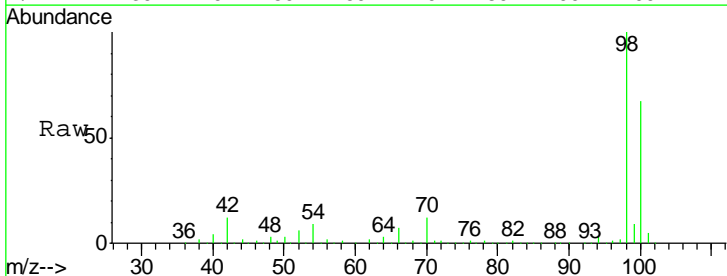


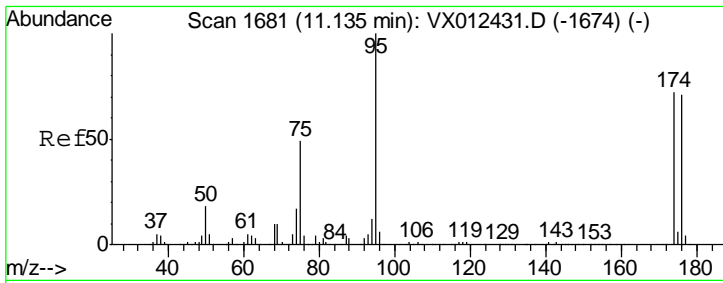

#62
 4-Bromofluorobenzene
 Concen: 43.301 ug/l
 RT: 11.14 min Scan# 1681
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36




Instrument : MSVOA_X
 ClientSampleId : SA-MW126S-20190926


Tgt Ion	Resp	Lower	Upper
95	112376		
174	68.7	0.0	140.0
176	67.1	0.0	135.4

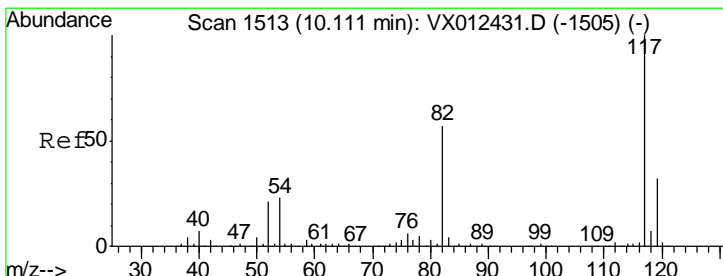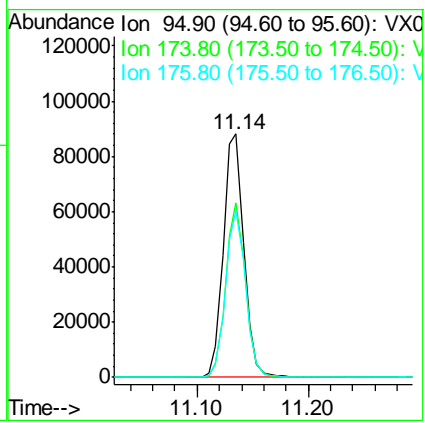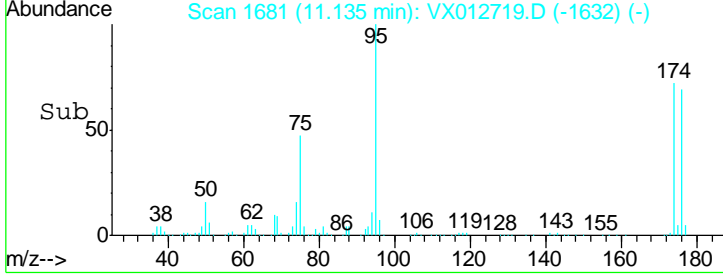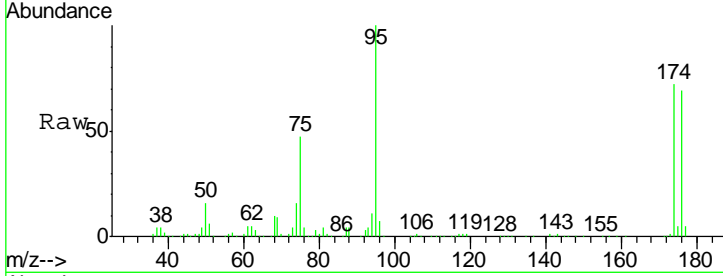

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.11 min Scan# 1513
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36

Tgt Ion	Resp	Lower	Upper
117	240093		
82	57.7	45.9	68.9
119	31.7	25.3	37.9

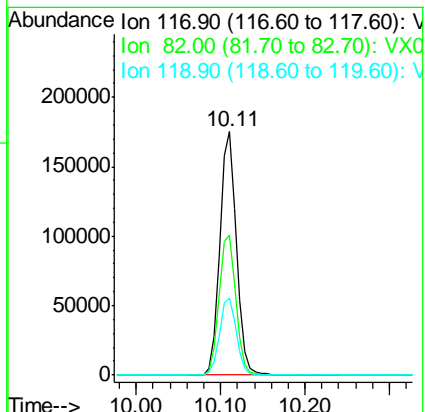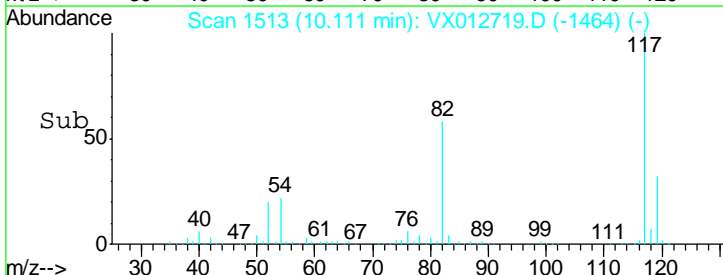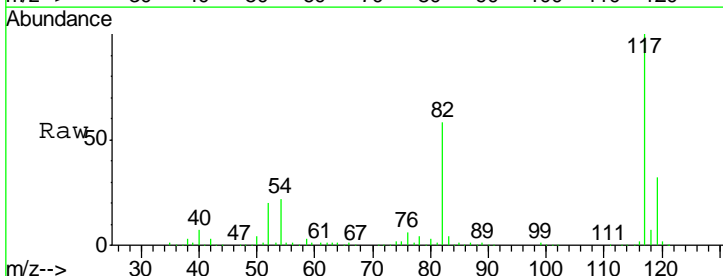

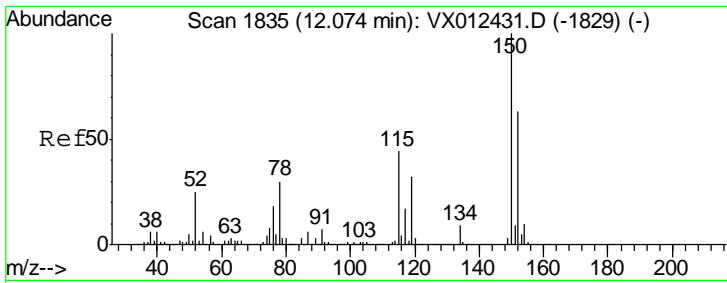

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.07 min Scan# 1835
 Delta R.T. 0.00 min
 Lab File: VX012719.D
 Acq: 30 Sep 2019 20:36

Instrument : MSVOA_X
 ClientSampleId : SA-MW126S-20190926

Tot Ion	Resp	Lower	Upper
152	100		
115	63.0	44.1	132.3
150	157.0	0.0	343.8

