

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012706.D
Acq On : 30 Sep 2019 15:32
Operator : JC/SP
Sample : K5081-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ118I-20190926

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	346110	431453	45.90%	8.145%
2	1.265	58	62	70	rBV	36091	44728	4.76%	0.844%
3	2.430	249	253	261	rBV	8125	12718	1.35%	0.240%
4	2.594	273	280	293	rBV	55906	100221	10.66%	1.892%
5	5.490	741	755	768	rBV2	101701	289958	30.84%	5.474%
6	5.649	768	781	794	rBV	190220	537521	57.18%	10.147%
7	6.051	836	847	863	rBV2	123374	329241	35.02%	6.215%
8	6.850	968	978	995	rBV	296356	700992	74.57%	13.233%
9	8.709	1276	1283	1301	rBV	591095	940053	100.00%	17.746%
10	10.111	1507	1513	1526	rBV	533362	769186	81.82%	14.521%
11	11.135	1675	1681	1697	rBV	404525	538511	57.29%	10.166%
12	12.074	1830	1835	1844	rVB	489231	602568	64.10%	11.375%


Sum of corrected areas: 5297150

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012706.D
Acq On : 30 Sep 2019 15:32
Operator : JC/SP
Sample : K5081-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ118I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

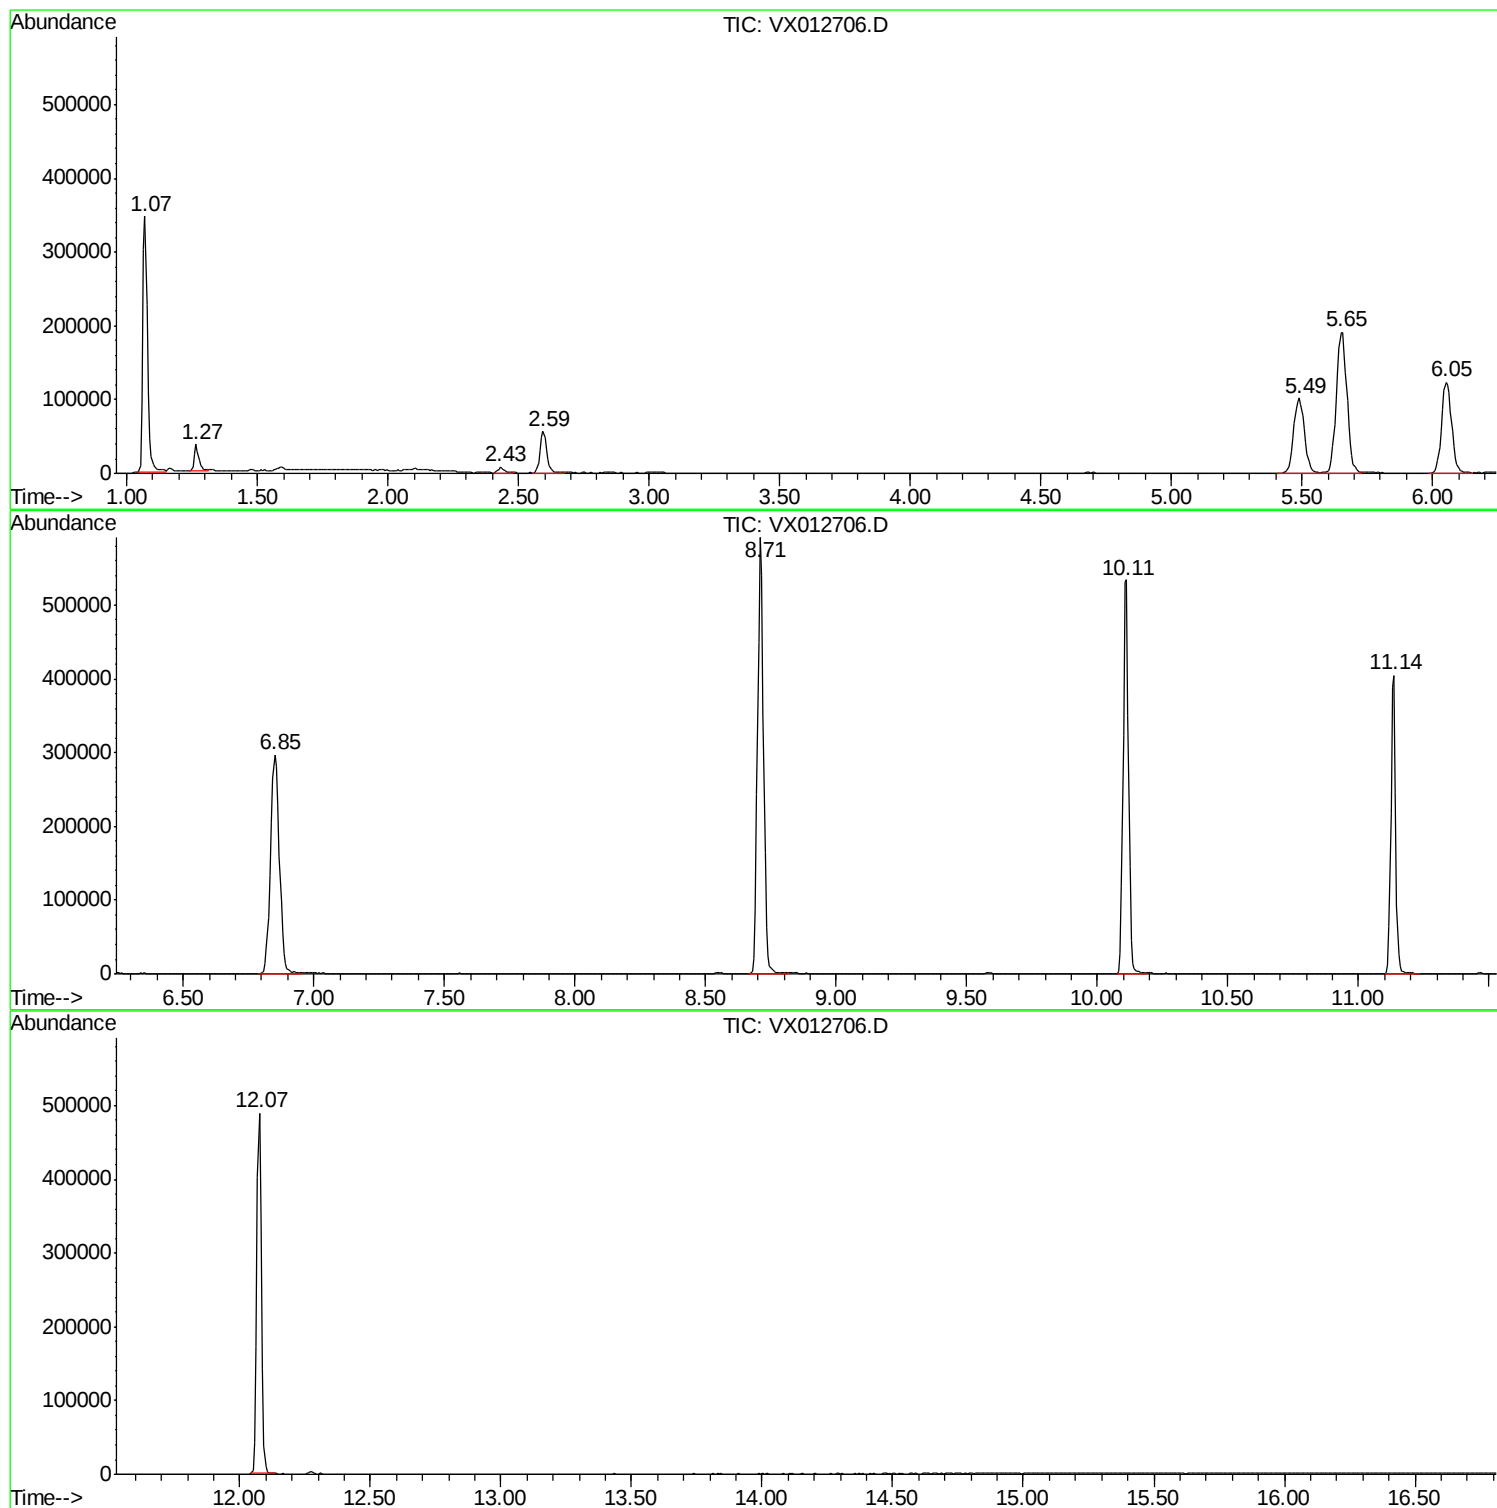

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012706.D
Acq On : 30 Sep 2019 15:32
Operator : JC/SP
Sample : K5081-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ118I-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	9.32 ug/l	100221	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4		Formamide	45	CH3NO	000075-12-7	5
5		Ethylamine	45	C2H7N	000075-04-7	5

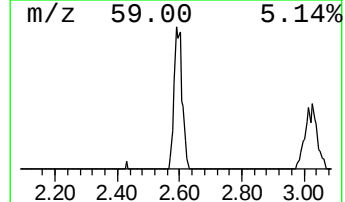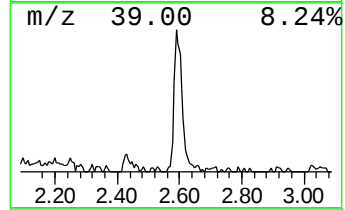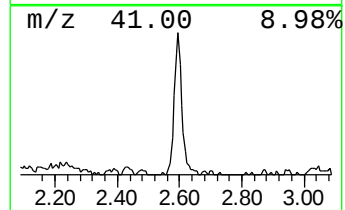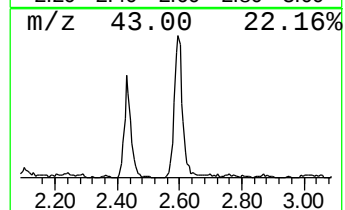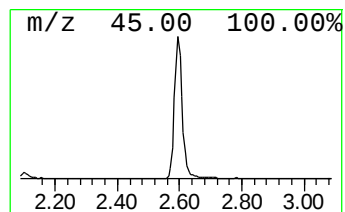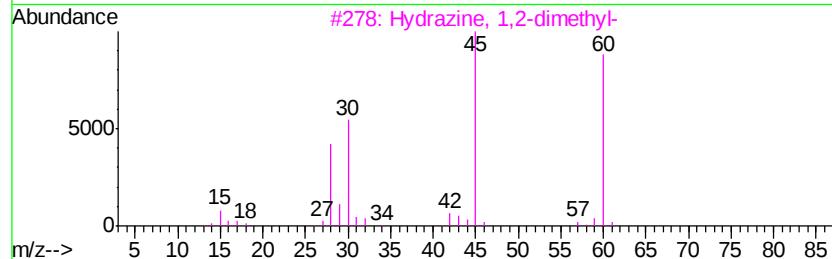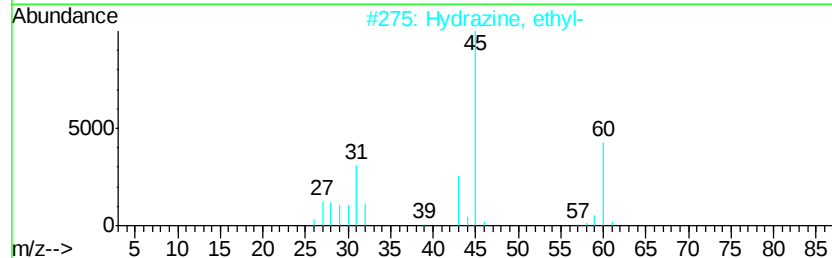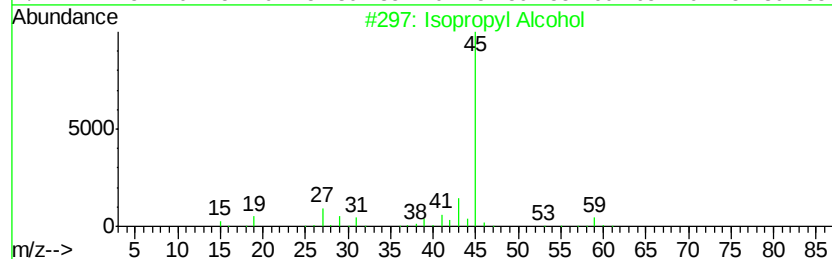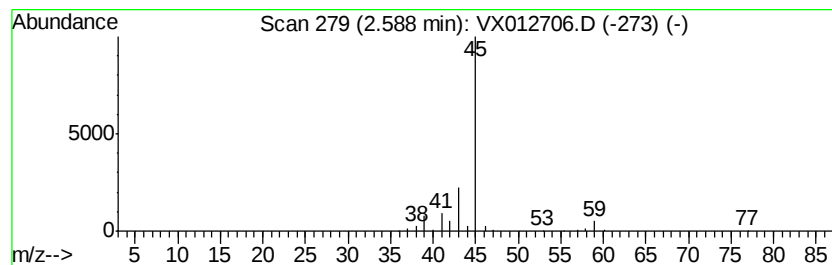

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX093019\
Data File : VX012706.D
Acq On : 30 Sep 2019 15:32
Operator : JC/SP
Sample : K5081-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ118I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	9.3	ug/l	100221	1	5.65	537521	50.0