

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
 Data File : VX012707.D
 Acq On : 30 Sep 2019 15:56
 Operator : JC/SP
 Sample : K5081-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ123S-20190926

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	350326	442951	45.95%	8.076%
2	1.265	58	62	68	rBV	37223	46790	4.85%	0.853%
3	1.332	68	73	77	rBV3	6576	17205	1.78%	0.314%
4	2.436	248	254	260	rBV	6691	11487	1.19%	0.209%
5	2.594	272	280	290	rBV	51621	94084	9.76%	1.715%
6	5.490	743	755	768	rBV	105551	296561	30.77%	5.407%
7	5.655	768	782	797	rBV	192714	543258	56.36%	9.905%
8	6.051	833	847	864	rBV	129514	336169	34.88%	6.129%
9	6.850	969	978	998	rBV	302186	720492	74.75%	13.136%
10	8.709	1275	1283	1301	rBV	596956	963912	100.00%	17.574%
11	10.111	1507	1513	1527	rBV	570937	797383	82.72%	14.538%
12	11.135	1675	1681	1691	rBV	436780	565080	58.62%	10.303%
13	12.074	1829	1835	1843	rBV	522879	649480	67.38%	11.841%


Sum of corrected areas: 5484852

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012707.D
Acq On : 30 Sep 2019 15:56
Operator : JC/SP
Sample : K5081-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ123S-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

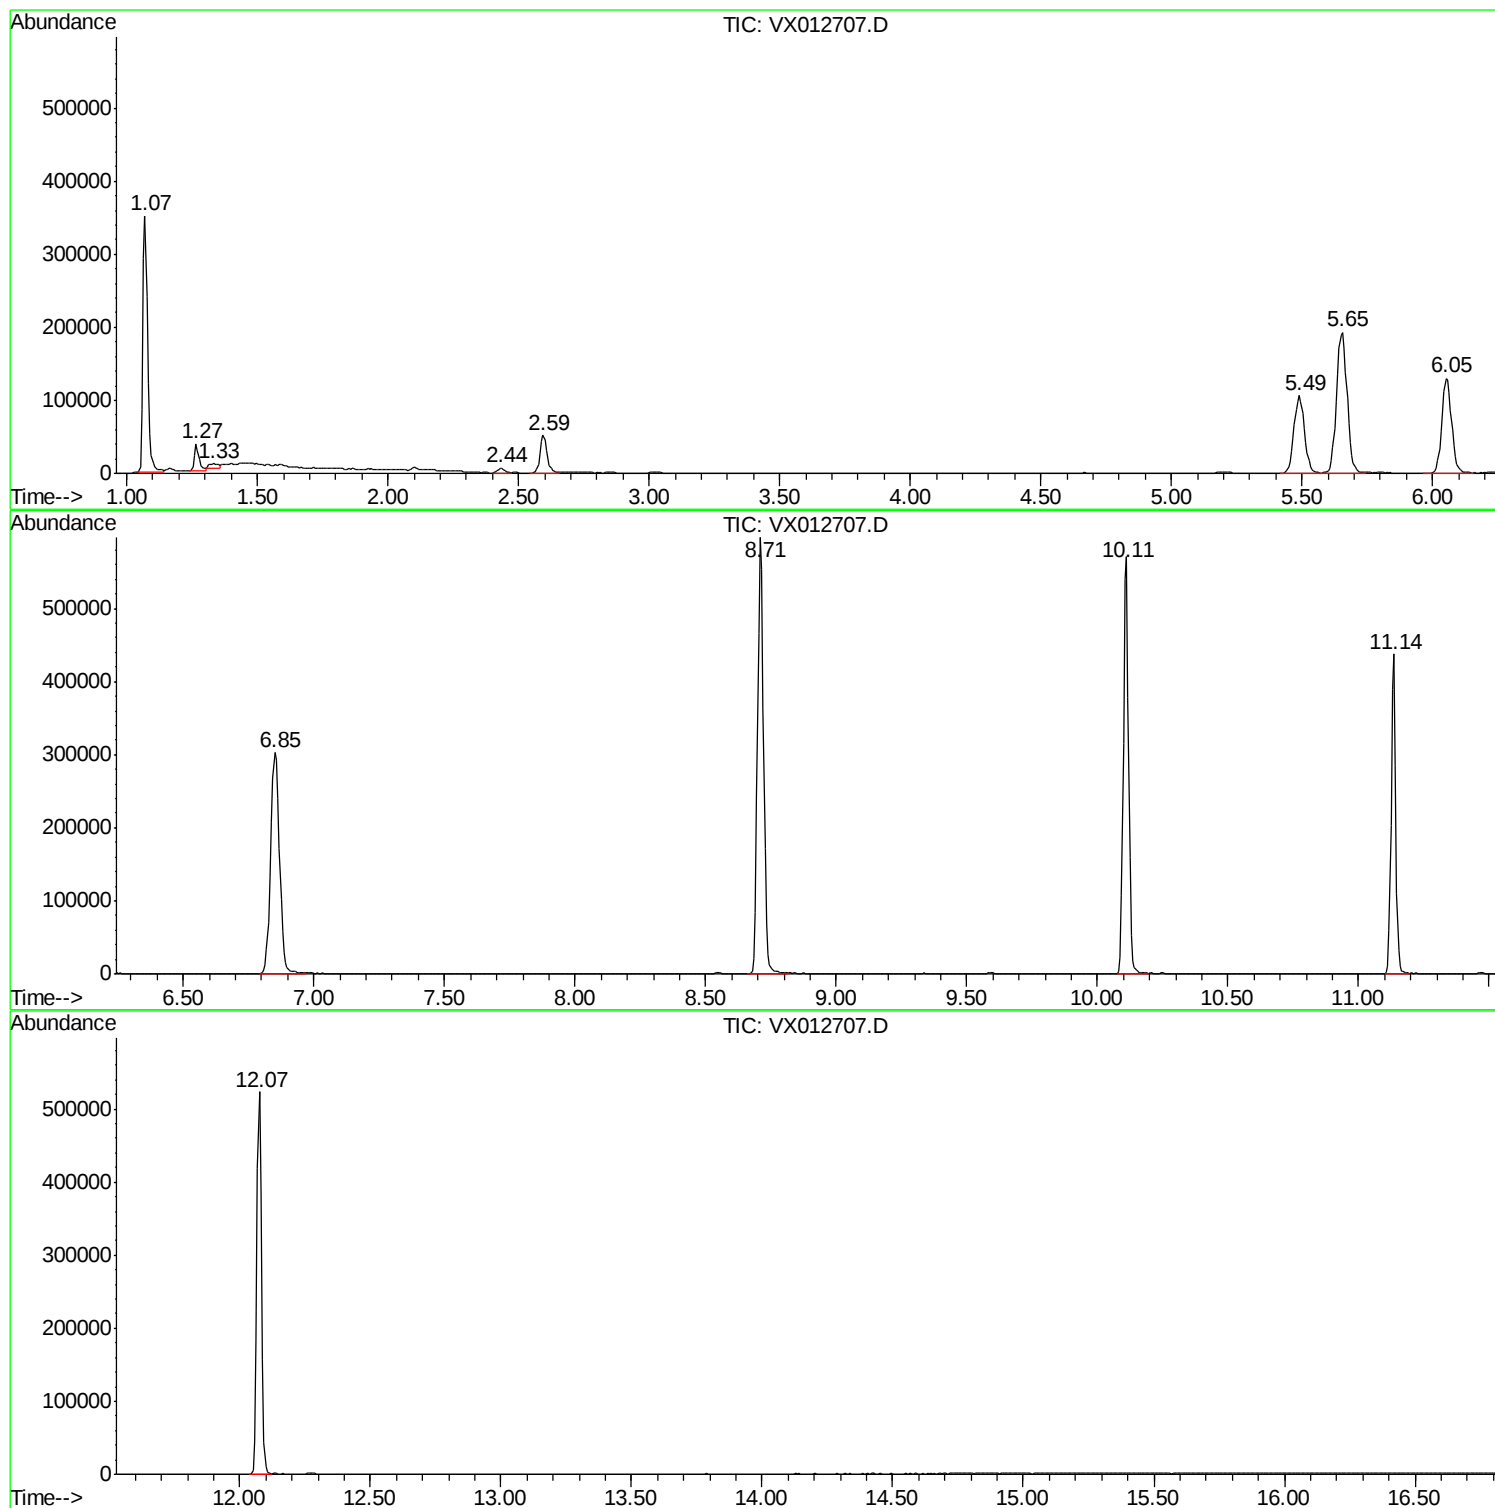

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012707.D
Acq On : 30 Sep 2019 15:56
Operator : JC/SP
Sample : K5081-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ123S-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	8.66 ug/l	94084	Pentafluorobenzene	5.65

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		4-Penten-2-ol	86	C5H10O	000625-31-0	9
4		Ethylamine	45	C2H7N	000075-04-7	5
5		Formamide	45	CH3NO	000075-12-7	5

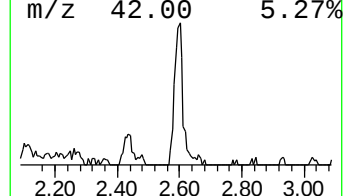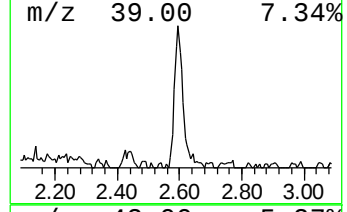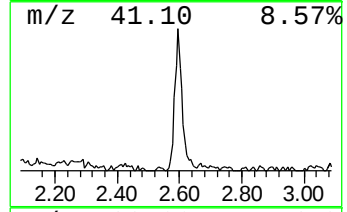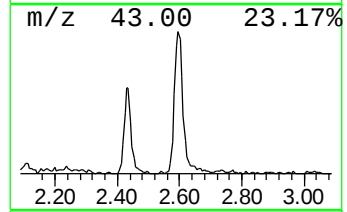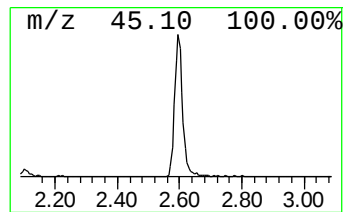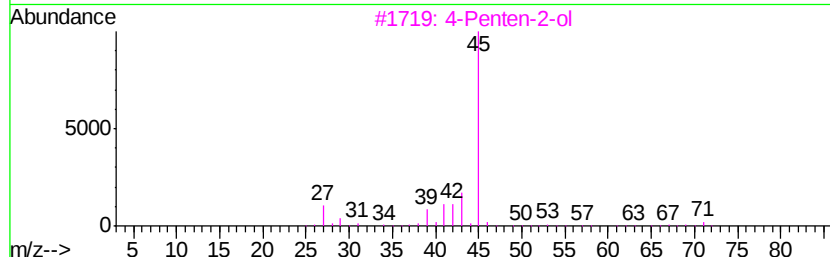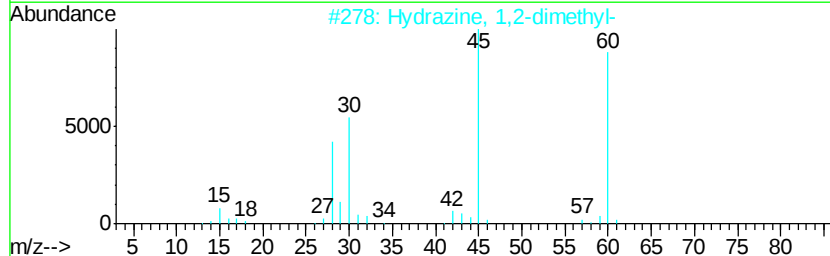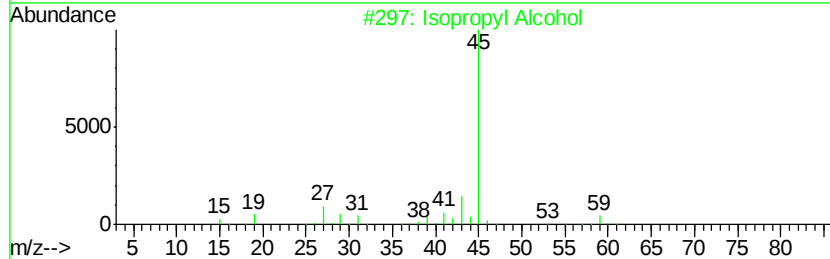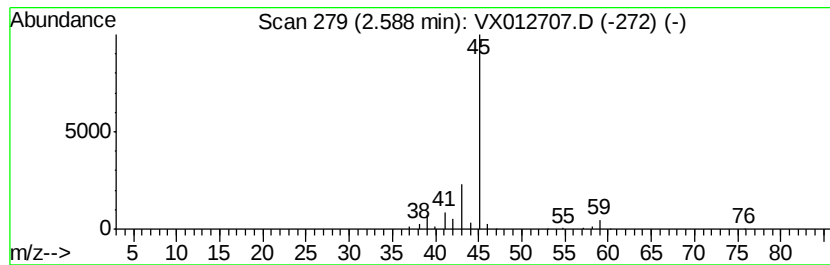

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX093019\
Data File : VX012707.D
Acq On : 30 Sep 2019 15:56
Operator : JC/SP
Sample : K5081-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ123S-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	8.7	ug/l	94084	1	5.65	543258	50.0