

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012709.D
Acq On : 30 Sep 2019 16:43
Operator : JC/SP
Sample : K5081-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ12311-20190926

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	44	rBV	372750	473385	52.16%	9.008%
2	1.265	58	62	69	rBV	39329	48196	5.31%	0.917%
3	2.594	270	280	293	rBV	67828	122811	13.53%	2.337%
4	3.691	453	460	467	rVB2	4139	9257	1.02%	0.176%
5	5.490	742	755	767	rBV	98661	280830	30.94%	5.344%
6	5.654	770	782	795	rBV	183654	518919	57.18%	9.875%
7	6.051	838	847	863	rBV	118764	320718	35.34%	6.103%
8	6.849	968	978	997	rBV	290145	687001	75.70%	13.073%
9	8.709	1276	1283	1295	rBV	569978	907527	100.00%	17.270%
10	10.111	1507	1513	1527	rBV	548224	753794	83.06%	14.345%
11	11.135	1675	1681	1692	rBV	399481	526576	58.02%	10.021%
12	12.074	1829	1835	1842	rBV	492149	605909	66.76%	11.530%


Sum of corrected areas: 5254923

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012709.D
Acq On : 30 Sep 2019 16:43
Operator : JC/SP
Sample : K5081-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ123I1-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

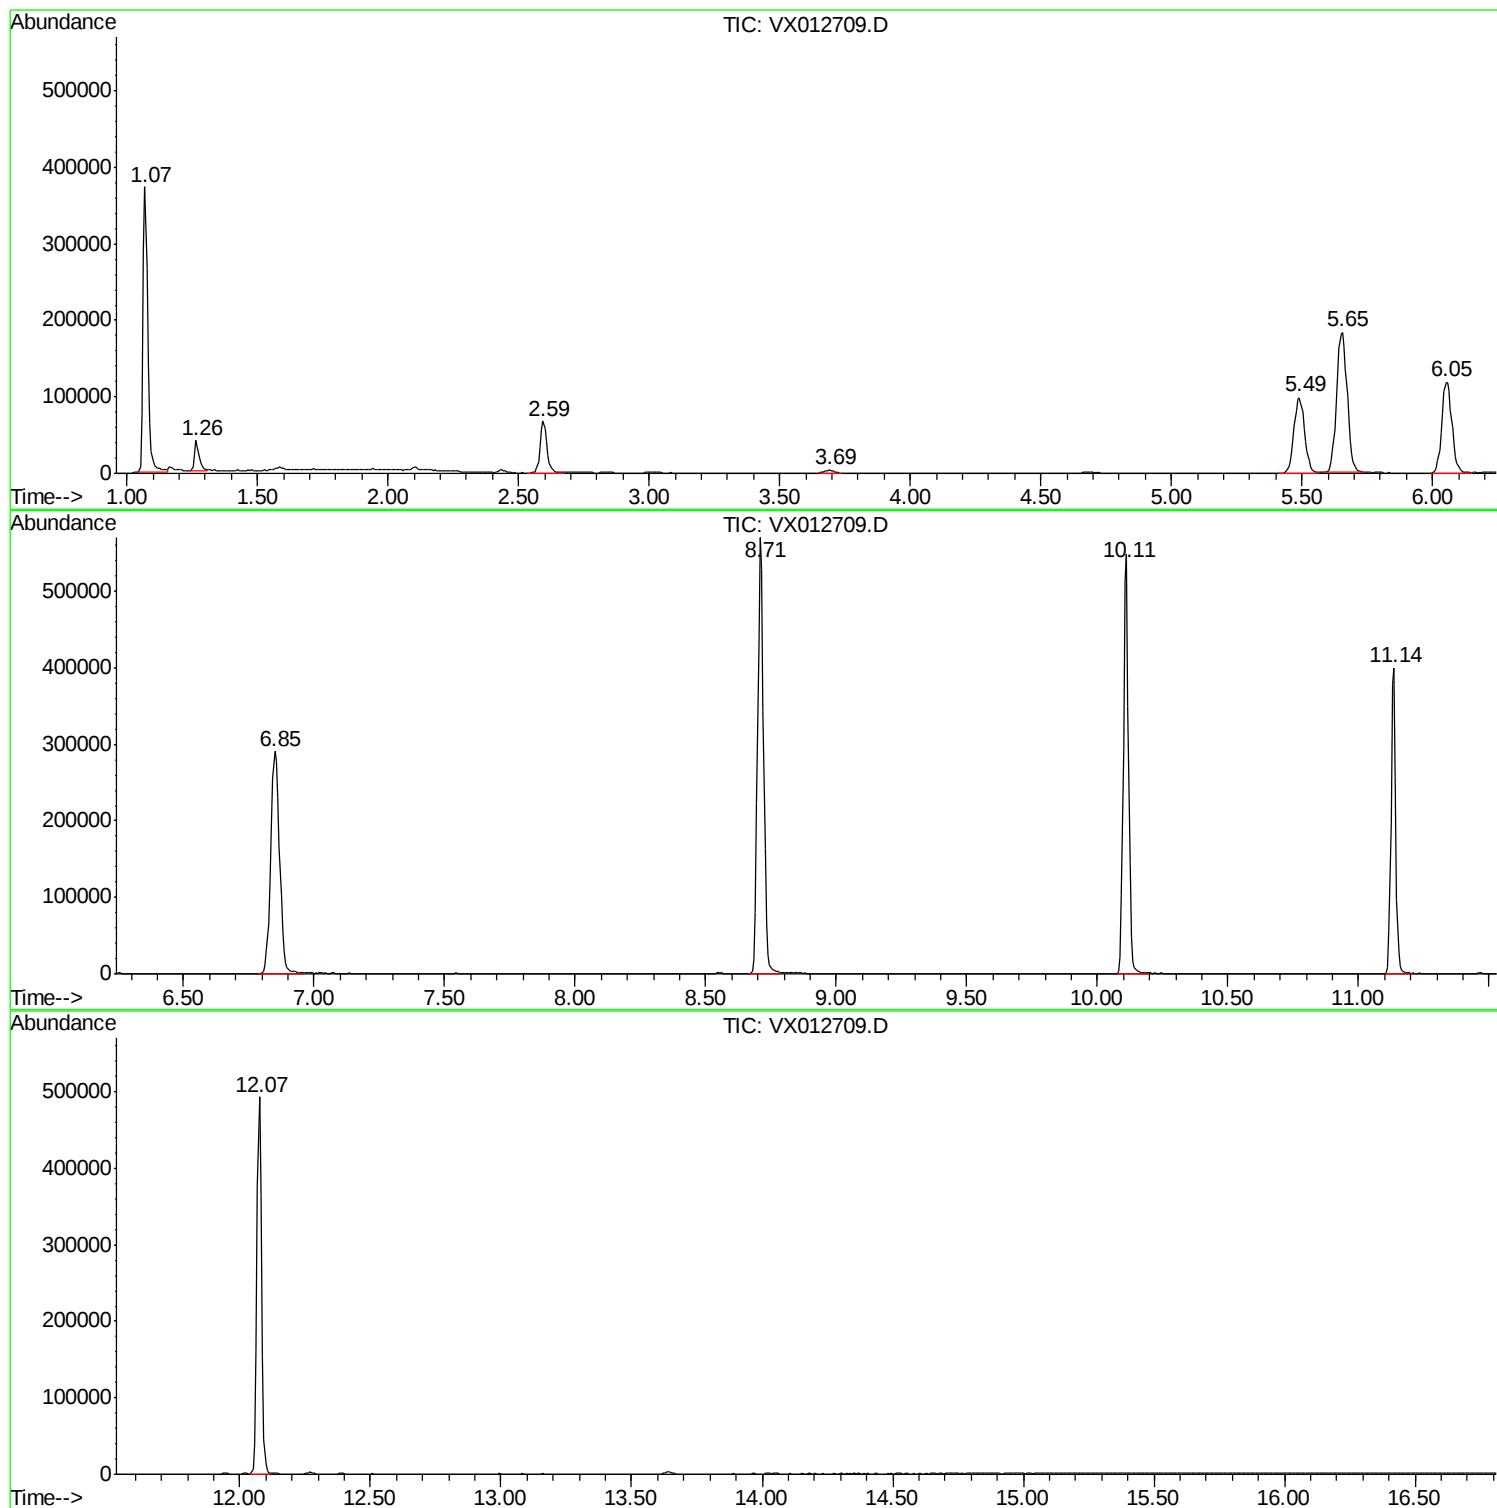

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012709.D
Acq On : 30 Sep 2019 16:43
Operator : JC/SP
Sample : K5081-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ123I1-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	11.83 ug/l	122811	Pentafluorobenzene	5.65

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4
4		Formamide	45	CH3NO	000075-12-7	4
5		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	4

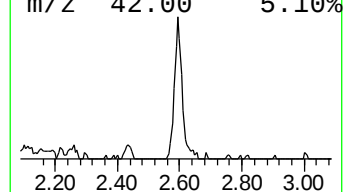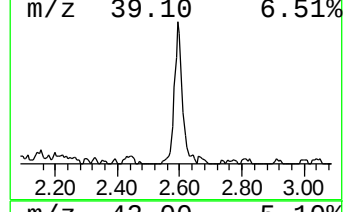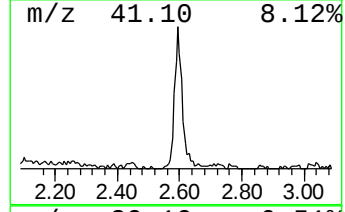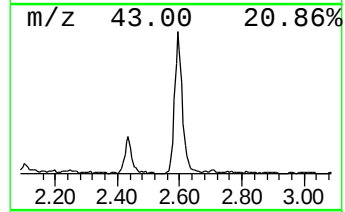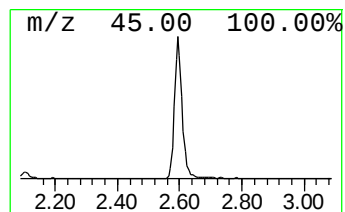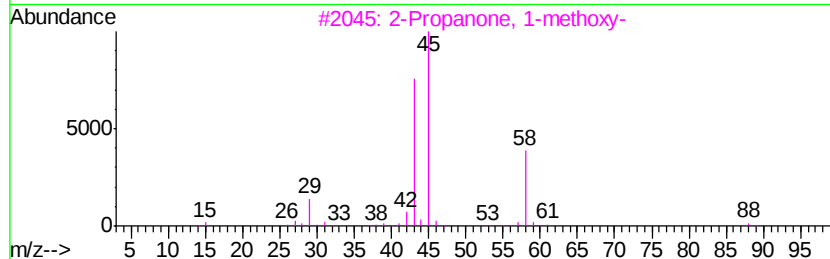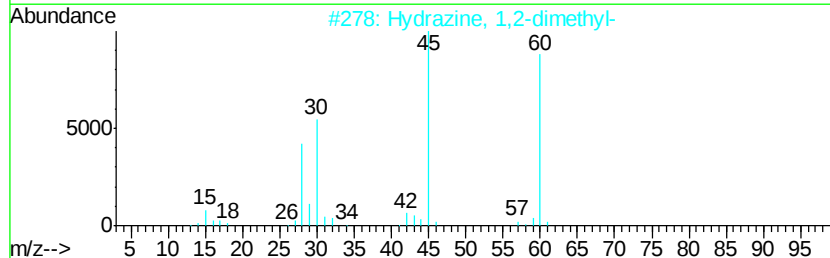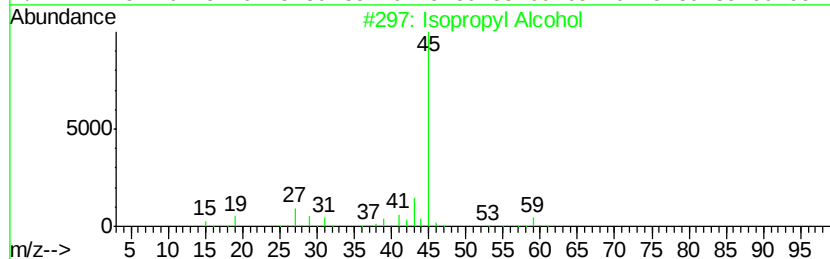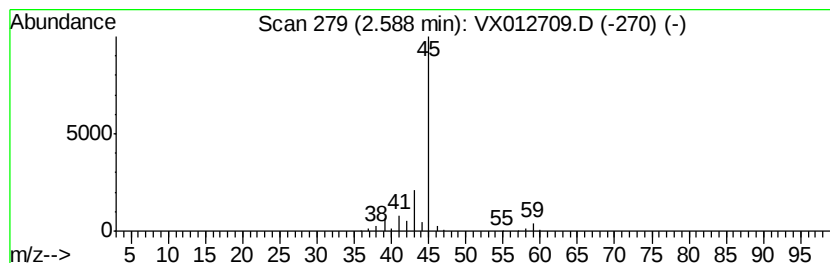

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX093019\
Data File : VX012709.D
Acq On : 30 Sep 2019 16:43
Operator : JC/SP
Sample : K5081-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ12311-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	11.8	ug/l	122811	1	5.65	518919	50.0