

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
 Data File : VX012710.D
 Acq On : 30 Sep 2019 17:06
 Operator : JC/SP
 Sample : K5081-16
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ122I-20190926

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	406024	502270	56.20%	9.843%
2	1.265	58	62	69	rBV	39200	46454	5.20%	0.910%
3	2.430	247	253	264	rVB	9064	16559	1.85%	0.324%
4	2.594	274	280	291	rBV	71443	127717	14.29%	2.503%
5	5.490	743	755	770	rBV	97627	284319	31.81%	5.572%
6	5.649	770	781	798	rVB	185504	519799	58.16%	10.186%
7	6.051	836	847	862	rBV2	120380	314790	35.22%	6.169%
8	6.850	968	978	992	rBV	287263	672993	75.30%	13.188%
9	8.709	1276	1283	1295	rBV	553464	893724	100.00%	17.514%
10	10.111	1507	1513	1530	rBV	513554	722765	80.87%	14.164%
11	11.135	1675	1681	1696	rBV	368744	486485	54.43%	9.533%
12	12.074	1830	1835	1844	rBV	412281	515065	57.63%	10.093%


Sum of corrected areas: 5102940

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012710.D
Acq On : 30 Sep 2019 17:06
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

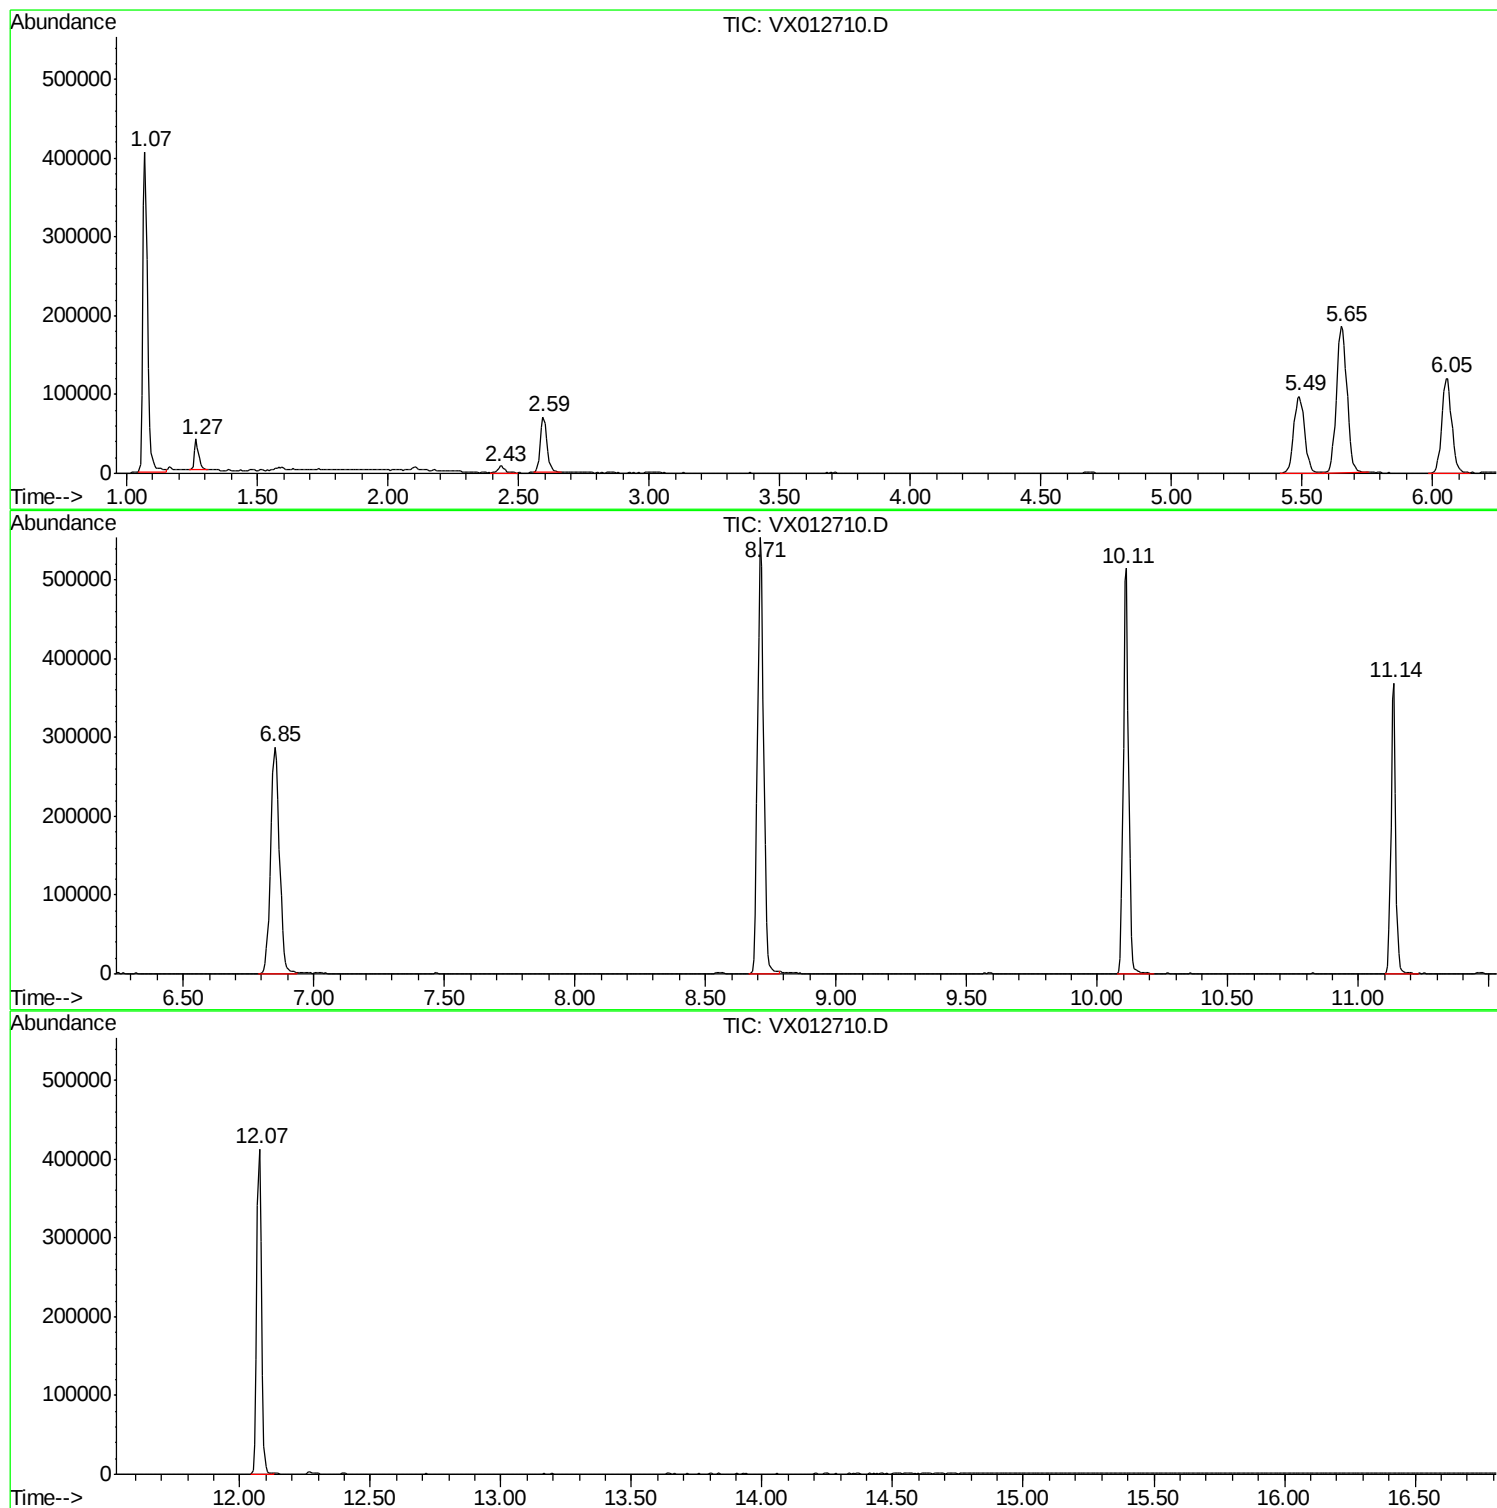

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012710.D
Acq On : 30 Sep 2019 17:06
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	12.29 ug/l	127717	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		Ethylamine	45	C2H7N	000075-04-7	5
4		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4
5		Formamide	45	CH3NO	000075-12-7	4

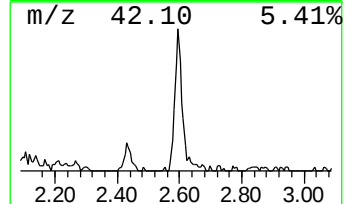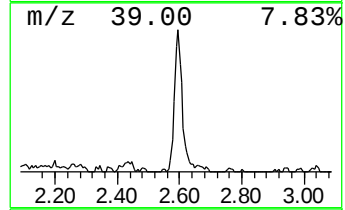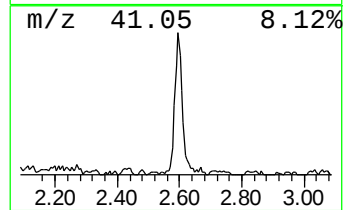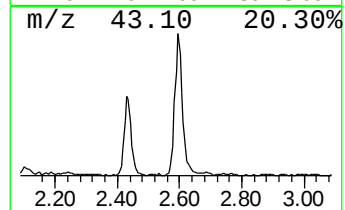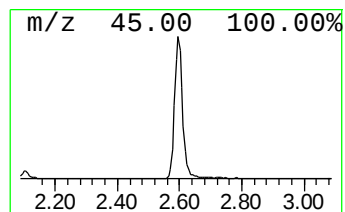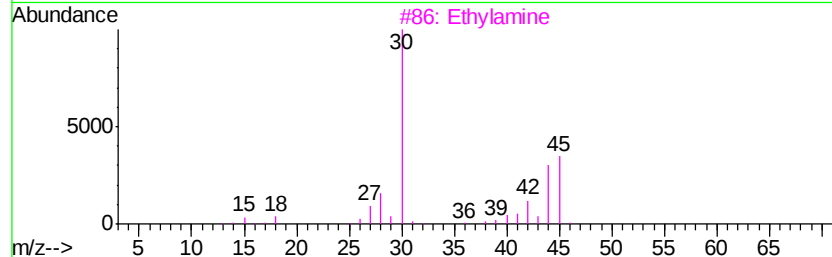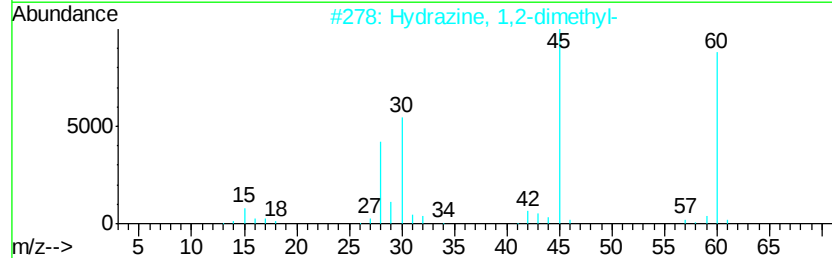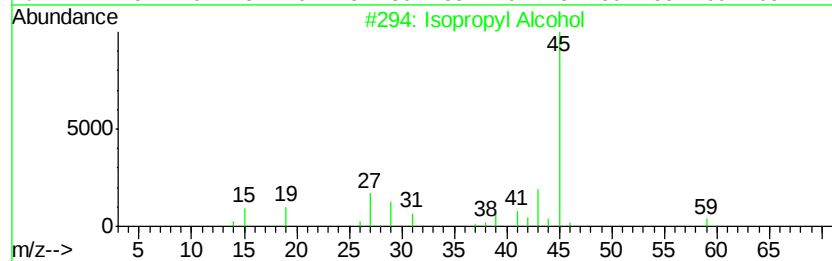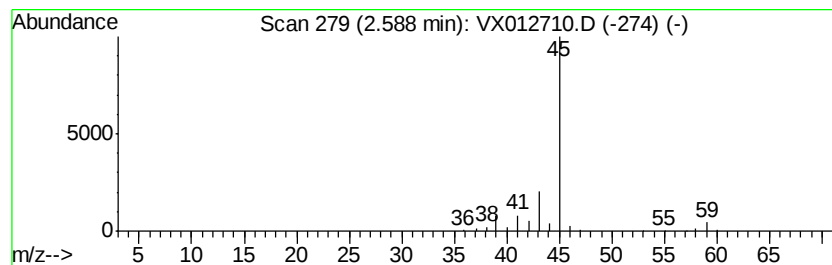

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX093019\
Data File : VX012710.D
Acq On : 30 Sep 2019 17:06
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	12.3	ug/l	127717	1	5.65	519799	50.0