

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093019\
 Data File : VX012715.D
 Acq On : 30 Sep 2019 19:03
 Operator : JC/SP
 Sample : K5081-21
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ147-20190926

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	312247	389134	44.50%	7.876%
2	1.265	59	62	69	rBV	38152	49203	5.63%	0.996%
3	1.594	108	116	122	rBV7	3630	8820	1.01%	0.179%
4	2.429	246	253	264	rVB	7712	13799	1.58%	0.279%
5	2.594	273	280	291	rBV	56862	101975	11.66%	2.064%
6	5.490	742	755	765	rBV	98679	275695	31.53%	5.580%
7	5.654	769	782	797	rVV	179255	505064	57.76%	10.222%
8	6.057	837	848	863	rBV	117252	311732	35.65%	6.309%
9	6.849	968	978	998	rBV	273119	658141	75.27%	13.320%
10	8.709	1275	1283	1300	rBV	544882	874420	100.00%	17.697%
11	10.111	1507	1513	1529	rVB	517782	708140	80.98%	14.332%
12	11.135	1675	1681	1691	rBV	378470	490228	56.06%	9.922%
13	12.074	1829	1835	1846	rBV	455434	554612	63.43%	11.225%


Sum of corrected areas: 4940963

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012715.D
Acq On : 30 Sep 2019 19:03
Operator : JC/SP
Sample : K5081-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ147-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

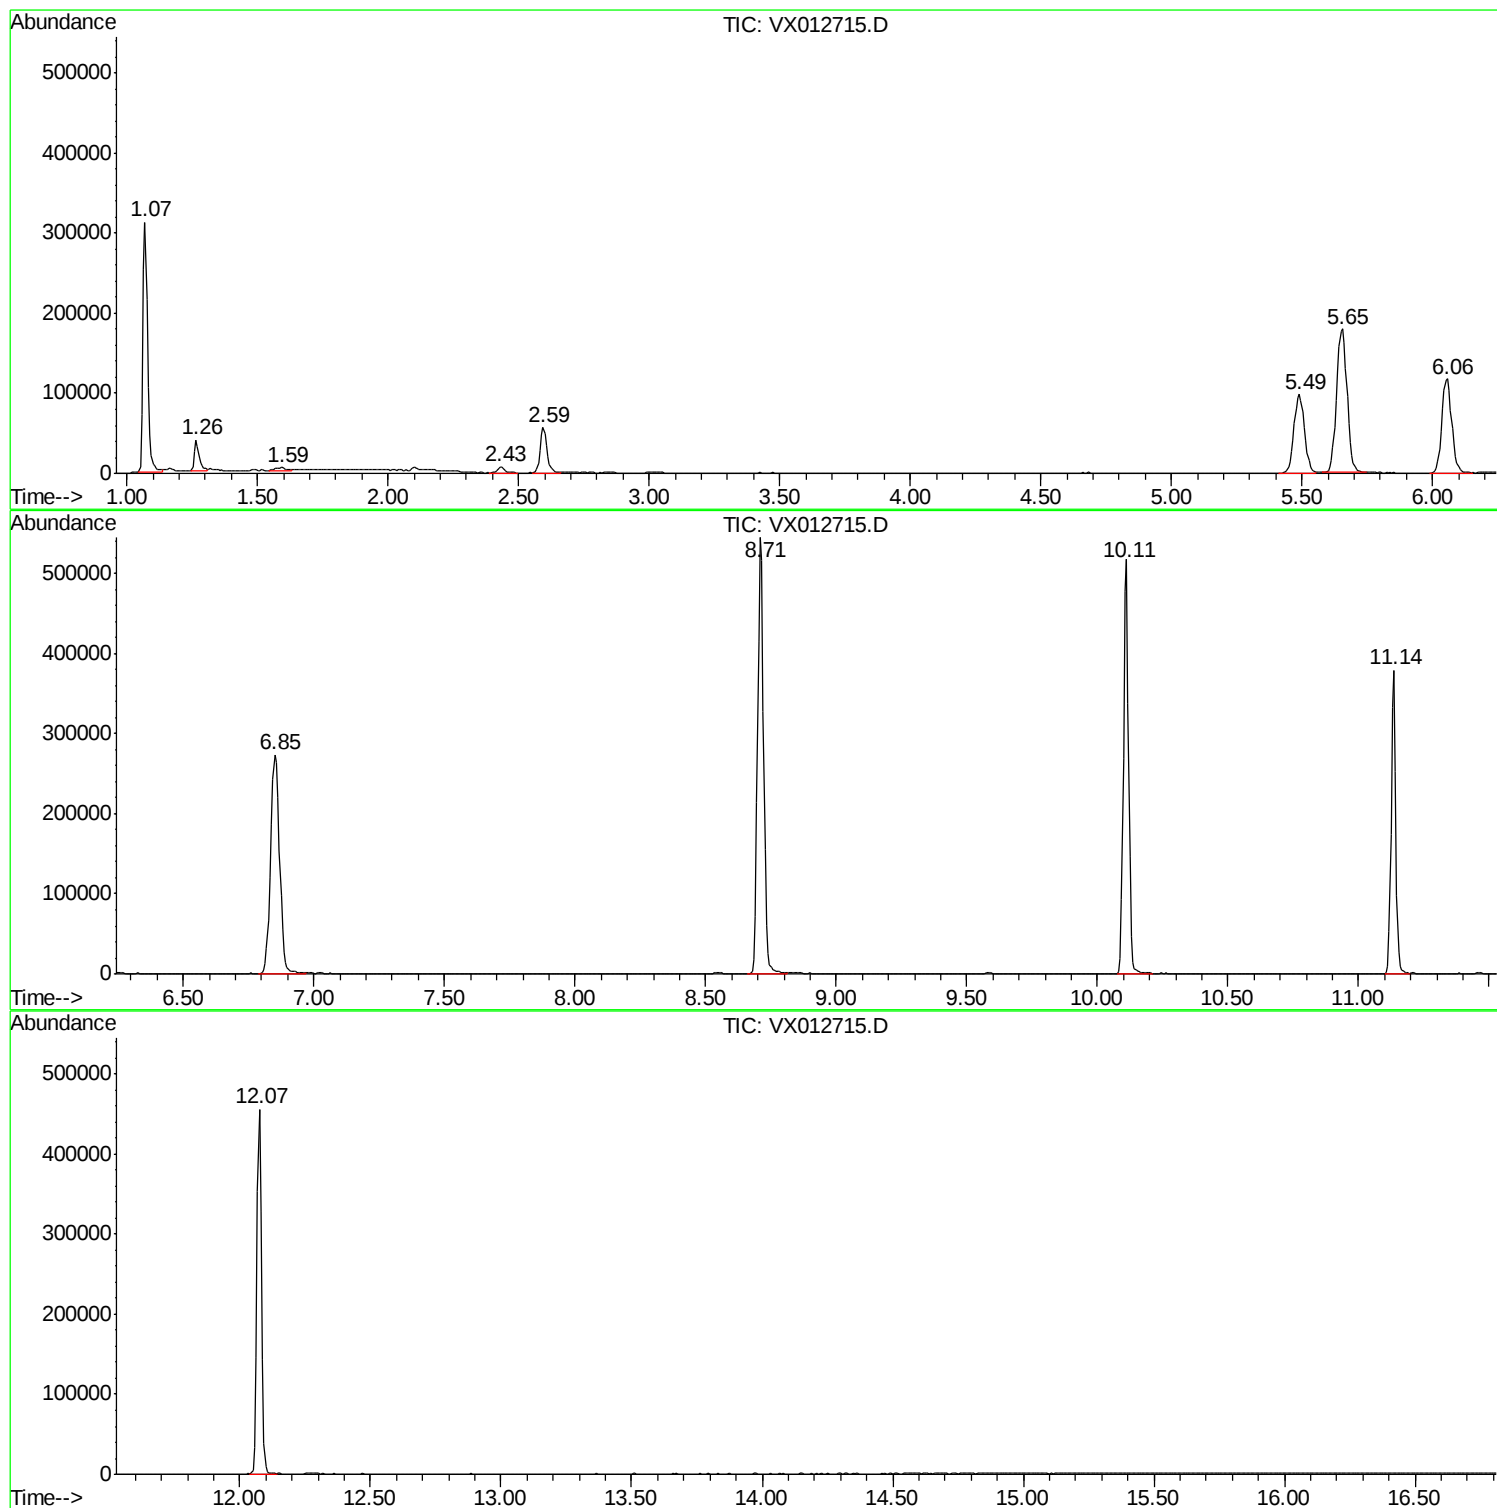

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX093019\
Data File : VX012715.D
Acq On : 30 Sep 2019 19:03
Operator : JC/SP
Sample : K5081-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ147-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	10.10 ug/l	101975	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4		Ethylamine	45	C2H7N	000075-04-7	5
5		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4

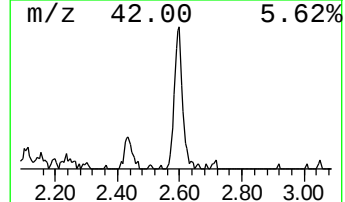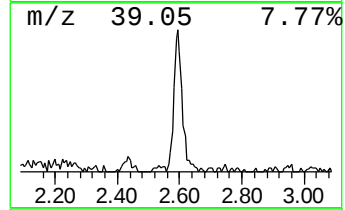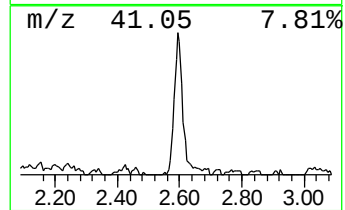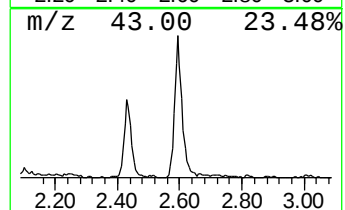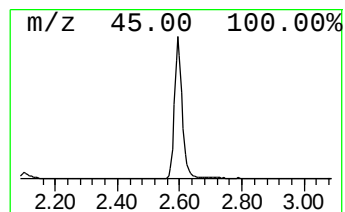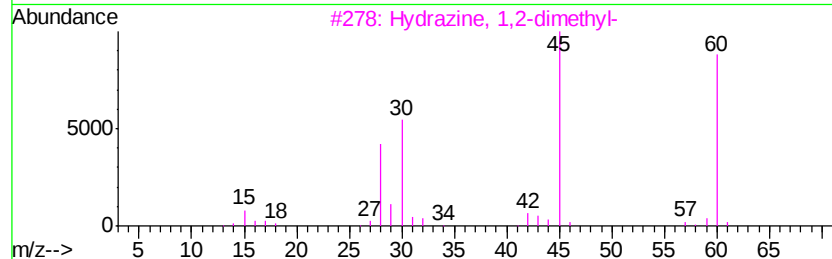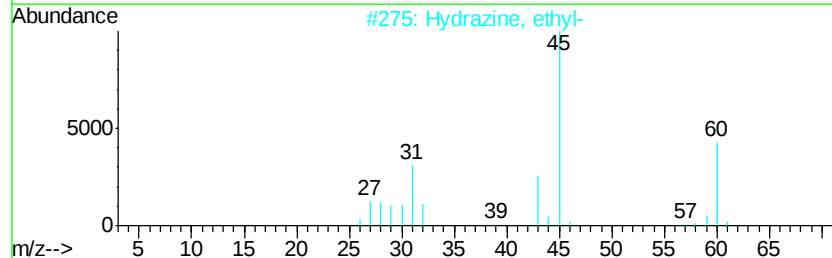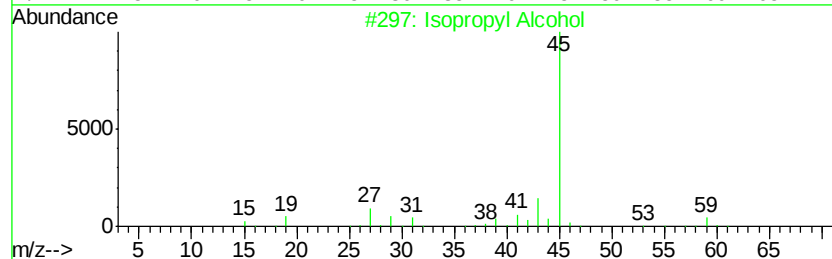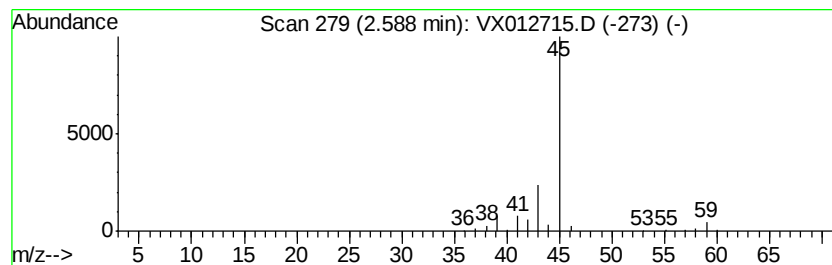

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX093019\
Data File : VX012715.D
Acq On : 30 Sep 2019 19:03
Operator : JC/SP
Sample : K5081-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ147-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	10.1	ug/l	101975	1	5.65	505064	50.0