

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX093020\
 Data File : VX018704.D
 Acq On : 30 Sep 2020 18:00
 Operator : JC/SP
 Sample : L4135-21
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK01

Quant Time: Oct 01 04:24:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 01 01:06:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	206845	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	195690	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	89544	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	40165	3.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.20%
7) Chloroethane-d5	1.70	69	39038	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.34	63	80339	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	4.56	46	158437	57.40	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.80%
24) Chloroform-d	5.15	84	126729	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	6.03	65	72769	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	6.05	84	212342	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	7.37	67	68116	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	8.70	98	183695	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
45) trans-1,3-Dichloropropene-	8.99	79	27488	4.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.80%
48) 2-Hexanone-d5	9.43	63	118532	54.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.14%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	57134	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.60%
65) 1,2-Dichlorobenzene-d4	12.36	152	76155	5.21	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.20%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	4655	0.337 ug/L	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093020\
Data File : VX018704.D
Acq On : 30 Sep 2020 18:00
Operator : JC/SP
Sample : L4135-21
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK01

Quant Time: Oct 01 04:24:15 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 01 01:06:26 2020
Response via : Initial Calibration

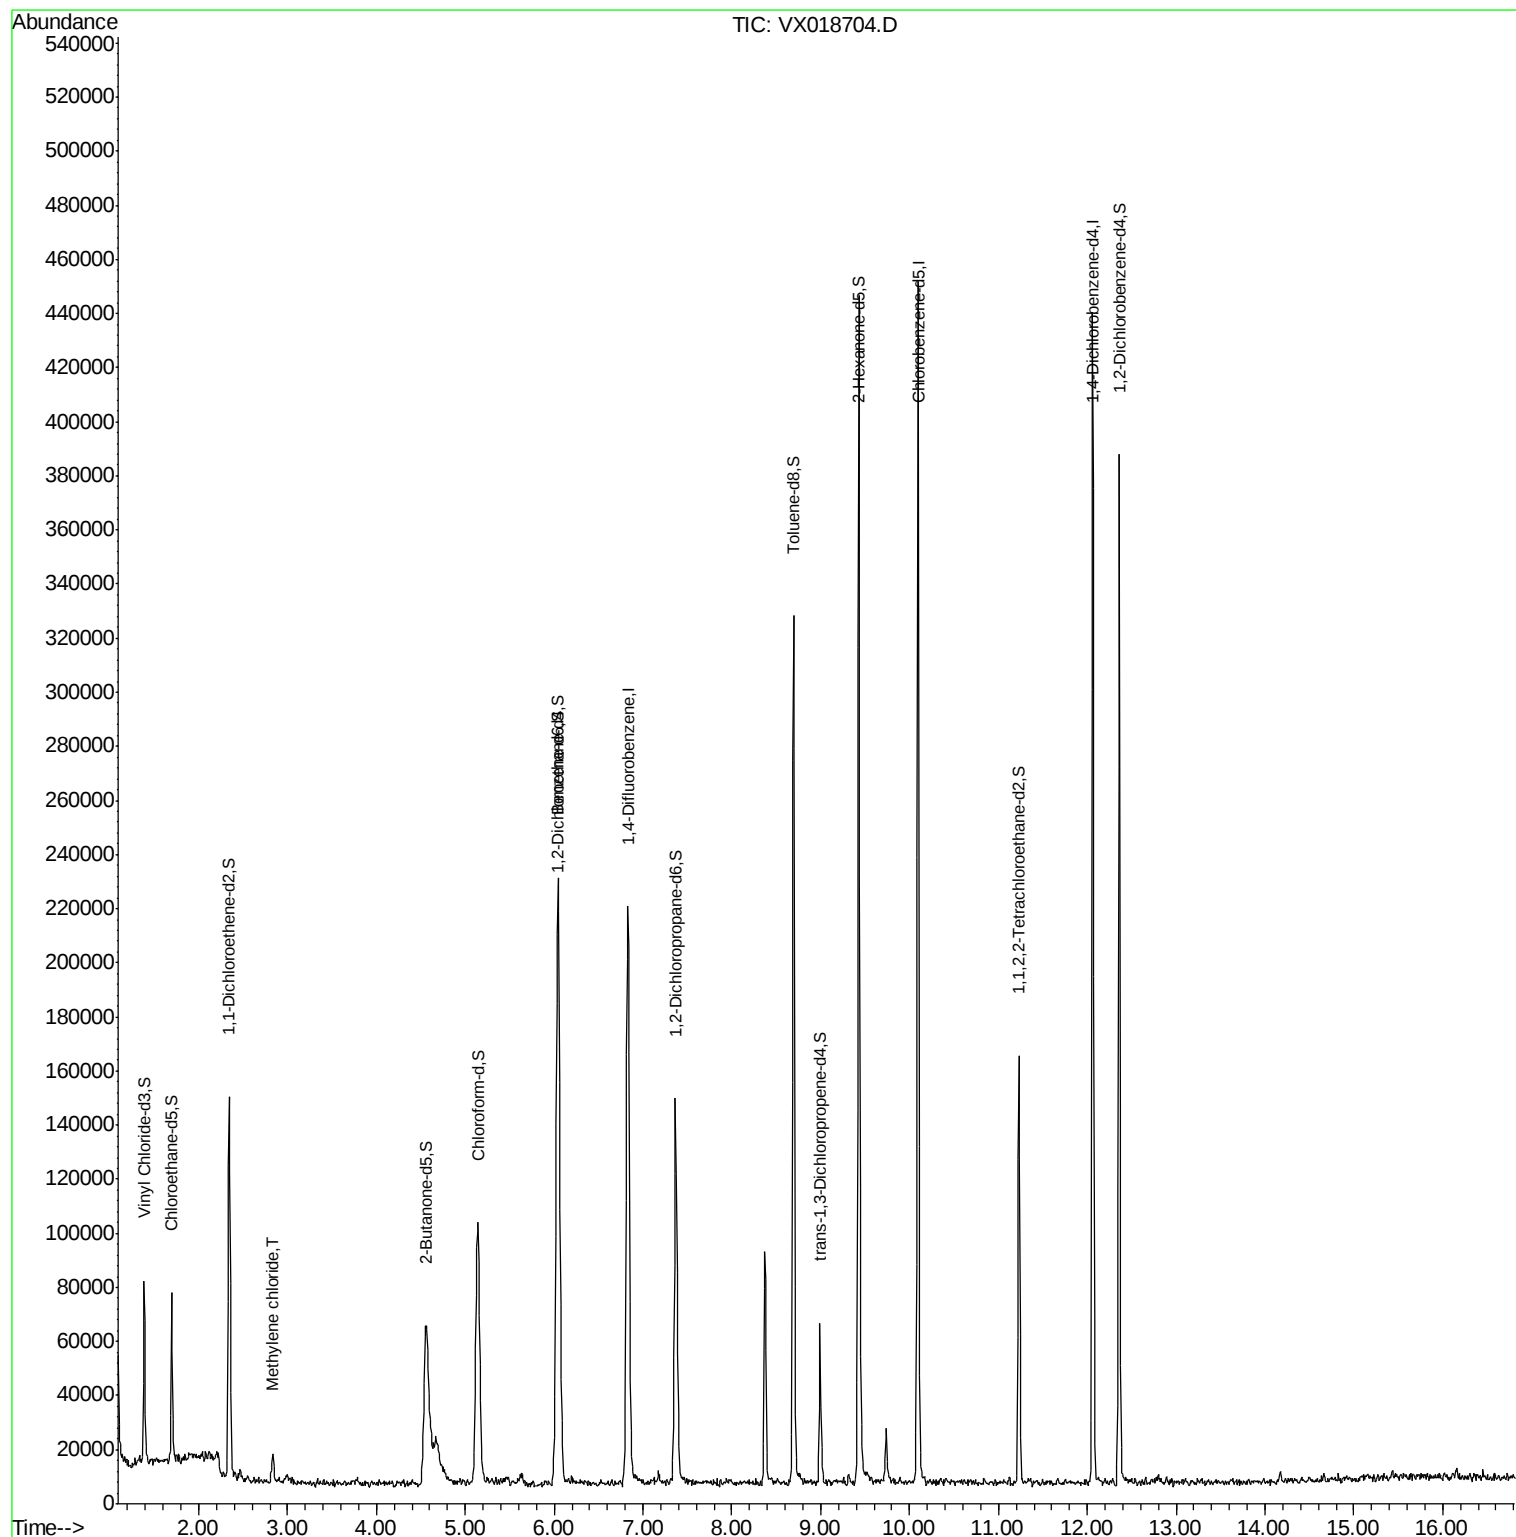

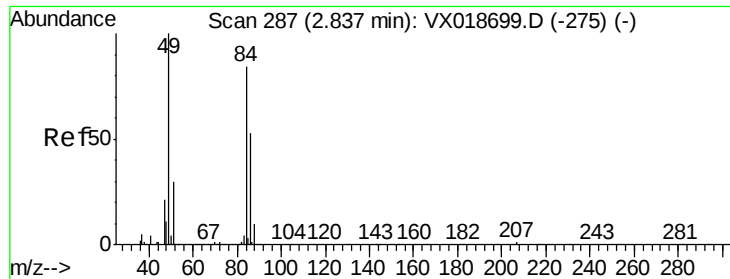

#16
 Methylene chloride
 Concen: 0.337 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. -0.01 min
 Lab File: VX018704.D
 Acq: 30 Sep 2020 18:00

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 4655
 Ion Ratio Lower Upper
 84 100
 86 80.1 41.9 77.7#
 49 121.2 80.8 150.2

