


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX093020\
 Data File : VX018698.D
 Acq On : 30 Sep 2020 14:37
 Operator : JC/SP
 Sample : BFB74
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB74

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Oct 05 17:17:28 2020

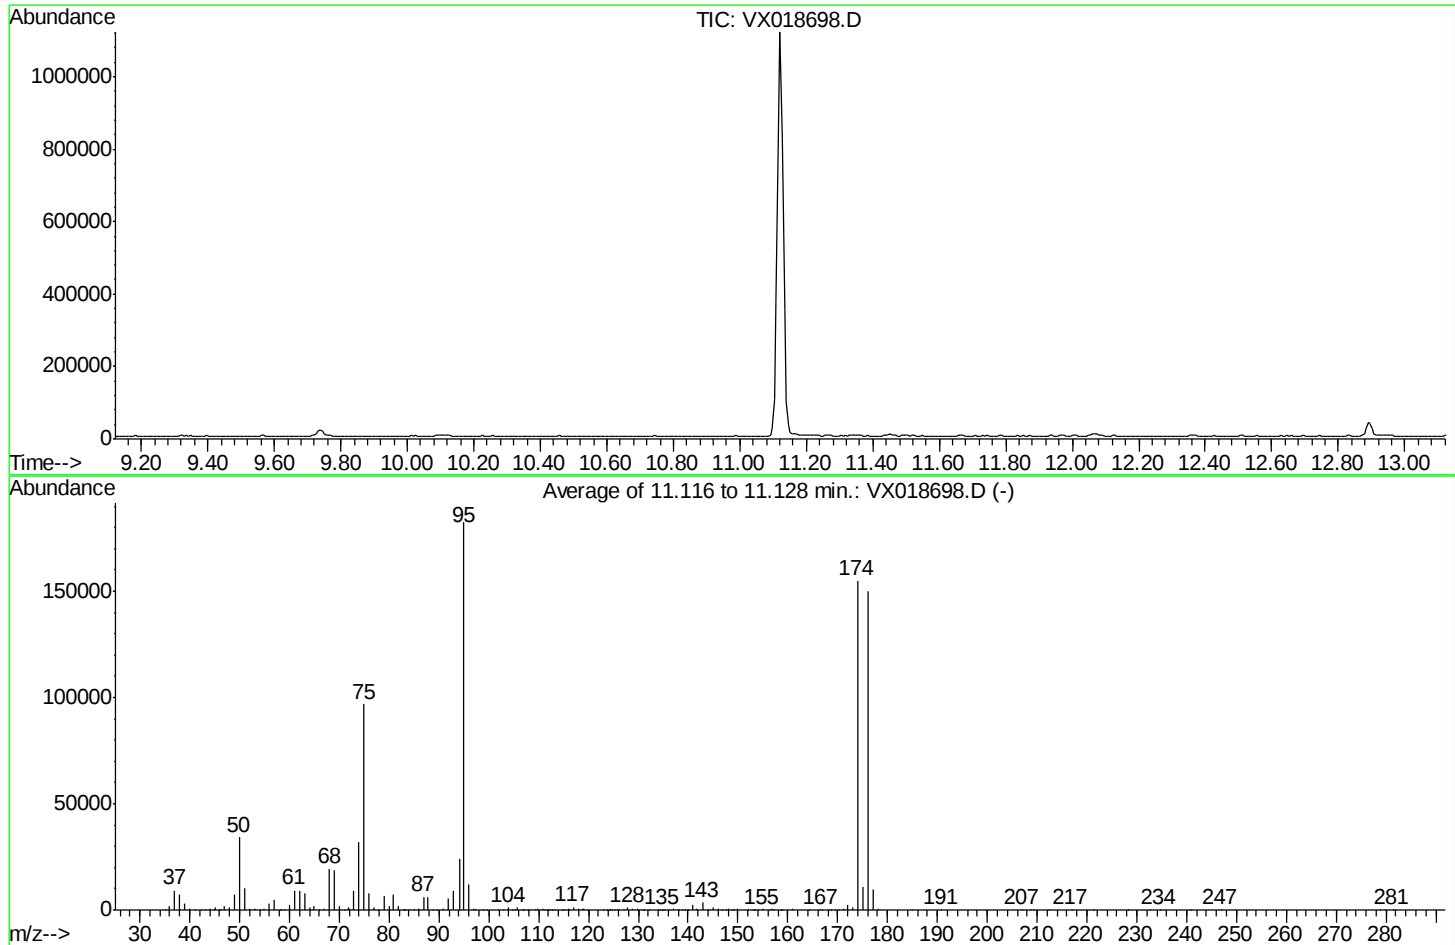

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	34120	PASS
75	95	30	80	53.0	96757	PASS
95	95	100	100	100.0	182421	PASS
96	95	5	9	6.6	12066	PASS
173	174	0.00	2	0.9	1329	PASS
174	95	50	120	85.0	155002	PASS
175	174	5	9	6.9	10690	PASS
176	174	95	101	96.8	150077	PASS
177	176	5	9	6.4	9559	PASS

m/z	Abundance
35.10	268.0
36.00	2108.0
37.00	9738.0
38.00	8187.0
39.00	3832.0
40.10	455.0
40.90	159.0
41.20	149.0
42.20	201.0
42.70	212.0
44.00	1254.0
44.90	1884.0
46.20	291.0
46.90	2354.0
48.00	1535.0
49.00	7697.0
50.00	36720.0
51.00	11392.0
52.00	582.0
52.90	400.0
54.20	153.0
54.90	1137.0
56.00	3108.0
57.00	4759.0
58.20	297.0
59.00	161.0
60.00	2213.0
61.00	10573.0
62.00	9507.0
63.00	8781.0
64.00	1739.0
65.00	2119.0
66.00	513.0
67.00	638.0
68.00	20008.0
69.00	18360.0
70.00	1827.0
71.10	104.0
71.80	1386.0
73.00	8819.0
74.00	31952.0
75.00	93136.0
76.00	7629.0
77.10	1110.0
78.90	6861.0
80.00	1502.0
80.90	6821.0
81.90	1523.0
82.80	121.0
84.00	143.0
86.00	482.0
86.90	6024.0
87.90	6391.0
90.90	839.0
92.00	5265.0
93.00	8066.0
94.10	23488.0
95.00	169024.0
96.00	11955.0
97.10	485.0
100.00	60.0
101.10	76.0
101.80	62.0
103.00	115.0
104.00	930.0
104.70	281.0
105.80	911.0
106.80	300.0
107.90	98.0
109.40	82.0
109.90	190.0
110.80	205.0
111.60	61.0
112.20	73.0
112.70	105.0
113.10	251.0
114.90	471.0
115.90	882.0
116.90	1497.0
117.90	827.0
118.80	1223.0
122.80	75.0
123.60	150.0
124.70	104.0
126.10	88.0
127.90	1096.0
128.90	484.0
129.90	847.0
130.80	288.0
132.70	81.0
134.00	140.0
134.70	207.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

135.20	326.0
137.00	582.0
138.80	151.0
139.70	171.0
141.00	2120.0
141.80	266.0
143.00	3445.0
143.90	350.0
145.10	1078.0
146.10	488.0
146.70	225.0
147.60	208.0
148.10	235.0
149.10	154.0
149.90	332.0
152.10	134.0
153.00	239.0
153.60	194.0
154.20	258.0
154.90	460.0
156.30	95.0
157.00	429.0
158.70	242.0
160.00	52.0
160.90	423.0
164.40	52.0
166.80	78.0
168.60	144.0
171.00	574.0
172.00	2878.0
173.00	1628.0
174.00	126768.0
175.00	8793.0
176.00	117688.0
177.00	7603.0
178.00	104.0
184.70	116.0
190.80	105.0
206.90	139.0
207.30	121.0
228.10	81.0
234.60	104.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

m/z	Abundance
36.00	2531.0
37.00	12645.0
38.00	8248.0
39.10	3809.0
40.10	585.0
41.00	396.0
42.30	233.0
43.10	298.0
44.00	1977.0
45.10	1766.0
45.90	434.0
47.00	2219.0
48.10	1292.0
49.00	9215.0
50.00	38992.0
51.00	12045.0
52.00	795.0
53.00	324.0
54.10	134.0
55.00	462.0
56.00	3554.0
57.00	6350.0
58.00	236.0
58.90	150.0
59.90	2803.0
61.00	10041.0
62.00	11190.0
63.00	9352.0
64.10	1769.0
65.00	2667.0
66.30	278.0
66.80	532.0
68.00	22144.0
69.00	22384.0
70.00	1835.0
71.20	80.0
71.90	1643.0
73.00	11360.0
74.00	37392.0
75.00	119504.0
76.00	9079.0
77.10	1063.0
78.90	7917.0
79.90	2820.0
80.90	8232.0
82.00	2125.0
83.00	418.0
84.00	108.0
86.10	775.0
87.00	7571.0
87.90	7034.0
90.90	874.0
92.00	7350.0
93.00	11168.0
94.00	28504.0
95.00	221248.0
96.00	14890.0
96.90	793.0
99.50	97.0
101.20	90.0
102.90	140.0
104.00	1509.0
104.80	250.0
105.90	1332.0
107.10	238.0
107.70	71.0
108.10	72.0
109.80	464.0
110.80	441.0
111.80	365.0
112.60	139.0
113.10	294.0
115.00	346.0
115.90	1272.0
116.90	1862.0
117.90	1092.0
119.00	1564.0
119.70	52.0
122.90	182.0
124.10	116.0
124.70	87.0
125.20	68.0
125.80	103.0
127.20	70.0
127.90	955.0
128.90	492.0
129.90	981.0
131.10	266.0
132.30	92.0
134.30	234.0
134.90	391.0
136.90	656.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

138.20	82.0
138.80	111.0
139.80	138.0
140.90	3303.0
141.90	530.0
142.90	3501.0
143.90	446.0
144.90	1023.0
146.00	527.0
146.70	124.0
148.00	692.0
148.80	107.0
149.90	408.0
151.90	131.0
153.20	85.0
154.00	316.0
154.90	467.0
156.90	398.0
158.90	408.0
160.00	58.0
160.90	353.0
164.30	75.0
166.80	78.0
168.00	107.0
168.60	258.0
171.10	652.0
172.10	2608.0
174.00	185088.0
175.00	13426.0
176.00	181760.0
177.00	12463.0
178.10	537.0
184.70	61.0
190.80	156.0
207.00	200.0
208.80	79.0
212.40	54.0
216.80	52.0
232.60	57.0
246.90	50.0
279.90	72.0
281.00	122.0
281.30	103.0
283.10	56.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

m/z	Abundance
35.20	134.0
36.00	1320.0
37.00	5865.0
38.00	5486.0
39.00	2566.0
39.90	499.0
41.00	239.0
42.90	257.0
44.00	1752.0
45.20	1091.0
45.90	291.0
47.10	888.0
48.00	1170.0
49.00	5998.0
50.00	26648.0
51.00	8156.0
52.10	537.0
53.10	375.0
54.10	86.0
55.10	363.0
56.00	2256.0
57.00	4104.0
58.30	325.0
58.90	143.0
60.00	2109.0
61.00	7105.0
62.00	7629.0
63.00	5971.0
64.20	692.0
65.10	1455.0
66.00	382.0
66.90	426.0
68.00	16168.0
69.00	15753.0
70.10	1212.0
72.10	1141.0
73.00	7059.0
74.00	27280.0
75.00	77856.0
76.00	7034.0
76.90	955.0
77.80	498.0
79.00	5444.0
80.10	1439.0
80.90	6249.0
82.00	1238.0
83.20	236.0
83.80	144.0
84.80	51.0
86.00	289.0
86.90	4930.0
87.90	4534.0
88.90	120.0
89.60	194.0
91.00	672.0
91.90	4518.0
93.00	8039.0
94.00	19904.0
95.00	156992.0
96.10	9354.0
97.20	170.0
98.70	74.0
99.50	77.0
101.30	73.0
102.90	194.0
103.90	1035.0
104.60	202.0
105.20	246.0
105.80	614.0
106.90	252.0
109.70	314.0
110.60	337.0
111.10	176.0
111.80	381.0
113.00	296.0
114.70	237.0
115.80	360.0
116.10	465.0
117.00	1234.0
118.00	804.0
118.80	1297.0
119.80	97.0
123.00	121.0
124.30	86.0
124.70	77.0
125.20	111.0
125.90	136.0
127.10	97.0
127.90	745.0
128.90	236.0
129.90	648.0
131.00	253.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

132.20	113.0
133.10	66.0
134.00	163.0
134.90	333.0
136.00	267.0
137.00	309.0
138.10	100.0
138.80	106.0
139.40	199.0
140.00	126.0
140.80	2248.0
141.70	353.0
143.00	3490.0
144.10	378.0
144.90	1085.0
146.10	406.0
147.00	62.0
147.70	321.0
148.00	331.0
148.90	257.0
149.80	266.0
153.10	147.0
153.90	165.0
155.00	583.0
156.80	323.0
157.20	382.0
158.80	178.0
160.00	54.0
160.70	217.0
166.30	65.0
168.10	149.0
168.70	102.0
169.50	136.0
170.20	191.0
171.20	529.0
172.00	2377.0
173.10	2361.0
174.00	153152.0
175.00	9851.0
176.00	150784.0
177.00	8612.0
177.90	337.0
207.30	285.0
209.30	84.0
212.30	60.0
216.80	53.0
221.30	73.0
240.90	59.0
278.90	65.0
279.90	62.0
281.40	80.0
281.90	64.0
283.10	135.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74

m/z	Abundance
35.70	197.0
37.10	58.0
38.10	152.0
39.10	155.0
39.80	315.0
41.30	167.0
41.90	161.0
42.70	78.0
44.00	806.0
45.00	316.0
45.80	122.0
46.20	68.0
47.30	67.0
48.00	72.0
49.00	169.0
51.30	143.0
52.60	101.0
53.40	90.0
54.70	72.0
55.30	85.0
56.10	76.0
56.60	65.0
57.70	117.0
60.60	191.0
62.20	127.0
63.40	87.0
64.00	62.0
66.50	133.0
67.20	135.0
71.90	52.0
72.80	149.0
73.80	237.0
75.10	75.0
76.10	97.0
77.20	88.0
80.50	82.0
87.70	82.0
89.70	62.0
93.10	62.0
99.80	104.0
101.30	97.0
113.10	71.0
116.20	57.0
117.00	68.0
119.30	55.0
126.60	91.0
132.60	69.0
133.10	112.0
145.20	82.0
147.20	104.0
152.40	90.0
167.50	63.0
178.70	58.0
179.40	88.0
181.80	89.0
196.20	77.0
203.60	54.0
207.30	159.0
208.30	138.0
216.40	61.0
223.70	121.0
237.30	87.0
270.80	65.0
280.90	103.0
283.20	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB74