

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
 Data File : VX038004.D
 Acq On : 30 Sep 2023 15:17
 Operator : JC/MD
 Sample : 04647-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 02 02:12:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	150357	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	265291	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	281537	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	149528	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	112945	57.174	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	114.340%
35) Dibromofluoromethane	5.385	113	87223	49.138	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.280%
50) Toluene-d8	8.647	98	340506	51.627	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	103.260%
62) 4-Bromofluorobenzene	11.079	95	137454	57.352	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	114.700%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.946	59	2769	6.530	ug/l #	84
13) Acrolein	2.233	56	402	0.960	ug/l #	39
16) Acetone	2.379	43	23024	24.228	ug/l	95
18) Methyl Acetate	2.709	43	1055	0.308	ug/l	93
20) Methylene Chloride	2.788	84	8276	4.688	ug/l	92
25) 2-Butanone	4.574	43	5466	4.076	ug/l #	85
29) Tetrahydrofuran	5.037	42	468	0.561	ug/l #	82
36) 1,1-Dichloropropene	5.550	75	13376	5.470	ug/l #	51
37) Ethyl Acetate	4.733	43	2054	0.764	ug/l #	90
38) Carbon Tetrachloride	5.556	117	15994	6.251	ug/l #	14
40) Benzene	6.043	78	35090	4.667	ug/l	97
43) Isopropyl Acetate	6.342	43	90492	21.052	ug/l	98
48) Methyl methacrylate	7.799	41	89622	43.615	ug/l #	50
49) 1,4-Dioxane	7.793	88	147	2.729	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	78752	28.876	ug/l #	46
52) Toluene	8.720	92	27354	5.644	ug/l	87
53) t-1,3-Dichloropropene	8.957	75	657	0.243	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	32502	10.856	ug/l #	61
56) Ethyl methacrylate	9.244	69	810	0.266	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	4248	1.285	ug/l #	42
59) 2-Hexanone	9.482	43	61447	28.938	ug/l #	54
67) Ethyl Benzene	10.195	91	6369	0.605	ug/l	94
68) m/p-Xylenes	10.305	106	10444	2.567	ug/l	93
69) o-Xylene	10.640	106	7383	1.810	ug/l	90
70) Styrene	10.658	104	4028	0.615	ug/l #	76
76) 1,2,3-Trichloropropane	11.079	75	76998	22.264	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	2121	0.229	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	76998	71.319	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	6812	0.739	ug/l	84
95) Naphthalene	13.774	128	80812	7.850	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038004.D
Acq On : 30 Sep 2023 15:17
Operator : JC/MD
Sample : 04647-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Oct 02 02:12:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration

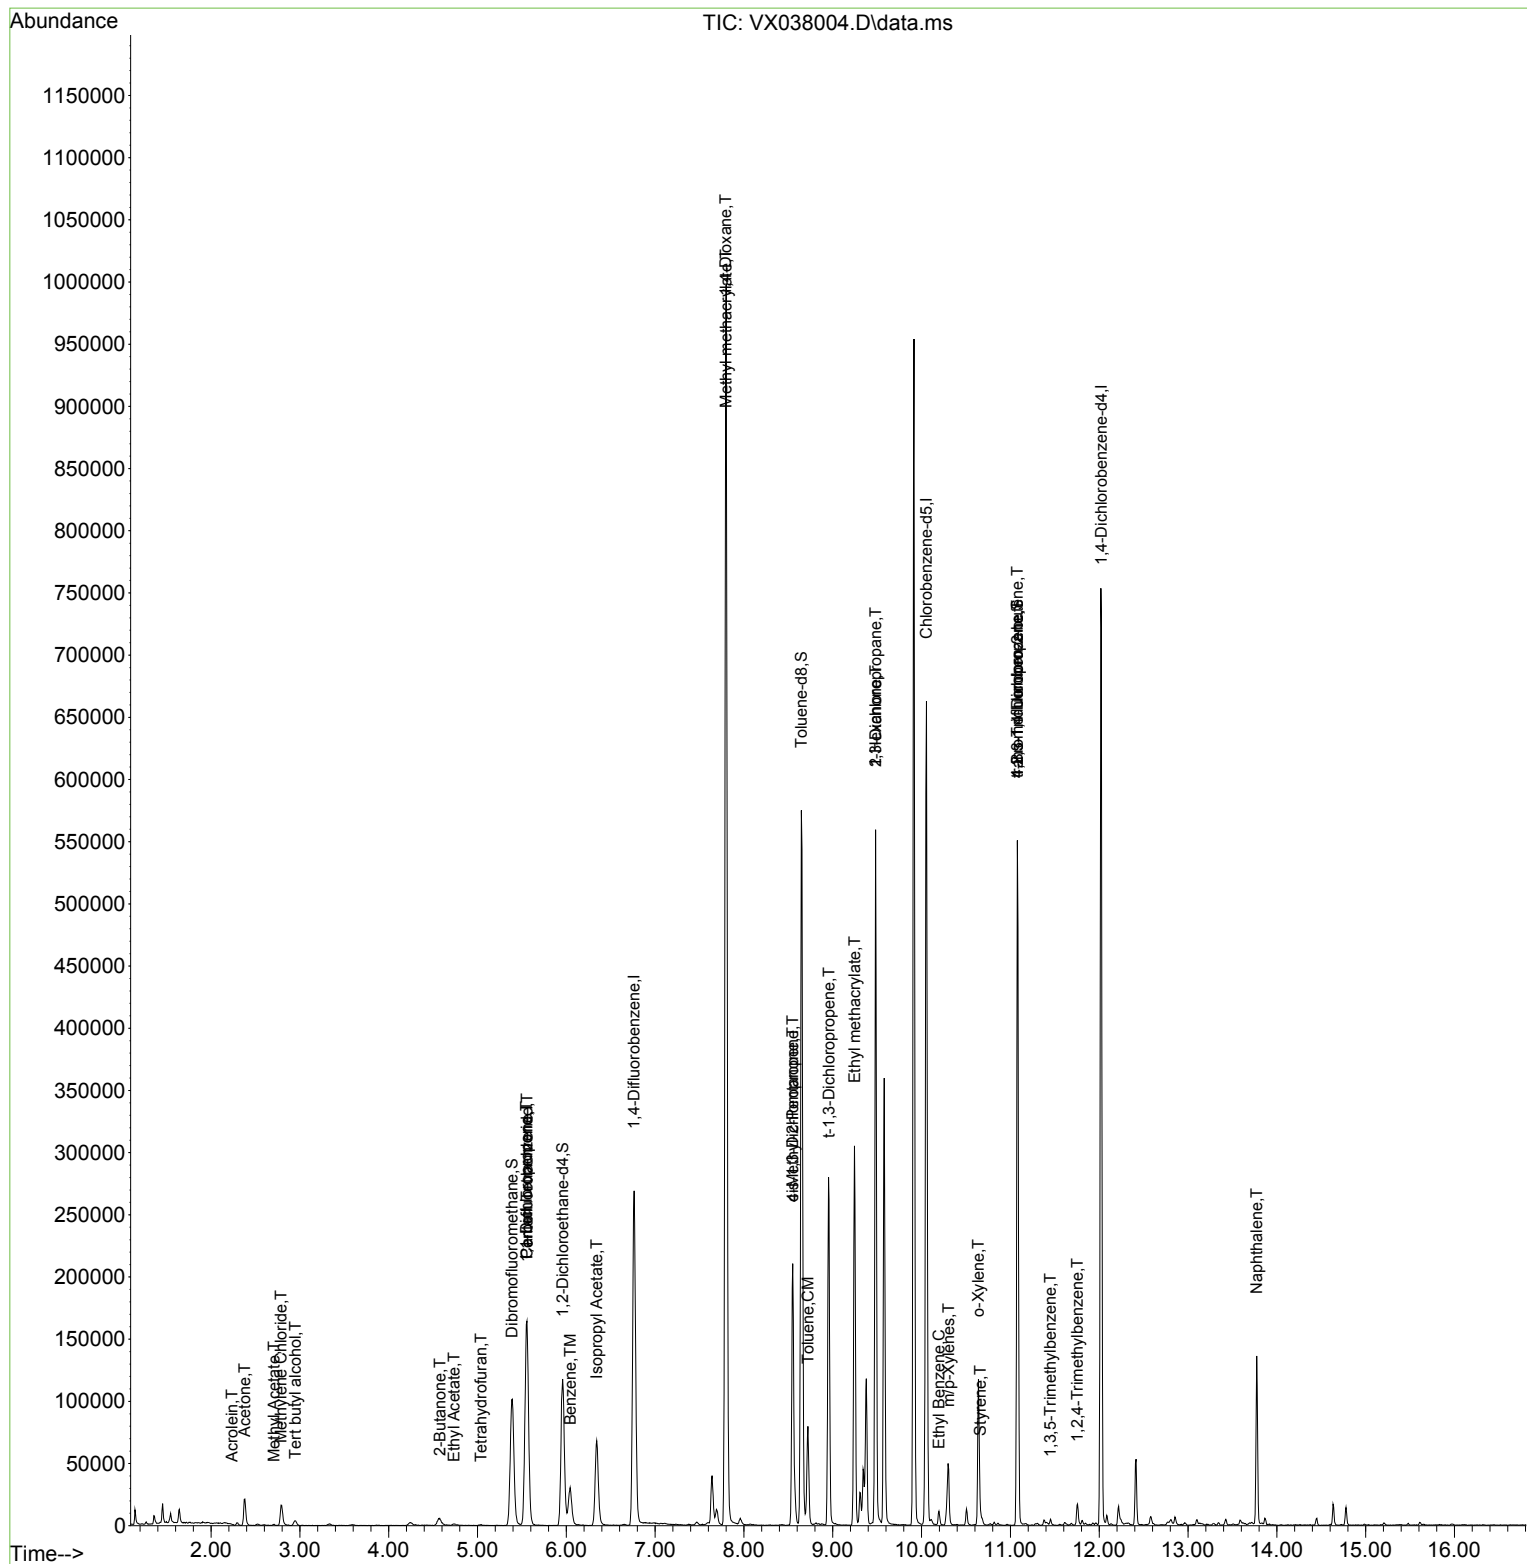






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Instrument :
MSVOA_X
ClientSampleId :



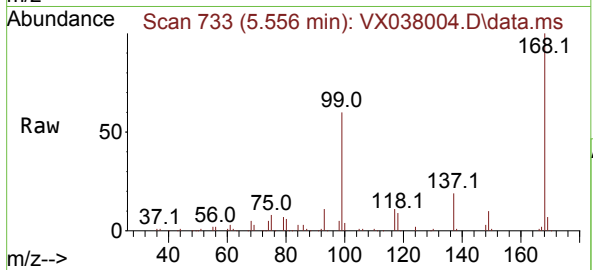



Tgt Ion:168 Resp: 150357
Ion Ratio Lower Upper
168 100
99 59.7 56.6 85.0

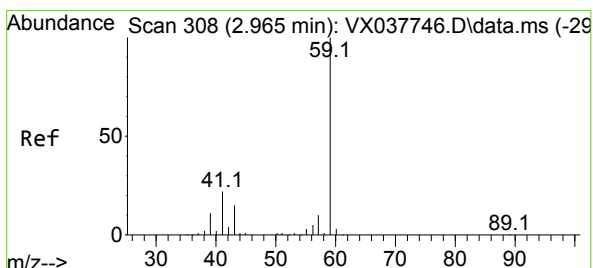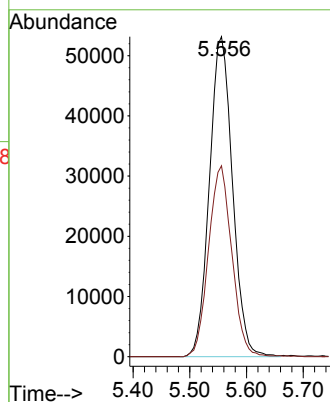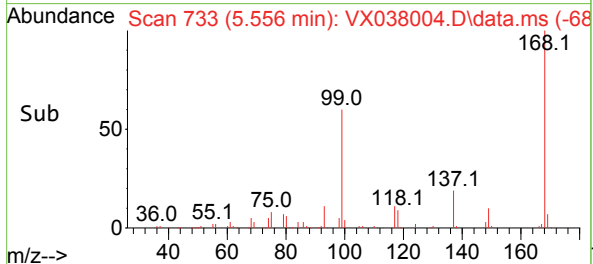

#11
Tert butyl alcohol
Concen: 6.530 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.018 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 59 Resp: 2769
Ion Ratio Lower Upper
59 100
57 1.9 6.0 9.0#

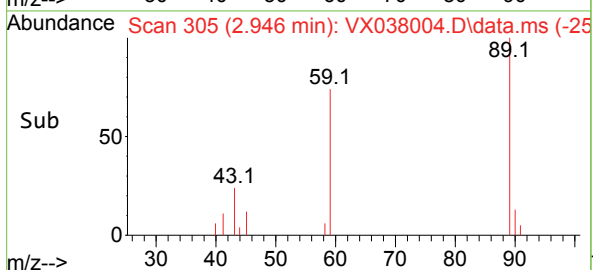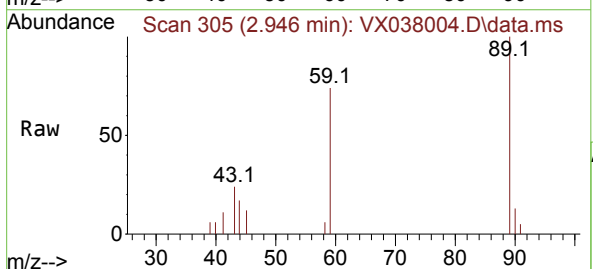



#13

Acrolein

Concen: 0.960 ug/l

RT: 2.233 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 402

Ion Ratio Lower Upper

56 100

55 122.4 57.1 85.7#

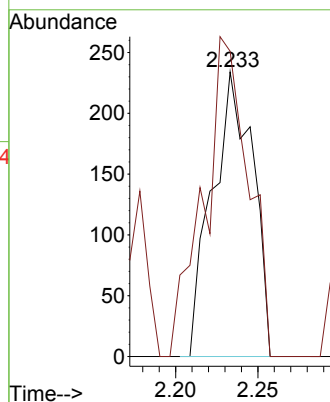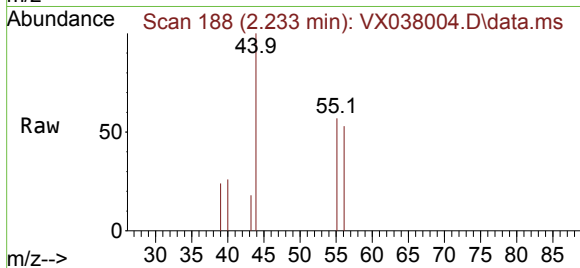

#16

Acetone

Concen: 24.228 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.000 min

Lab File: VX038004.D




Acq: 30 Sep 2023 15:17


Tgt Ion: 43 Resp: 23024

Ion Ratio Lower Upper

43 100

58 29.9 21.9 32.9




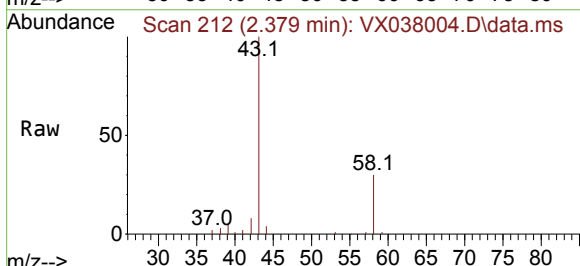




#18
Methyl Acetate
Concen: 0.308 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1055
Ion Ratio Lower Upper
43 100
74 19.0 17.8 26.8

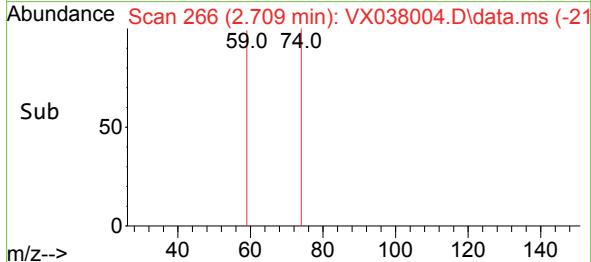

#20
Methylene Chloride
Concen: 4.688 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 84 Resp: 8276
Ion Ratio Lower Upper
84 100
49 114.8 103.6 155.4
51 41.9 33.8 50.6
86 65.3 49.4 74.0

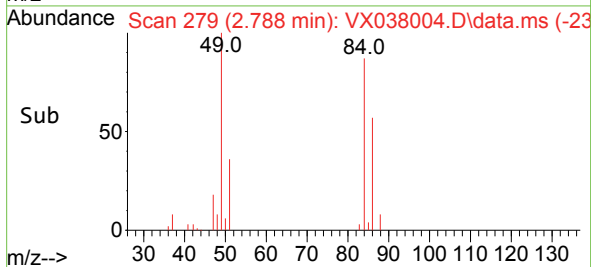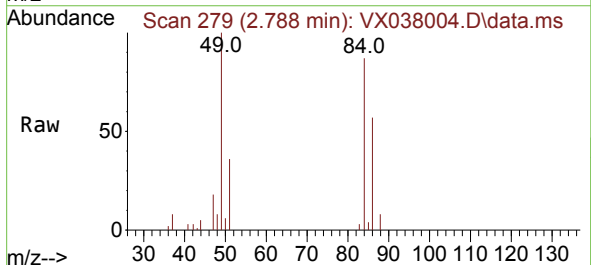

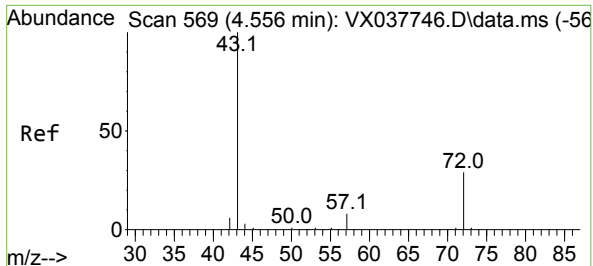

#25

2-Butanone

Concen: 4.076 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 5466

Ion Ratio Lower Upper

43 100

72 31.7 19.4 29.2#

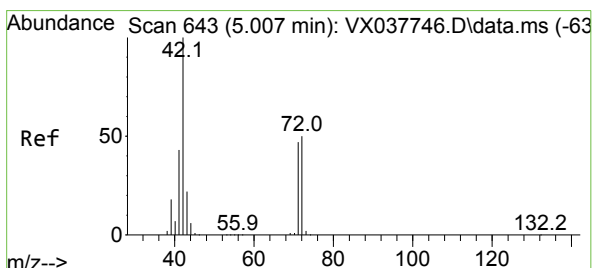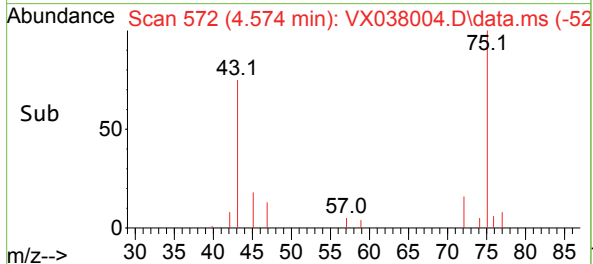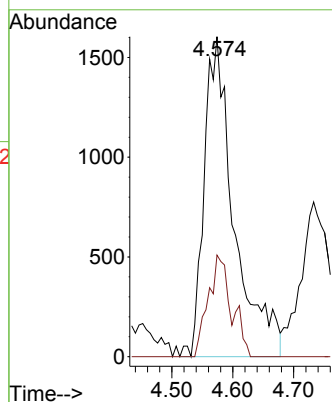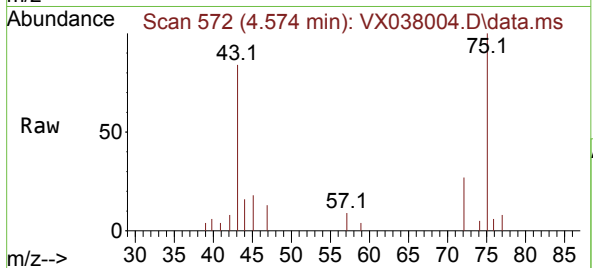

#29

Tetrahydrofuran

Concen: 0.561 ug/l

RT: 5.037 min Scan# 648

Delta R.T. 0.024 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17




Tgt Ion: 42 Resp: 468


Ion Ratio Lower Upper

42 100

72 31.8 34.2 51.4#

71 28.2 32.2 48.2#

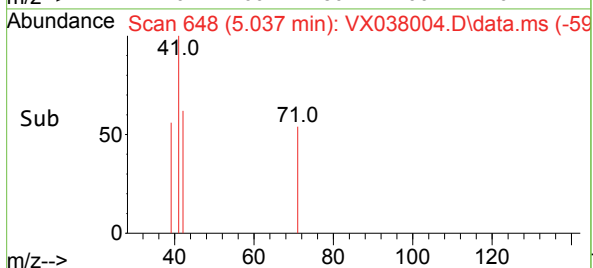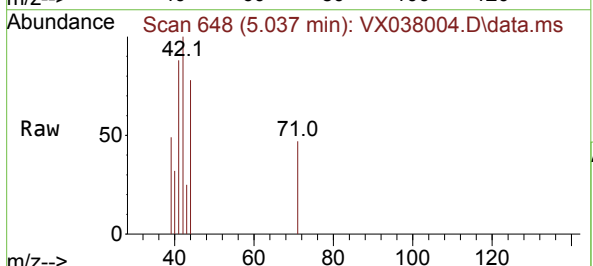



#33

1,2-Dichloroethane-d4

Concen: 57.174 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 112945

Ion Ratio Lower Upper

65 100

67 51.7 0.0 100.2



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17




Tgt Ion: 114 Resp: 265291


Ion Ratio Lower Upper

114 100

63 20.6 0.0 45.0


88 16.1 0.0 36.6





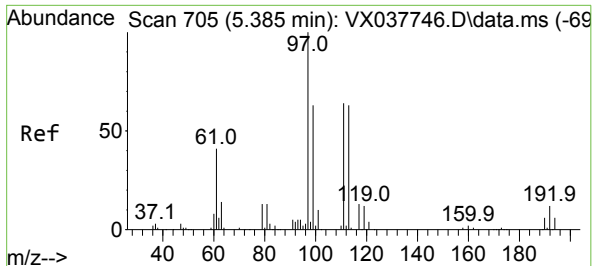


#35
Dibromofluoromethane
Concen: 49.138 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Instrument :
MSVOA_X
ClientSampleId :



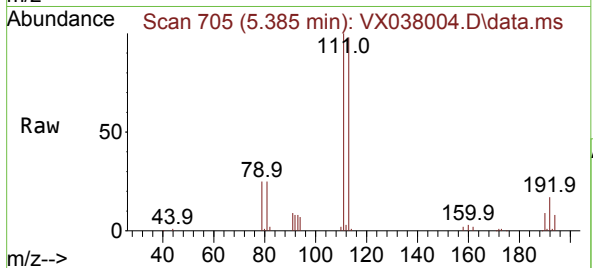



Tgt Ion:113 Resp: 87223
Ion Ratio Lower Upper
113 100
111 103.7 82.9 124.3
192 18.4 13.3 19.9

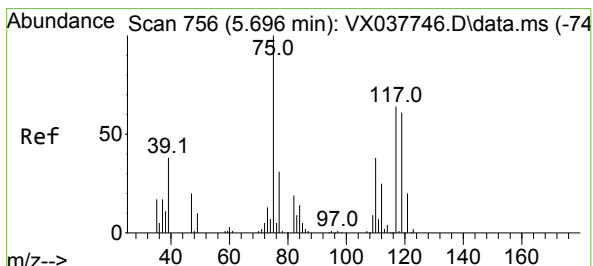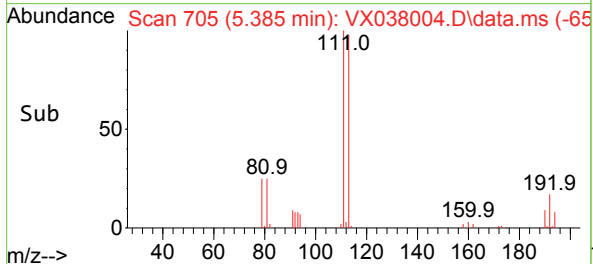

#36
1,1-Dichloropropene
Concen: 5.470 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.147 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 75 Resp: 13376
Ion Ratio Lower Upper
75 100
110 9.5 17.0 50.9#
77 0.0 24.7 37.1#

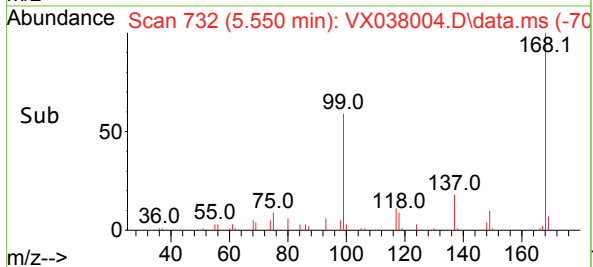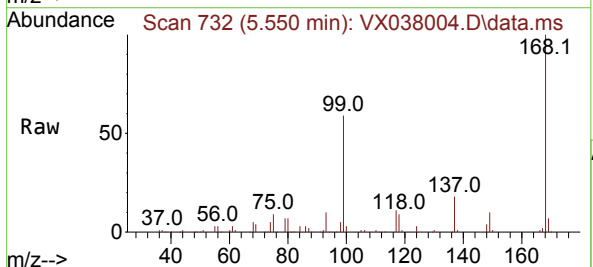



#37

Ethyl Acetate

Concen: 0.764 ug/l

RT: 4.733 min Scan# 595

Delta R.T. -0.000 min


Lab File: VX038004.D

Acq: 30 Sep 2023 15:17




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:	43	Resp:	2054
Ion	Ratio	Lower	Upper
43	100		
61	7.1	10.6	16.0#
70	9.0	8.3	12.5



#38

Carbon Tetrachloride

Concen: 6.251 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.122 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Tgt Ion:	117	Resp:	15994
Ion	Ratio	Lower	Upper
117	100		
119	3.3	78.2	117.2#
121	0.0	24.4	36.6#



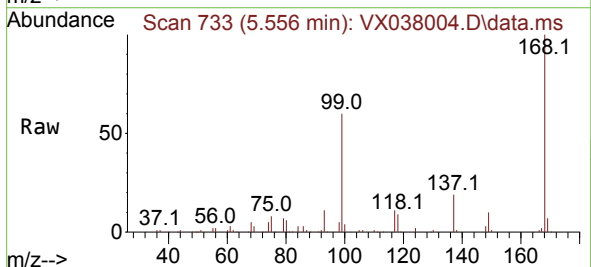



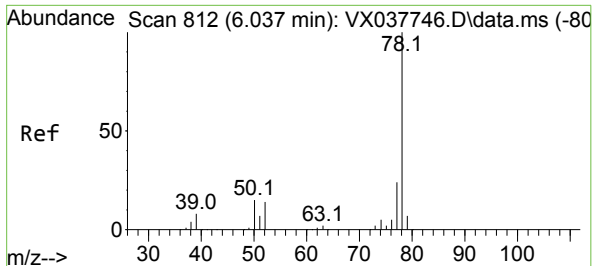

#40
Benzene
Concen: 4.667 ug/l
RT: 6.043 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 35090
Ion Ratio Lower Upper
78 100
77 22.8 19.3 28.9

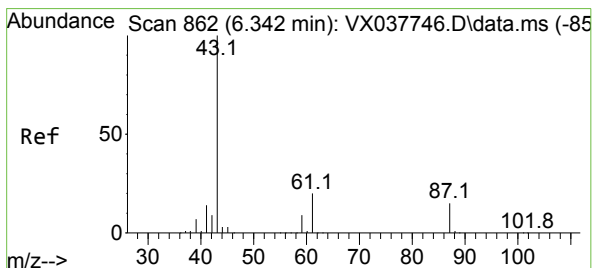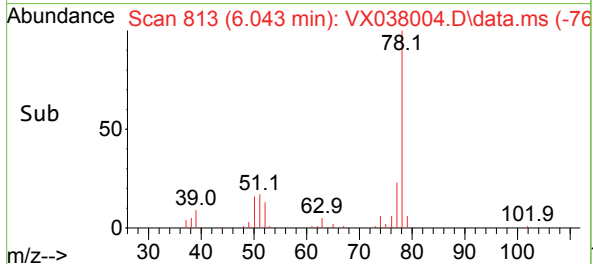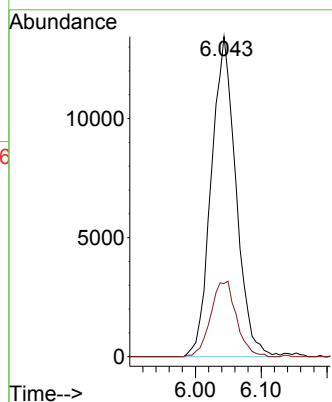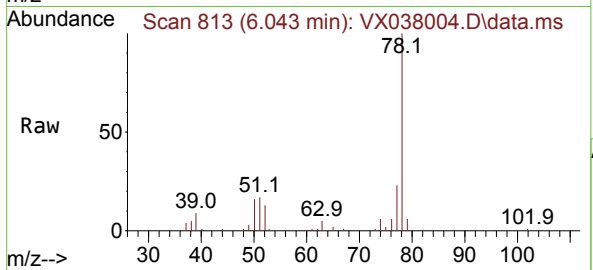

#43
Isopropyl Acetate
Concen: 21.052 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 43 Resp: 90492
Ion Ratio Lower Upper
43 100
61 19.2 15.2 22.8
87 14.0 9.8 14.6


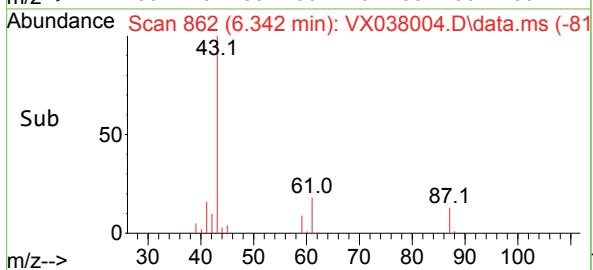

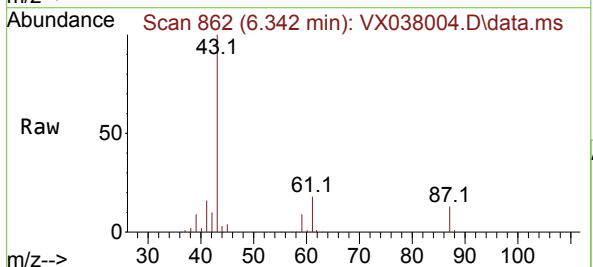




#48
Methyl methacrylate
Concen: 43.615 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.097 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 41 Resp: 89622
Ion Ratio Lower Upper
41 100
69 0.2 59.2 88.8#
39 57.6 47.7 71.5

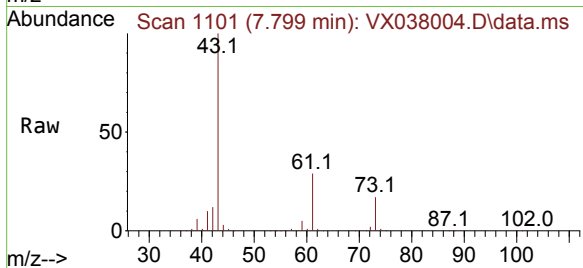

#49
1,4-Dioxane
Concen: 2.729 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.122 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 88 Resp: 147
Ion Ratio Lower Upper
88 100
43 607169.4 0.0 0.0#
58 2732.7 60.1 90.1#


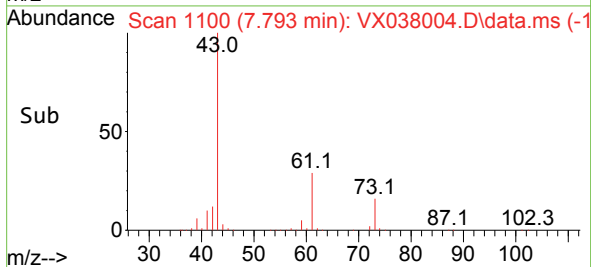

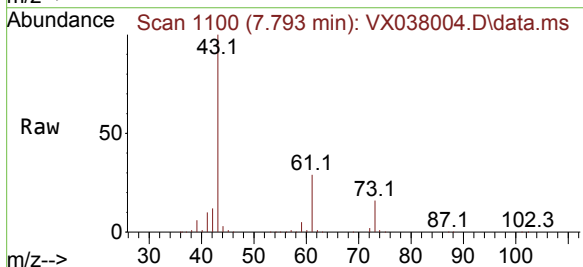




#50
Toluene-d8
Concen: 51.627 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 340506
Ion Ratio Lower Upper
98 100
100 62.8 53.1 79.7

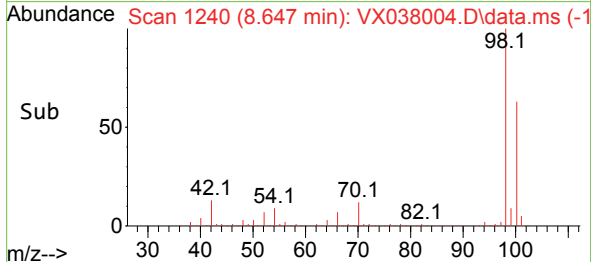

#51
4-Methyl-2-Pentanone
Concen: 28.876 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 43 Resp: 78752
Ion Ratio Lower Upper
43 100
58 5.5 30.4 45.6#


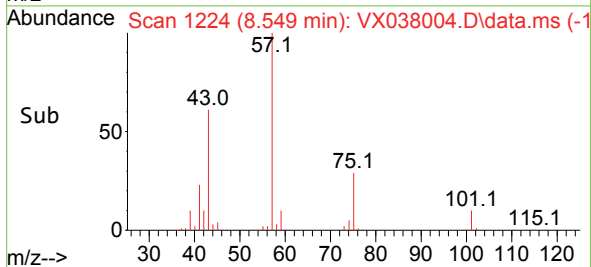

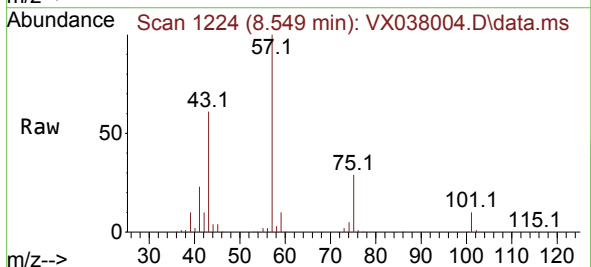




#52
Toluene
Concen: 5.644 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 27354
Ion Ratio Lower Upper
92 100
91 185.1 134.2 201.2

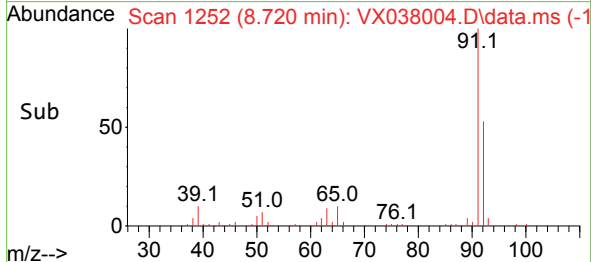

#53
t-1,3-Dichloropropene
Concen: 0.243 ug/l
RT: 8.957 min Scan# 1291
Delta R.T. -0.031 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 75 Resp: 657
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#


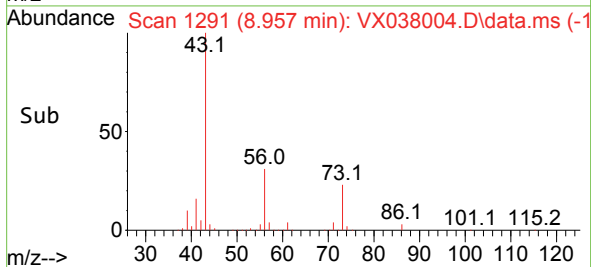

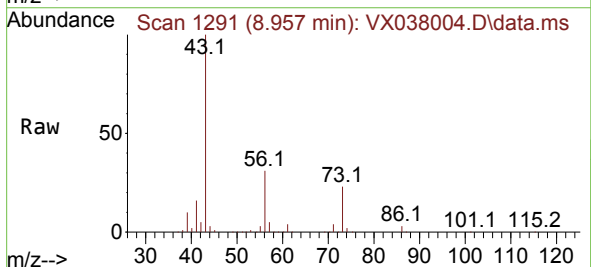




#54
 cis-1,3-Dichloropropene
 Concen: 10.856 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.177 min
 Lab File: VX038004.D
 Acq: 30 Sep 2023 15:17




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 32502
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.3 37.9#
 39 36.2 46.7 70.1#



#56
 Ethyl methacrylate
 Concen: 0.266 ug/l
 RT: 9.244 min Scan# 1338
 Delta R.T. 0.122 min
 Lab File: VX038004.D
 Acq: 30 Sep 2023 15:17

Tgt Ion: 69 Resp: 810
 Ion Ratio Lower Upper
 69 100
 41 6074.2 56.8 85.2#
 39 2894.7 32.0 48.0#

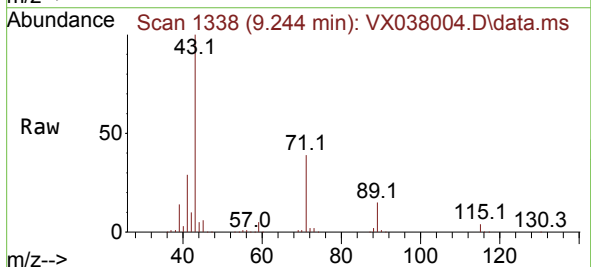



#57

1,3-Dichloropropane

Concen: 1.285 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.176 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 4248

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

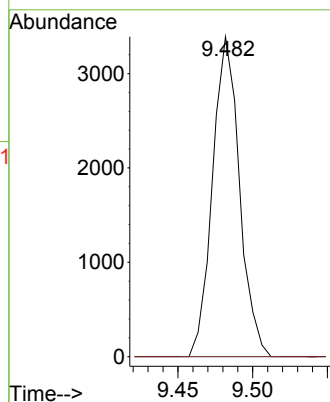

#59

2-Hexanone

Concen: 28.938 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.048 min

Lab File: VX038004.D




Acq: 30 Sep 2023 15:17


Tgt Ion: 43 Resp: 61447

Ion Ratio Lower Upper

43 100

58 19.7 26.2 78.5#









#62
4-Bromofluorobenzene
Concen: 57.352 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 137454
Ion Ratio Lower Upper
95 100
174 79.9 0.0 135.6
176 75.3 0.0 131.0

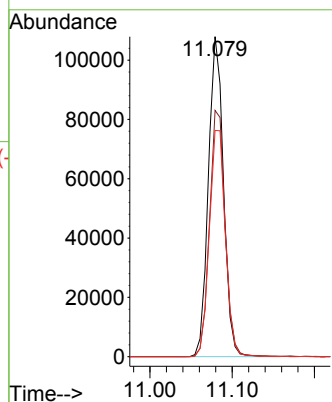

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX038004.D
Acq: 30 Sep 2023 15:17

Tgt Ion: 117 Resp: 281537
Ion Ratio Lower Upper
117 100
82 56.1 46.2 69.4
119 31.7 25.5 38.3





#67

Ethyl Benzene

Concen: 0.605 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 6369

Ion Ratio Lower Upper

91 100

106 34.2 24.9 37.3



#68

m/p-Xylenes

Concen: 2.567 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX038004.D




Acq: 30 Sep 2023 15:17


Tgt Ion: 106 Resp: 10444

Ion Ratio Lower Upper

106 100

91 217.0 165.5 248.3





#69

o-Xylene

Concen: 1.810 ug/l

RT: 10.640 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 7383

Ion Ratio Lower Upper

106 100

91 233.7 108.9 326.8



#70

Styrene

Concen: 0.615 ug/l

RT: 10.658 min Scan# 1570

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17




Tgt Ion:104 Resp: 4028


Ion Ratio Lower Upper

104 100

78 71.0 43.6 65.4#

103 73.0 43.6 65.4#

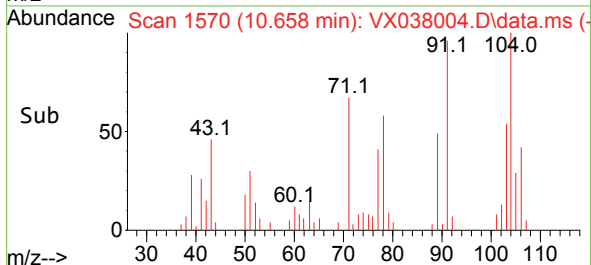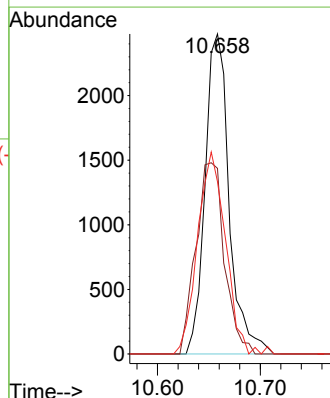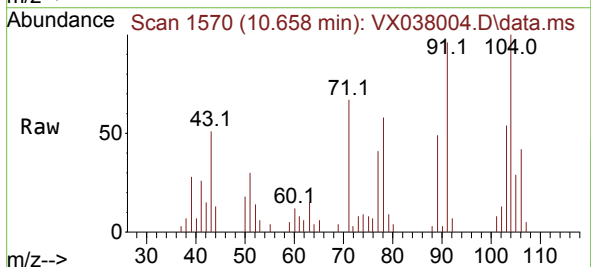



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 149528

Ion Ratio Lower Upper

152 100

115 60.7 43.3 129.9

150 157.7 0.0 345.0

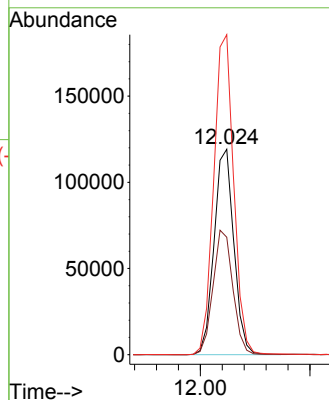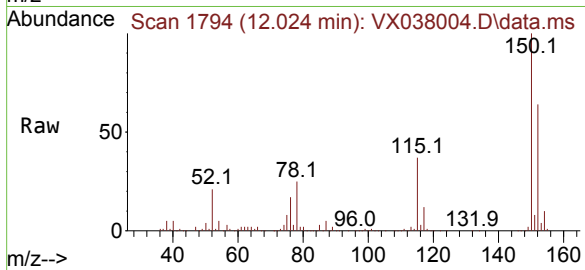

#76

1,2,3-Trichloropropane

Concen: 22.264 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX038004.D




Acq: 30 Sep 2023 15:17


Tgt Ion: 75 Resp: 76998

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

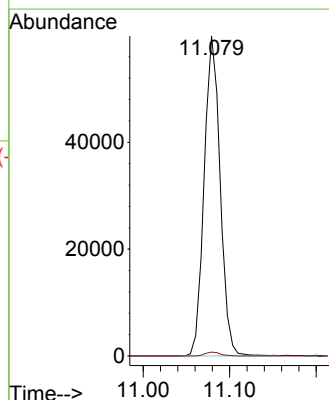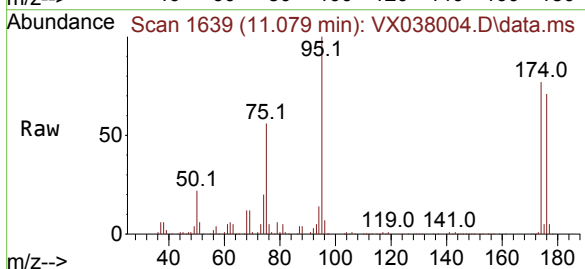



#80

1,3,5-Trimethylbenzene

Concen: 0.229 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.000 min


Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion:105 Resp: 2121

Ion Ratio Lower Upper

105 100

120 46.0 24.1 72.3

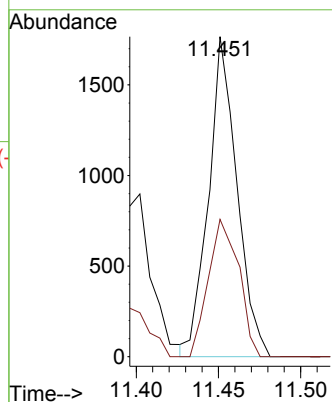

#81

trans-1,4-Dichloro-2-butene

Concen: 71.319 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17




Tgt Ion: 75 Resp: 76998


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#





#84

1,2,4-Trimethylbenzene

Concen: 0.739 ug/l

RT: 11.756 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 6812

Ion Ratio Lower Upper

105 100

120 32.5 21.2 63.6

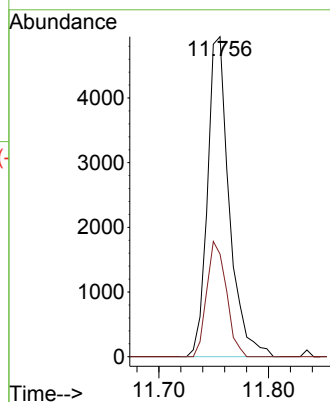

#95

Naphthalene

Concen: 7.850 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. -0.006 min

Lab File: VX038004.D

Acq: 30 Sep 2023 15:17

Tgt Ion:128 Resp: 80812

Ion Ratio Lower Upper

128 100

127 12.8 10.3 15.5

129 11.1 8.8 13.2

