

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
 Data File : VX038011.D
 Acq On : 30 Sep 2023 17:59
 Operator : JC/MD
 Sample : 04647-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 02 02:16:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	152924	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	274757	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	289109	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	153697	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	116584	58.025	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 116.060%			
35) Dibromofluoromethane	5.391	113	90551	49.255	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.500%			
50) Toluene-d8	8.647	98	350156	51.261	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.520%			
62) 4-Bromofluorobenzene	11.079	95	141314	56.931	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 113.860%			
Target Compounds					Qvalue	
6) Chloroethane	1.679	64	292	0.224	ug/l #	43
11) Tert butyl alcohol	2.947	59	4742	10.995	ug/l #	84
13) Acrolein	2.239	56	458	1.075	ug/l #	79
16) Acetone	2.373	43	25220	26.093	ug/l	97
18) Methyl Acetate	2.709	43	1191	0.342	ug/l #	80
20) Methylene Chloride	2.794	84	8624	4.803	ug/l	92
25) 2-Butanone	4.562	43	5393	3.954	ug/l	98
29) Tetrahydrofuran	5.032	42	500	0.589	ug/l #	41
36) 1,1-Dichloropropene	5.550	75	12892	5.091	ug/l #	51
37) Ethyl Acetate	4.739	43	2362	0.848	ug/l #	69
38) Carbon Tetrachloride	5.550	117	16028	6.049	ug/l #	15
40) Benzene	6.044	78	43314	5.562	ug/l	98
43) Isopropyl Acetate	6.342	43	95265	21.399	ug/l	98
48) Methyl methacrylate	7.799	41	91782	43.127	ug/l #	51
49) 1,4-Dioxane	7.793	88	74	1.326	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	84430	29.892	ug/l #	46
52) Toluene	8.720	92	33252	6.625	ug/l	92
53) t-1,3-Dichloropropene	8.958	75	804	0.287	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	34712	11.195	ug/l #	59
56) Ethyl methacrylate	9.244	69	770	0.244	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	4691	1.370	ug/l #	42
59) 2-Hexanone	9.482	43	62612	28.471	ug/l #	55
67) Ethyl Benzene	10.195	91	7402	0.685	ug/l	93
68) m/p-Xylenes	10.299	106	12657	3.030	ug/l	98
69) o-Xylene	10.646	106	8773	2.094	ug/l	94
70) Styrene	10.659	104	4304	0.640	ug/l #	70
76) 1,2,3-Trichloropropane	11.079	75	79775	22.441	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.451	105	2204	0.231	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	79775	71.887	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.750	105	8333	0.880	ug/l	82
95) Naphthalene	13.774	128	95867	9.060	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038011.D
Acq On : 30 Sep 2023 17:59
Operator : JC/MD
Sample : 04647-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Oct 02 02:16:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration

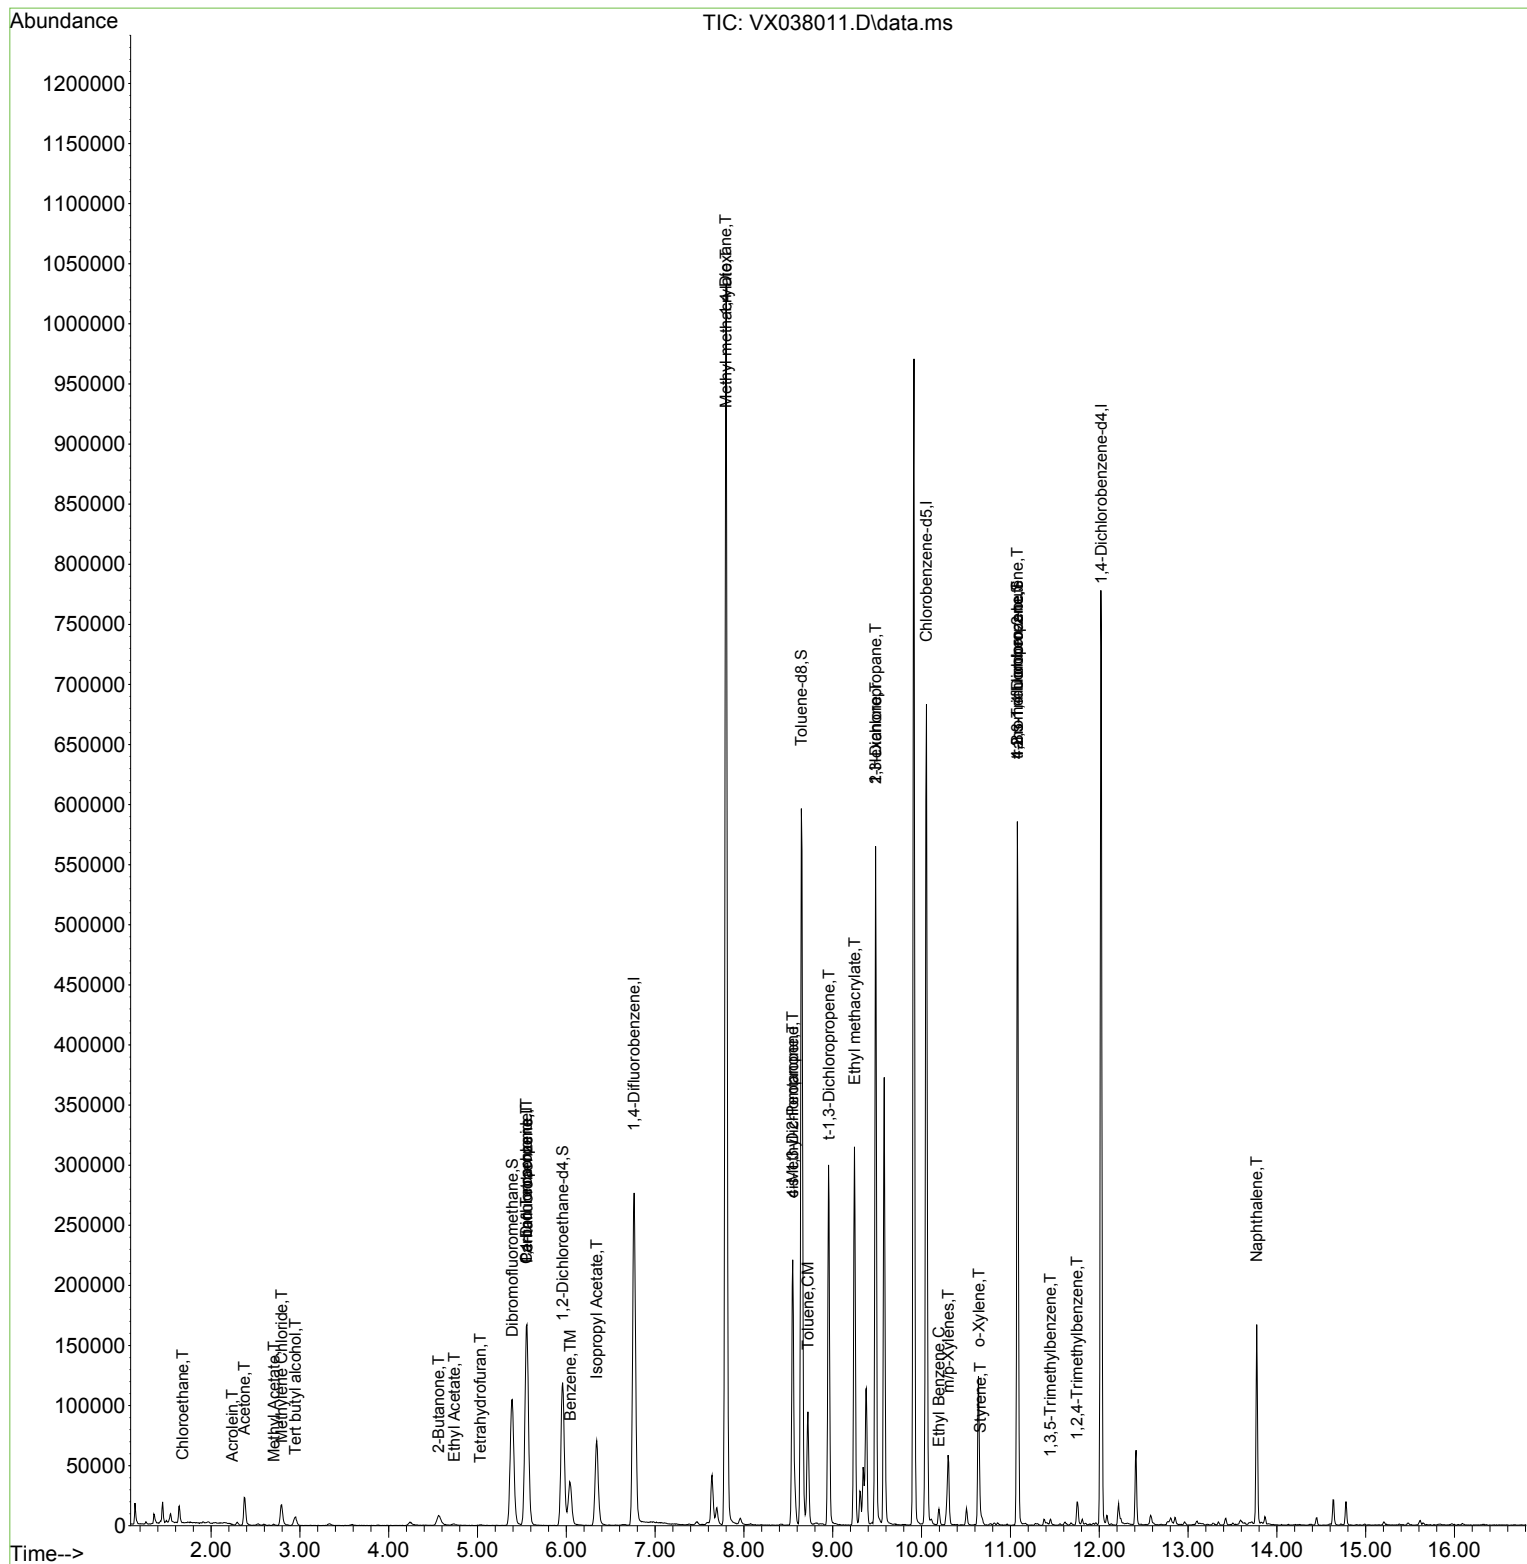






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 152924
Ion Ratio Lower Upper
168 100
99 59.8 56.6 85.0

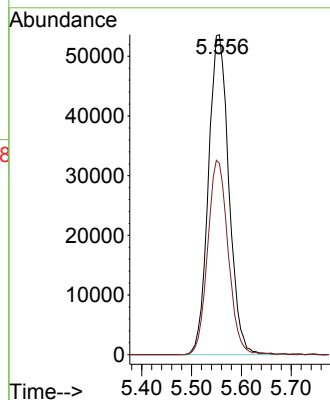

#6
Chloroethane
Concen: 0.224 ug/l
RT: 1.679 min Scan# 97
Delta R.T. -0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 64 Resp: 292
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

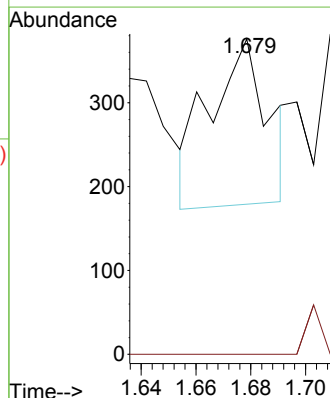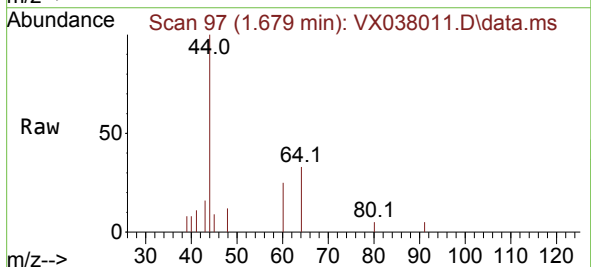

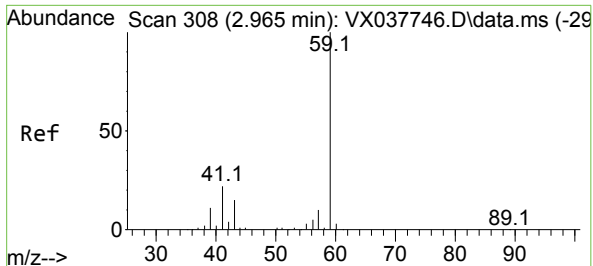

#11

Tert butyl alcohol

Concen: 10.995 ug/l

RT: 2.947 min Scan# 308

Delta R.T. -0.018 min


Lab File: VX038011.D

Acq: 30 Sep 2023 17:59

Instrument :

MSVOA_X

ClientSampleId :



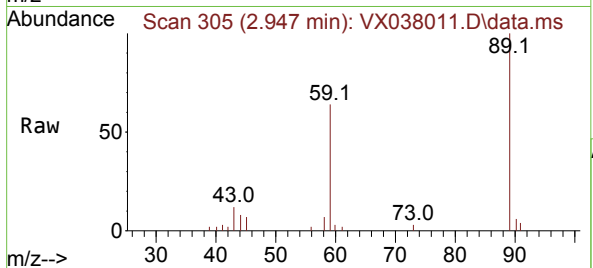


Tgt Ion: 59 Resp: 4742

Ion Ratio Lower Upper

59 100

57 2.0 6.0 9.0#

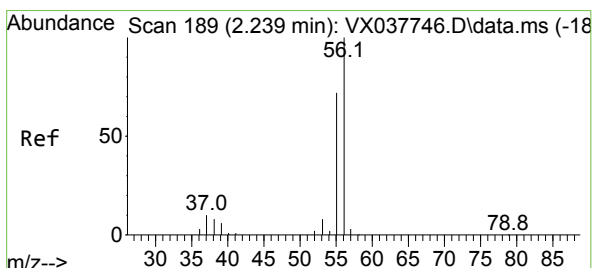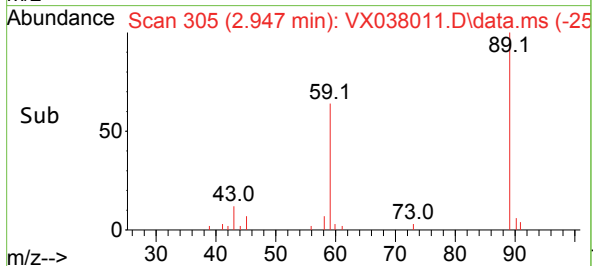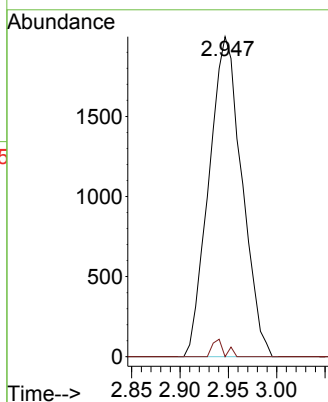

#13

Acrolein

Concen: 1.075 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX038011.D




Acq: 30 Sep 2023 17:59


Tgt Ion: 56 Resp: 458

Ion Ratio Lower Upper

56 100

55 54.4 57.1 85.7#


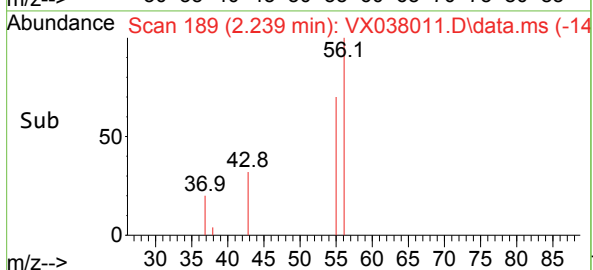
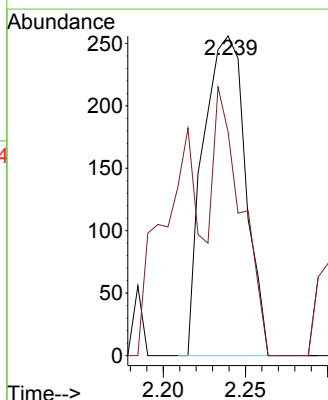
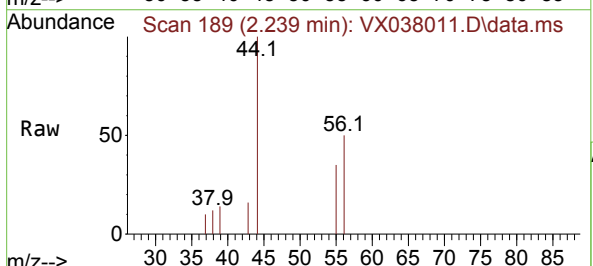




#16
Acetone
Concen: 26.093 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 25220
Ion Ratio Lower Upper
43 100
58 28.8 21.9 32.9

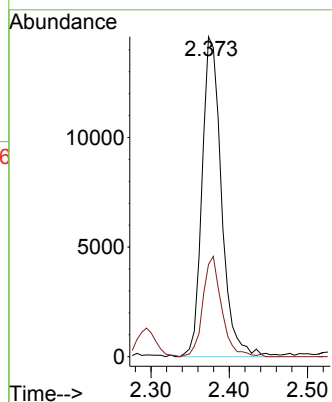

#18
Methyl Acetate
Concen: 0.342 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59


Tgt Ion: 43 Resp: 1191
Ion Ratio Lower Upper
43 100
74 12.8 17.8 26.8#

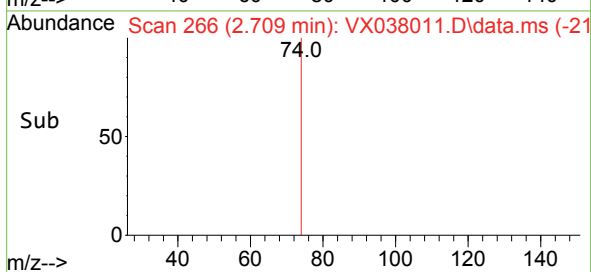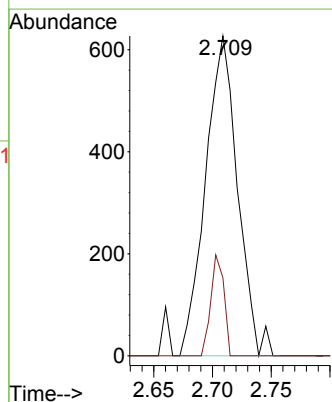






#20
Methylene Chloride
Concen: 4.803 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84	Resp: 8624
Ion Ratio	Lower Upper
84 100	
49 115.2	103.6 155.4
51 39.1	33.8 50.6
86 60.2	49.4 74.0

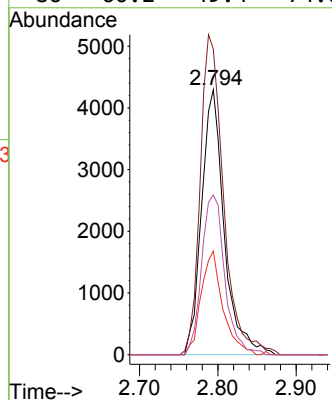

#25
2-Butanone
Concen: 3.954 ug/l
RT: 4.562 min Scan# 570
Delta R.T. -0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 43	Resp: 5393
Ion Ratio	Lower Upper
43 100	
72 25.1	19.4 29.2

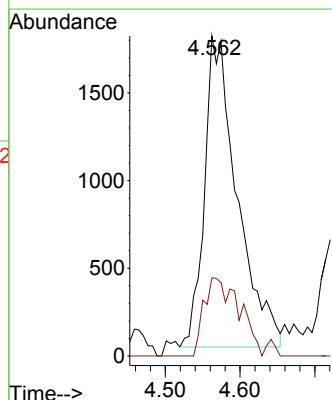

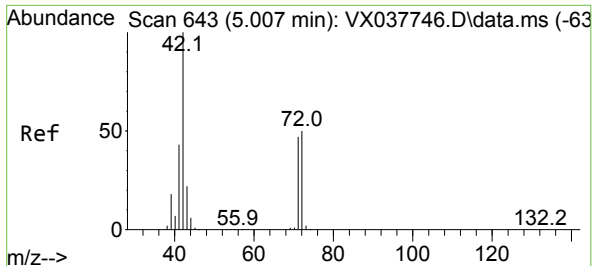

#29

Tetrahydrofuran

Concen: 0.589 ug/l

RT: 5.032 min Scan# 643

Delta R.T. 0.018 min


Lab File: VX038011.D

Acq: 30 Sep 2023 17:59




Instrument :

MSVOA_X

ClientSampleId :

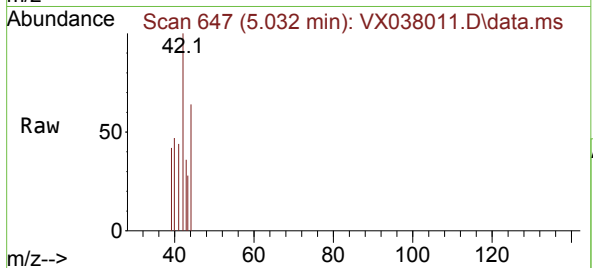

Tgt Ion:	42	Resp:	500
Ion	Ratio	Lower	Upper
42	100		
72	0.0	34.2	51.4#
71	8.8	32.2	48.2#

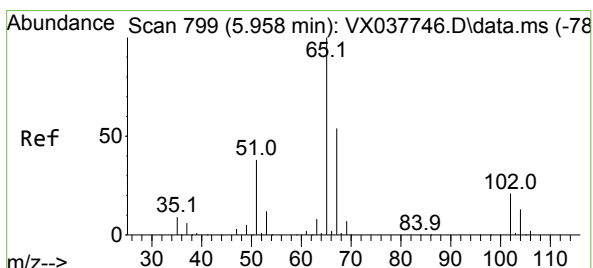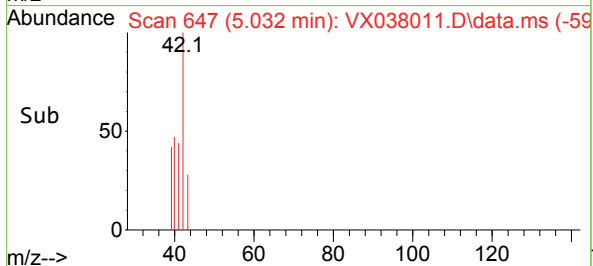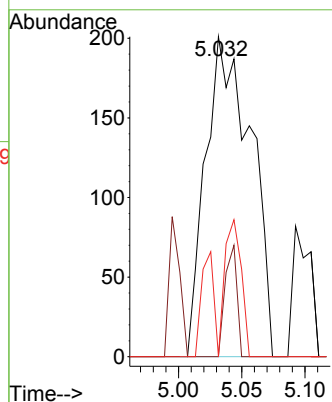

#33

1,2-Dichloroethane-d4

Concen: 58.025 ug/l




RT: 5.958 min Scan# 799


Delta R.T. 0.000 min

Lab File: VX038011.D

Acq: 30 Sep 2023 17:59

Tgt Ion:	65	Resp:	116584
Ion	Ratio	Lower	Upper
65	100		
67	51.7	0.0	100.2


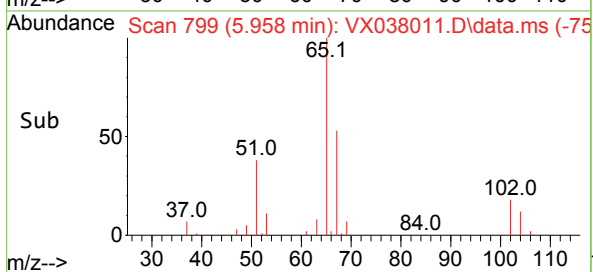
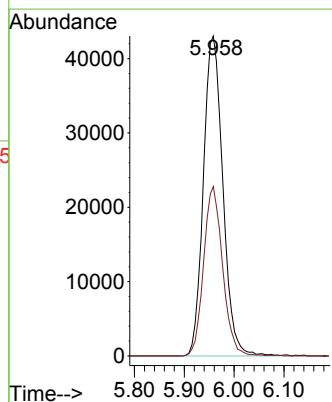
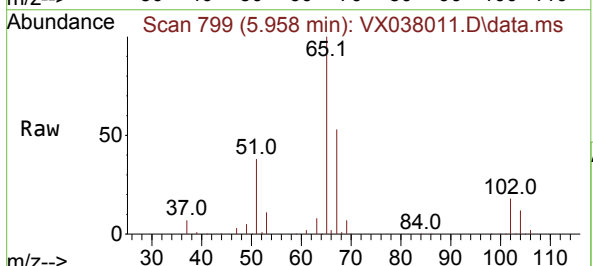




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 274757
Ion Ratio Lower Upper
114 100
63 20.5 0.0 45.0
88 15.1 0.0 36.6

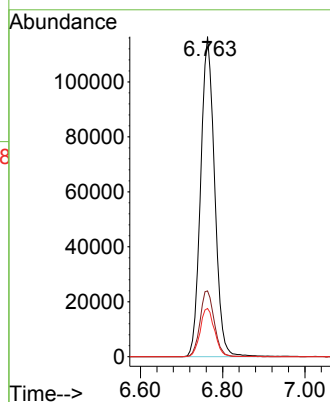

#35
Dibromofluoromethane
Concen: 49.255 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59


Tgt Ion:113 Resp: 90551
Ion Ratio Lower Upper
113 100
111 102.3 82.9 124.3
192 18.4 13.3 19.9

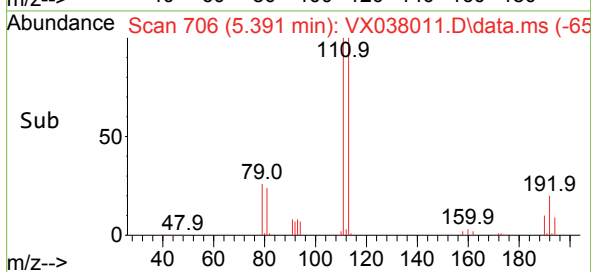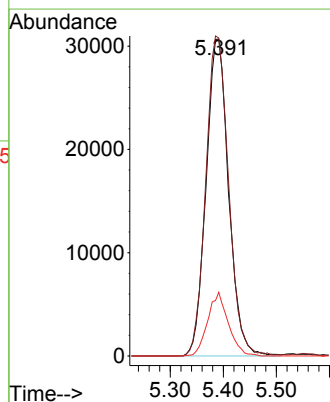






#36
1,1-Dichloropropene
Concen: 5.091 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 12892
Ion Ratio Lower Upper
75 100
110 9.2 17.0 50.9#
77 0.0 24.7 37.1#

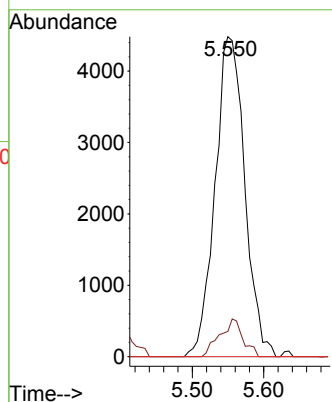

#37
Ethyl Acetate
Concen: 0.848 ug/l
RT: 4.739 min Scan# 599
Delta R.T. 0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59


Tgt Ion: 43 Resp: 2362
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#

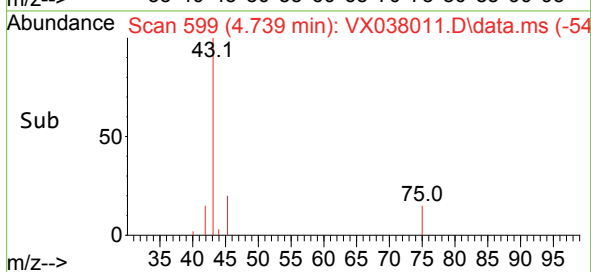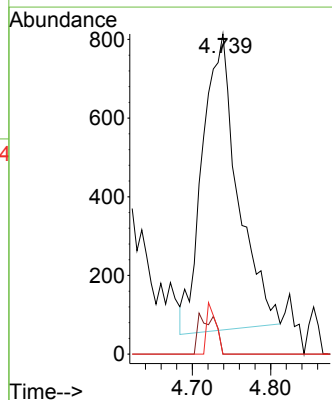



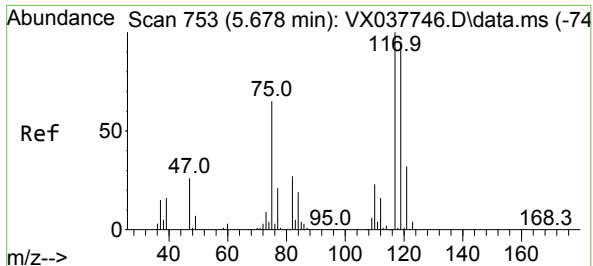


#38
Carbon Tetrachloride
Concen: 6.049 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Instrument :
MSVOA_X
ClientSampleId :



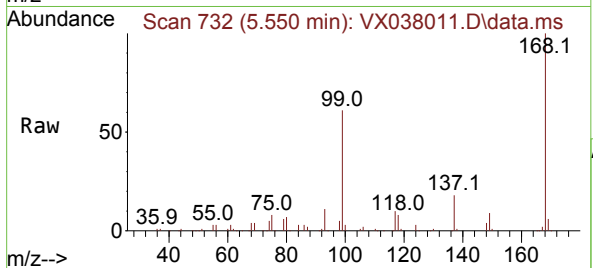



Tgt Ion:117 Resp: 16028
Ion Ratio Lower Upper
117 100
119 5.0 78.2 117.2#
121 0.0 24.4 36.6#

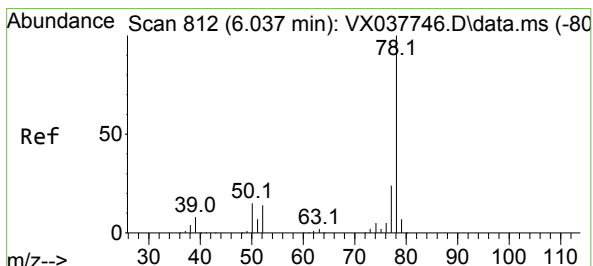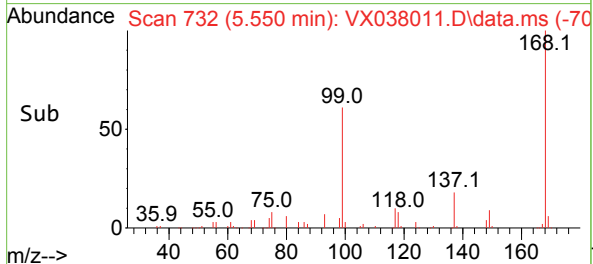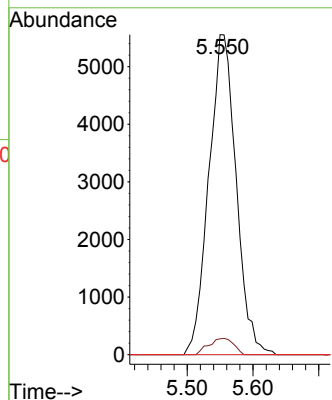

#40
Benzene
Concen: 5.562 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 78 Resp: 43314
Ion Ratio Lower Upper
78 100
77 23.0 19.3 28.9


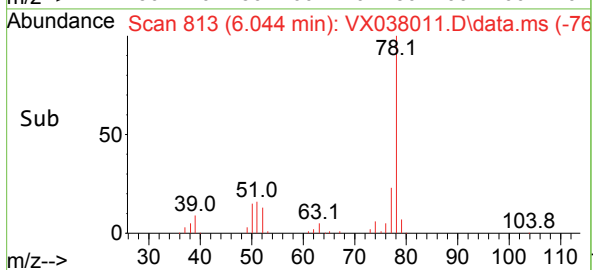
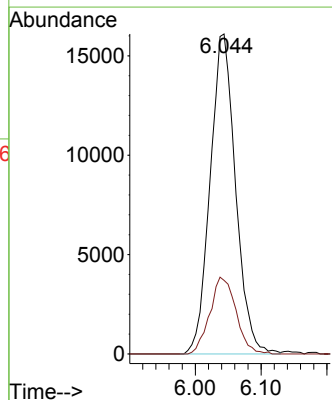
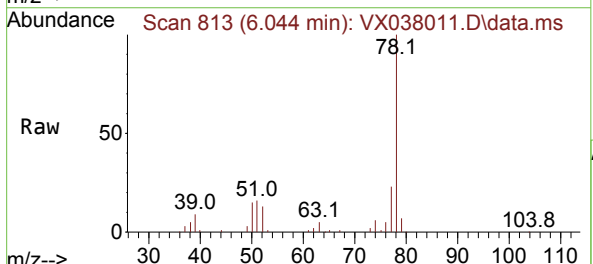




#43
Isopropyl Acetate
Concen: 21.399 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
43	100		
61	18.8	15.2	22.8
87	13.6	9.8	14.6

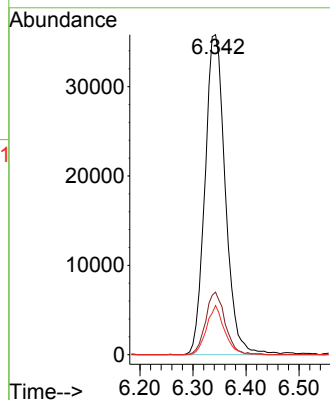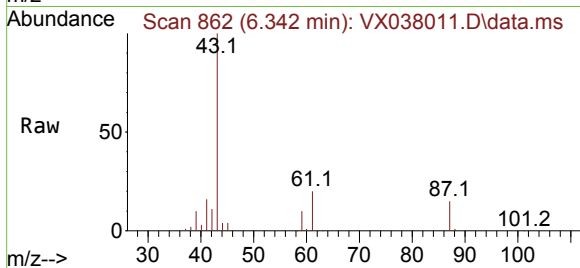

#48
Methyl methacrylate
Concen: 43.127 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.097 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion	Ratio	Lower	Upper
41	100		
69	0.1	59.2	88.8#
39	57.8	47.7	71.5

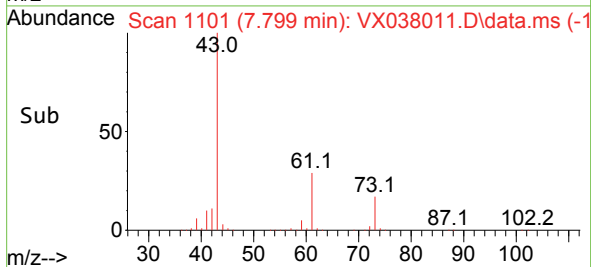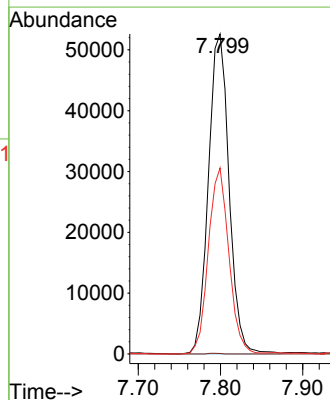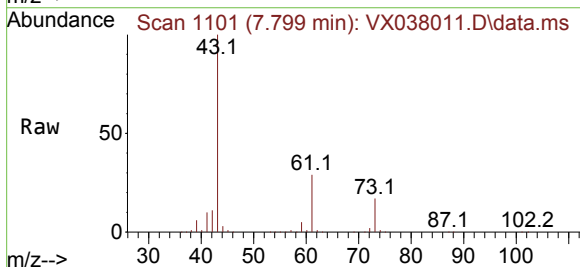



#49

1,4-Dioxane

Concen: 1.326 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.122 min

Lab File: VX038011.D

Acq: 30 Sep 2023 17:59

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 88 Resp: 74

Ion Ratio Lower Upper

88 100

43 1245773.0 0.0 0.0#

58 5782.4 60.1 90.1#

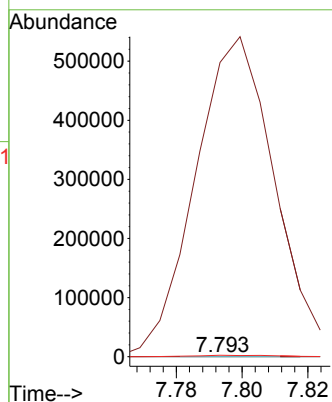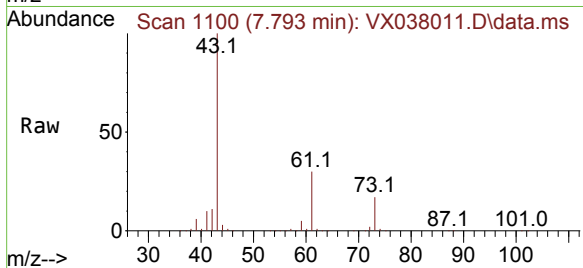

#50

Toluene-d8

Concen: 51.261 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX038011.D




Acq: 30 Sep 2023 17:59


Tgt Ion: 98 Resp: 350156

Ion Ratio Lower Upper

98 100

100 63.4 53.1 79.7



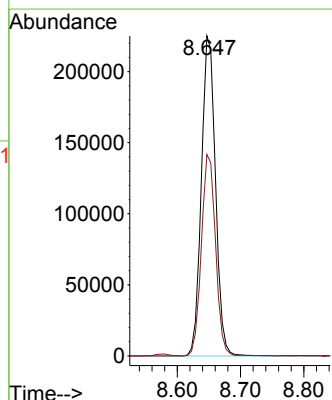
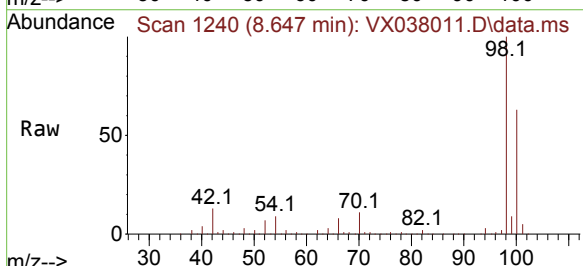




#51
4-Methyl-2-Pentanone
Concen: 29.892 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 84430
Ion Ratio Lower Upper
43 100
58 5.7 30.4 45.6#

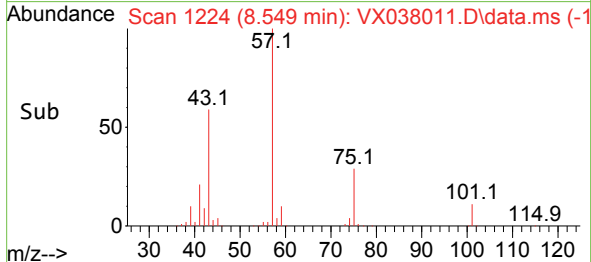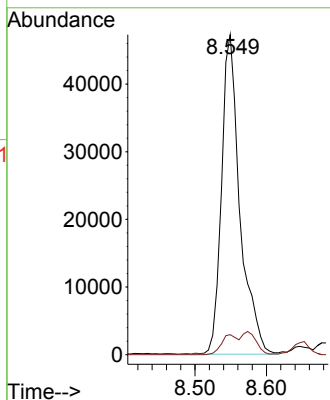

#52
Toluene
Concen: 6.625 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 92 Resp: 33252
Ion Ratio Lower Upper
92 100
91 179.1 134.2 201.2


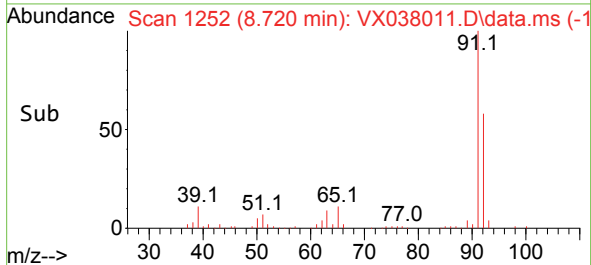
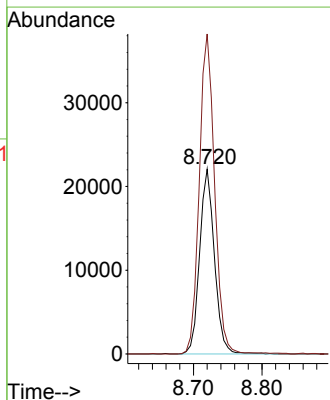
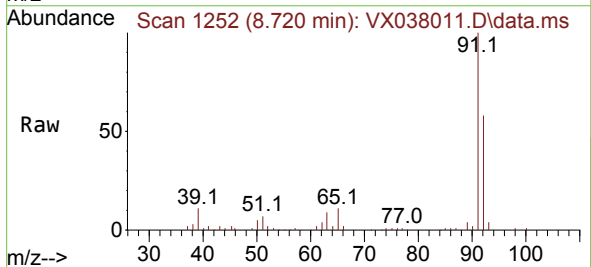




#53
 t-1,3-Dichloropropene
 Concen: 0.287 ug/l
 RT: 8.958 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VX038011.D
 Acq: 30 Sep 2023 17:59




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 804
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#

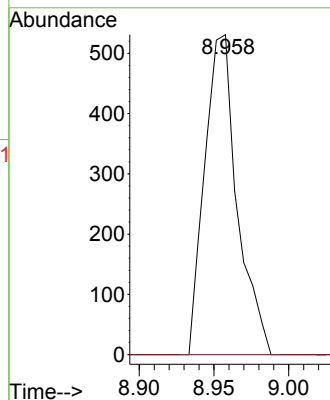

#54
 cis-1,3-Dichloropropene
 Concen: 11.195 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.177 min
 Lab File: VX038011.D
 Acq: 30 Sep 2023 17:59

Tgt Ion: 75 Resp: 34712
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.3 37.9#
 39 34.2 46.7 70.1#



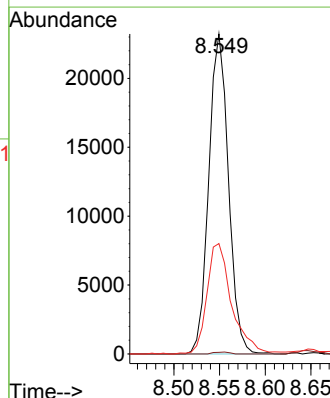
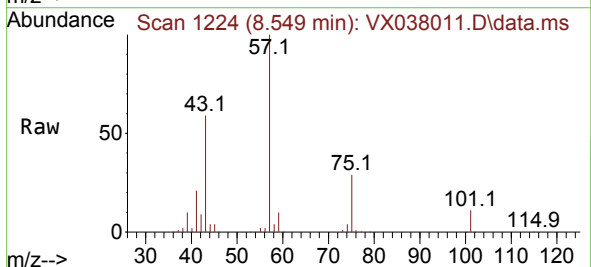




#56
Ethyl methacrylate
Concen: 0.244 ug/l
RT: 9.244 min Scan# 1338
Delta R.T. 0.122 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 69 Resp: 770
Ion Ratio Lower Upper
69 100
41 6553.6 56.8 85.2#
39 3011.6 32.0 48.0#

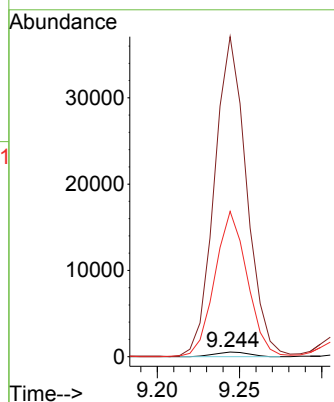

#57
1,3-Dichloropropane
Concen: 1.370 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 76 Resp: 4691
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#



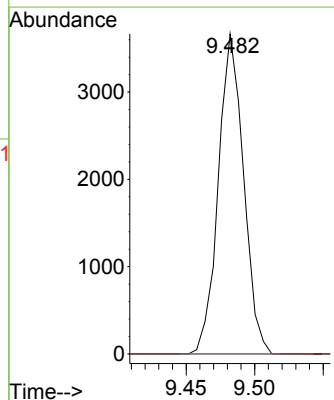





#59
2-Hexanone
Concen: 28.471 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.049 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 62612
Ion Ratio Lower Upper
43 100
58 20.7 26.2 78.5#

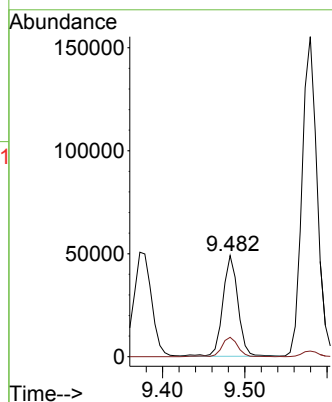

#62
4-Bromofluorobenzene
Concen: 56.931 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 95 Resp: 141314
Ion Ratio Lower Upper
95 100
174 78.0 0.0 135.6
176 76.3 0.0 131.0



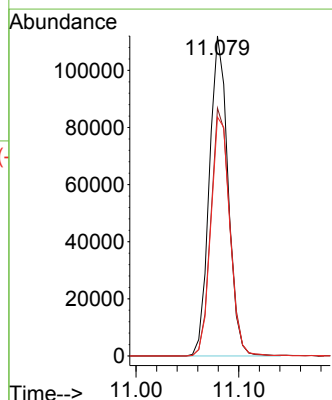
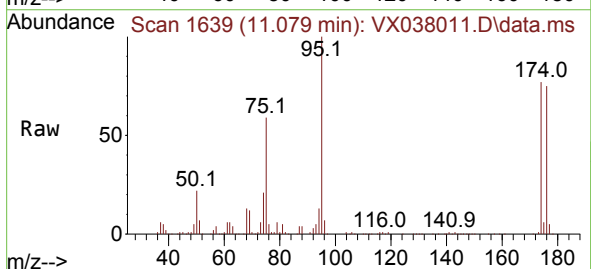




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 289109
Ion Ratio Lower Upper
117 100
82 55.7 46.2 69.4
119 32.3 25.5 38.3

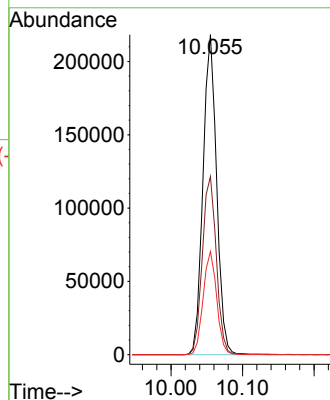

#67
Ethyl Benzene
Concen: 0.685 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Tgt Ion: 91 Resp: 7402
Ion Ratio Lower Upper
91 100
106 34.8 24.9 37.3



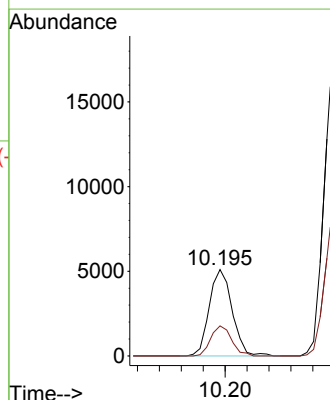
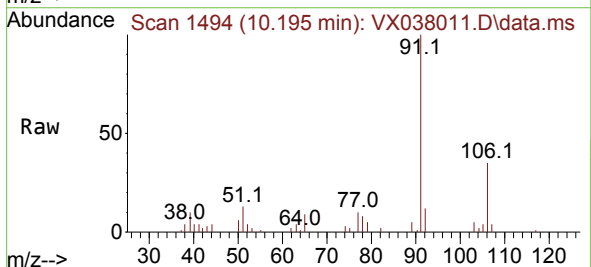


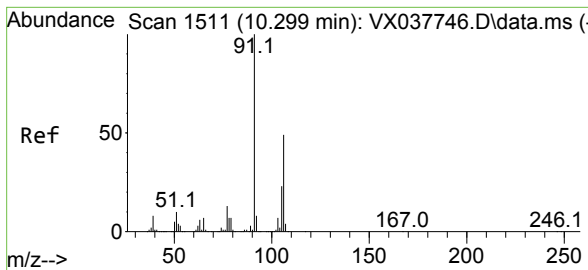

#68
m/p-Xylenes
Concen: 3.030 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 12657
Ion Ratio Lower Upper
106 100
91 209.9 165.5 248.3

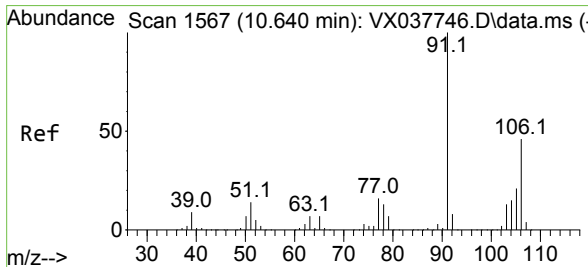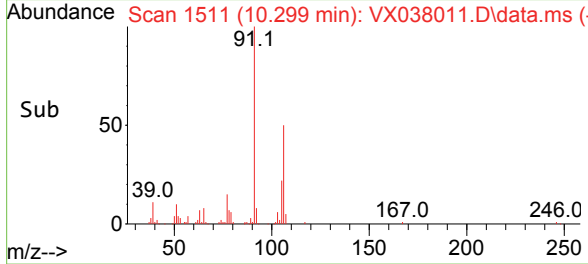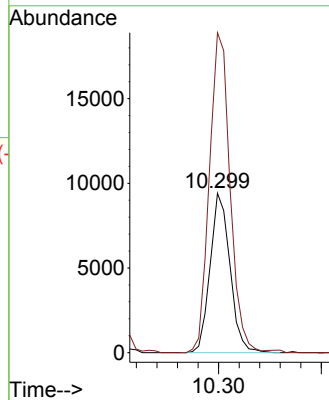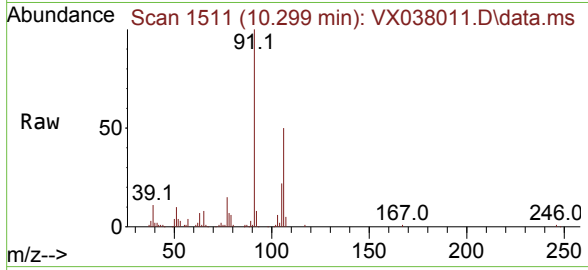

#69
o-Xylene
Concen: 2.094 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59


Tgt Ion:106 Resp: 8773
Ion Ratio Lower Upper
106 100
91 227.2 108.9 326.8

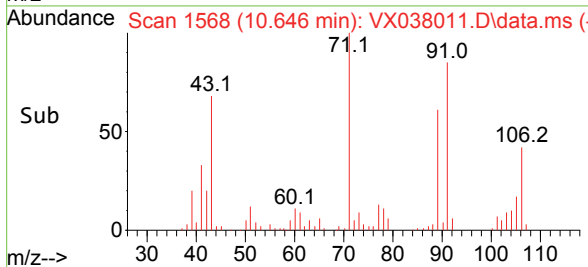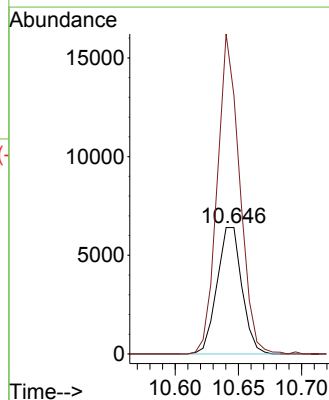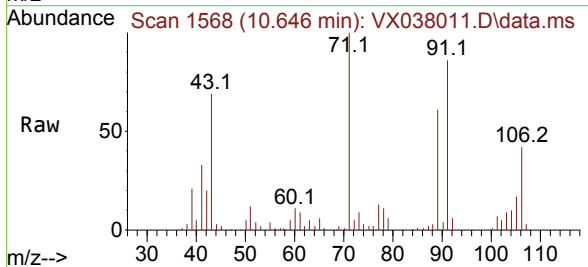






#70
Styrene
Concen: 0.640 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:104 Resp: 4304
Ion Ratio Lower Upper
104 100
78 74.5 43.6 65.4#
103 77.5 43.6 65.4#

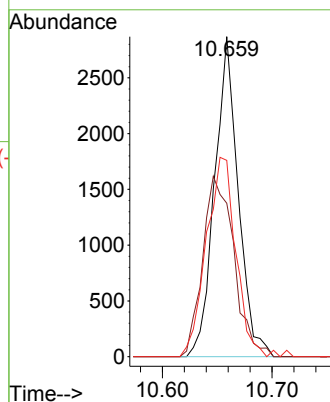


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59



Tgt Ion:152 Resp: 153697
Ion Ratio Lower Upper
152 100
115 60.5 43.3 129.9
150 155.1 0.0 345.0

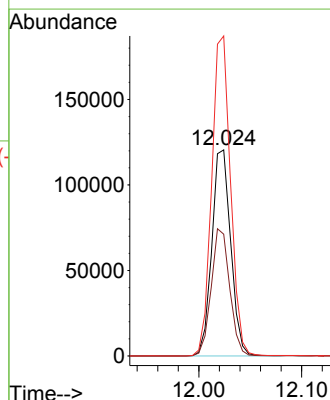



#76

1,2,3-Trichloropropane

Concen: 22.441 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX038011.D

Acq: 30 Sep 2023 17:59

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 79775

Ion Ratio Lower Upper

75 100

77 1.0 19.1 57.5#

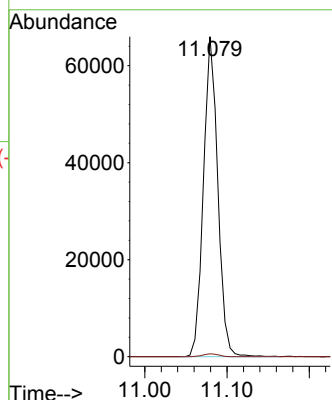

#80

1,3,5-Trimethylbenzene

Concen: 0.231 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX038011.D




Acq: 30 Sep 2023 17:59


Tgt Ion:105 Resp: 2204

Ion Ratio Lower Upper

105 100

120 46.1 24.1 72.3



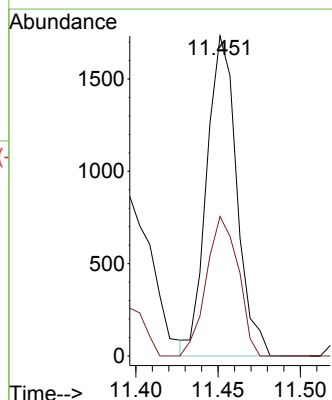





#81
 trans-1,4-Dichloro-2-butene
 Concen: 71.887 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX038011.D
 Acq: 30 Sep 2023 17:59




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 79775
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.0 36.9 55.3#

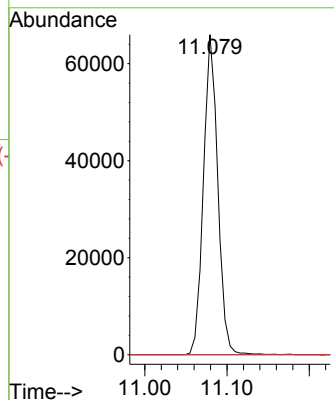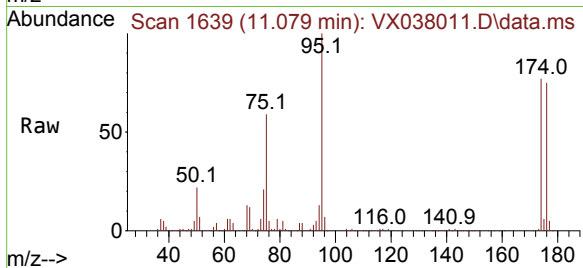

#84
 1,2,4-Trimethylbenzene
 Concen: 0.880 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.006 min
 Lab File: VX038011.D
 Acq: 30 Sep 2023 17:59


Tgt Ion:105 Resp: 8333
 Ion Ratio Lower Upper
 105 100
 120 30.9 21.2 63.6

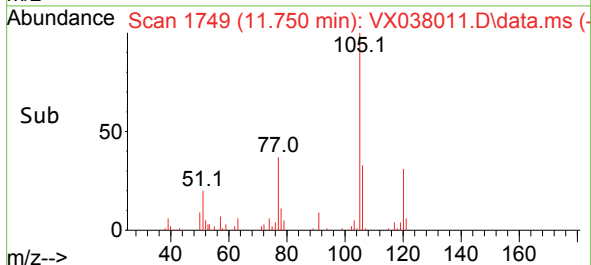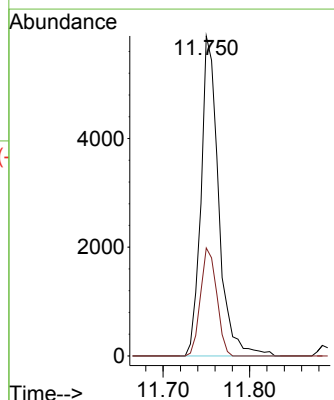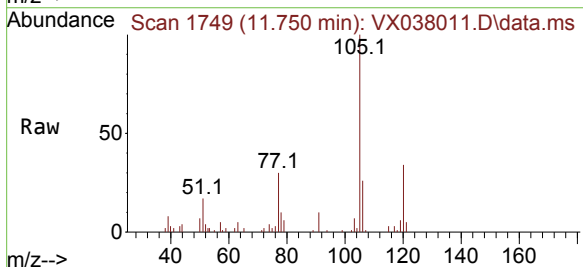

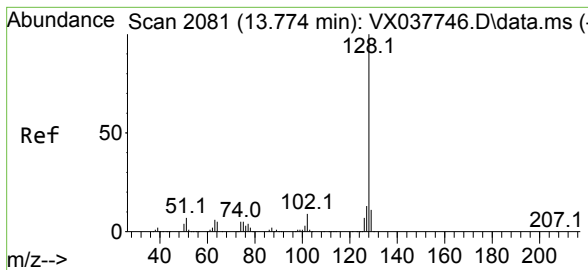

#95
Naphthalene
Concen: 9.060 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX038011.D
Acq: 30 Sep 2023 17:59

Instrument :
MSVOA_X
ClientSampleId :

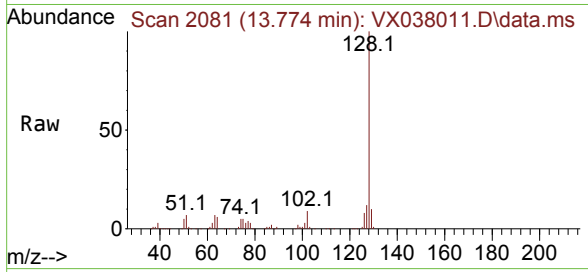

Tgt Ion:	128	Resp:	95867
Ion	Ratio	Lower	Upper
128	100		
127	12.6	10.3	15.5
129	11.2	8.8	13.2

