

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
 Data File : VX038013.D
 Acq On : 30 Sep 2023 18:45
 Operator : JC/MD
 Sample : 04639-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1036

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Title : SW846 8260

Signal : TIC: VX038013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.374	205	211	222	rBV	41094	69128	6.66%	1.039%
2	2.526	230	236	244	rBV	6491	12386	1.19%	0.186%
3	4.568	563	571	584	rBV2	4413	14019	1.35%	0.211%
4	5.385	694	705	721	rBV2	113747	332962	32.10%	5.005%
5	5.550	721	732	752	rVB	186398	528341	50.93%	7.941%
6	5.958	788	799	811	rBV2	128721	349533	33.69%	5.254%
7	6.763	921	931	949	rBV	309712	727217	70.10%	10.930%
8	8.647	1234	1240	1248	rBV	631045	987943	95.23%	14.849%
9	8.720	1248	1252	1259	rVB	15367	25036	2.41%	0.376%
10	9.525	1375	1384	1392	rBV2	8421	13780	1.33%	0.207%
11	10.055	1465	1471	1491	rBV	699023	948894	91.47%	14.262%
12	10.640	1561	1567	1574	rBV	51645	70563	6.80%	1.061%
13	10.768	1584	1588	1598	rBV	9628	14494	1.40%	0.218%
14	11.079	1634	1639	1653	rBV	620758	772734	74.49%	11.614%
15	11.402	1682	1692	1696	rBV	6868	11670	1.12%	0.175%
16	11.451	1696	1700	1704	rBV	8839	11013	1.06%	0.166%
17	11.616	1719	1727	1732	rBV	13022	17423	1.68%	0.262%
18	12.018	1788	1793	1800	rBV	816809	1037422	100.00%	15.593%
19	12.085	1800	1804	1810	rVB	29593	35857	3.46%	0.539%
20	12.244	1822	1830	1838	rBV2	17732	31310	3.02%	0.471%
21	12.317	1838	1842	1852	rVB2	8531	13471	1.30%	0.202%
22	12.610	1885	1890	1894	rBV	10932	12980	1.25%	0.195%
23	12.701	1900	1905	1912	rBV2	6778	10974	1.06%	0.165%
24	12.920	1936	1941	1944	rVV	10710	12720	1.23%	0.191%
25	12.963	1944	1948	1954	rVB	14639	17975	1.73%	0.270%
26	13.164	1974	1981	1985	rBV3	11667	17578	1.69%	0.264%
27	13.292	1997	2002	2007	rVB2	40772	54262	5.23%	0.816%
28	13.420	2019	2023	2030	rVB	24386	31337	3.02%	0.471%
29	13.579	2046	2049	2056	rBV4	9169	17174	1.66%	0.258%
30	13.658	2059	2062	2068	rVB3	9227	15606	1.50%	0.235%
31	13.774	2074	2081	2090	rBV	36142	50120	4.83%	0.753%
32	13.853	2090	2094	2099	rVB	13781	16565	1.60%	0.249%
33	13.926	2101	2106	2110	rBV2	15176	20701	2.00%	0.311%
34	14.073	2126	2130	2134	rBV	10431	12834	1.24%	0.193%
35	14.225	2149	2155	2160	rBV2	32902	57108	5.50%	0.858%
36	14.371	2175	2179	2183	rVB2	15666	19328	1.86%	0.291%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038013.D
Acq On : 30 Sep 2023 18:45
Operator : JC/MD
Sample : 04639-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1036

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M

Title : SW846 8260

37	14.481	2192	2197	2202	rBV2	29510	38804	3.74%	0.583%
38	14.634	2209	2222	2226	rBV2	30480	59990	5.78%	0.902%
39	14.670	2226	2228	2234	rVB2	9013	10432	1.01%	0.157%
40	14.780	2240	2246	2249	rBV	21992	29463	2.84%	0.443%
41	14.902	2260	2266	2273	rVB4	6211	10599	1.02%	0.159%
42	15.182	2308	2312	2314	rBV2	10450	16158	1.56%	0.243%
43	15.201	2314	2315	2321	rVB2	13097	13760	1.33%	0.207%
44	15.365	2338	2342	2351	rVB6	8279	18639	1.80%	0.280%
45	15.475	2356	2360	2364	rBV2	7597	10413	1.00%	0.157%
46	15.609	2378	2382	2385	rBV2	13416	19265	1.86%	0.290%
47	15.646	2385	2388	2397	rVB2	12508	20054	1.93%	0.301%
48	15.841	2413	2420	2426	rVB3	6858	13187	1.27%	0.198%




Sum of corrected areas: 6653222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038013.D
Acq On : 30 Sep 2023 18:45
Operator : JC/MD
Sample : 04639-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

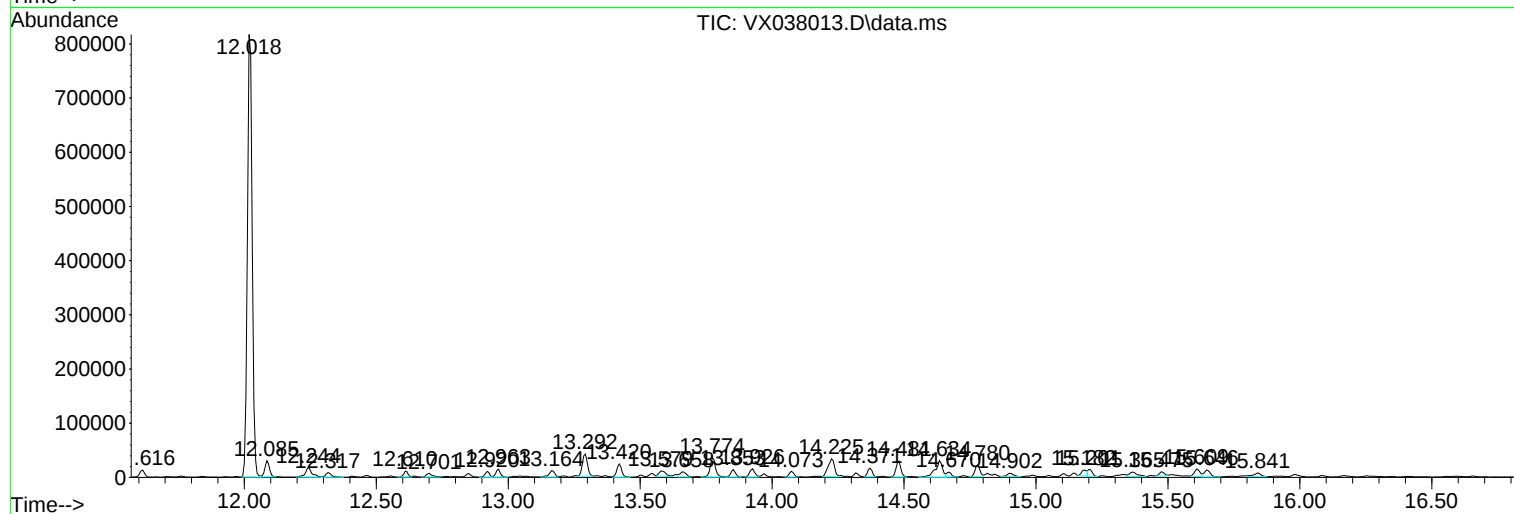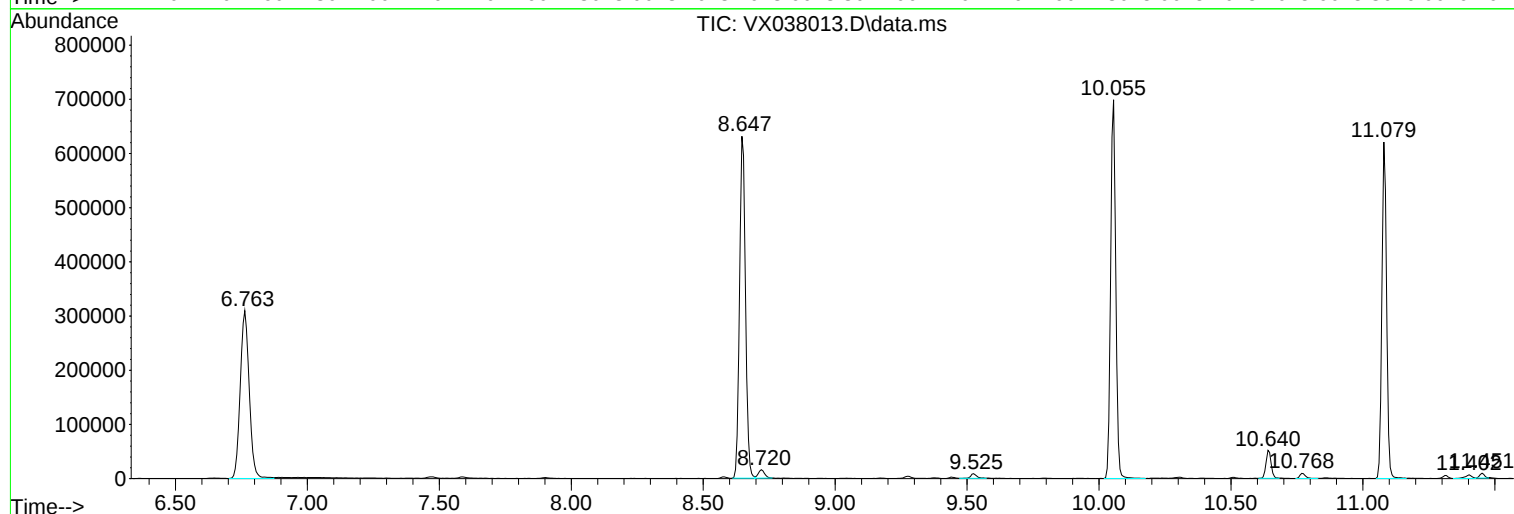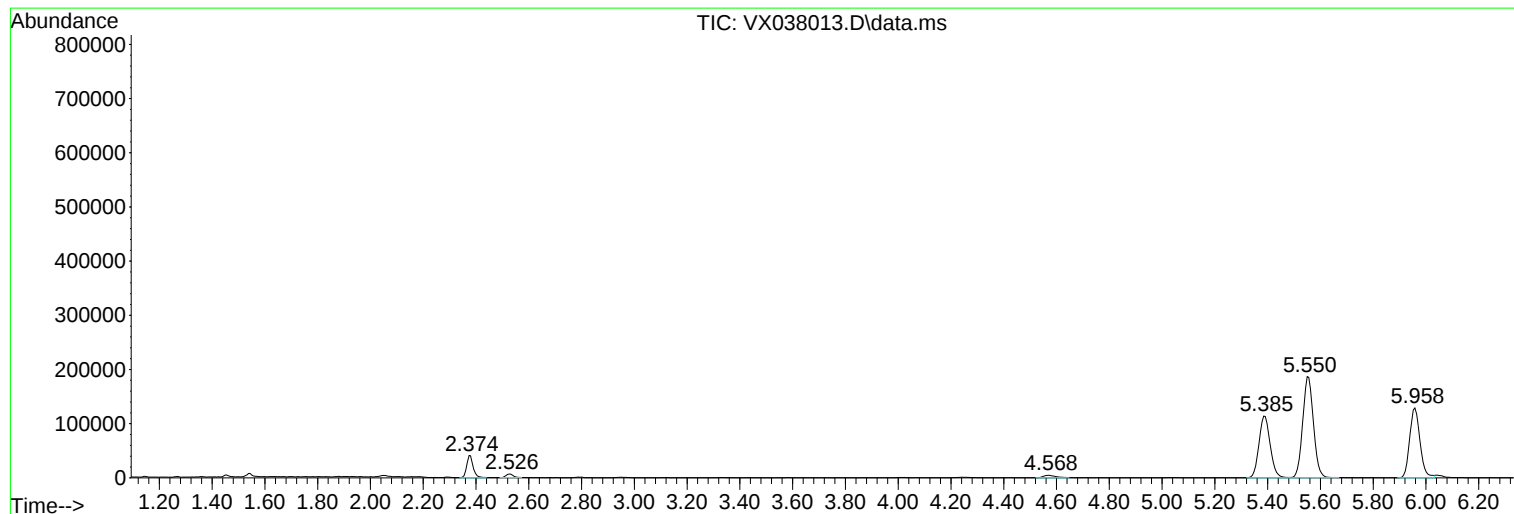

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038013.D
Acq On : 30 Sep 2023 18:45
Operator : JC/MD
Sample : 04639-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093023\
Data File : VX038013.D
Acq On : 30 Sep 2023 18:45
Operator : JC/MD
Sample : 04639-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------