

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100118\
 Data File : VX004864.D
 Acq On : 01 Oct 2018 12:21
 Operator : JC/MD
 Sample : J5135-21
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB03-20180926

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	66	76	79	rBV4	10400	24476	1.78%	0.340%
2	2.446	207	212	220	rBV	11841	19669	1.43%	0.273%
3	2.617	234	240	250	rVB	77829	142717	10.35%	1.980%
4	3.019	298	306	314	rBV	20980	49431	3.59%	0.686%
5	4.763	581	592	603	rBV2	8834	29839	2.16%	0.414%
6	5.500	702	713	728	rBV	169657	482178	34.98%	6.689%
7	5.665	728	740	760	rBV	209607	611888	44.39%	8.489%
8	6.067	795	806	822	rBV	182806	475358	34.48%	6.594%
9	6.860	926	936	971	rBV	335054	857919	62.24%	11.902%
10	8.719	1233	1241	1263	rBV	791994	1378513	100.00%	19.124%
11	10.116	1463	1470	1489	rBV	736043	1048928	76.09%	14.551%
12	11.140	1632	1638	1652	rBV	748226	949808	68.90%	13.176%
13	12.079	1786	1792	1804	rVB	937389	1137690	82.53%	15.783%


Sum of corrected areas: 7208414

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100118\
Data File : VX004864.D
Acq On : 01 Oct 2018 12:21
Operator : JC/MD
Sample : J5135-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB03-20180926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

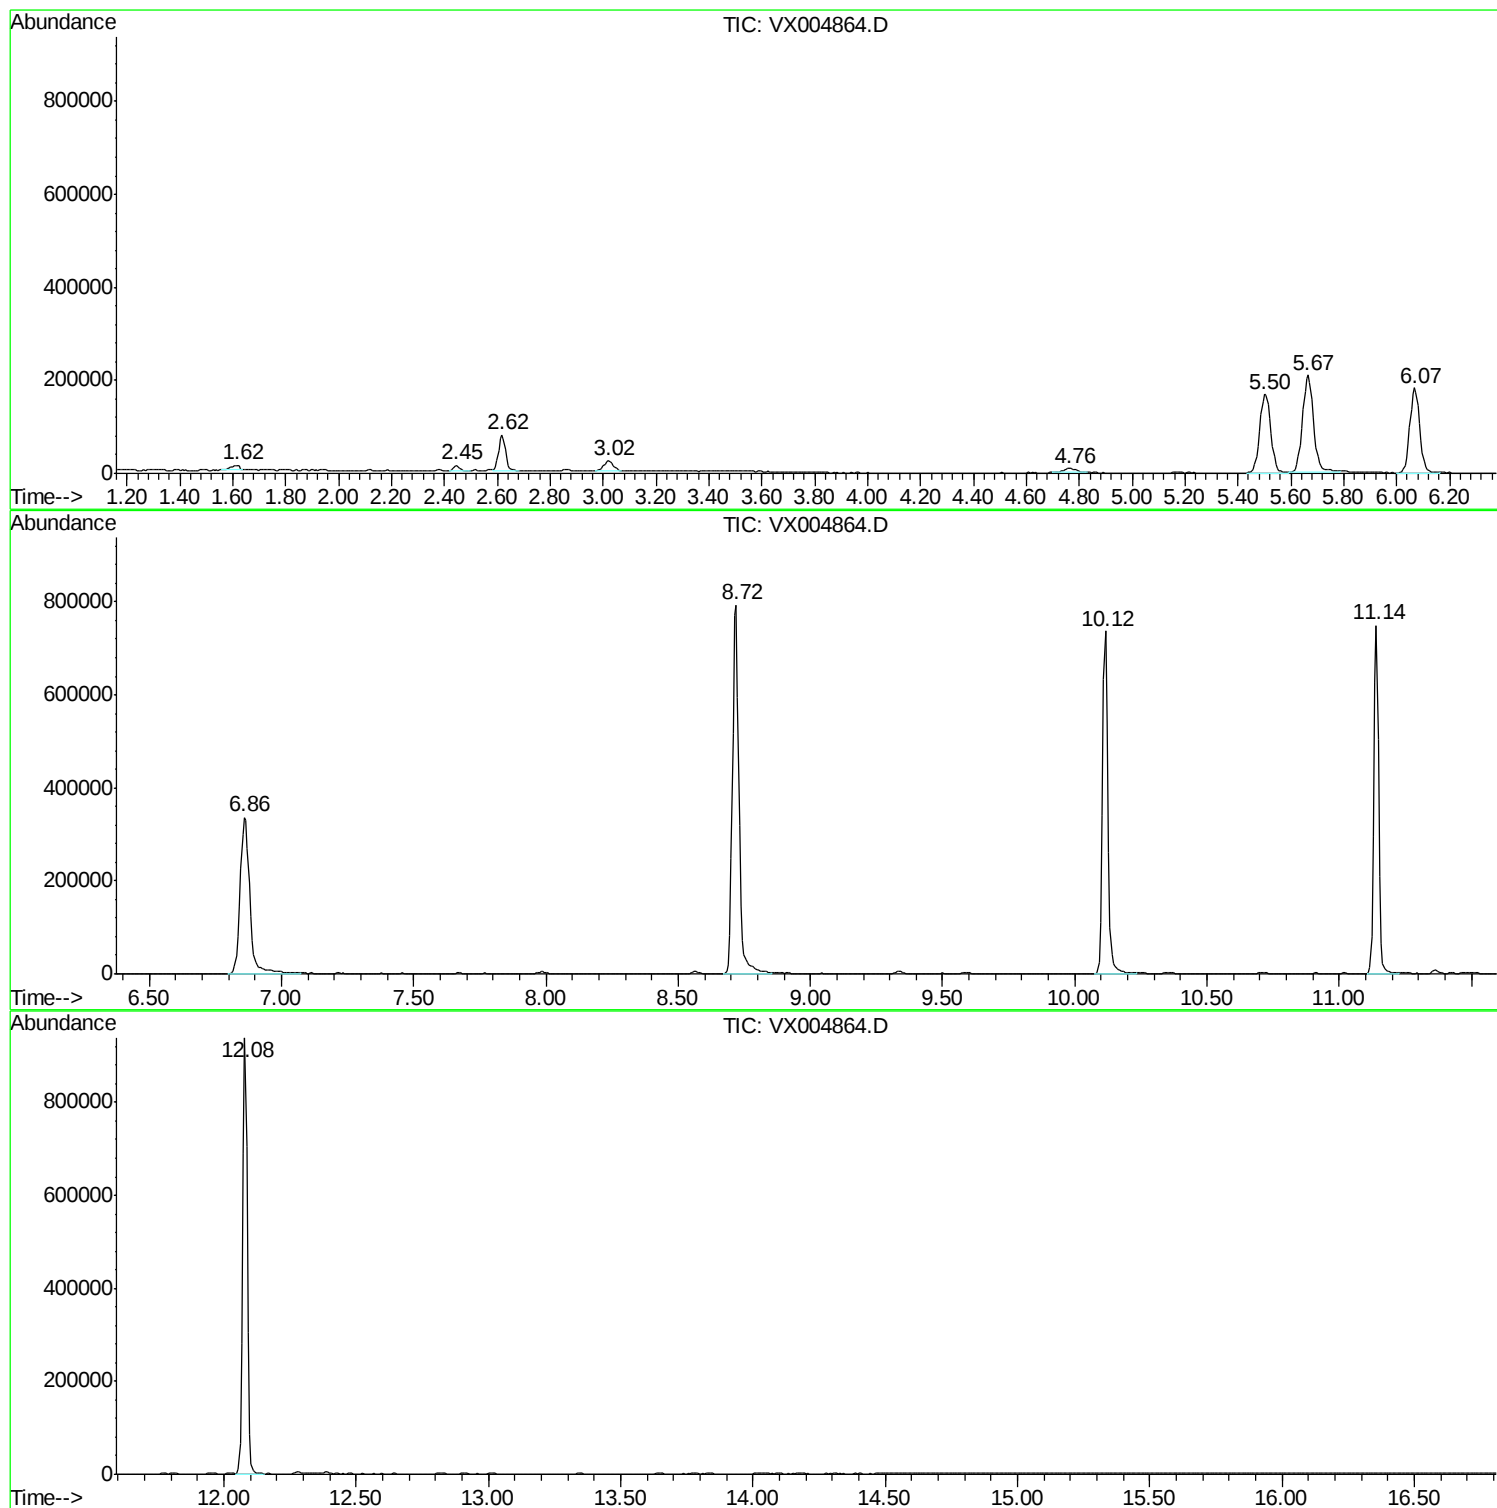

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100118\
Data File : VX004864.D
Acq On : 01 Oct 2018 12:21
Operator : JC/MD
Sample : J5135-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB03-20180926










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.62	11.66 ug/l	142717	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4		Methoxyacetyl chloride	108	C3H5ClO2	038870-89-2	4
5		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4

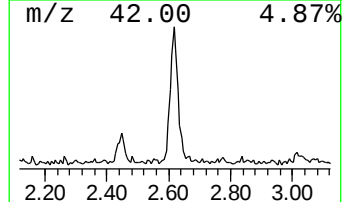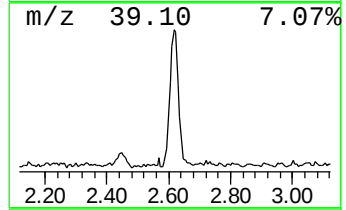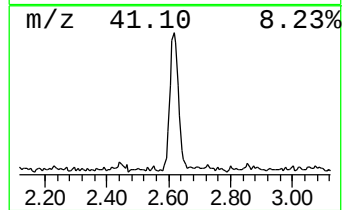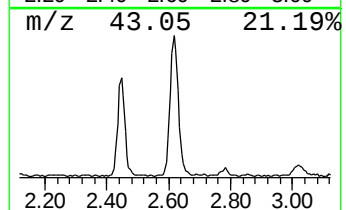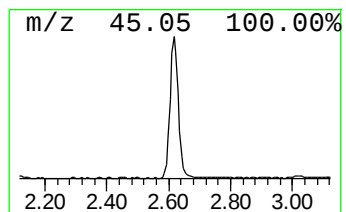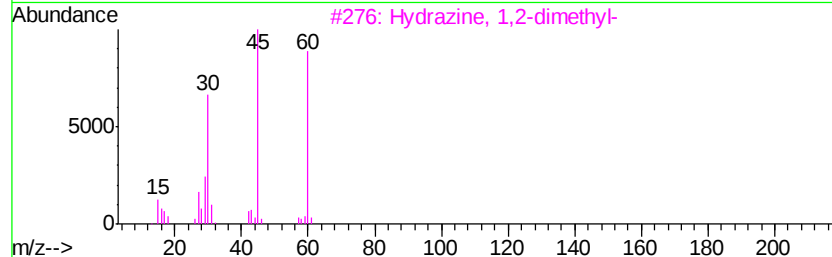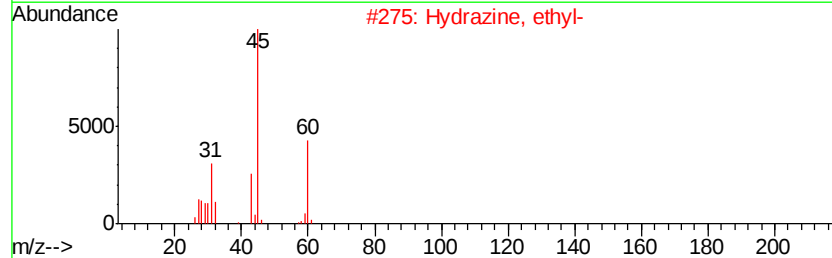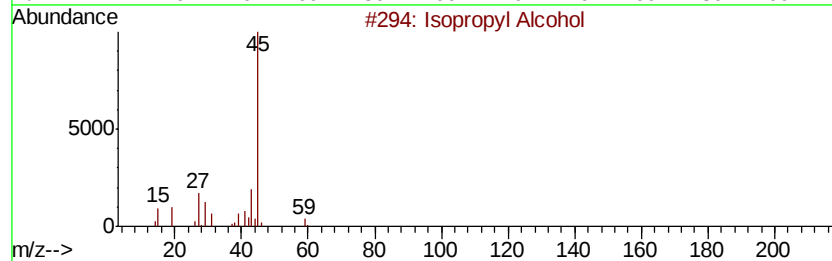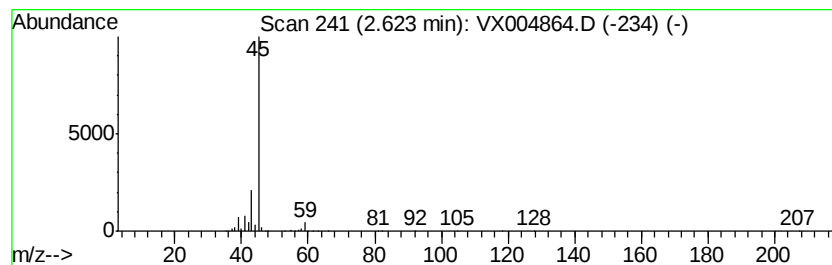

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100118\
Data File : VX004864.D
Acq On : 01 Oct 2018 12:21
Operator : JC/MD
Sample : J5135-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB03-20180926

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.62	11.7	ug/l	142717	1	5.67	611888	50.0