

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100118\
 Data File : VX004877.D
 Acq On : 01 Oct 2018 18:09
 Operator : JC/MD
 Sample : J5135-17
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-TW508-2327

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.611	67	75	78	rBV5	9694	18329	1.40%	0.271%
2	2.617	235	240	248	rVB	54577	98508	7.50%	1.456%
3	3.696	409	417	427	rVB	9711	28084	2.14%	0.415%
4	5.500	701	713	725	rBV	164884	471436	35.89%	6.968%
5	5.665	729	740	752	rBV	198915	572102	43.56%	8.455%
6	6.067	795	806	821	rBV	176500	459436	34.98%	6.790%
7	6.860	926	936	954	rBV	320862	802602	61.11%	11.862%
8	8.719	1233	1241	1257	rBV	767269	1313455	100.00%	19.412%
9	10.116	1464	1470	1490	rBV	708446	998008	75.98%	14.750%
10	11.140	1632	1638	1651	rBV	705470	892751	67.97%	13.194%
11	12.079	1786	1792	1800	rBV	877850	1072471	81.65%	15.851%
12	12.755	1899	1903	1910	rVB3	11218	16905	1.29%	0.250%
13	13.645	2044	2049	2053	rBV	17924	22002	1.68%	0.325%


Sum of corrected areas: 6766089

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100118\
Data File : VX004877.D
Acq On : 01 Oct 2018 18:09
Operator : JC/MD
Sample : J5135-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-TW508-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

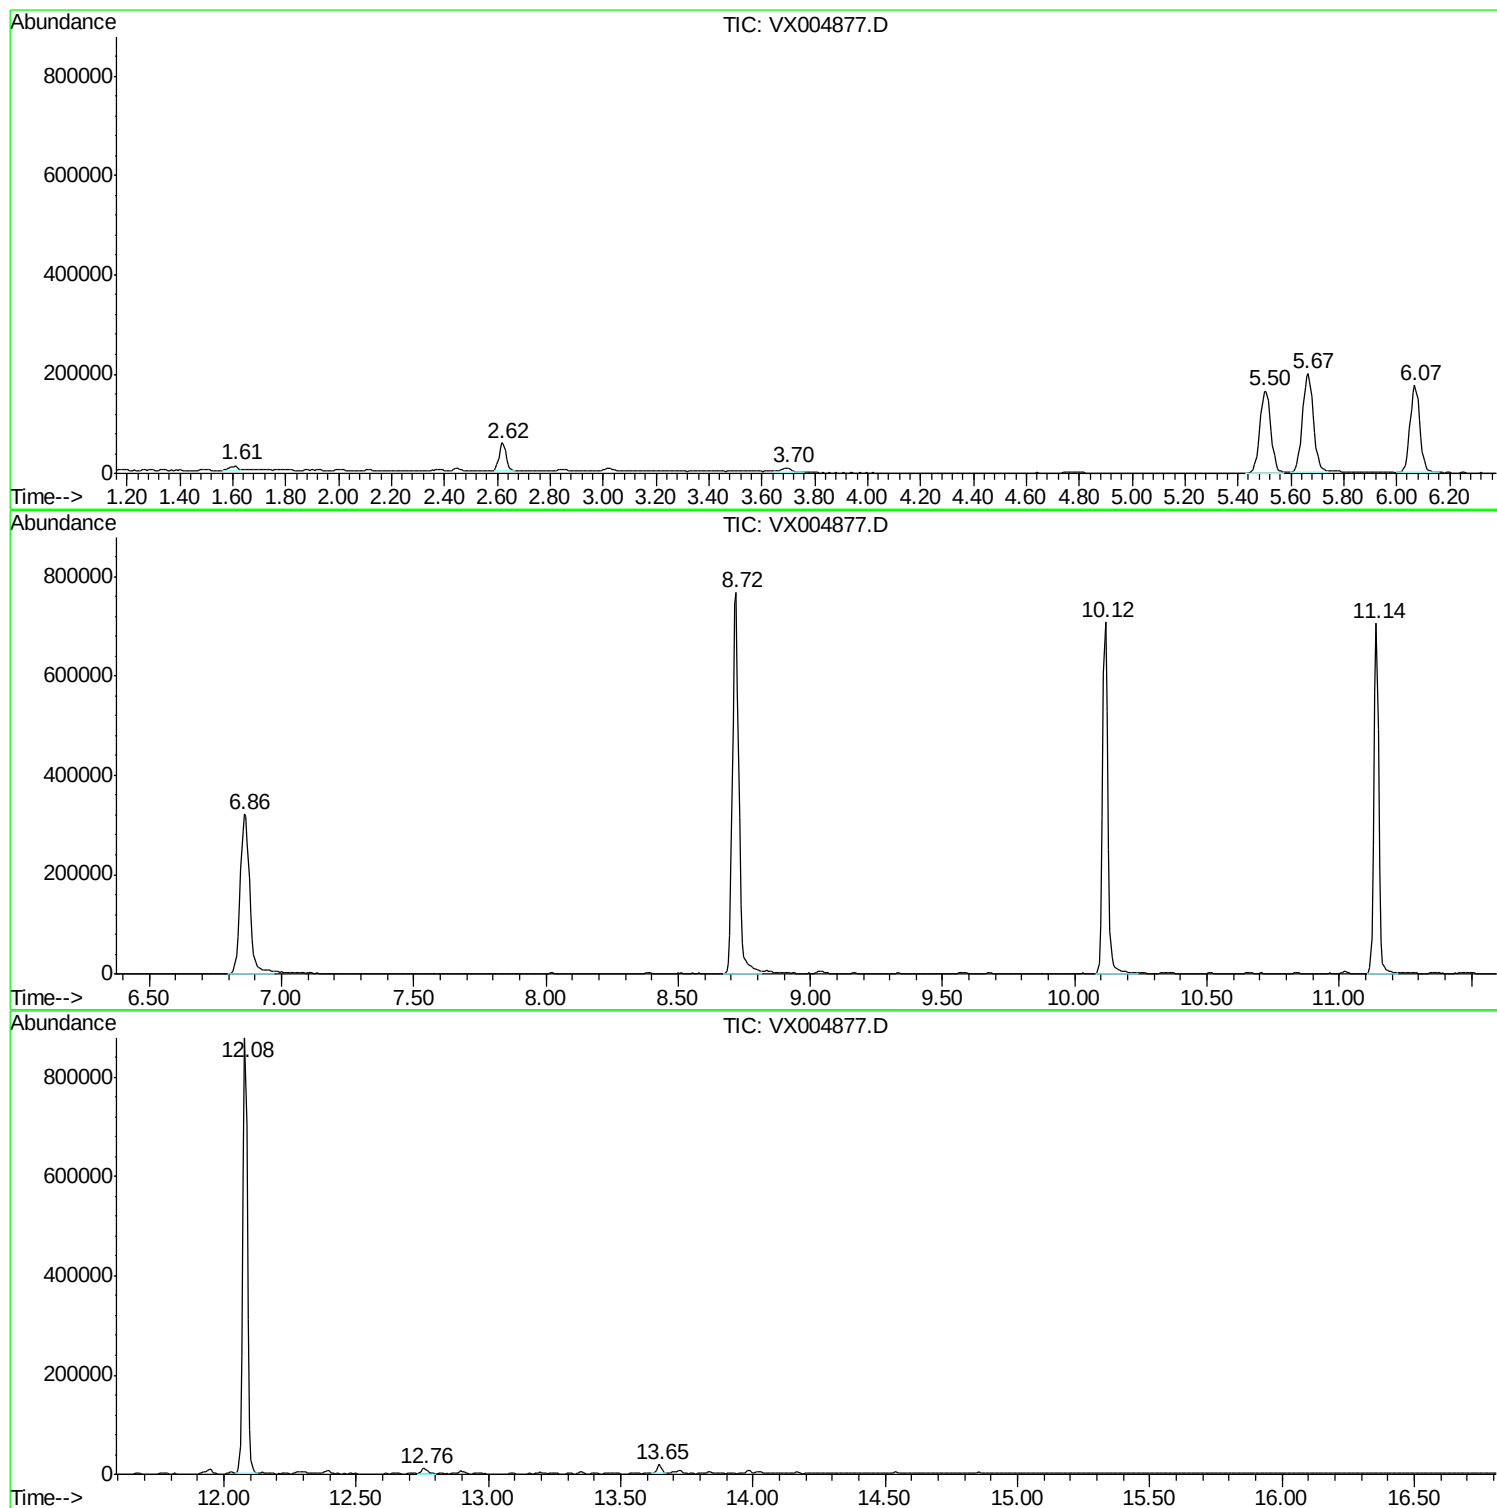

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100118\
Data File : VX004877.D
Acq On : 01 Oct 2018 18:09
Operator : JC/MD
Sample : J5135-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
SA-TW508-2327










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.62	8.61 ug/l	98508	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		Ethylamine	45	C2H7N	000075-04-7	7
4		Formamide	45	CH3NO	000075-12-7	4
5		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	4

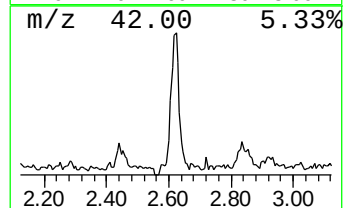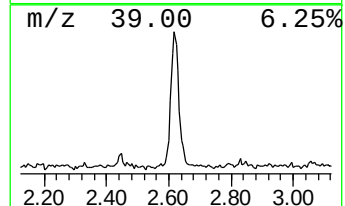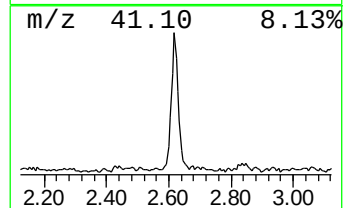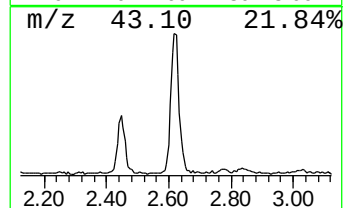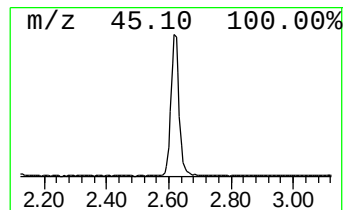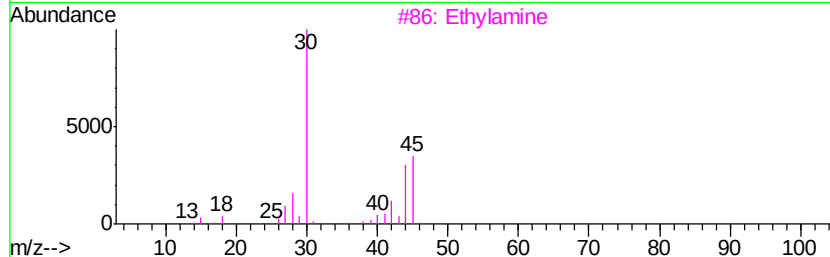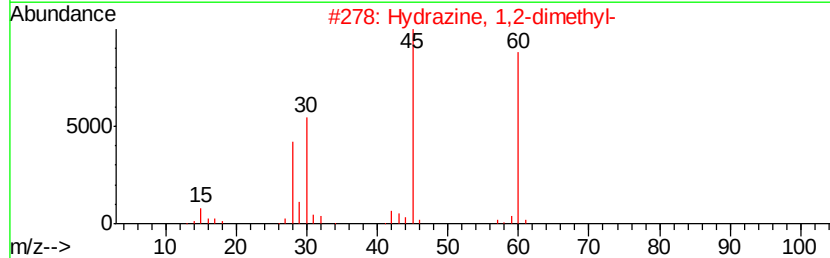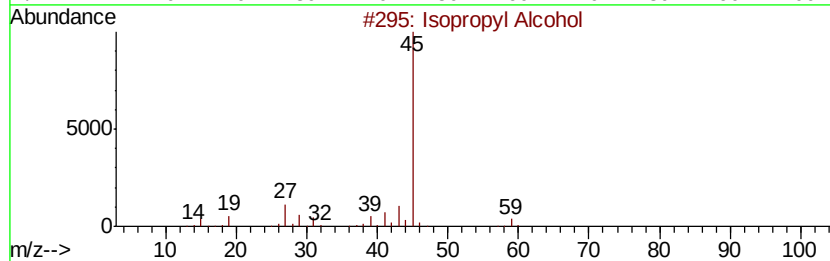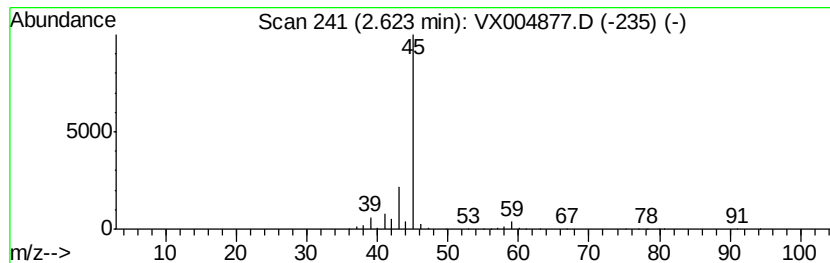

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100118\
Data File : VX004877.D
Acq On : 01 Oct 2018 18:09
Operator : JC/MD
Sample : J5135-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-TW508-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.62	8.6	ug/l	98508	1	5.67	572102	50.0