

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012728.D
Acq On : 01 Oct 2019 13:17
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	378125	474428	52.56%	9.209%
2	1.265	58	62	69	rBV	28144	36882	4.09%	0.716%
3	2.436	247	254	261	rBV	8487	14784	1.64%	0.287%
4	2.594	271	280	289	rBV	53824	99087	10.98%	1.923%
5	5.490	742	755	770	rBV2	99360	283781	31.44%	5.509%
6	5.648	770	781	795	rBV	181213	508536	56.33%	9.871%
7	6.051	836	847	863	rBV2	119538	316395	35.05%	6.142%
8	6.849	968	978	992	rBV	285370	673524	74.61%	13.074%
9	8.709	1273	1283	1301	rBV	563560	902720	100.00%	17.523%
10	10.111	1507	1513	1527	rBV	522105	741168	82.10%	14.387%
11	11.135	1675	1681	1694	rBV	406936	514211	56.96%	9.982%
12	12.074	1830	1835	1846	rBV	468511	586081	64.92%	11.377%


Sum of corrected areas: 5151597

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012728.D
Acq On : 01 Oct 2019 13:17
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

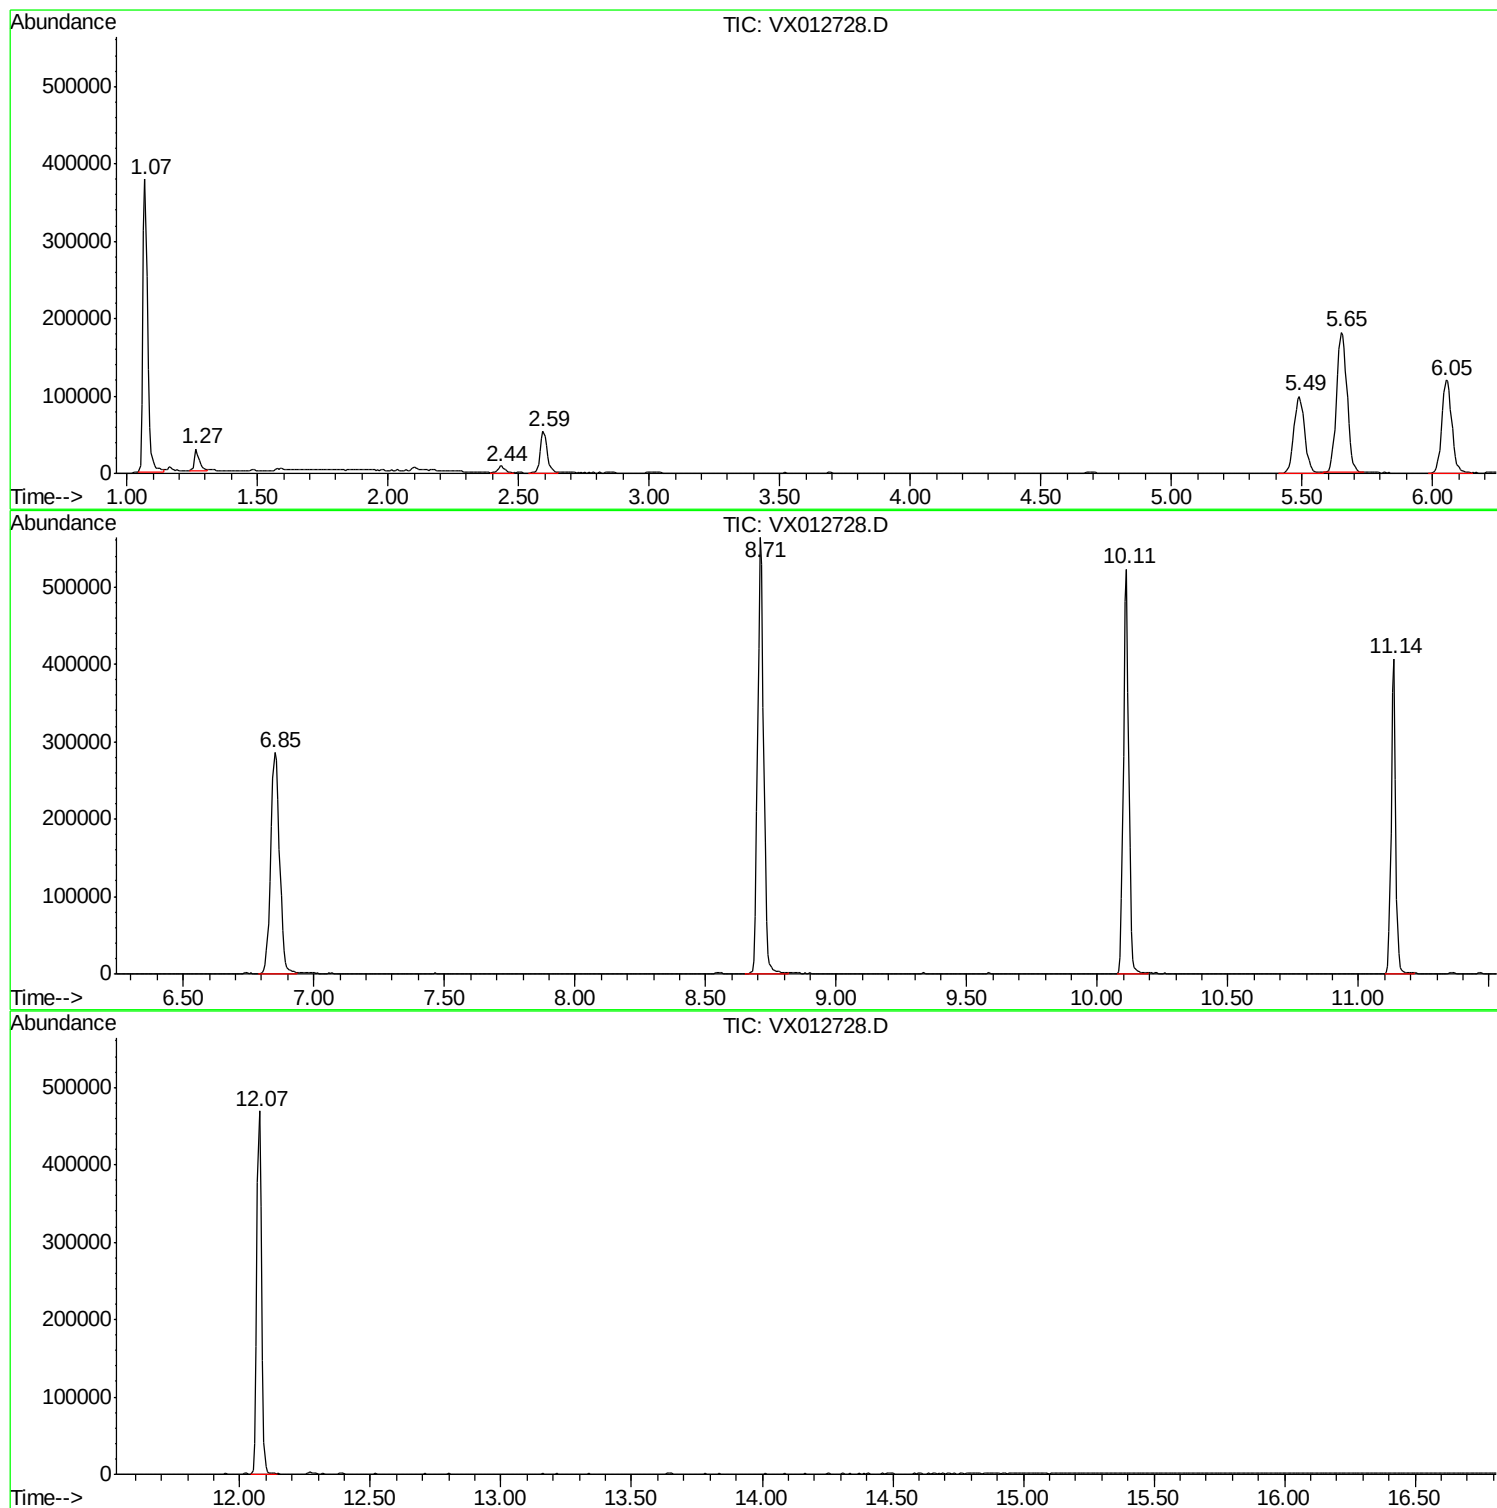

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012728.D
Acq On : 01 Oct 2019 13:17
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	9.74 ug/l	99087	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Formamide	45	CH3NO	000075-12-7	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

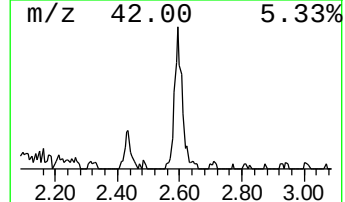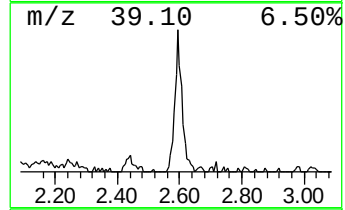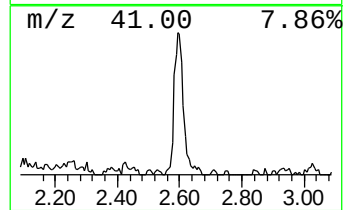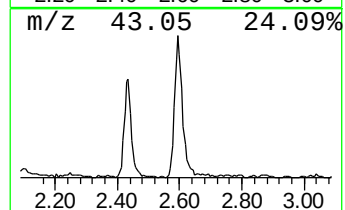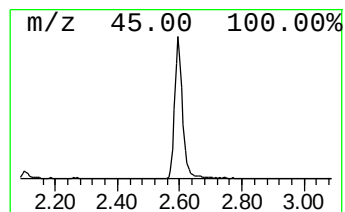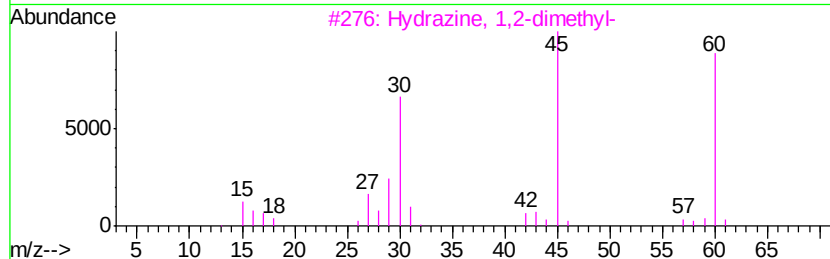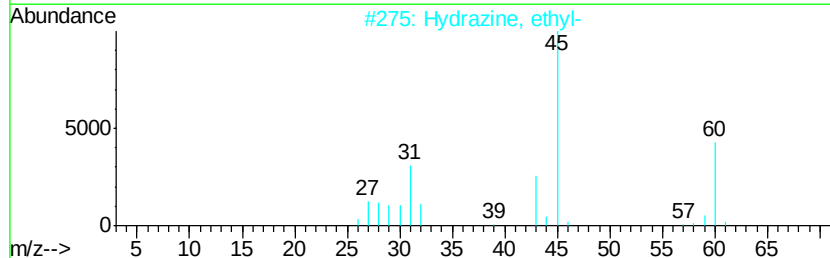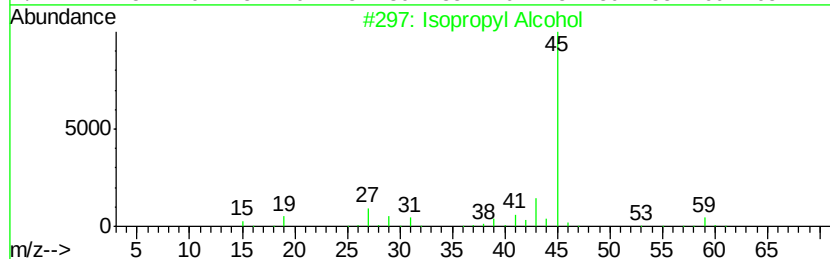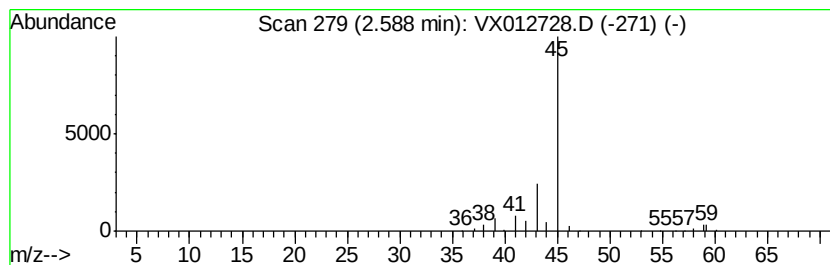

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100119\
Data File : VX012728.D
Acq On : 01 Oct 2019 13:17
Operator : JC/SP
Sample : K5081-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ122I-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	9.7	ug/l	99087	1	5.65	508536	50.0