

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100119\
 Data File : VX012730.D
 Acq On : 01 Oct 2019 14:04
 Operator : JC/SP
 Sample : K5081-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ183I-20190925

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	409949	514242	57.45%	9.979%
2	1.265	58	62	69	rBV	28567	38953	4.35%	0.756%
3	2.436	248	254	262	rBV	10210	17440	1.95%	0.338%
4	2.594	272	280	293	rBV	88220	164576	18.39%	3.194%
5	5.490	742	755	770	rBV2	97289	280881	31.38%	5.450%
6	5.655	770	782	795	rBV	180625	510129	56.99%	9.899%
7	6.051	837	847	859	rBV	116970	310901	34.73%	6.033%
8	6.849	968	978	991	rBV	280075	673035	75.19%	13.060%
9	8.709	1276	1283	1296	rBV	557356	895078	100.00%	17.369%
10	10.111	1507	1513	1525	rBV	517746	724380	80.93%	14.057%
11	11.135	1675	1681	1693	rBV	375862	489595	54.70%	9.501%
12	12.074	1830	1835	1845	rBV	437738	534117	59.67%	10.365%


Sum of corrected areas: 5153327

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012730.D
Acq On : 01 Oct 2019 14:04
Operator : JC/SP
Sample : K5081-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ183I-20190925

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

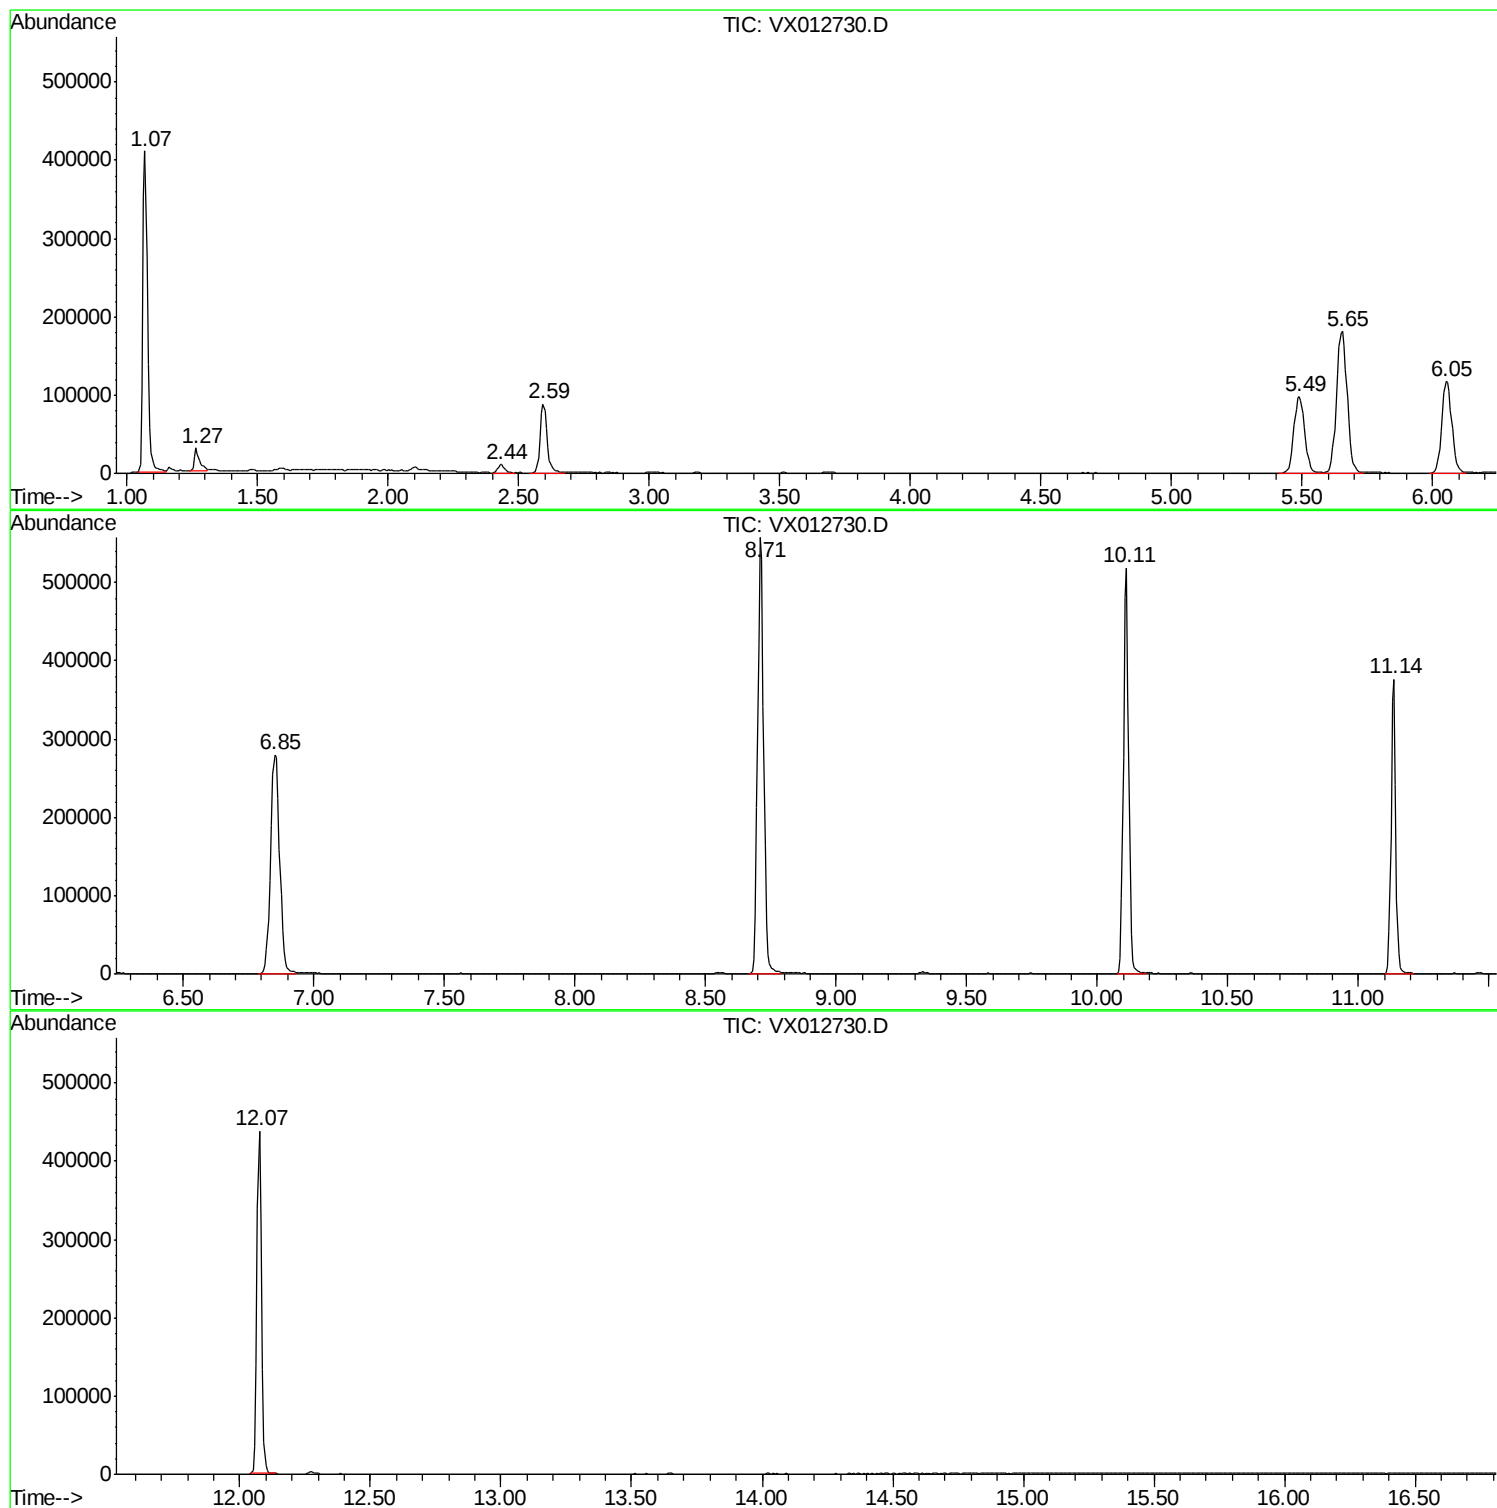

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012730.D
Acq On : 01 Oct 2019 14:04
Operator : JC/SP
Sample : K5081-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ183I-20190925










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	16.13 ug/l	164576	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4
4		Formamide	45	CH3NO	000075-12-7	4
5		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	4

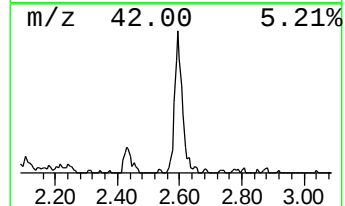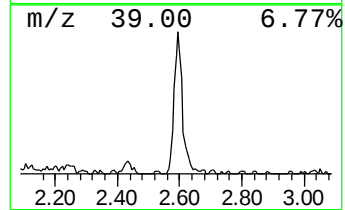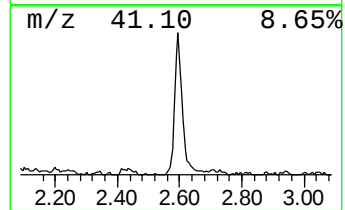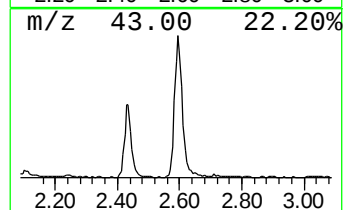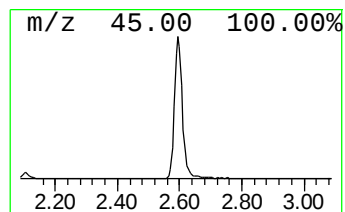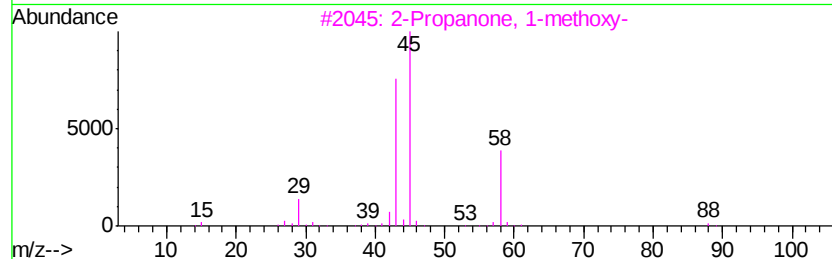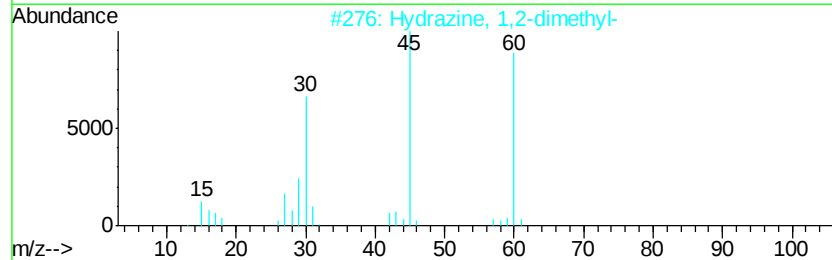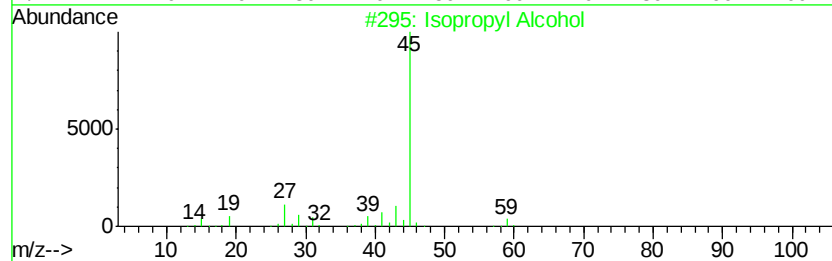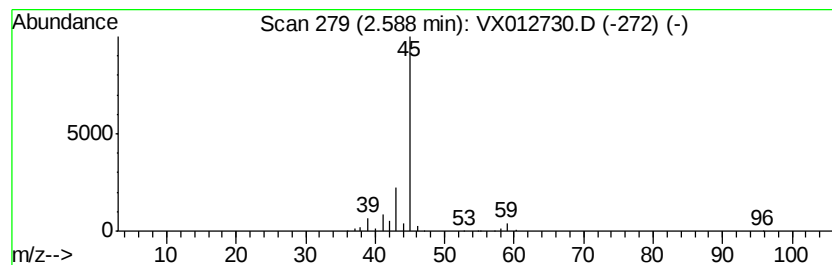

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100119\
Data File : VX012730.D
Acq On : 01 Oct 2019 14:04
Operator : JC/SP
Sample : K5081-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ183I-20190925

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	16.1	ug/l	164576	1	5.65	510129	50.0