

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100119\
 Data File : VX012736.D
 Acq On : 01 Oct 2019 16:25
 Operator : JC/SP
 Sample : K5082-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-DUP05-20190926

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	352772	442655	51.01%	8.886%
2	1.265	58	62	67	rBV	27773	36068	4.16%	0.724%
3	1.320	67	71	76	rBV2	10036	23329	2.69%	0.468%
4	2.435	249	254	261	rVB	7716	12792	1.47%	0.257%
5	2.594	270	280	295	rBV	86497	160713	18.52%	3.226%
6	5.490	744	755	768	rBV	99726	278577	32.10%	5.592%
7	5.654	770	782	800	rVV	177929	499340	57.54%	10.024%
8	6.057	838	848	864	rBV	117510	311772	35.93%	6.259%
9	6.849	969	978	990	rBV	273785	654963	75.47%	13.148%
10	8.709	1277	1283	1299	rBV	529892	867827	100.00%	17.421%
11	10.111	1507	1513	1531	rBV	504785	701295	80.81%	14.078%
12	11.135	1675	1681	1691	rBV	356724	468951	54.04%	9.414%
13	12.074	1829	1835	1850	rVB	426274	523093	60.28%	10.501%


Sum of corrected areas: 4981375

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012736.D
Acq On : 01 Oct 2019 16:25
Operator : JC/SP
Sample : K5082-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-DUP05-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

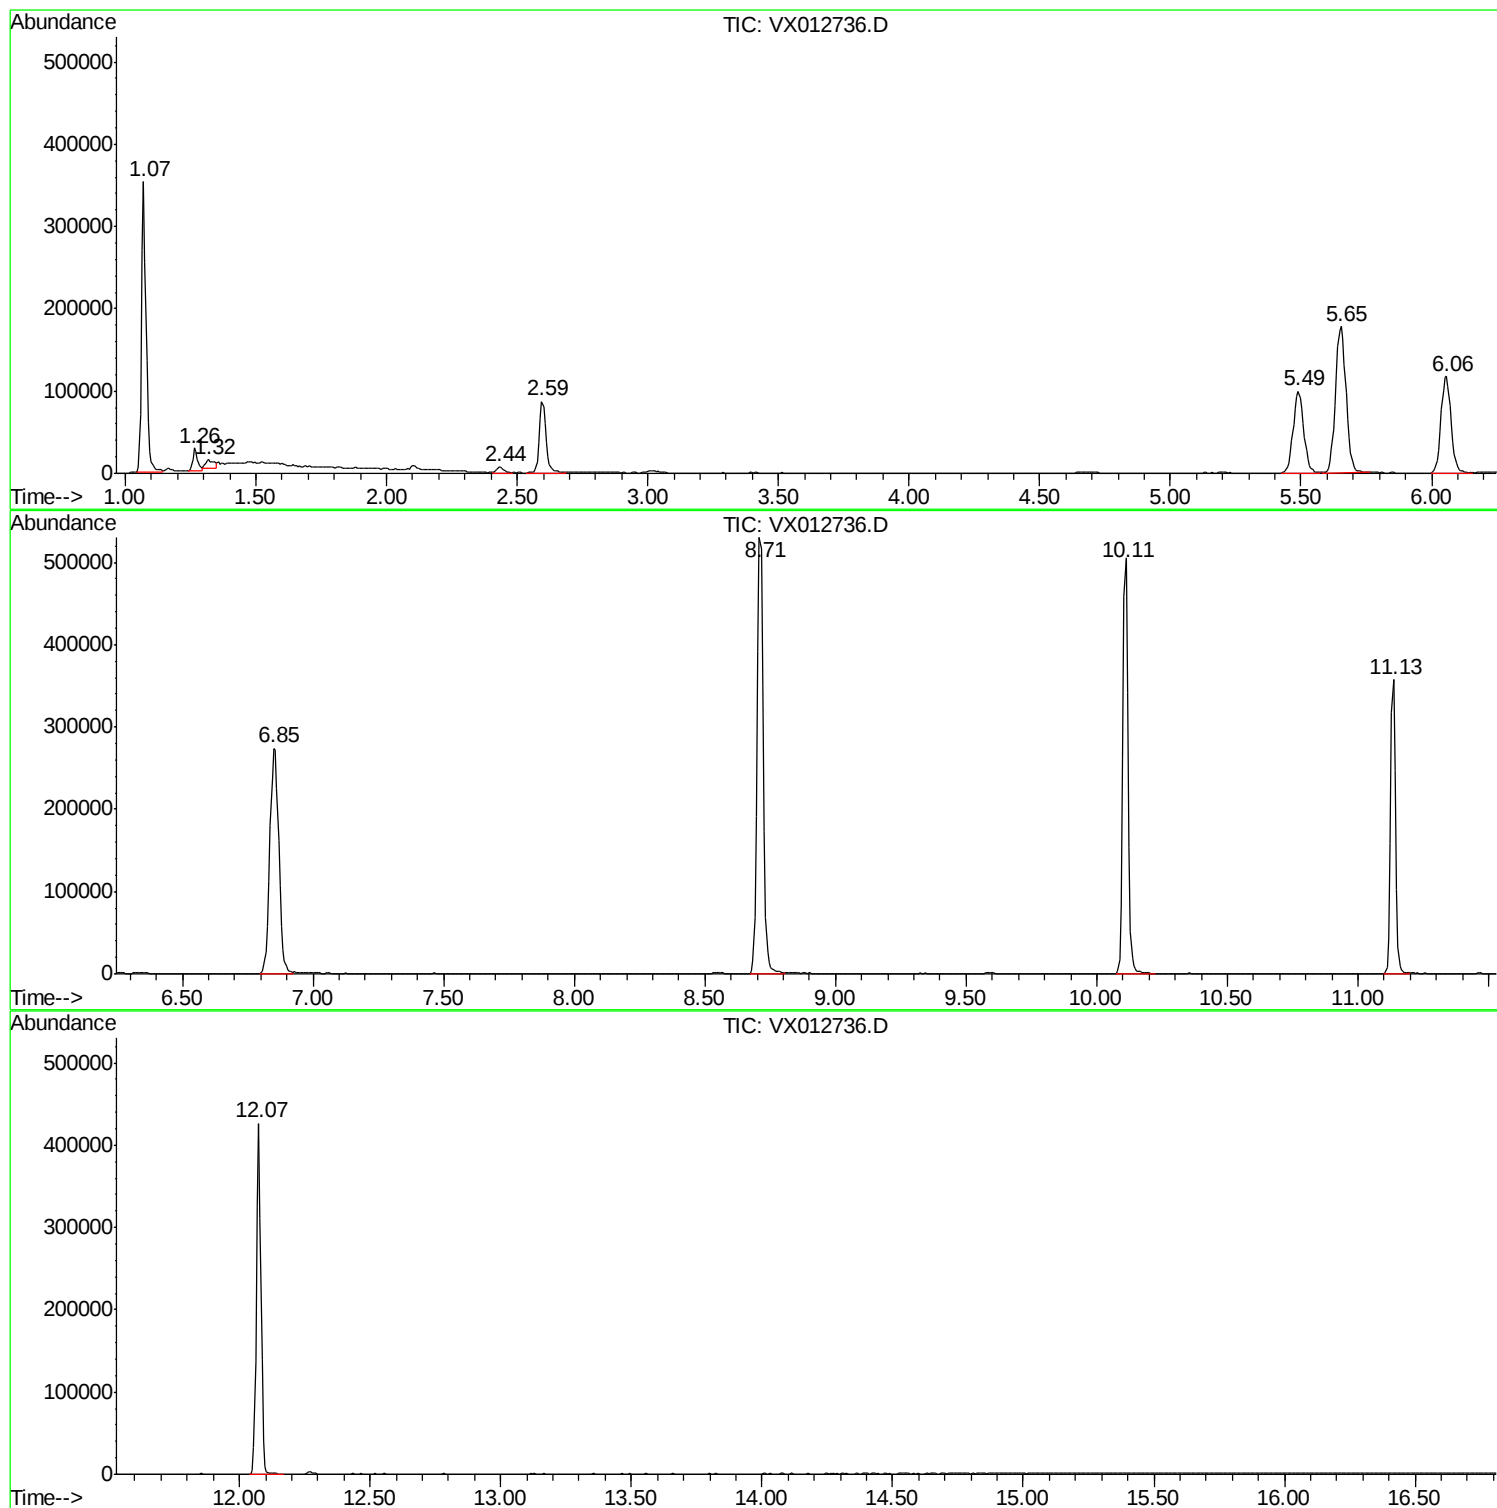

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100119\
Data File : VX012736.D
Acq On : 01 Oct 2019 16:25
Operator : JC/SP
Sample : K5082-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-DUP05-20190926










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	16.09 ug/l	160713	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2		Propylene Glycol	76	C3H8O2	000057-55-6	9
3		2-Pentanol	88	C5H12O	006032-29-7	9
4		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5		(R)-(-)-2-Pentanol	88	C5H12O	031087-44-2	9

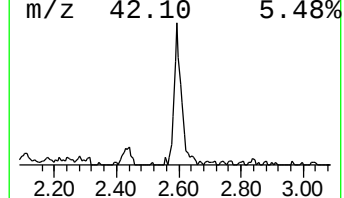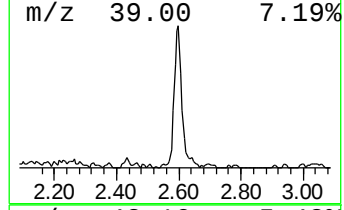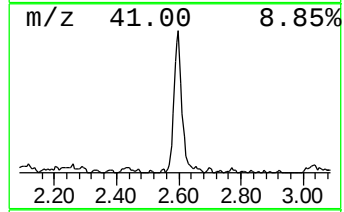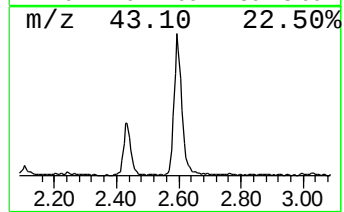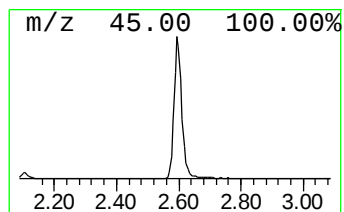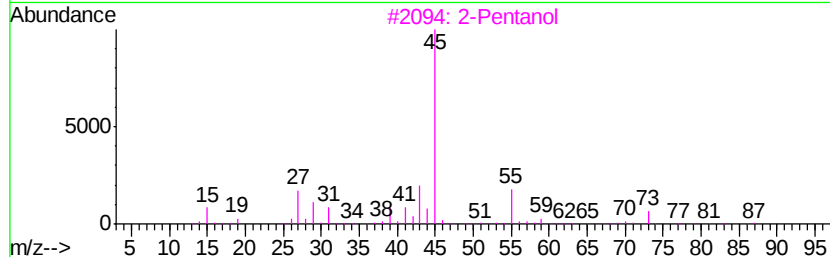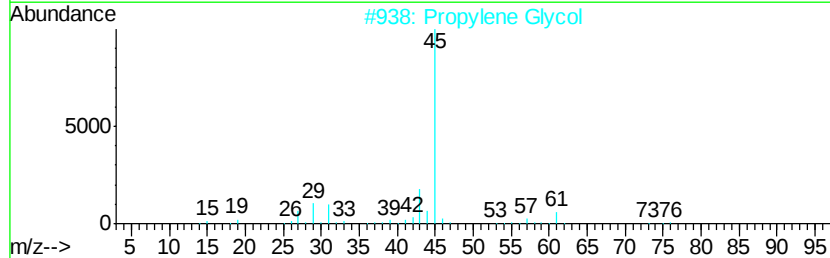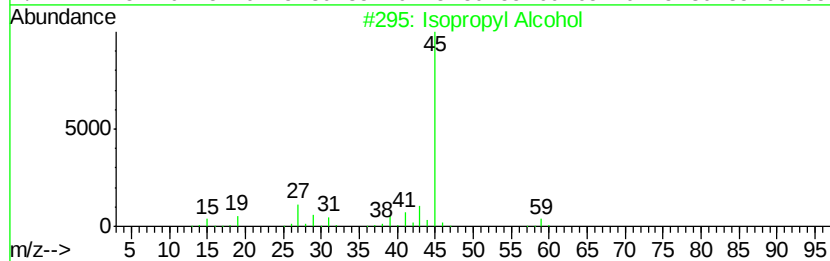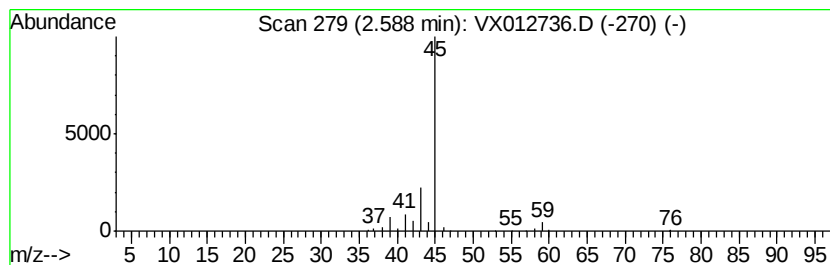

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100119\
Data File : VX012736.D
Acq On : 01 Oct 2019 16:25
Operator : JC/SP
Sample : K5082-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-DUP05-20190926

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	16.1	ug/l	160713	1	5.65	499340	50.0