

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100120\
 Data File : VX018732.D
 Acq On : 01 Oct 2020 19:40
 Operator : JC/SP
 Sample : L4135-21
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK01

Quant Time: Oct 02 09:14:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 08:54:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	183739	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	183640	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	86799	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	71095	7.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	147.80%#
7) Chloroethane-d5	1.70	69	55457	6.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	136.80%#
11) 1,1-Dichloroethene-d2	2.34	63	121743	5.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	114.60%
20) 2-Butanone-d5	4.57	46	179160	73.07	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	146.14%#
24) Chloroform-d	5.14	84	150324	6.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	132.00%#
26) 1,2-Dichloroethane-d4	6.03	65	94352	7.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	142.20%#
32) Benzene-d6	6.05	84	269869	6.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.40%#
36) 1,2-Dichloropropane-d6	7.37	67	78296	6.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	121.20%
41) Toluene-d8	8.70	98	247211	5.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.20%
45) trans-1,3-Dichloropropene-	8.99	79	38486	6.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	134.00%#
48) 2-Hexanone-d5	9.43	63	141746	68.90	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	137.80%#
59) 1,1,2,2-Tetrachloroethane-	11.23	84	60548	6.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	126.00%#
65) 1,2-Dichlorobenzene-d4	12.36	152	97784	6.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	137.80%#


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	4892	0.399 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100120\
Data File : VX018732.D
Acq On : 01 Oct 2020 19:40
Operator : JC/SP
Sample : L4135-21
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK01

Quant Time: Oct 02 09:14:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 08:54:14 2020
Response via : Initial Calibration

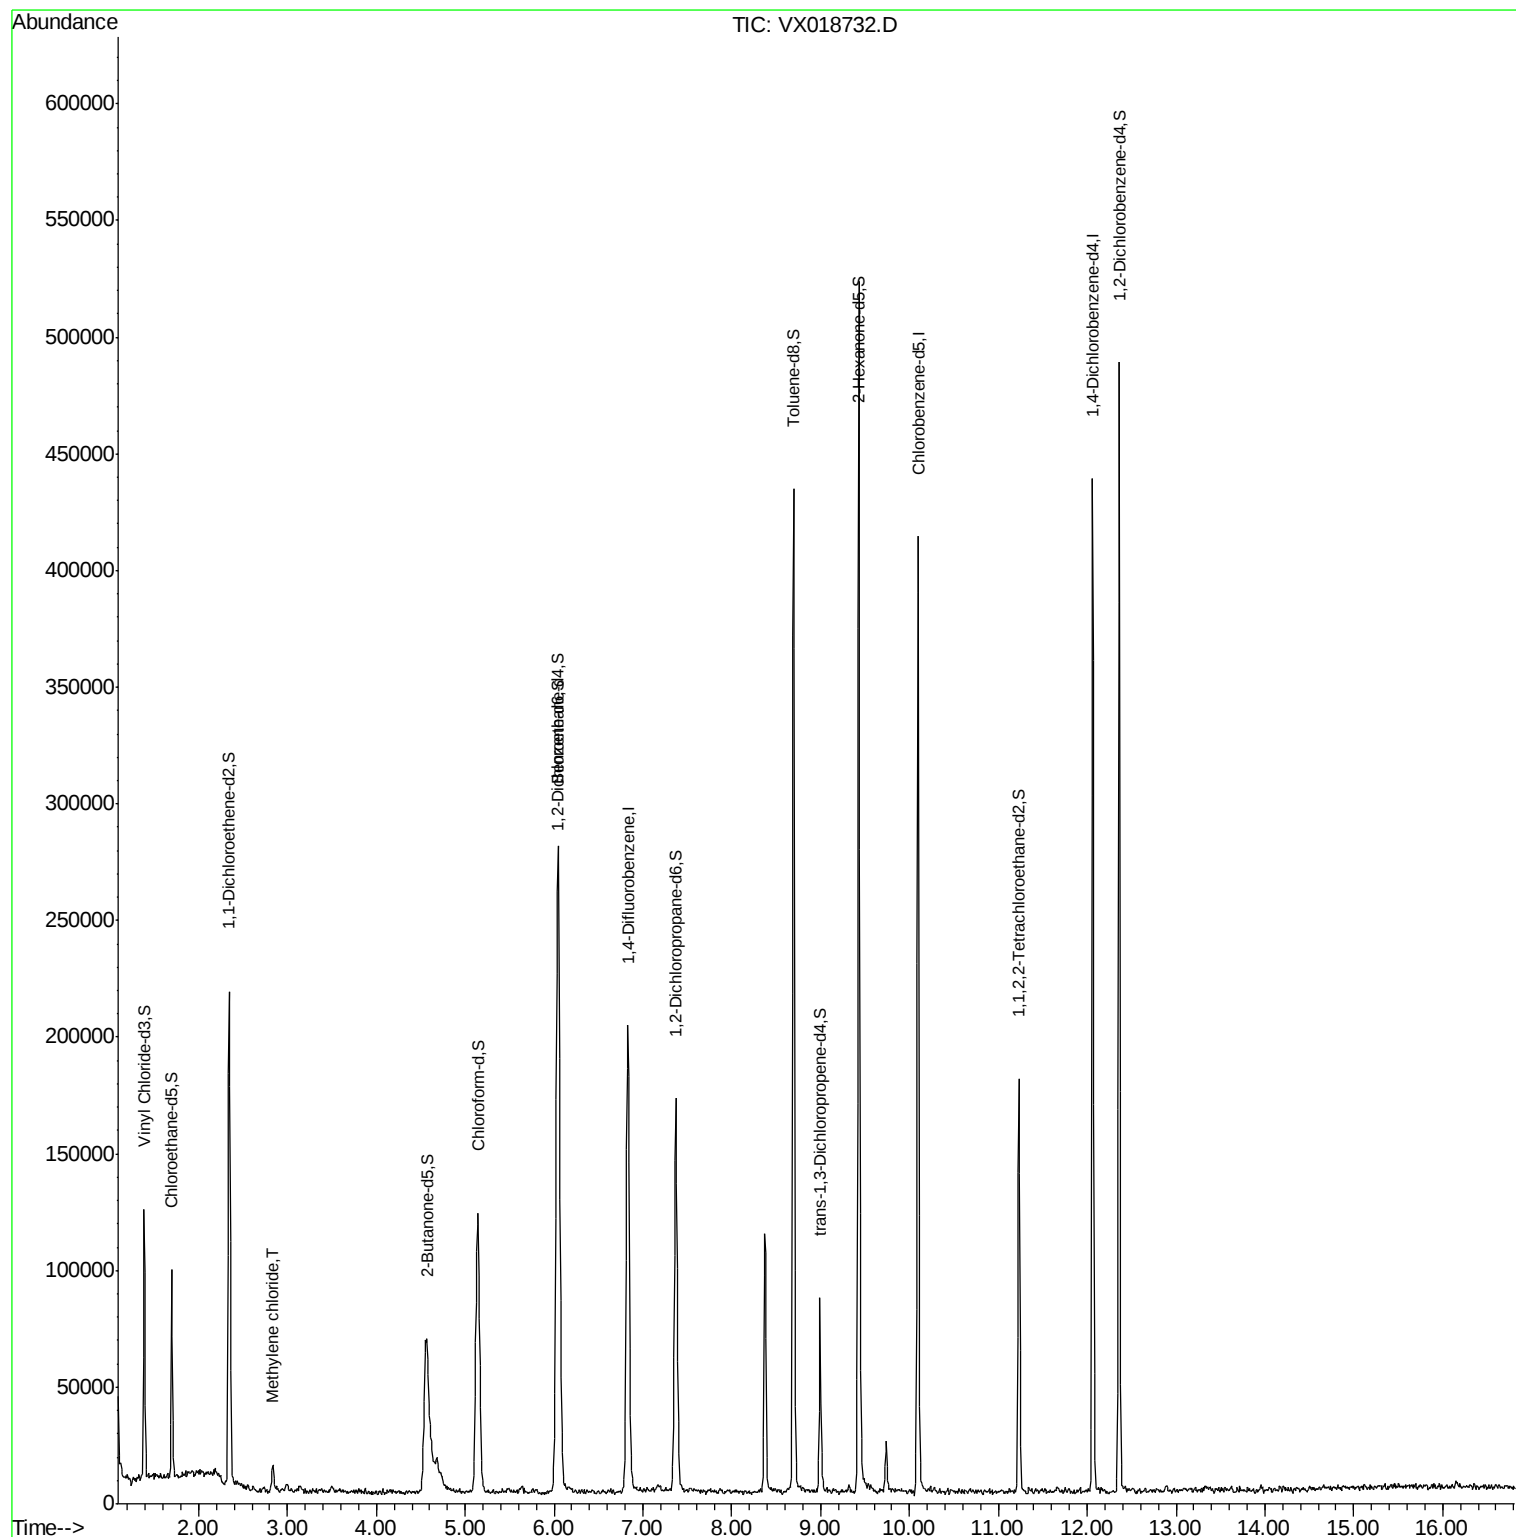

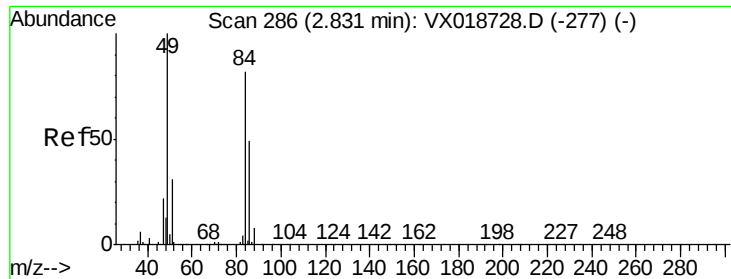

#16
 Methvlene chloride
 Concen: 0.399 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. 0.00 min
 Lab File: VX018732.D
 Acq: 01 Oct 2020 19:40

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 4892
 Ion Ratio Lower Upper
 84 100
 86 53.8 41.9 77.7
 49 135.2 80.8 150.2

