


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100120\
 Data File : VX018726.D
 Acq On : 01 Oct 2020 13:21
 Operator : JC/SP
 Sample : BFB75
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR092820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 02 08:54:14 2020

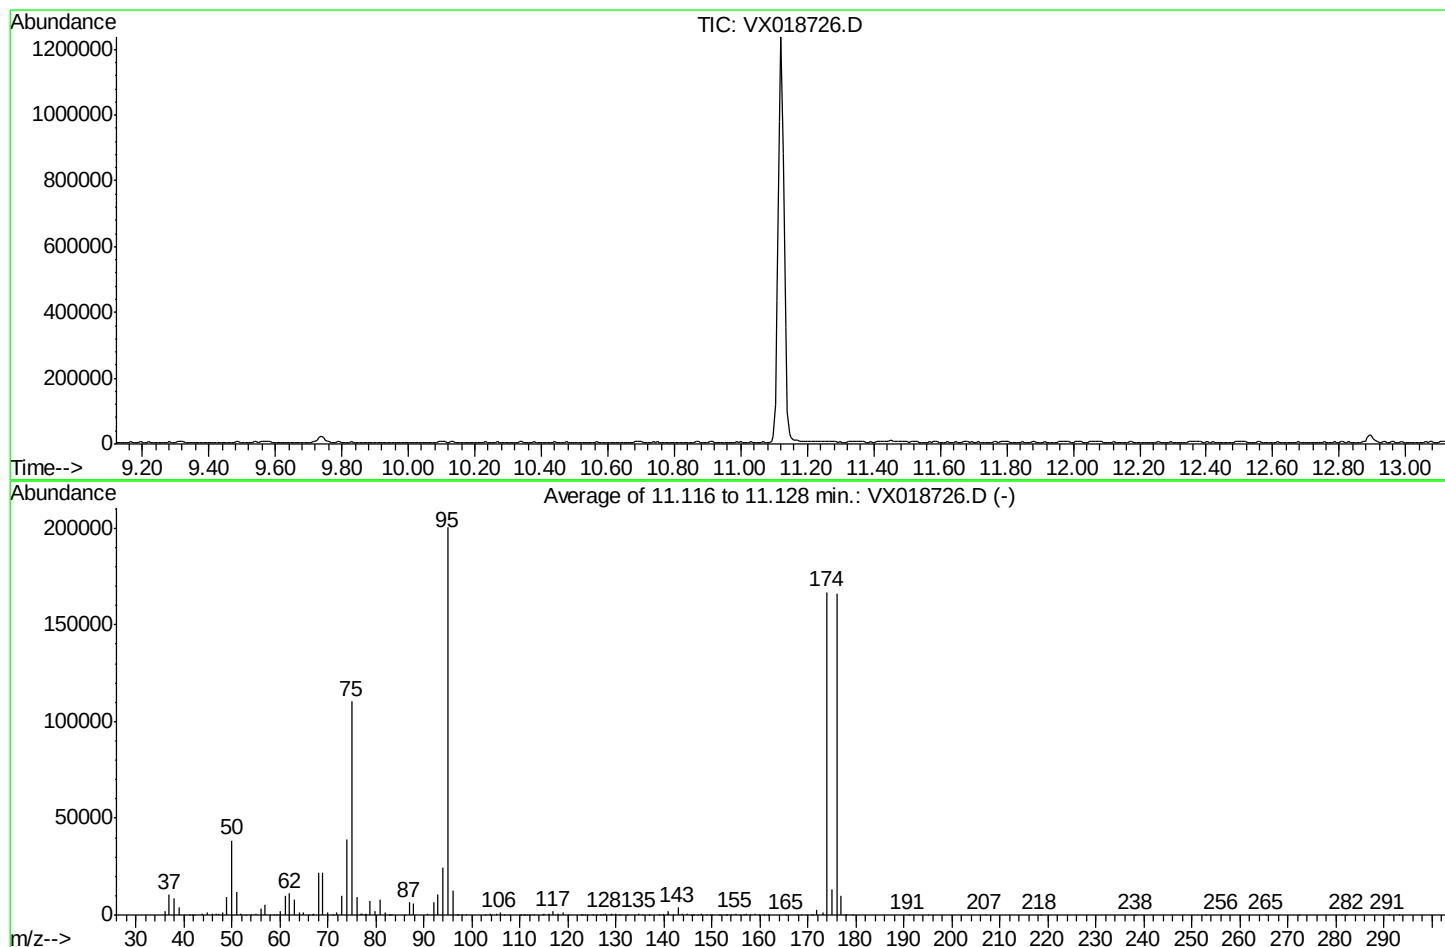

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	38641	PASS
75	95	30	80	55.0	110301	PASS
95	95	100	100	100.0	200426	PASS
96	95	5	9	6.2	12512	PASS
173	174	0.00	2	0.6	1066	PASS
174	95	50	120	83.3	166890	PASS
175	174	5	9	7.9	13248	PASS
176	174	95	101	99.6	166165	PASS
177	176	5	9	6.1	10209	PASS

m/z	Abundance
35.90	2173.0
37.00	11878.0
38.00	9436.0
39.00	4667.0
40.30	460.0
41.00	236.0
41.60	152.0
42.10	238.0
43.00	162.0
43.90	1242.0
45.00	1671.0
45.90	179.0
46.90	2161.0
48.00	1364.0
49.00	8863.0
50.00	39024.0
51.00	12586.0
51.90	675.0
52.90	301.0
53.80	134.0
55.00	1034.0
56.10	2972.0
57.00	5101.0
58.00	523.0
58.80	82.0
60.10	1951.0
61.10	10142.0
62.00	12425.0
63.00	8163.0
64.00	1388.0
64.90	1518.0
66.00	214.0
67.10	702.0
68.00	22792.0
69.00	25136.0
70.00	1938.0
71.20	166.0
71.90	1413.0
73.00	10303.0
74.00	38672.0
75.00	111256.0
76.00	9393.0
77.00	1529.0
78.10	648.0
78.90	6758.0
79.90	2048.0
80.90	7303.0
81.90	1786.0
83.10	276.0
85.90	304.0
87.00	6317.0
88.00	6248.0
90.80	1032.0
92.00	6259.0
93.00	10024.0
94.00	24464.0
95.00	193088.0
96.00	11645.0
97.00	372.0
98.00	100.0
102.80	103.0
103.80	689.0
105.00	564.0
105.90	984.0
106.80	156.0
109.80	105.0
110.30	111.0
111.10	280.0
111.70	217.0
112.90	407.0
114.80	293.0
116.10	789.0
116.90	1877.0
118.00	1045.0
118.90	1136.0
120.00	165.0
122.80	119.0
124.10	278.0
125.30	125.0
125.90	156.0
127.80	845.0
128.80	205.0
129.20	242.0
129.80	784.0
130.80	227.0
134.90	827.0
135.60	108.0
136.80	608.0
139.70	141.0
140.80	2490.0
142.90	2935.0
143.90	565.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

145.00	866.0
145.60	270.0
146.20	252.0
147.10	177.0
148.10	361.0
148.90	123.0
149.80	180.0
152.00	92.0
152.90	104.0
153.80	183.0
155.10	872.0
157.10	319.0
159.00	360.0
161.00	207.0
169.90	131.0
170.90	384.0
172.00	2661.0
174.00	145216.0
175.00	11460.0
176.00	140480.0
177.00	9898.0
177.80	300.0
206.90	145.0
272.20	70.0
281.20	202.0
282.30	196.0
293.00	56.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

m/z	Abundance
35.30	143.0
36.00	2251.0
37.10	11149.0
38.00	10288.0
39.10	4444.0
40.20	353.0
41.10	142.0
41.80	199.0
42.30	232.0
43.10	162.0
44.00	1306.0
45.00	1963.0
45.90	758.0
47.20	1744.0
48.00	1565.0
49.10	11339.0
50.00	46816.0
51.00	13998.0
52.00	615.0
53.20	232.0
54.10	89.0
55.10	745.0
56.00	4420.0
57.00	7029.0
58.10	159.0
59.20	51.0
60.00	2656.0
61.00	12428.0
62.00	12653.0
63.00	10203.0
63.90	1526.0
64.90	2073.0
66.00	433.0
67.10	1151.0
68.00	25304.0
69.00	25472.0
70.10	1729.0
71.20	198.0
71.90	1284.0
73.00	11984.0
74.00	47160.0
75.00	134016.0
76.10	10964.0
77.20	1449.0
78.00	1071.0
79.00	9023.0
79.90	2225.0
81.00	9511.0
81.90	1974.0
82.80	143.0
83.30	176.0
87.00	8291.0
88.00	7284.0
90.90	1197.0
92.00	8825.0
93.00	12928.0
94.00	29800.0
95.00	238656.0
96.00	15193.0
97.20	486.0
98.90	51.0
102.90	188.0
104.00	1406.0
105.10	491.0
105.80	1451.0
106.80	354.0
107.90	161.0
109.90	209.0
110.70	268.0
111.60	254.0
112.10	330.0
113.00	351.0
115.00	633.0
116.00	1062.0
117.00	2554.0
117.90	869.0
118.90	1475.0
120.00	111.0
123.00	66.0
124.10	140.0
125.30	123.0
125.80	214.0
126.70	64.0
127.20	101.0
127.80	901.0
129.00	873.0
129.90	1001.0
130.70	371.0
134.80	739.0
137.10	486.0
139.10	57.0
139.90	240.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

141.00	3623.0
142.10	427.0
142.90	5085.0
143.90	220.0
145.10	919.0
145.90	567.0
147.00	310.0
147.90	772.0
148.90	225.0
150.00	332.0
151.90	194.0
152.70	132.0
153.10	124.0
153.90	213.0
154.90	745.0
155.90	167.0
157.10	616.0
157.80	74.0
158.90	539.0
160.80	423.0
161.70	101.0
167.70	55.0
168.70	101.0
169.70	390.0
171.10	483.0
172.00	3275.0
174.00	199488.0
175.00	15261.0
176.00	200832.0
177.00	11145.0
178.00	422.0
179.20	54.0
191.00	71.0
195.00	51.0
206.90	185.0
218.40	64.0
238.30	162.0
256.10	72.0
281.20	184.0
291.00	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

m/z	Abundance
35.10	57.0
36.10	1514.0
37.00	8213.0
38.00	6540.0
39.00	2693.0
39.90	430.0
41.20	262.0
41.90	92.0
42.20	88.0
43.00	199.0
43.90	1136.0
45.10	1266.0
46.00	336.0
47.20	1388.0
47.90	923.0
49.00	7092.0
50.00	30344.0
51.00	8353.0
52.00	594.0
53.00	187.0
54.00	144.0
54.90	494.0
56.10	1845.0
57.00	4047.0
58.10	198.0
59.20	149.0
59.90	1498.0
61.00	8056.0
62.00	8249.0
63.00	6210.0
64.10	781.0
65.00	1686.0
65.80	155.0
66.80	443.0
67.20	520.0
68.00	16728.0
69.00	16195.0
70.10	943.0
71.10	279.0
71.90	1167.0
73.00	7620.0
74.00	30880.0
75.00	85632.0
76.10	7049.0
77.00	1154.0
77.80	397.0
79.00	6363.0
79.90	1554.0
80.90	6850.0
81.90	1147.0
83.10	225.0
86.00	527.0
87.10	4906.0
87.90	5160.0
91.00	751.0
92.00	5602.0
93.00	8807.0
94.00	18832.0
95.00	169536.0
96.00	10698.0
97.00	579.0
102.80	175.0
103.90	878.0
105.00	278.0
105.90	869.0
106.80	160.0
110.00	293.0
110.80	157.0
111.20	138.0
111.70	86.0
112.20	108.0
113.00	182.0
114.90	497.0
116.00	712.0
117.00	1220.0
118.00	849.0
119.00	1026.0
123.70	63.0
124.20	342.0
125.20	89.0
127.80	907.0
129.00	481.0
129.90	810.0
130.90	418.0
132.40	89.0
134.90	479.0
137.00	472.0
139.10	55.0
140.00	215.0
140.90	2762.0
141.90	389.0
142.90	2974.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

144.00	328.0
144.90	718.0
145.80	270.0
146.90	332.0
148.00	614.0
148.90	129.0
149.80	238.0
151.60	161.0
153.10	241.0
154.00	162.0
155.00	474.0
156.00	77.0
156.70	406.0
157.20	306.0
157.90	175.0
158.90	300.0
159.70	182.0
160.80	382.0
161.70	65.0
165.50	105.0
168.80	118.0
169.80	194.0
170.70	194.0
171.90	2682.0
173.10	3200.0
174.00	155968.0
175.00	13023.0
176.00	157184.0
177.00	9585.0
178.10	602.0
179.20	52.0
191.00	74.0
195.00	58.0
207.00	210.0
253.00	142.0
256.10	116.0
265.50	85.0
281.20	103.0
282.10	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75

m/z	Abundance
35.20	218.0
36.20	70.0
37.20	103.0
38.00	194.0
38.70	190.0
39.90	300.0
41.40	157.0
42.10	83.0
43.00	175.0
43.90	461.0
45.70	65.0
46.20	128.0
47.30	96.0
49.30	131.0
50.00	87.0
50.70	112.0
51.90	151.0
53.10	87.0
53.80	139.0
54.70	140.0
56.40	81.0
56.90	94.0
57.60	70.0
61.60	63.0
62.20	89.0
64.90	99.0
67.00	67.0
67.60	84.0
69.00	80.0
71.00	77.0
72.90	216.0
73.80	50.0
74.50	72.0
76.20	76.0
78.30	63.0
78.90	59.0
81.00	220.0
82.30	72.0
86.00	61.0
88.00	59.0
88.90	52.0
90.30	79.0
92.10	60.0
96.80	177.0
99.90	68.0
102.40	52.0
114.60	82.0
129.30	53.0
131.20	84.0
137.00	64.0
140.90	70.0
167.10	51.0
169.80	54.0
197.10	108.0
207.00	131.0
281.30	78.0
288.70	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB75