

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100121\
 Data File : VX024503.D
 Acq On : 01 Oct 2021 16:11
 Operator : JC/MD
 Sample : M3970-01
 Misc : 5.08g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR-04-092821

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	21	28	41	rVB3	11899	27923	3.40%	0.586%
2	1.599	68	84	85	rBV7	7943	26692	3.25%	0.560%
3	1.904	132	134	147	rVB3	10477	15196	1.85%	0.319%
4	5.391	692	706	719	rBV2	91643	268968	32.80%	5.643%
5	5.550	721	732	746	rVB	159615	452289	55.15%	9.490%
6	5.964	789	800	814	rBV	103397	279870	34.13%	5.872%
7	6.373	857	867	880	rBV5	4600	14711	1.79%	0.309%
8	6.763	921	931	945	rBV	253689	602485	73.47%	12.641%
9	8.653	1233	1241	1249	rBV	523515	820096	100.00%	17.207%
10	10.055	1465	1471	1481	rBV	530706	741889	90.46%	15.566%
11	11.085	1634	1640	1654	rVB	462657	600892	73.27%	12.608%
12	12.024	1789	1794	1803	rBV	576254	744027	90.72%	15.611%
13	12.987	1944	1952	1956	rVB6	5044	8207	1.00%	0.172%
14	13.292	1995	2002	2008	rVB8	6602	13854	1.69%	0.291%
15	14.426	2185	2188	2194	rVB6	6455	11575	1.41%	0.243%
16	14.755	2239	2242	2245	rVB4	7678	8608	1.05%	0.181%
17	14.792	2245	2248	2254	rVB8	5790	10518	1.28%	0.221%
18	14.963	2269	2276	2282	rVB	45189	70911	8.65%	1.488%
19	15.420	2347	2351	2357	rVB2	19661	29751	3.63%	0.624%
20	15.743	2402	2404	2411	rVB5	11672	17654	2.15%	0.370%


Sum of corrected areas: 4766116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100121\
Data File : VX024503.D
Acq On : 01 Oct 2021 16:11
Operator : JC/MD
Sample : M3970-01
Misc : 5.08g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-04-092821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

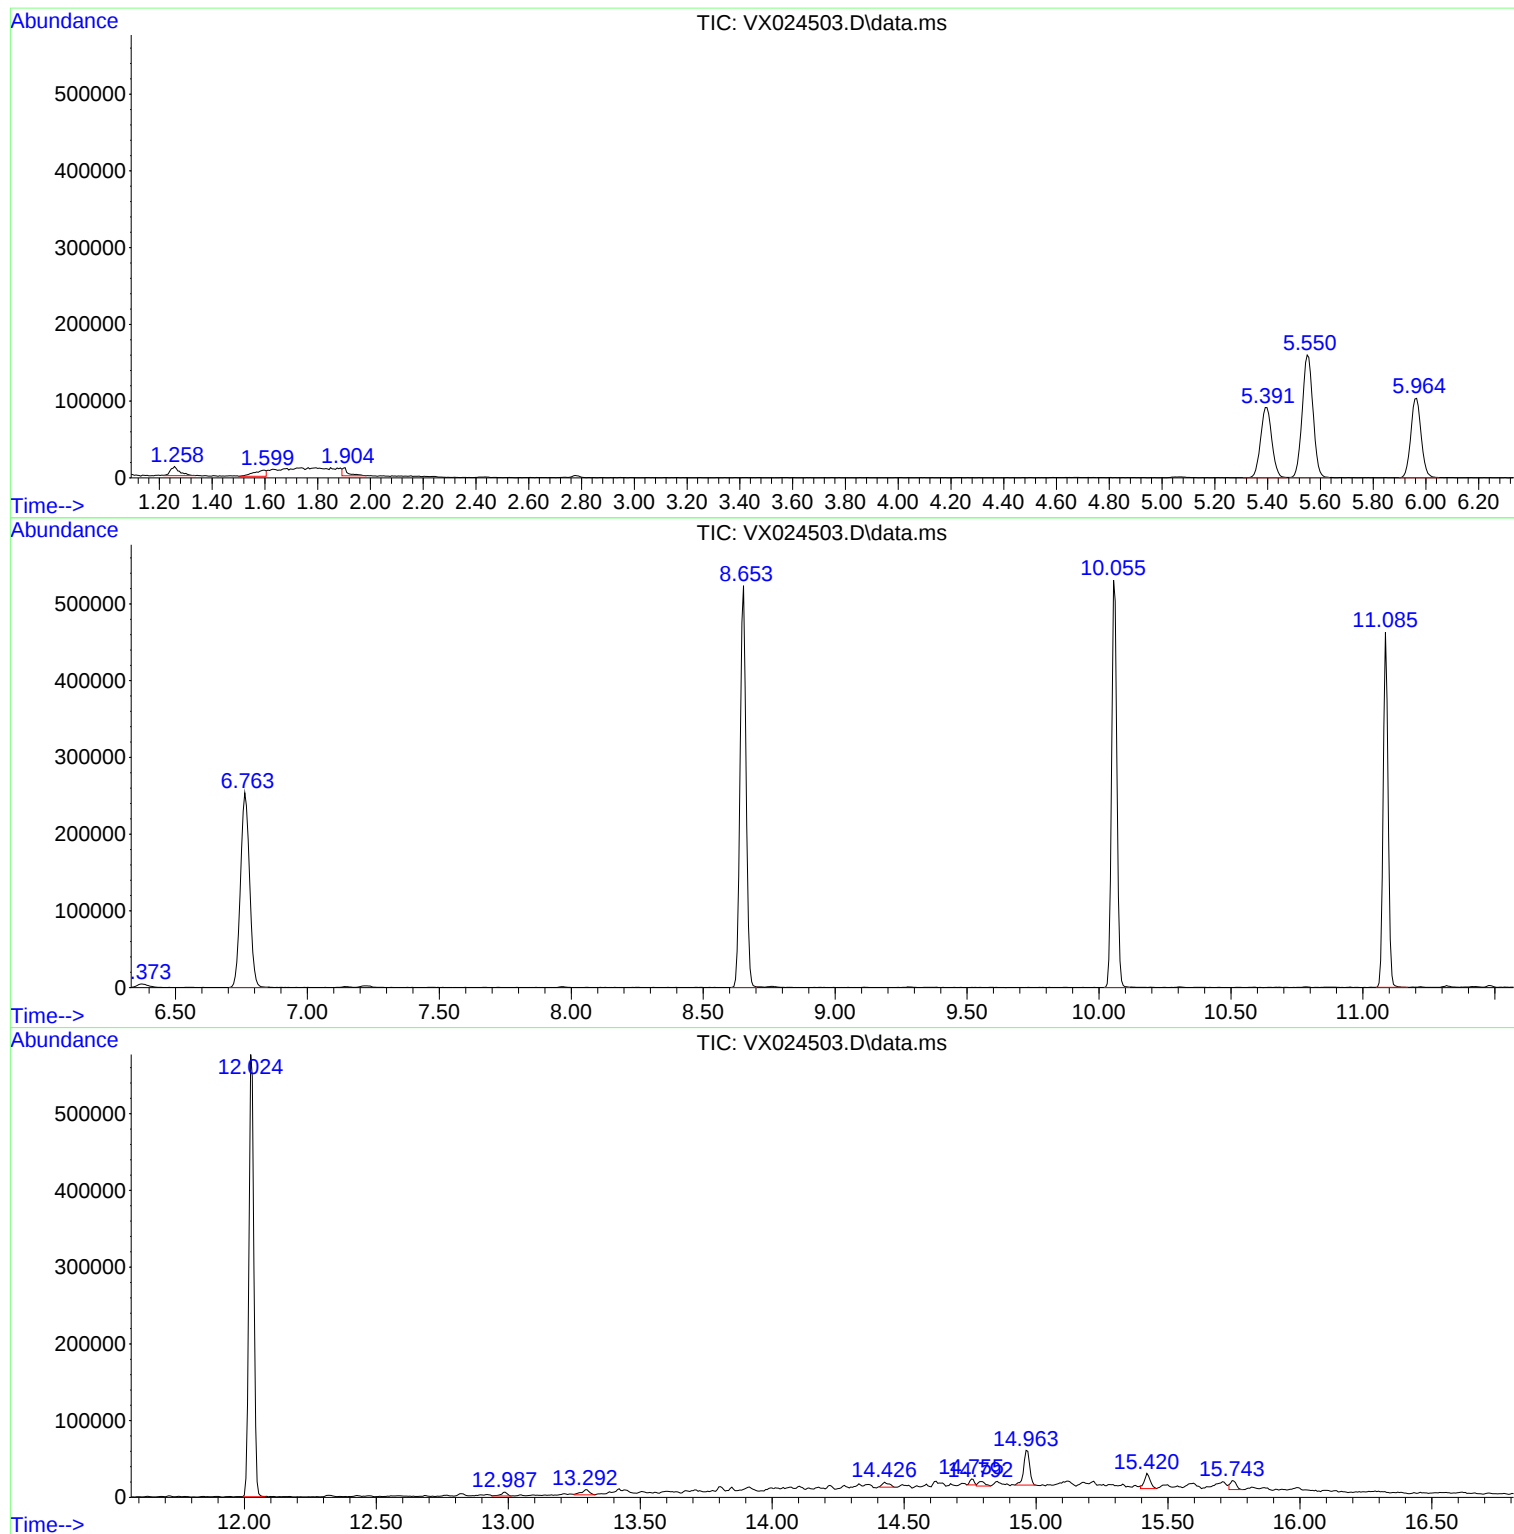

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100121\
Data File : VX024503.D
Acq On : 01 Oct 2021 16:11
Operator : JC/MD
Sample : M3970-01
Misc : 5.08g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-04-092821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100121\
Data File : VX024503.D
Acq On : 01 Oct 2021 16:11
Operator : JC/MD
Sample : M3970-01
Misc : 5.08g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-04-092821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
