

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100124\
 Data File : VX043206.D
 Acq On : 01 Oct 2024 10:50
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Oct 02 04:27:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 04:21:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	83986	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	159476	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	140594	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	57656	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	71380	49.376	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.760%		
35) Dibromofluoromethane	5.379	113	54111	47.590	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.180%		
50) Toluene-d8	8.647	98	191875	50.343	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.680%		
62) 4-Bromofluorobenzene	11.079	95	68315	49.338	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.680%		
Target Compounds					Qvalue	
5) Bromomethane	1.605	94	259	0.629	ug/l	89
11) Tert butyl alcohol	2.941	59	4104	15.448	ug/l #	71
13) Acrolein	2.240	56	244	0.990	ug/l	87
15) Acrylonitrile	3.081	53	389	0.730	ug/l #	75
16) Acetone	2.392	43	1058	1.847	ug/l	94
17) Carbon Disulfide	2.502	76	1495	0.659	ug/l	98
18) Methyl Acetate	2.709	43	380	0.264	ug/l #	51
20) Methylene Chloride	2.782	84	303	0.287	ug/l #	77
21) trans-1,2-Dichloroethene	3.081	96	289	0.311	ug/l	83
23) Vinyl Acetate	3.764	43	1059	0.325	ug/l #	71
25) 2-Butanone	4.617	43	591	0.752	ug/l #	49
29) Tetrahydrofuran	5.038	42	311	0.622	ug/l #	31
31) Cyclohexane	5.538	56	2098	1.418	ug/l #	21
36) 1,1-Dichloropropene	5.538	75	7179	5.167	ug/l #	50
38) Carbon Tetrachloride	5.538	117	9449	5.745	ug/l #	17
49) 1,4-Dioxane	7.702	88	22	0.837	ug/l #	16
51) 4-Methyl-2-Pentanone	8.586	43	513	0.306	ug/l #	82
59) 2-Hexanone	9.464	43	668	0.528	ug/l #	55
68) m/p-Xylenes	10.317	106	456	0.231	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	37823	29.575	ug/l #	34
79) 2-Chlorotoluene	11.463	91	827	0.261	ug/l	76
81) trans-1,4-Dichloro-2-b...	11.079	75	37823	76.649	ug/l #	8
82) 4-Chlorotoluene	11.463	91	827	0.229	ug/l	83
87) 1,3-Dichlorobenzene	11.976	146	586	0.305	ug/l	93
88) 1,4-Dichlorobenzene	11.976	146	586	0.304	ug/l	93
89) n-Butylbenzene	12.335	91	953	0.302	ug/l	92
93) 1,2,4-Trichlorobenzene	13.591	180	991	0.875	ug/l	92
94) Hexachlorobutadiene	13.731	225	160	0.356	ug/l #	73
95) Naphthalene	13.780	128	6383	1.533	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	1078	0.922	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100124\
Data File : VX043206.D
Acq On : 01 Oct 2024 10:50
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Oct 02 04:27:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 04:21:52 2024
Response via : Initial Calibration




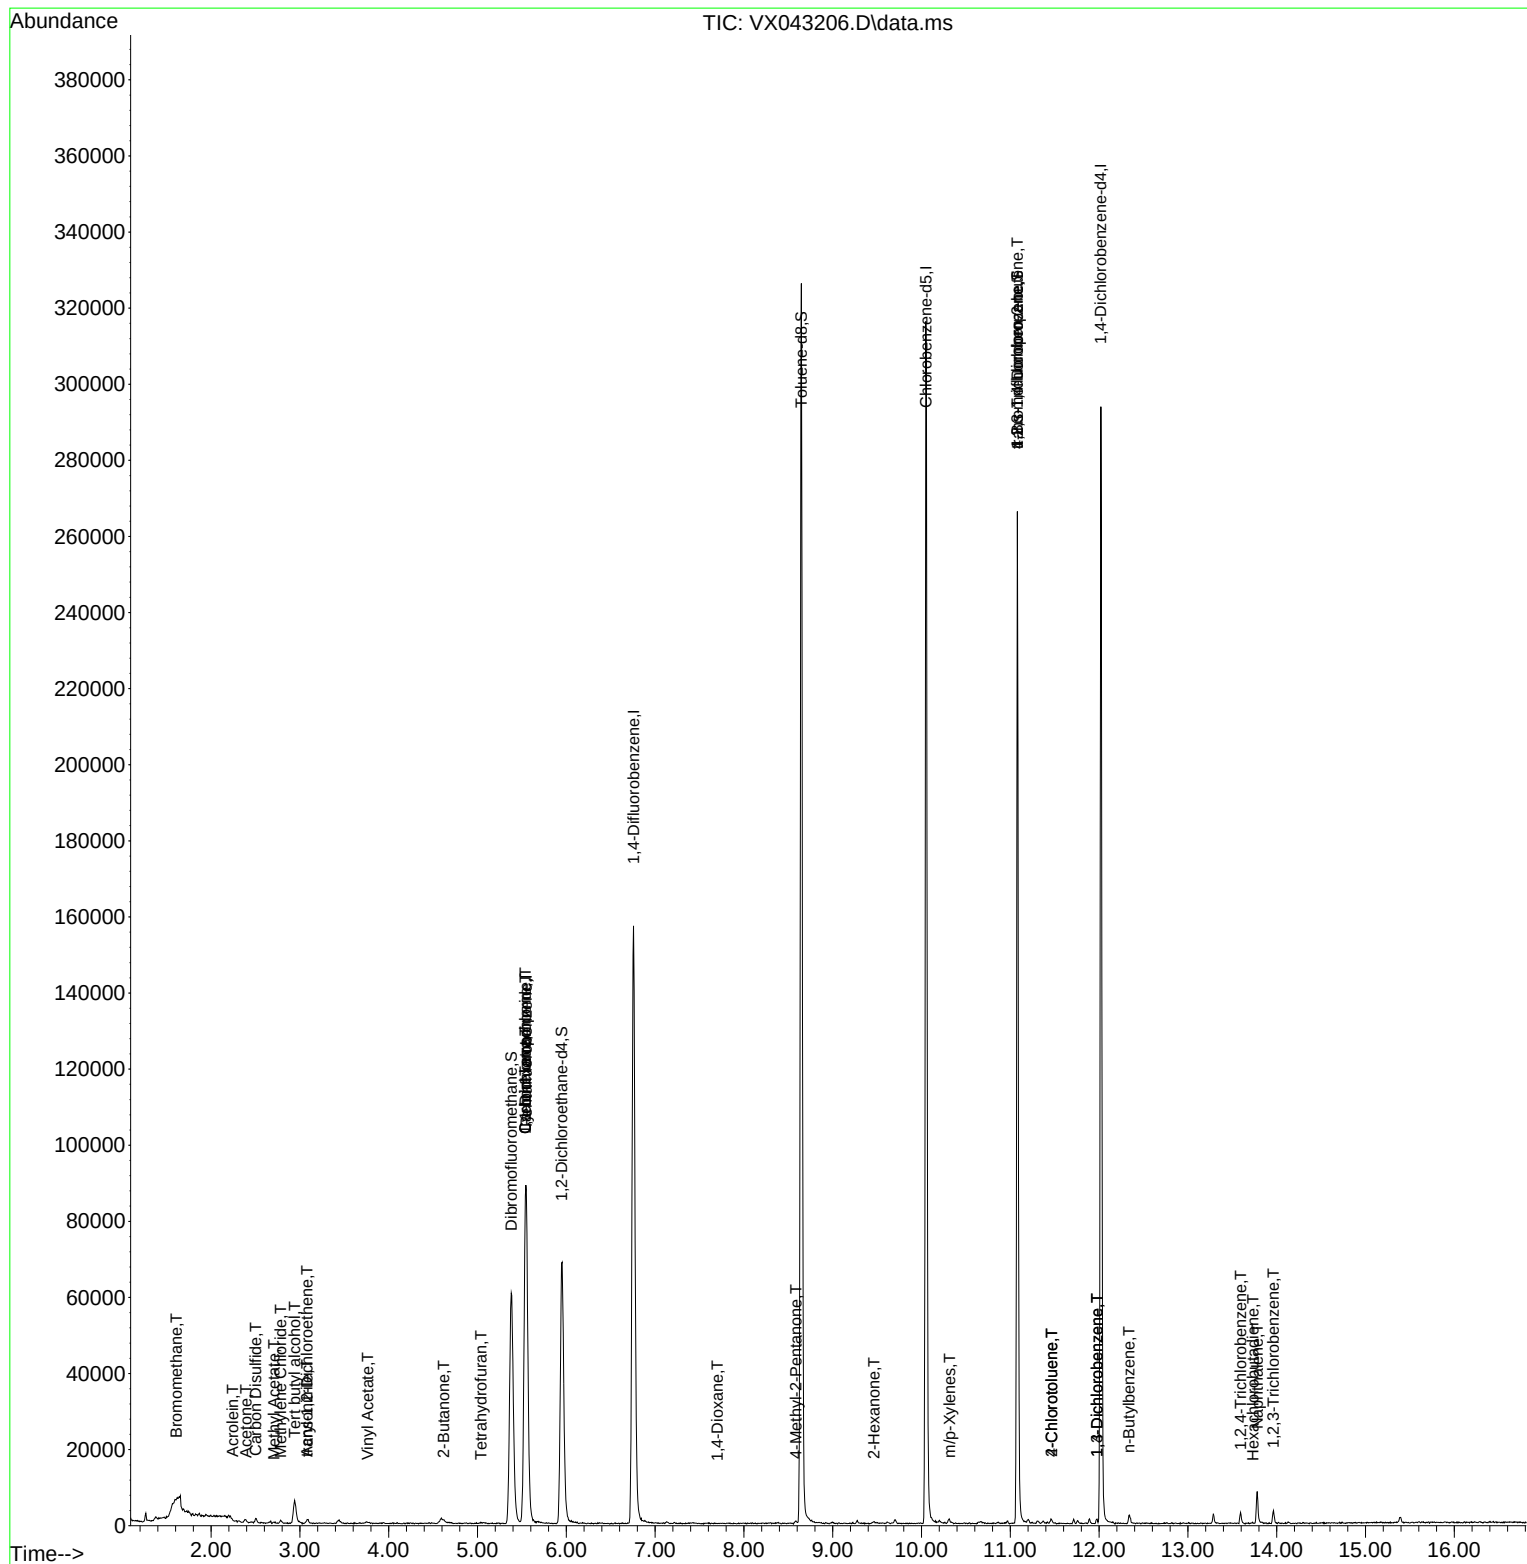




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 83986
Ion Ratio Lower Upper
168 100
99 63.7 49.7 74.5

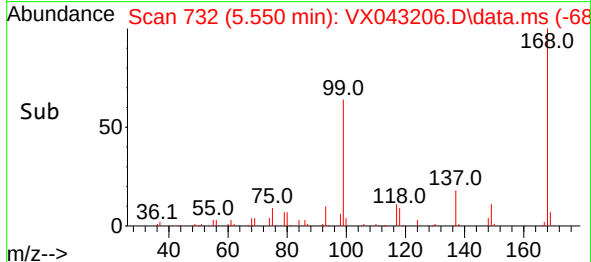

#5
Bromomethane
Concen: 0.629 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 94 Resp: 259
Ion Ratio Lower Upper
94 100
96 85.1 76.6 115.0


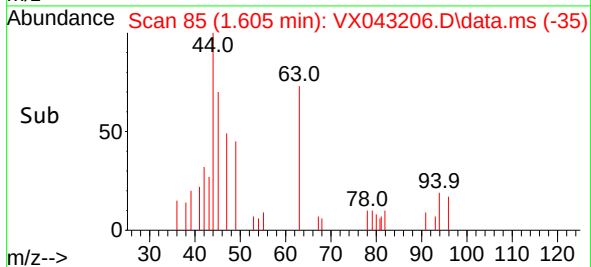

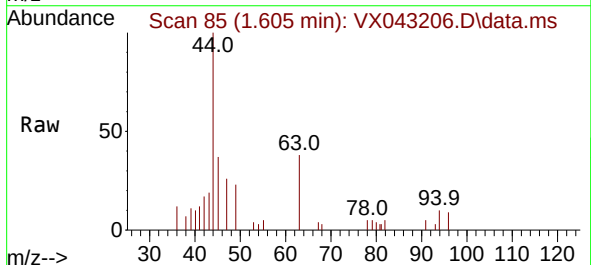




#11
Tert butyl alcohol
Concen: 15.448 ug/l
RT: 2.941 min Scan# 30
Delta R.T. -0.055 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 59 Resp: 4104
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0#

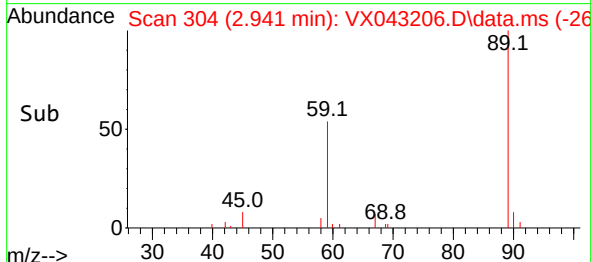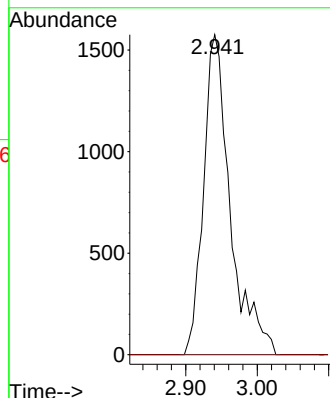

#13
Acrolein
Concen: 0.990 ug/l
RT: 2.240 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 56 Resp: 244
Ion Ratio Lower Upper
56 100
55 61.1 57.4 86.0

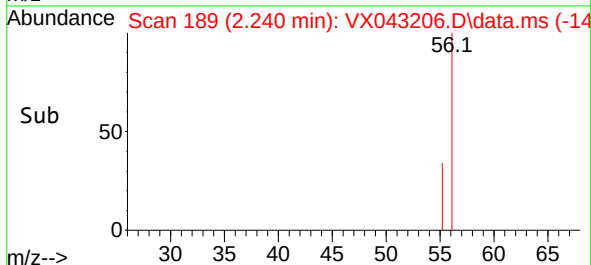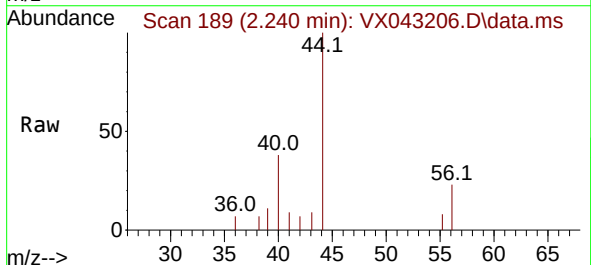



#15

Acrylonitrile

Concen: 0.730 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion: 53 Resp: 389

Ion Ratio Lower Upper

53 100

52 76.6 67.6 101.4

51 0.0 30.3 45.5#

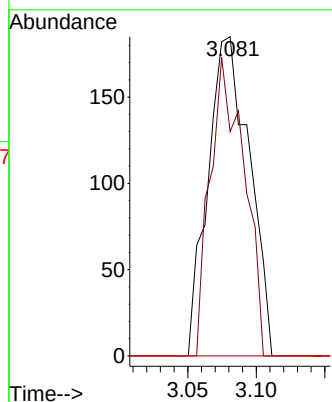

#16

Acetone

Concen: 1.847 ug/l

RT: 2.392 min Scan# 214

Delta R.T. 0.006 min

Lab File: VX043206.D




Acq: 01 Oct 2024 10:50


Tgt Ion: 43 Resp: 1058

Ion Ratio Lower Upper

43 100

58 25.1 22.6 33.8


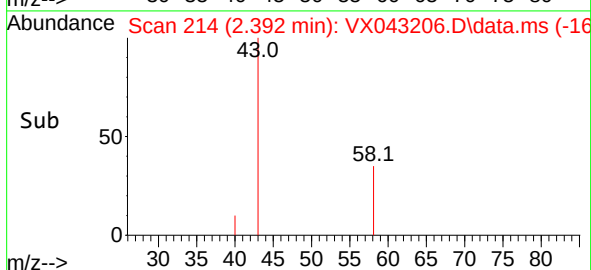
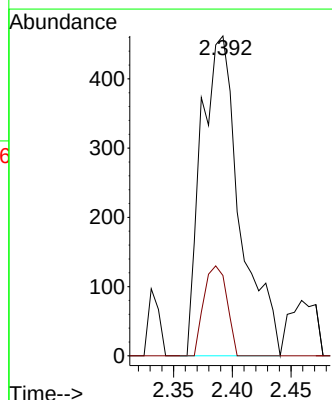





#17
Carbon Disulfide
Concen: 0.659 ug/l
RT: 2.502 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 76 Resp: 1495
Ion Ratio Lower Upper
76 100
78 9.3 6.7 10.1

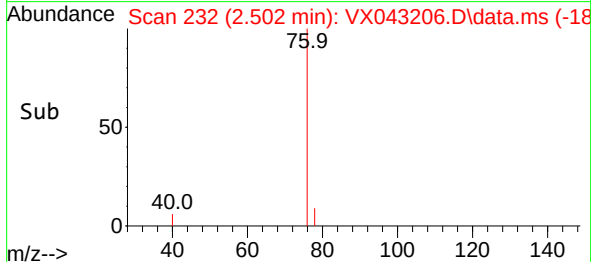

#18
Methyl Acetate
Concen: 0.264 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 43 Resp: 380
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#

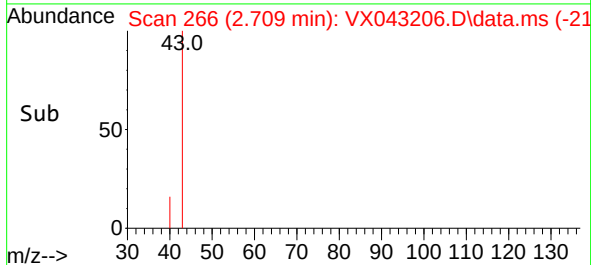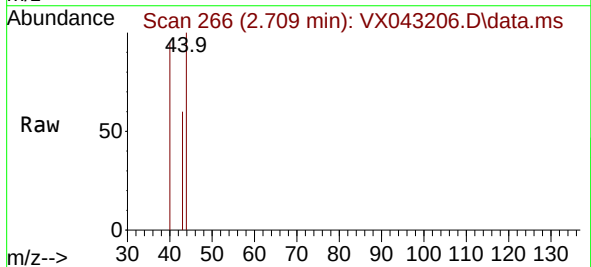



#20

Methylene Chloride

Concen: 0.287 ug/l

RT: 2.782 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion: 84 Resp: 303





Ion Ratio Lower Upper

84 100

49 89.9 96.7 145.1#

51 39.6 30.4 45.6

86 48.8 54.7 82.1#

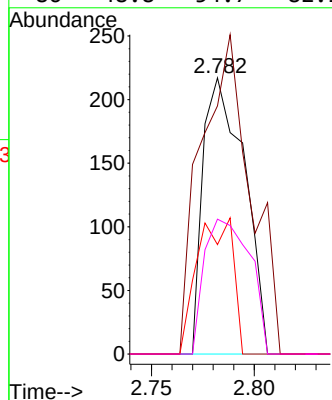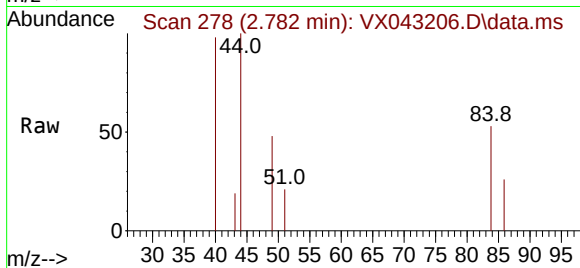

#21

trans-1,2-Dichloroethene

Concen: 0.311 ug/l

RT: 3.081 min Scan# 327

Delta R.T. -0.012 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion: 96 Resp: 289


Ion Ratio Lower Upper

96 100

61 114.2 112.3 168.5

98 75.4 54.6 82.0


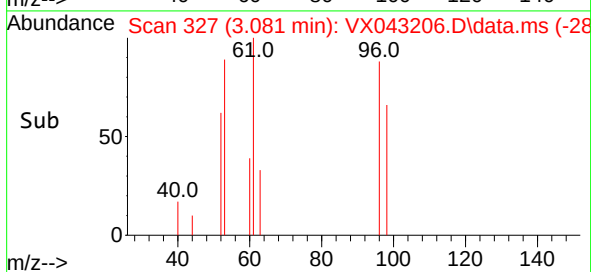
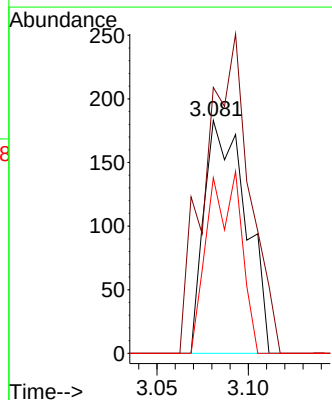
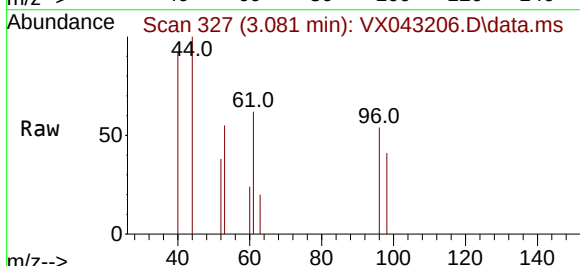


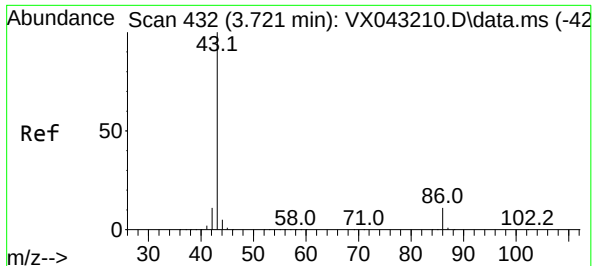

#23
 Vinyl Acetate
 Concen: 0.325 ug/l
 RT: 3.764 min Scan# 41
 Delta R.T. 0.031 min
 Lab File: VX043206.D
 Acq: 01 Oct 2024 10:50




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion: 43 Resp: 1059
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.8 13.2#

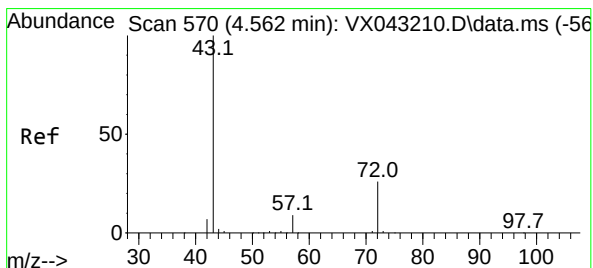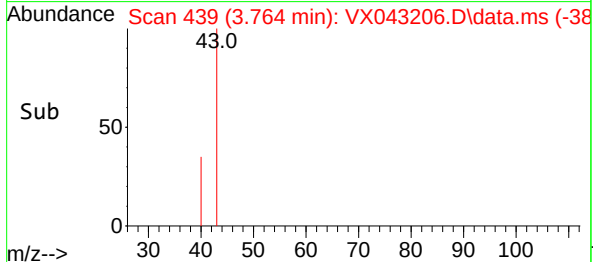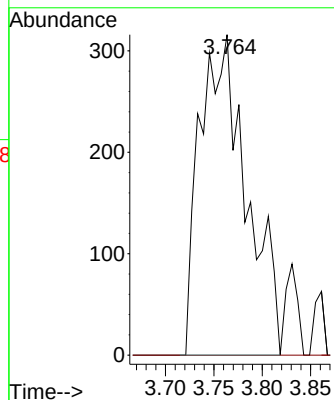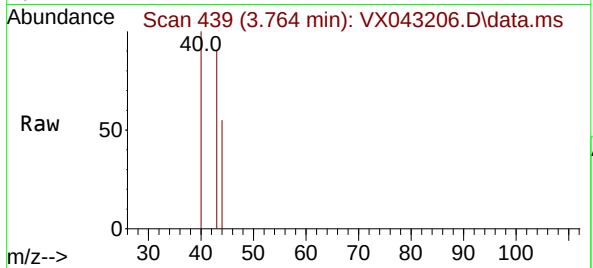

#25
 2-Butanone
 Concen: 0.752 ug/l
 RT: 4.617 min Scan# 579
 Delta R.T. 0.037 min
 Lab File: VX043206.D
 Acq: 01 Oct 2024 10:50

Tgt Ion: 43 Resp: 591
 Ion Ratio Lower Upper
 43 100
 72 0.0 20.6 31.0#

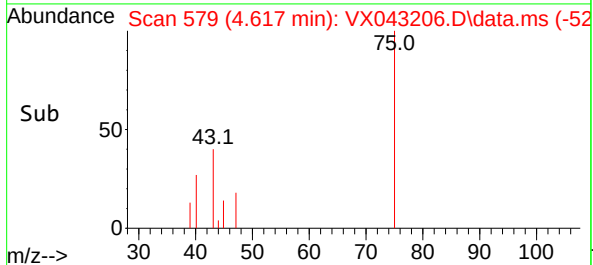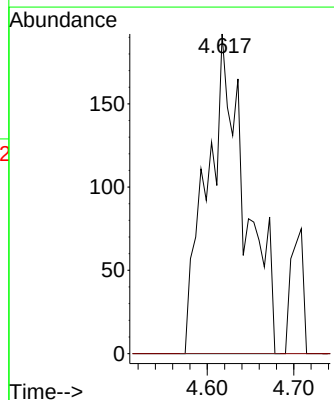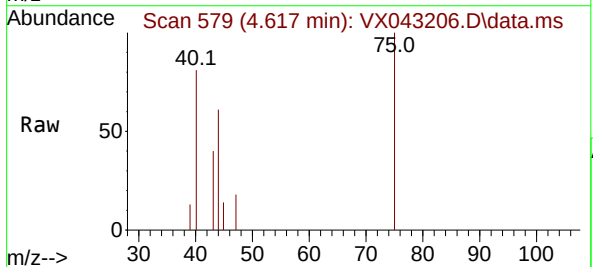

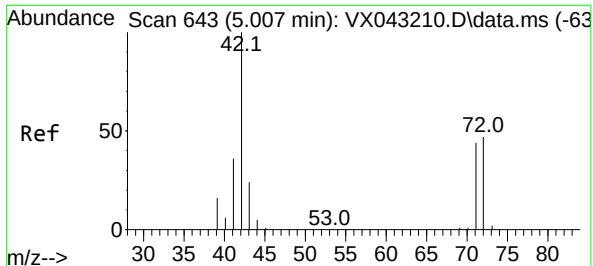

#29

Tetrahydrofuran

Concen: 0.622 ug/l

RT: 5.038 min Scan# 64

Delta R.T. 0.006 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion: 42 Resp: 311

Ion Ratio Lower Upper

42 100

72 0.0 37.7 56.5#

71 0.0 34.6 52.0#

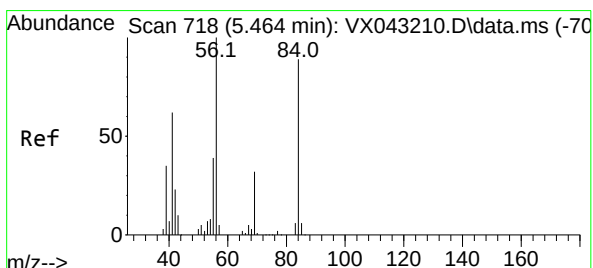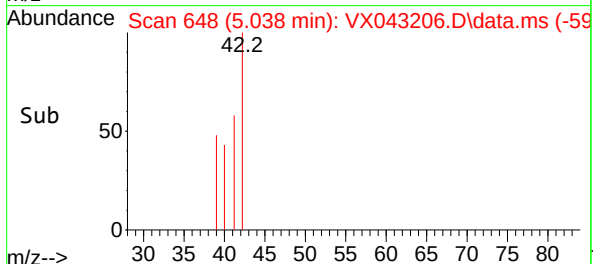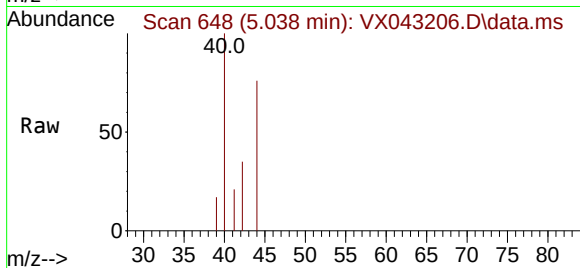

#31

Cyclohexane

Concen: 1.418 ug/l

RT: 5.538 min Scan# 730

Delta R.T. 0.073 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion: 56 Resp: 2098


Ion Ratio Lower Upper

56 100

69 156.6 25.8 38.6#

84 114.4 71.1 106.7#

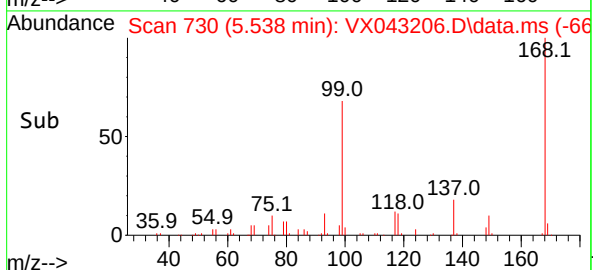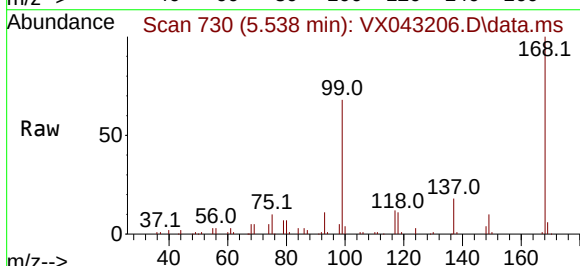



#33

1,2-Dichloroethane-d4

Concen: 49.376 ug/l

RT: 5.946 min Scan# 798

Delta R.T. -0.006 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 65 Resp: 71380

Ion Ratio Lower Upper

65 100

67 49.2 0.0 99.0

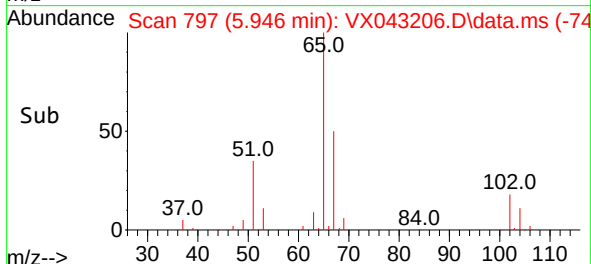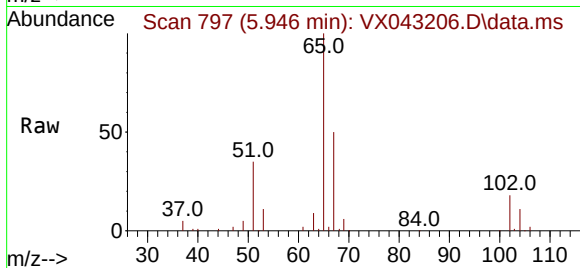

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion: 114 Resp: 159476


Ion Ratio Lower Upper

114 100

63 21.5 0.0 43.0

88 17.2 0.0 33.0


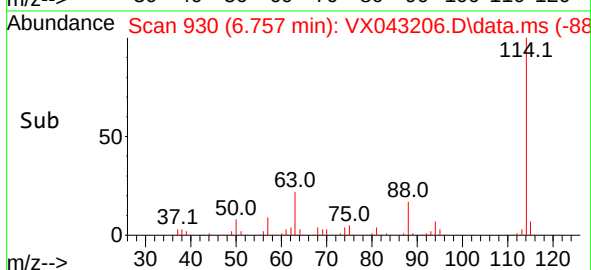

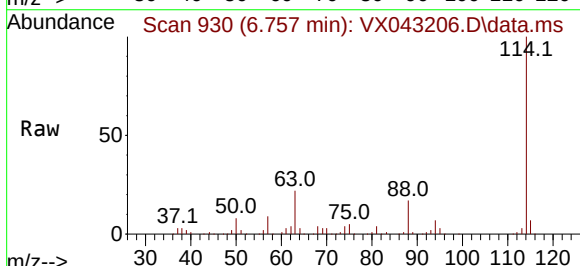


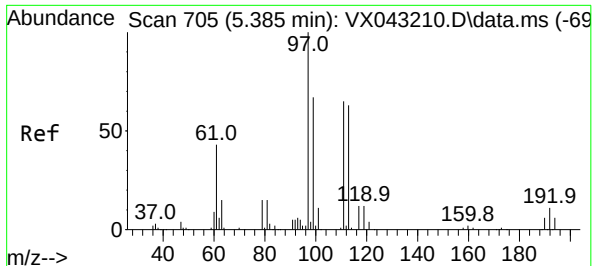

#35
Dibromofluoromethane
Concen: 47.590 ug/l
RT: 5.379 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:113 Resp: 54111
Ion Ratio Lower Upper
113 100
111 102.7 83.4 125.0
192 17.9 14.1 21.1

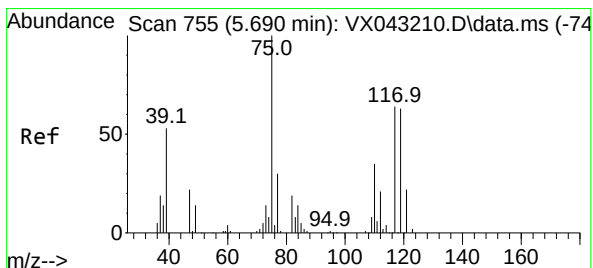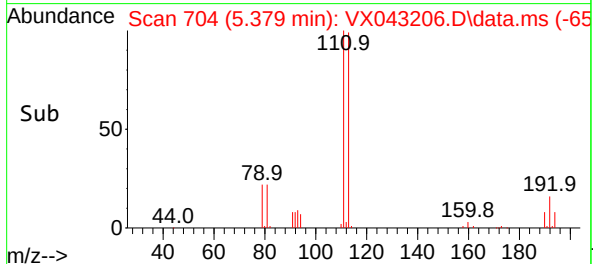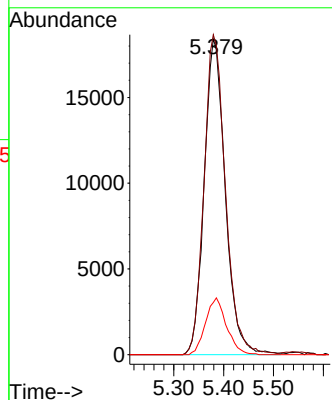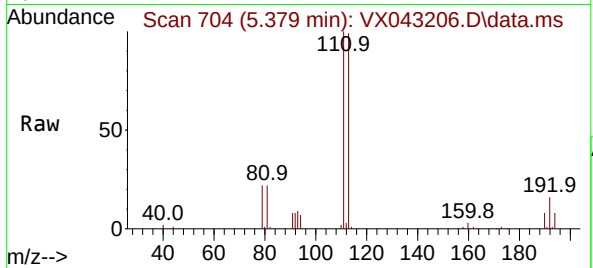

#36
1,1-Dichloropropene
Concen: 5.167 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.152 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 75 Resp: 7179
Ion Ratio Lower Upper
75 100
110 9.6 17.8 53.3#
77 0.0 24.9 37.3#


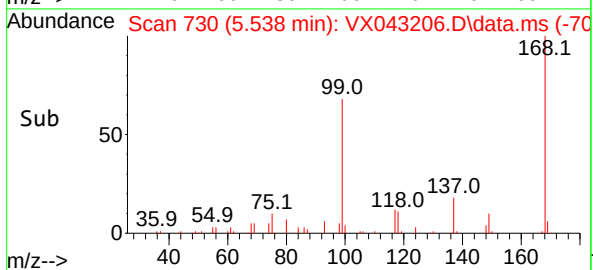
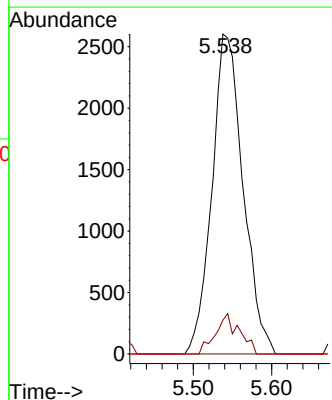
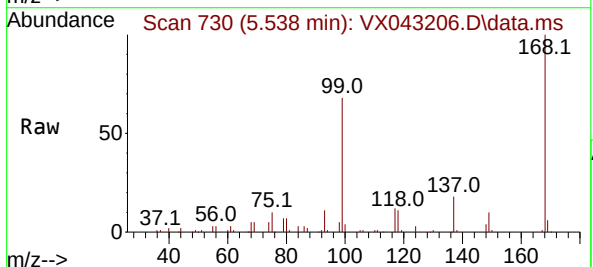




#38
Carbon Tetrachloride
Concen: 5.745 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 9449
Ion Ratio Lower Upper
117 100
119 6.6 77.7 116.5#
121 0.0 24.3 36.5#

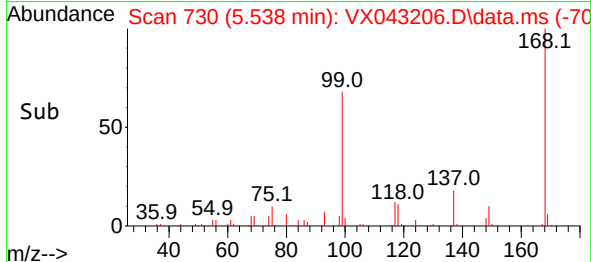

#49
1,4-Dioxane
Concen: 0.837 ug/l
RT: 7.702 min Scan# 1085
Delta R.T. 0.018 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 88 Resp: 22
Ion Ratio Lower Upper
88 100
43 86.4 29.5 44.3#
58 0.0 55.2 82.8#


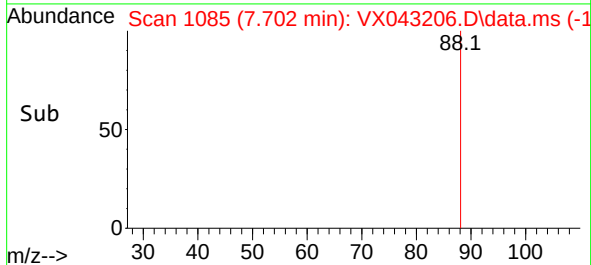

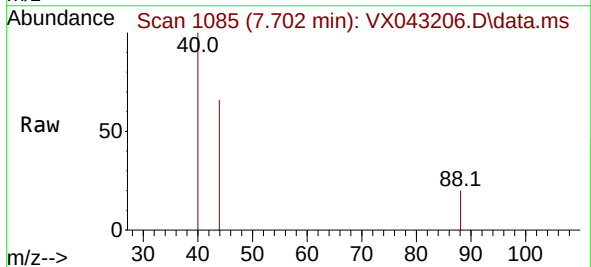


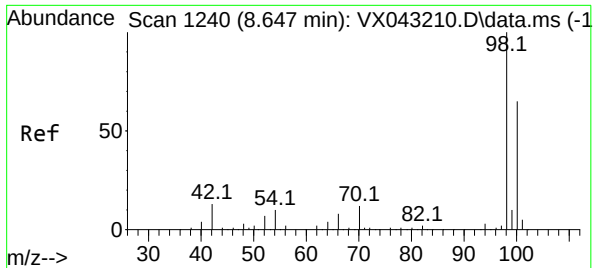

#50
Toluene-d8
Concen: 50.343 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 191875
Ion Ratio Lower Upper
98 100
100 65.6 52.4 78.6

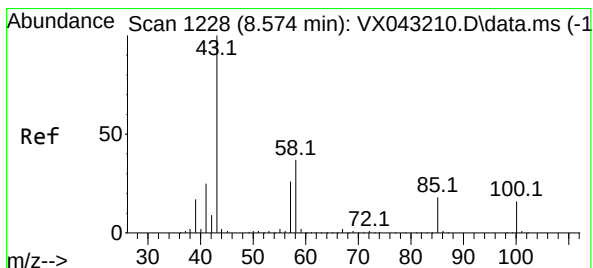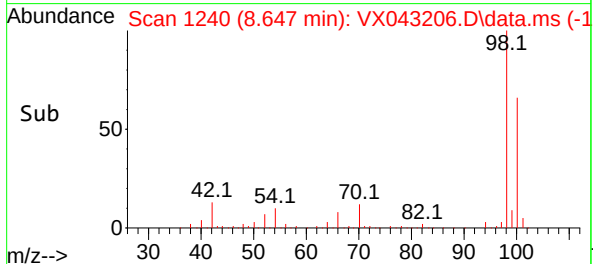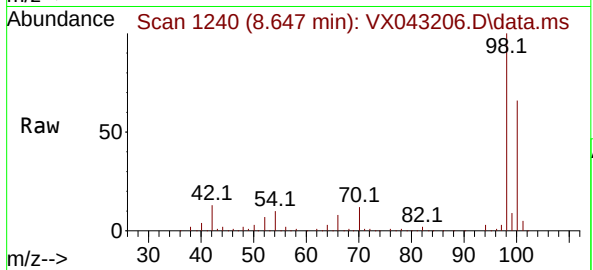

#51
4-Methyl-2-Pentanone
Concen: 0.306 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.006 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 43 Resp: 513
Ion Ratio Lower Upper
43 100
58 26.7 30.0 45.0#

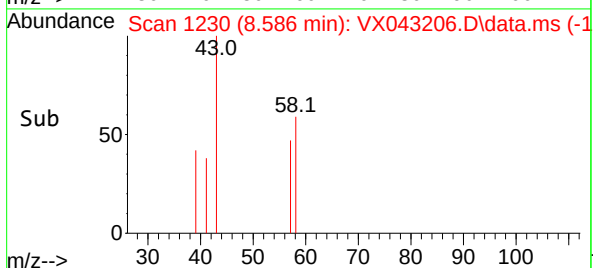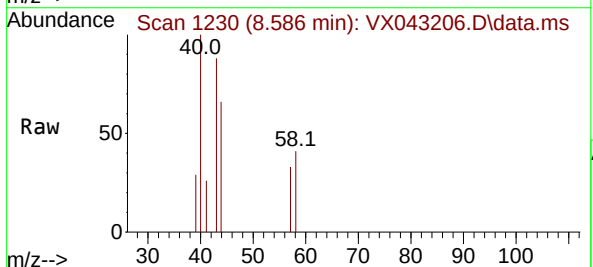

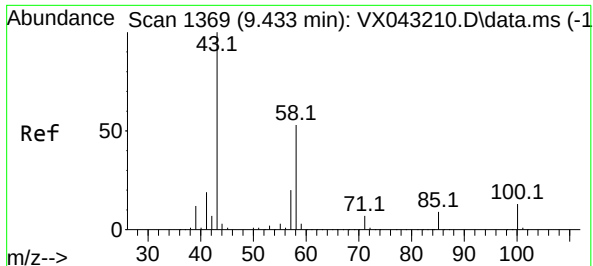

#59

2-Hexanone

Concen: 0.528 ug/l

RT: 9.464 min Scan# 1374

Delta R.T. 0.025 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 43 Resp: 668

Ion Ratio Lower Upper

43 100

58 20.5 26.1 78.3#

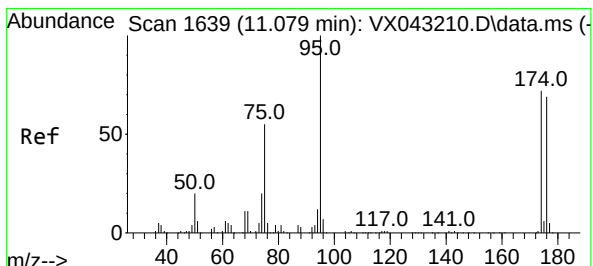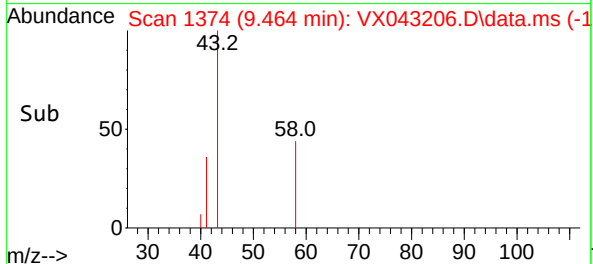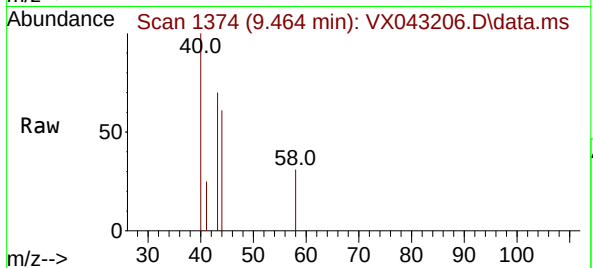

#62

4-Bromofluorobenzene

Concen: 49.338 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion: 95 Resp: 68315


Ion Ratio Lower Upper

95 100

174 72.6 0.0 145.0

176 71.1 0.0 143.0


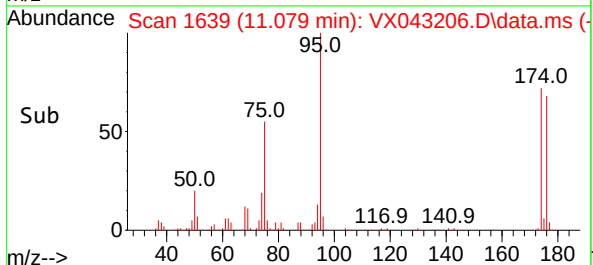
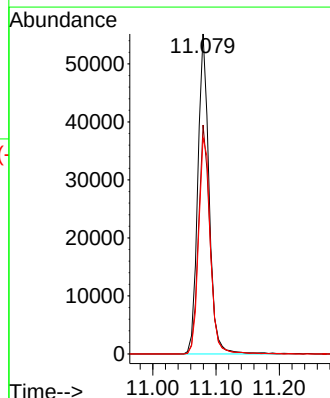
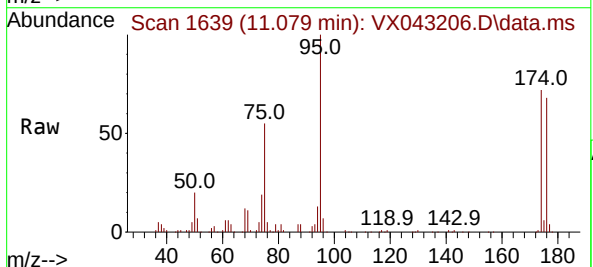




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 140594
Ion Ratio Lower Upper
117 100
82 57.9 45.0 67.6
119 32.1 25.3 37.9

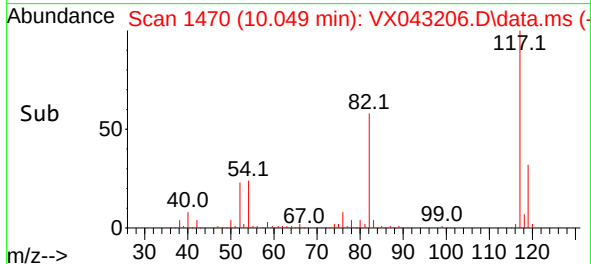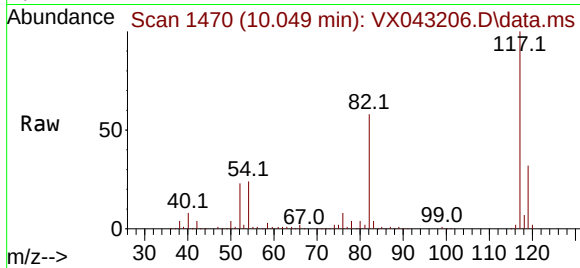

#68
m/p-Xylenes
Concen: 0.231 ug/l
RT: 10.317 min Scan# 1514
Delta R.T. 0.012 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion:106 Resp: 456
Ion Ratio Lower Upper
106 100
91 210.7 167.0 250.6




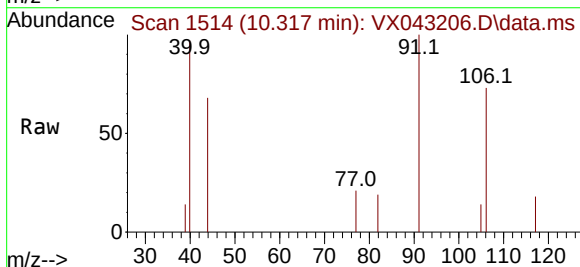




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VX043206.D
 Acq: 01 Oct 2024 10:50




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:152 Resp: 57656
 Ion Ratio Lower Upper
 152 100
 115 65.4 44.1 132.3
 150 164.1 0.0 347.4

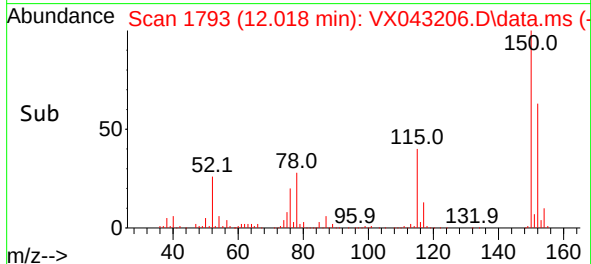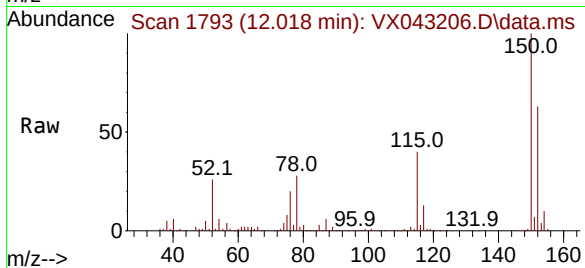

#76
 1,2,3-Trichloropropane
 Concen: 29.575 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.164 min
 Lab File: VX043206.D
 Acq: 01 Oct 2024 10:50

Tgt Ion: 75 Resp: 37823
 Ion Ratio Lower Upper
 75 100
 77 1.1 22.0 66.0#

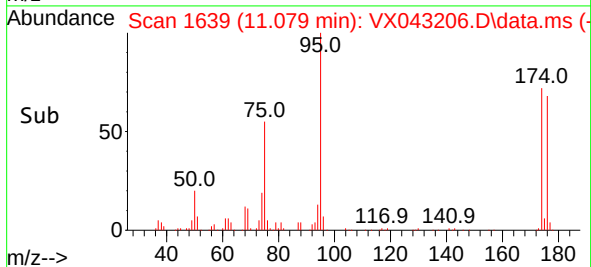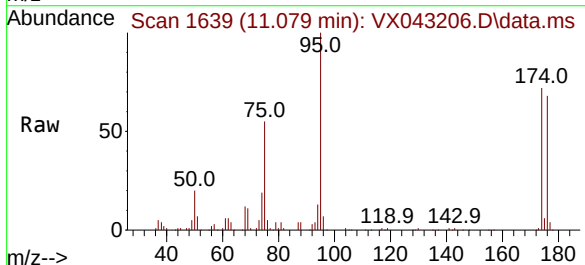



#79

2-Chlorotoluene

Concen: 0.261 ug/l

RT: 11.463 min Scan# 11

Delta R.T. 0.098 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 91 Resp: 827

Ion Ratio Lower Upper

91 100

126 19.3 16.6 49.7

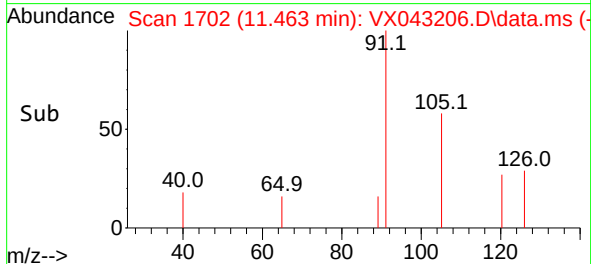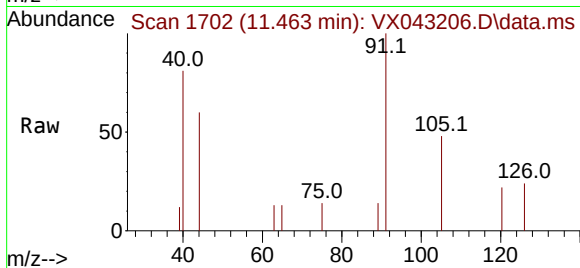

#81

trans-1,4-Dichloro-2-butene

Concen: 76.649 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion: 75 Resp: 37823


Ion Ratio Lower Upper

75 100

53 0.0 83.9 125.9#

89 0.0 38.6 58.0#

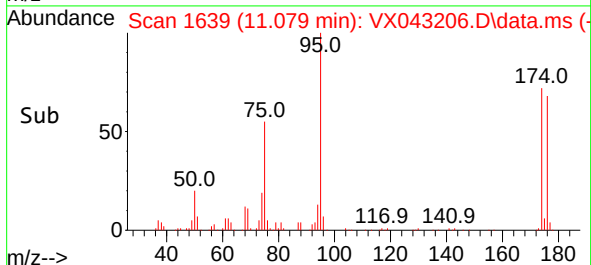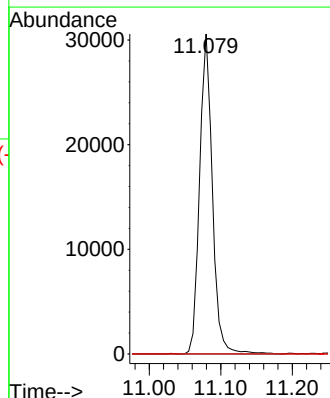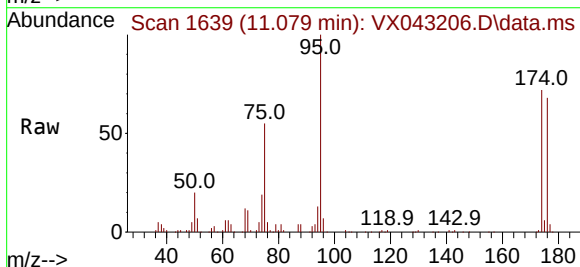



#82

4-Chlorotoluene

Concen: 0.229 ug/l

RT: 11.463 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 91 Resp: 827

Ion Ratio Lower Upper

91 100

126 19.3 14.1 42.3

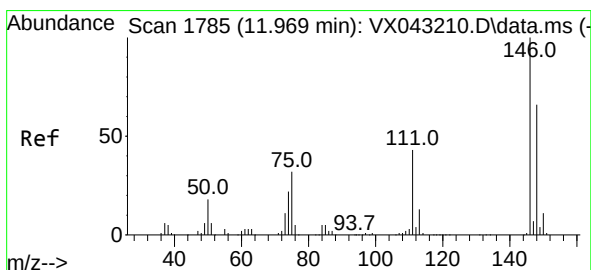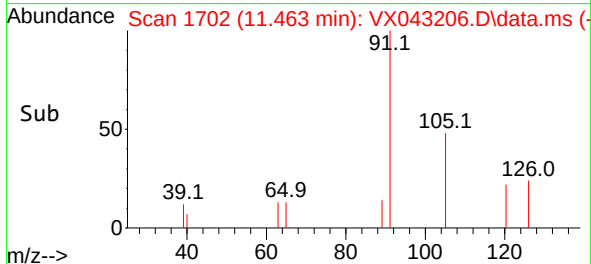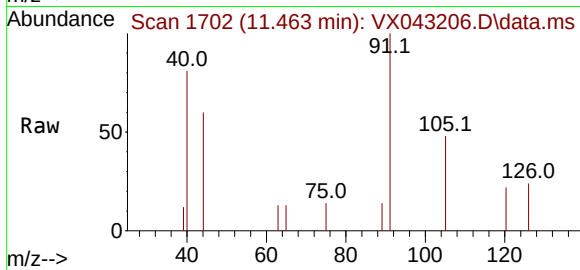

#87

1,3-Dichlorobenzene

Concen: 0.305 ug/l

RT: 11.976 min Scan# 1786

Delta R.T. 0.000 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion:146 Resp: 586


Ion Ratio Lower Upper

146 100

111 42.2 21.8 65.3

148 56.1 32.4 97.2




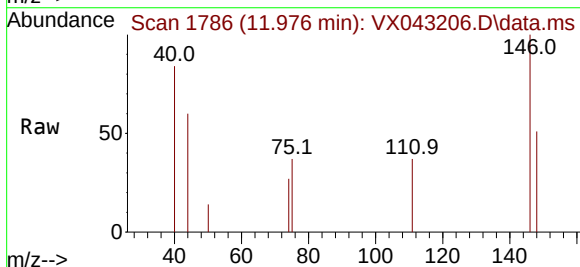




#88
1,4-Dichlorobenzene
Concen: 0.304 ug/l
RT: 11.976 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:146 Resp: 586
Ion Ratio Lower Upper
146 100
111 42.2 20.8 62.5
148 56.1 32.4 97.0

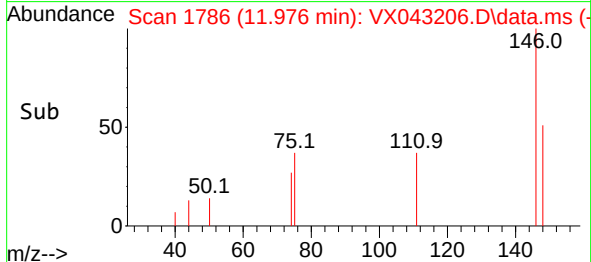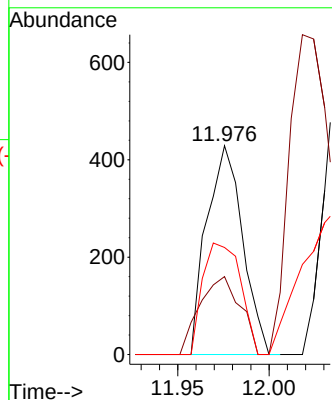

#89
n-Butylbenzene
Concen: 0.302 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion: 91 Resp: 953
Ion Ratio Lower Upper
91 100
92 58.6 27.0 81.0
134 19.7 12.9 38.6

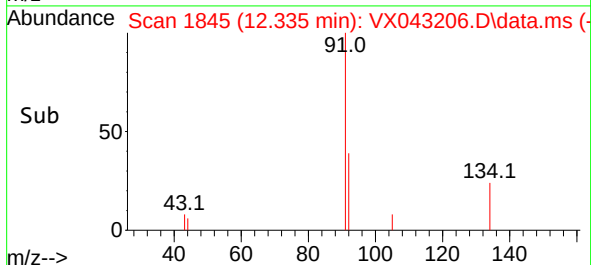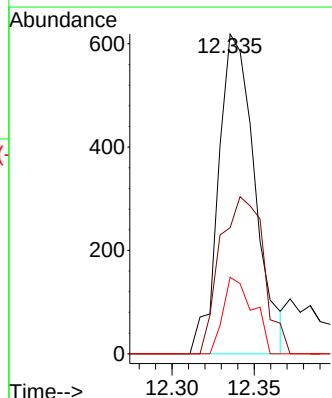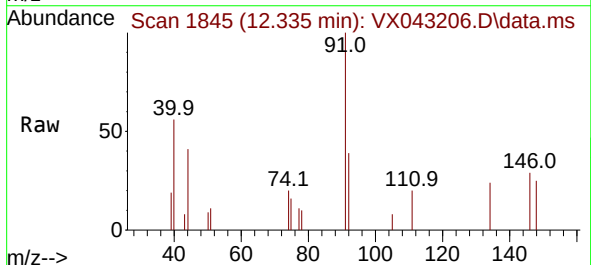



#93

1,2,4-Trichlorobenzene

Concen: 0.875 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.000 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:180 Resp: 991

Ion Ratio Lower Upper

180 100

182 85.0 47.1 141.3

145 30.6 16.6 49.8

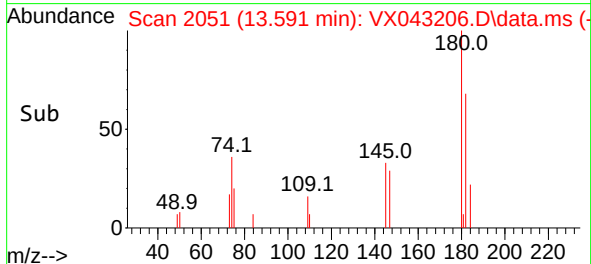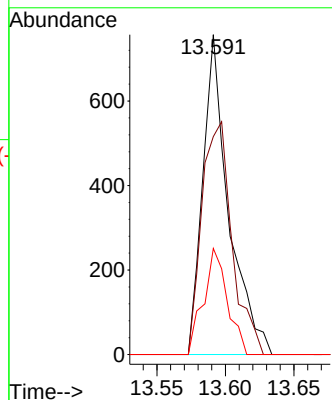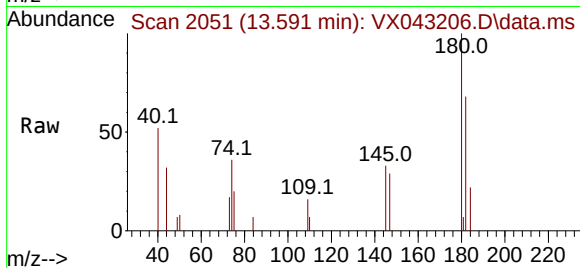

#94

Hexachlorobutadiene

Concen: 0.356 ug/l

RT: 13.731 min Scan# 2074

Delta R.T. 0.006 min

Lab File: VX043206.D

Acq: 01 Oct 2024 10:50




Tgt Ion:225 Resp: 160


Ion Ratio Lower Upper

225 100

223 25.0 30.8 92.4#

227 58.1 32.2 96.6


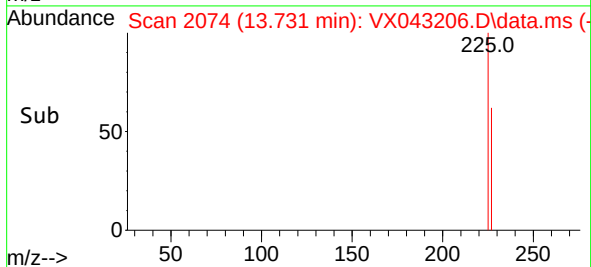
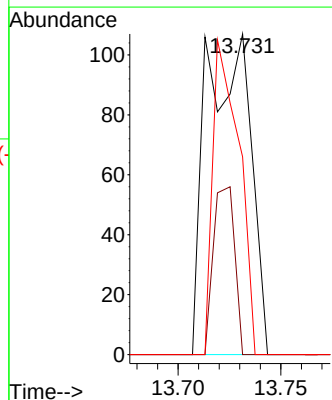
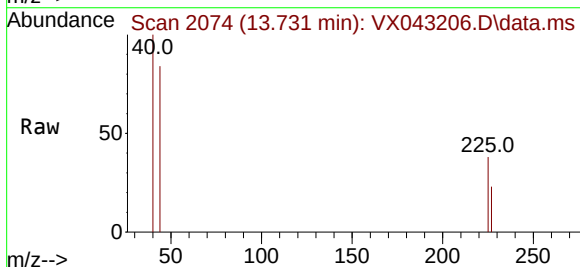




#95
Naphthalene
Concen: 1.533 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:128	Resp: 6383
Ion Ratio	Lower Upper
128 100	
127 13.6	10.2 15.2
129 10.6	8.6 13.0

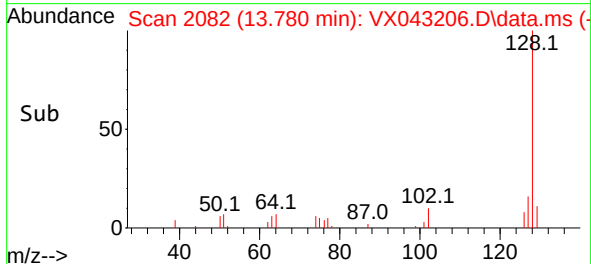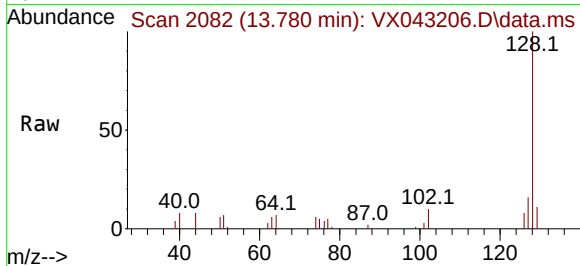

#96
1,2,3-Trichlorobenzene
Concen: 0.922 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.000 min
Lab File: VX043206.D
Acq: 01 Oct 2024 10:50

Tgt Ion:180	Resp:	1078	
Ion	Ratio	Lower	Upper
180	100		
182	97.9	46.5	139.3
145	36.1	17.2	51.6

