

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
 Data File : VX047939.D
 Acq On : 01 Oct 2025 14:48
 Operator : JC/MD
 Sample : Q3193-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT162S1-20250924

Quant Time: Oct 03 01:23:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	119386	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	245473	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	248853	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	118778	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	96274	50.662	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.320%	
35) Dibromofluoromethane	5.379	113	81734	49.648	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 99.300%	
50) Toluene-d8	8.635	98	276805	48.593	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.180%	
62) 4-Bromofluorobenzene	11.067	95	112879	52.213	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 104.420%	

Target Compounds				Qvalue		
5) Bromomethane	1.630	94	286	0.284	ug/l	86
9) 1,1,2-Trichlorotrifluo...	2.331	101	293	0.212	ug/l #	79
10) Methyl Iodide	2.465	142	964	0.448	ug/l #	86
11) Tert butyl alcohol	2.940	59	891	4.210	ug/l #	72
12) 1,1-Dichloroethene	2.331	96	385	0.271	ug/l #	59
13) Acrolein	2.245	56	109	0.559	ug/l #	14
15) Acrylonitrile	3.068	53	217	0.277	ug/l #	76
16) Acetone	2.380	43	1877	2.272	ug/l #	87
17) Carbon Disulfide	2.520	76	920	0.237	ug/l #	76
18) Methyl Acetate	2.703	43	433	0.235	ug/l #	66
20) Methylene Chloride	2.800	84	371	0.212	ug/l #	55
24) 1,1-Dichloroethane	3.605	63	4345	1.441	ug/l #	86
27) cis-1,2-Dichloroethene	4.483	96	404	0.216	ug/l	54
29) Tetrahydrofuran	5.013	42	233	0.376	ug/l #	34
30) Chloroform	5.086	83	1513	0.497	ug/l	92
31) Cyclohexane	5.537	56	2825	1.125	ug/l #	1
36) 1,1-Dichloropropene	5.537	75	10246	4.259	ug/l #	51
38) Carbon Tetrachloride	5.544	117	12873	4.925	ug/l #	18
44) Trichloroethene	7.110	130	18483	10.464	ug/l	98
49) 1,4-Dioxane	7.659	88	229	10.769	ug/l #	62
51) 4-Methyl-2-Pentanone	8.567	43	688	0.294	ug/l #	56
52) Toluene	8.708	92	1222	0.271	ug/l	89
60) Dibromochloromethane	9.256	129	919	0.460	ug/l #	11
64) Tetrachloroethene	9.256	164	853	0.526	ug/l #	87
76) 1,2,3-Trichloropropane	11.067	75	58810	24.454	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.067	75	58810	62.362	ug/l #	8
86) p-Isopropyltoluene	11.994	119	1688	0.221	ug/l #	79
89) n-Butylbenzene	12.317	91	2095	0.296	ug/l	99
93) 1,2,4-Trichlorobenzene	13.573	180	1060	0.414	ug/l	93
94) Hexachlorobutadiene	13.707	225	1017	1.171	ug/l	98
95) Naphthalene	13.762	128	2561	0.329	ug/l	98
96) 1,2,3-Trichlorobenzene	13.945	180	1081	0.454	ug/l	92





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion:168 Resp: 119386
Ion Ratio Lower Upper
168 100
99 62.9 48.8 73.2

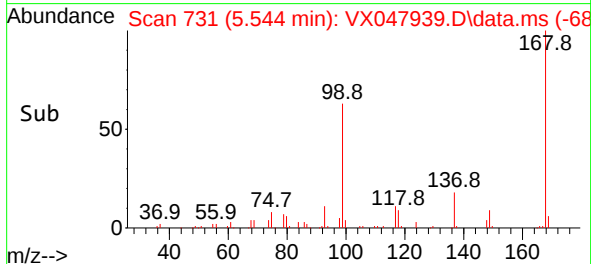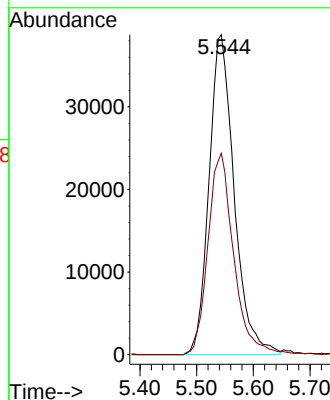

#5
Bromomethane
Concen: 0.284 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.012 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 94 Resp: 286
Ion Ratio Lower Upper
94 100
96 109.6 76.6 115.0


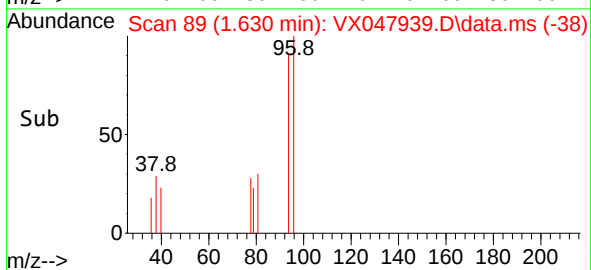
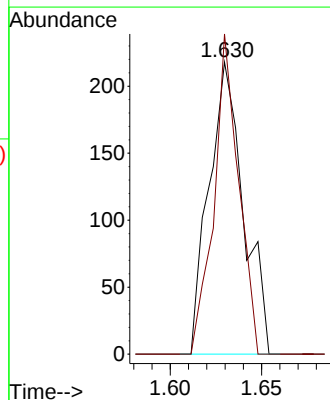





#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.212 ug/l
RT: 2.331 min Scan# 205
Delta R.T. -0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion:101 Resp: 293
Ion Ratio Lower Upper
101 100
85 46.1 35.5 53.3
151 46.4 59.4 89.0#

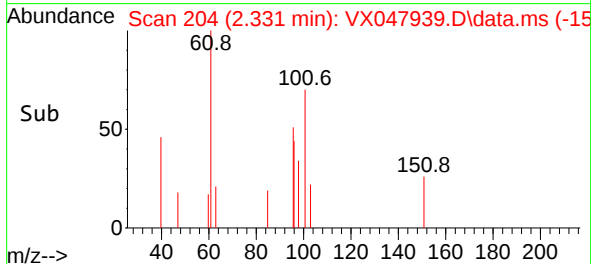

#10
Methyl Iodide
Concen: 0.448 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion:142 Resp: 964
Ion Ratio Lower Upper
142 100
127 38.9 37.2 55.8
141 4.6 11.4 17.0#




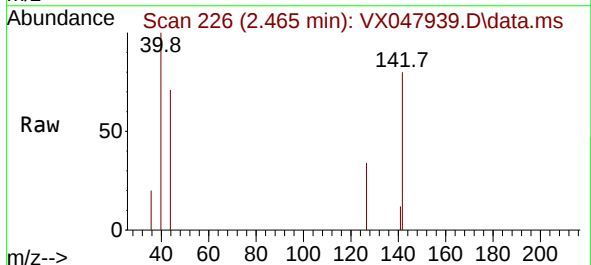


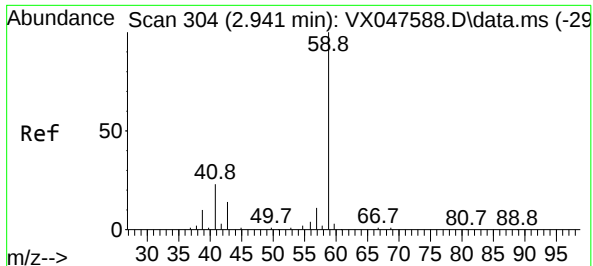

#11
Tert butyl alcohol
Concen: 4.210 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 59 Resp: 891
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

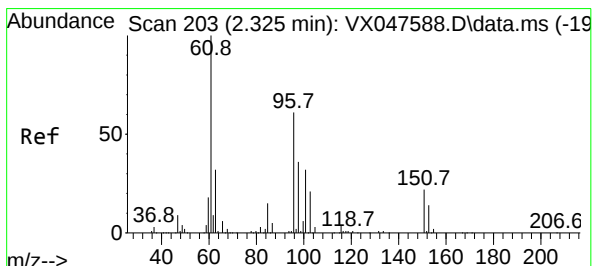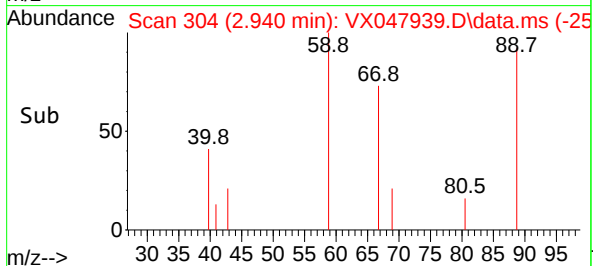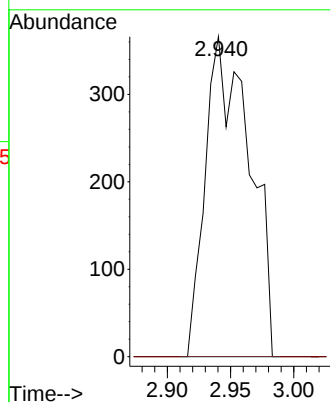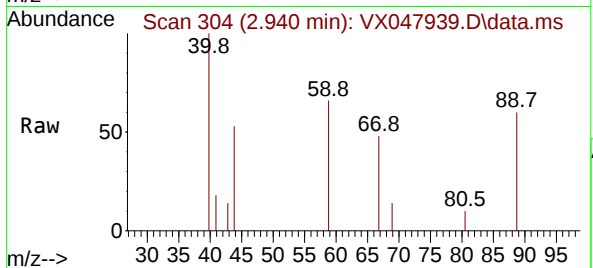

#12
1,1-Dichloroethene
Concen: 0.271 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 96 Resp: 385
Ion Ratio Lower Upper
96 100
61 105.1 131.0 196.6#
98 35.2 47.7 71.5#

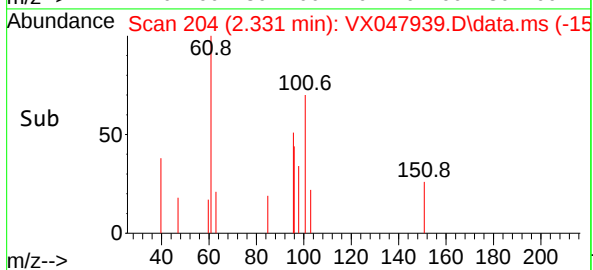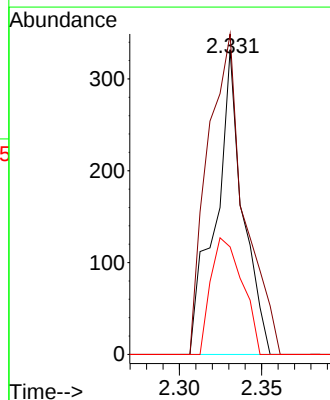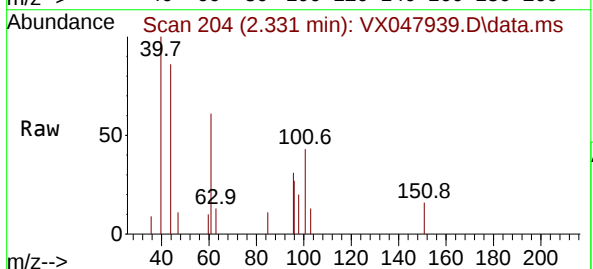

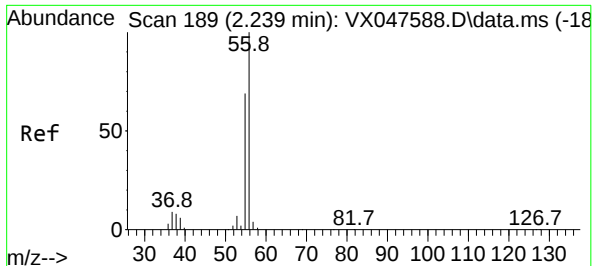

#13

Acrolein

Concen: 0.559 ug/l

RT: 2.245 min Scan# 190

Delta R.T. 0.006 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48

Instrument :

MSVOA_X

ClientSampleId :





TT162S1-20250924

Tgt Ion: 56 Resp: 109

Ion Ratio Lower Upper

56 100

55 0.0 57.2 85.8#

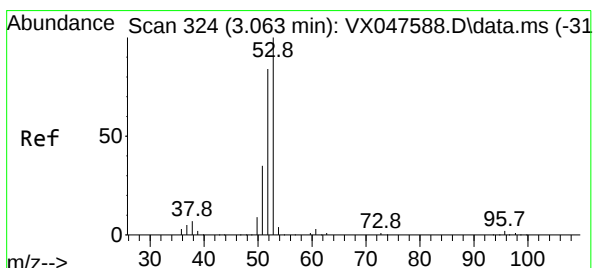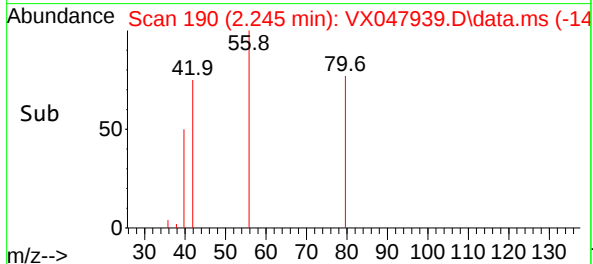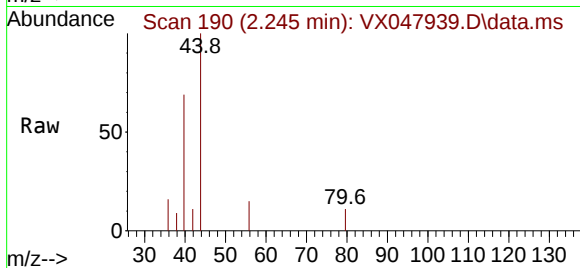

#15

Acrylonitrile

Concen: 0.277 ug/l

RT: 3.068 min Scan# 325

Delta R.T. 0.006 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48




Tgt Ion: 53 Resp: 217


Ion Ratio Lower Upper

53 100

52 76.5 66.4 99.6

51 0.0 29.5 44.3#


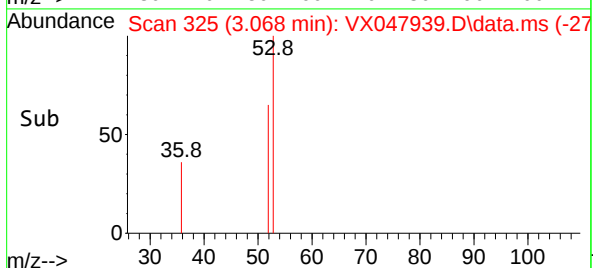

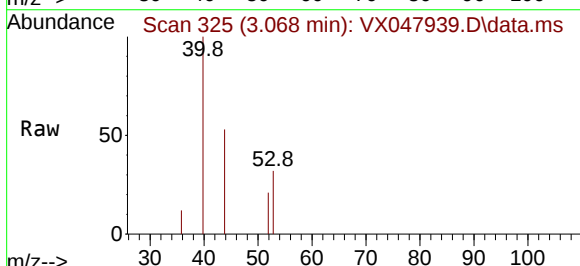




#16
Acetone
Concen: 2.272 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 43 Resp: 1877
Ion Ratio Lower Upper
43 100
58 36.0 23.4 35.0#

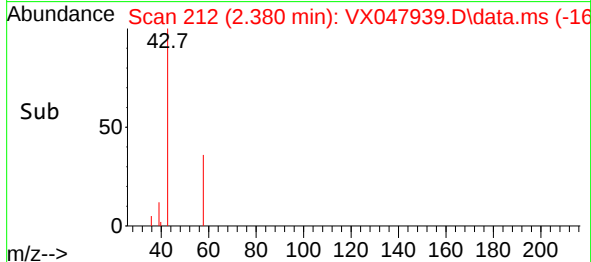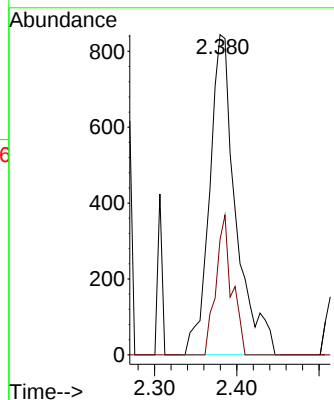

#17
Carbon Disulfide
Concen: 0.237 ug/l
RT: 2.520 min Scan# 235
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 76 Resp: 920
Ion Ratio Lower Upper
76 100
78 0.0 6.8 10.2#


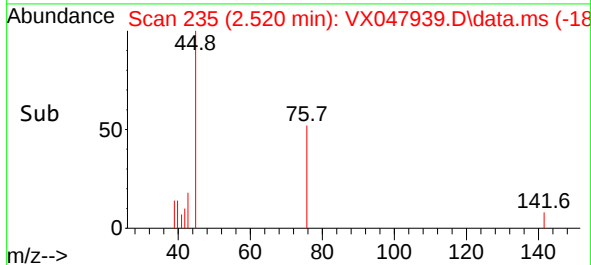
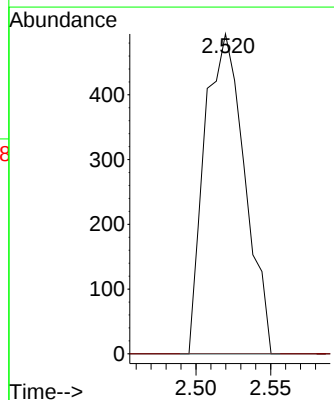





#18
Methyl Acetate
Concen: 0.235 ug/l
RT: 2.703 min Scan# 218
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 43 Resp: 433
Ion Ratio Lower Upper
43 100
74 5.8 17.4 26.2#

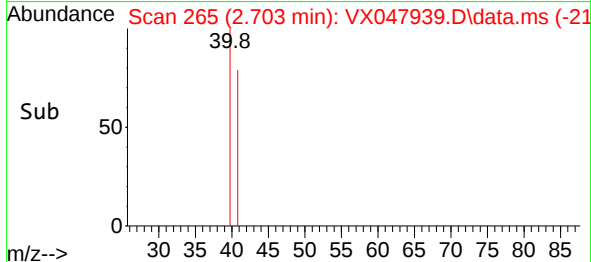

#20
Methylene Chloride
Concen: 0.212 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.012 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 84 Resp: 371
Ion Ratio Lower Upper
84 100
49 96.5 108.6 162.8#
51 25.5 32.6 48.8#
86 0.0 52.0 78.0#




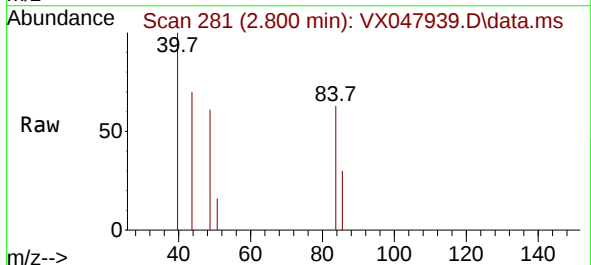




#24
 1,1-Dichloroethane
 Concen: 1.441 ug/l
 RT: 3.605 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VX047939.D
 Acq: 01 Oct 2025 14:48




Instrument :
 MSVOA_X
 ClientSampleId :
 TT162S1-20250924


Tgt Ion: 63 Resp: 4345
 Ion Ratio Lower Upper
 63 100
 98 0.0 3.8 11.2#
 100 3.7 2.3 6.9

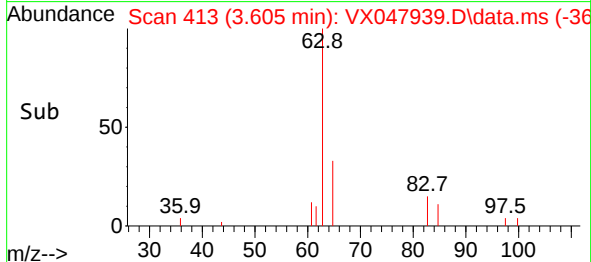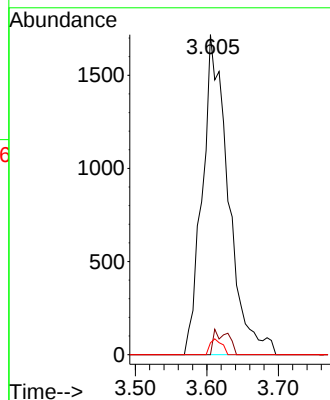

#27
 cis-1,2-Dichloroethene
 Concen: 0.216 ug/l
 RT: 4.483 min Scan# 557
 Delta R.T. -0.000 min
 Lab File: VX047939.D
 Acq: 01 Oct 2025 14:48

Tgt Ion: 96 Resp: 404
 Ion Ratio Lower Upper
 96 100
 61 103.5 0.0 303.2
 98 11.4 0.0 127.8

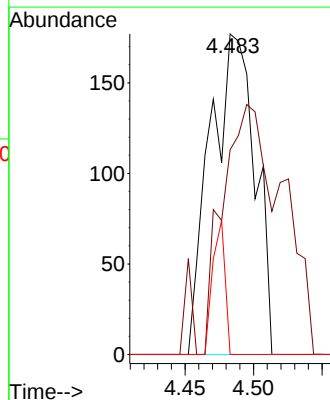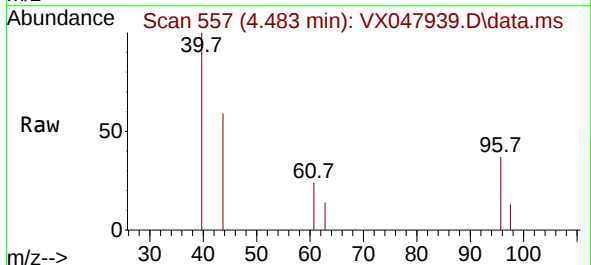



#29

Tetrahydrofuran

Concen: 0.376 ug/l

RT: 5.013 min Scan# 64

Delta R.T. 0.024 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48

Instrument :

MSVOA_X

ClientSampleId :

TT162S1-20250924





Tgt Ion: 42 Resp: 233

Ion Ratio Lower Upper

42 100

72 0.0 34.2 51.2#

71 0.0 31.9 47.9#

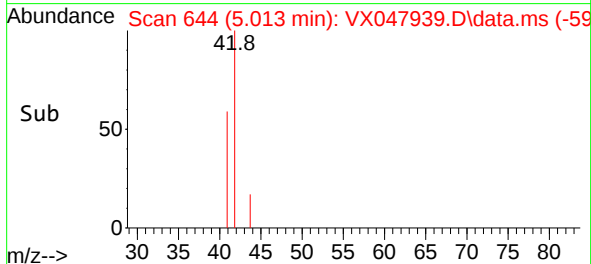

#30

Chloroform

Concen: 0.497 ug/l

RT: 5.086 min Scan# 656

Delta R.T. 0.006 min

Lab File: VX047939.D




Acq: 01 Oct 2025 14:48


Tgt Ion: 83 Resp: 1513

Ion Ratio Lower Upper

83 100

85 71.0 51.8 77.6


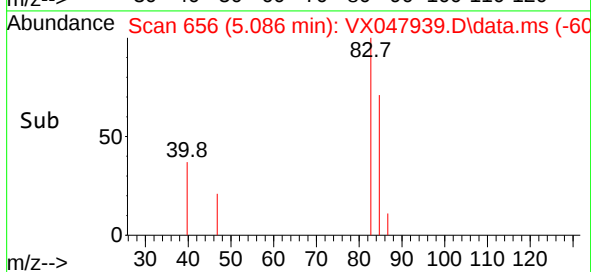






#31
Cyclohexane
Concen: 1.125 ug/l
RT: 5.537 min Scan# 717
Delta R.T. 0.079 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 56 Resp: 2825
Ion Ratio Lower Upper
56 100
69 187.3 23.8 35.8#
84 139.9 64.6 97.0#



#33
1,2-Dichloroethane-d4
Concen: 50.662 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48


Tgt Ion: 65 Resp: 96274
Ion Ratio Lower Upper
65 100
67 52.4 0.0 103.0

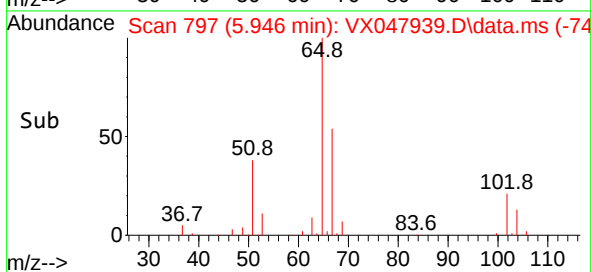






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924







Tgt Ion:114 Resp: 245473
Ion Ratio Lower Upper
114 100
63 21.9 0.0 44.0
88 16.1 0.0 34.2

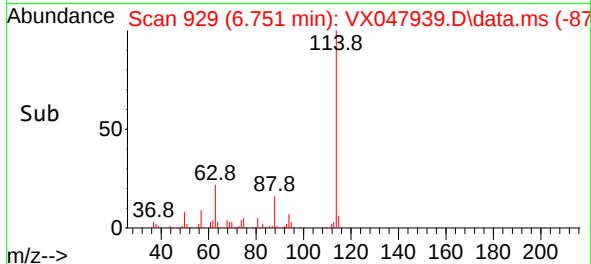

#35
Dibromofluoromethane
Concen: 49.648 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion:113 Resp: 81734
Ion Ratio Lower Upper
113 100
111 100.3 80.9 121.3
192 18.0 14.2 21.4


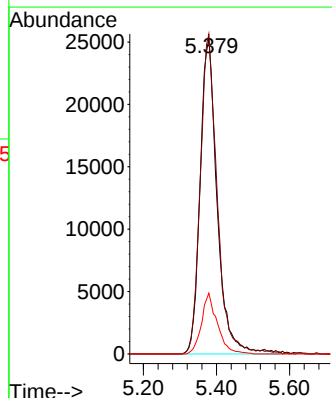
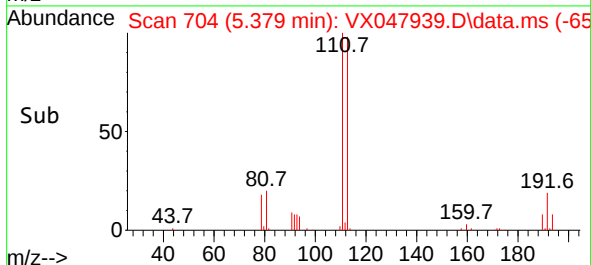
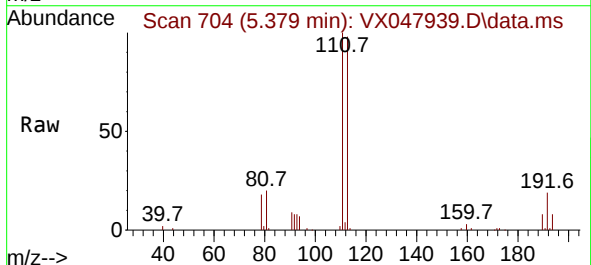




#36
1,1-Dichloropropene
Concen: 4.259 ug/l
RT: 5.537 min Scan# 710
Delta R.T. -0.147 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 75 Resp: 10246
Ion Ratio Lower Upper
75 100
110 9.3 16.7 50.1#
77 0.0 24.3 36.5#

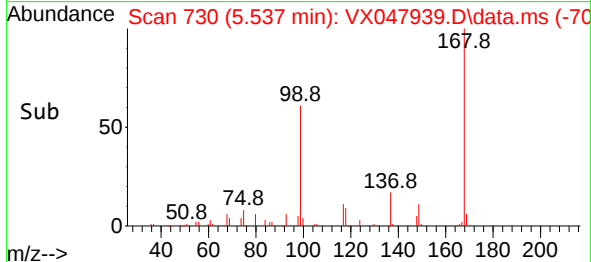

#38
Carbon Tetrachloride
Concen: 4.925 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.128 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 117 Resp: 12873
Ion Ratio Lower Upper
117 100
119 5.6 73.4 110.2#
121 0.0 23.8 35.6#


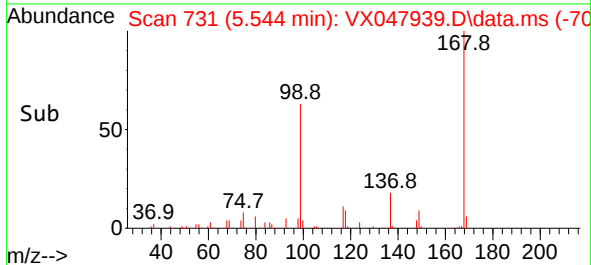






#44
Trichloroethene
Concen: 10.464 ug/l
RT: 7.110 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion:130 Resp: 18483
Ion Ratio Lower Upper
130 100
95 107.3 0.0 210.8

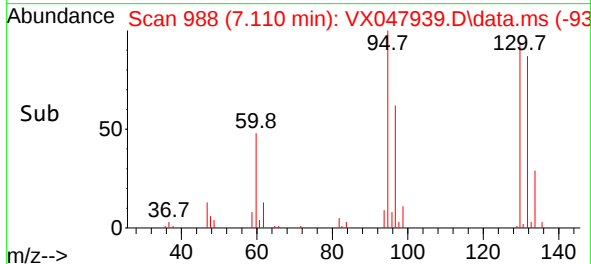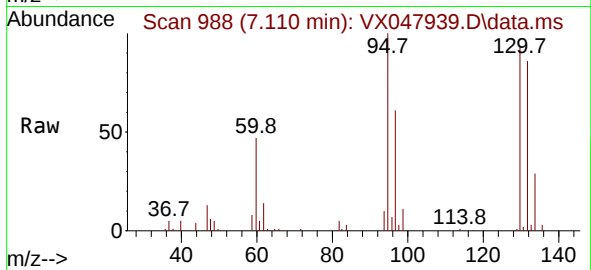

#49
1,4-Dioxane
Concen: 10.769 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. 0.012 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 88 Resp: 229
Ion Ratio Lower Upper
88 100
43 0.0 30.2 45.2#
58 52.8 59.5 89.3#


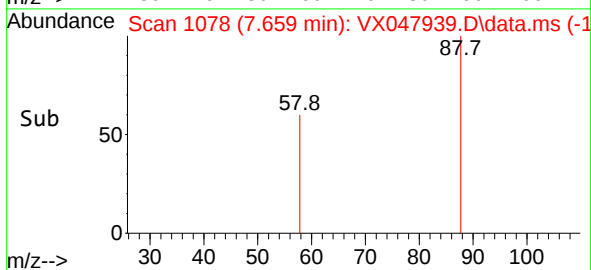






#50
Toluene-d8
Concen: 48.593 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 98 Resp: 276805
Ion Ratio Lower Upper
98 100
100 66.4 53.0 79.4

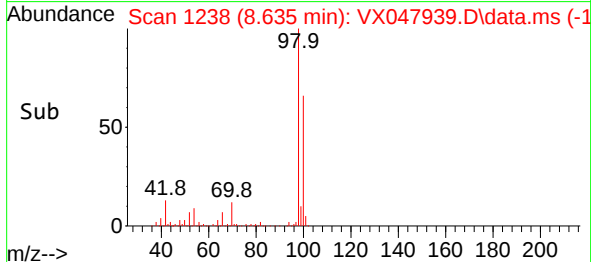

#51
4-Methyl-2-Pentanone
Concen: 0.294 ug/l
RT: 8.567 min Scan# 1227
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 43 Resp: 688
Ion Ratio Lower Upper
43 100
58 11.3 30.3 45.5#




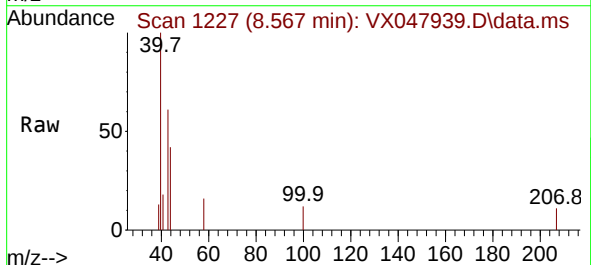




#52
Toluene
Concen: 0.271 ug/l
RT: 8.708 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 92 Resp: 1222
Ion Ratio Lower Upper
92 100
91 186.8 137.1 205.7

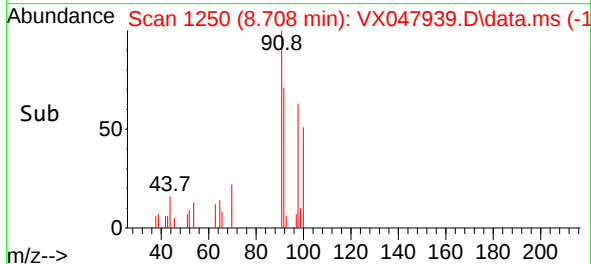

#60
Dibromochloromethane
Concen: 0.460 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. -0.250 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion:129 Resp: 919
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


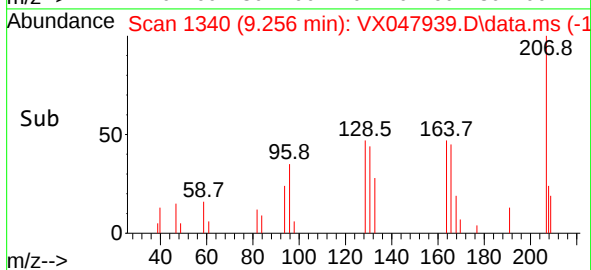




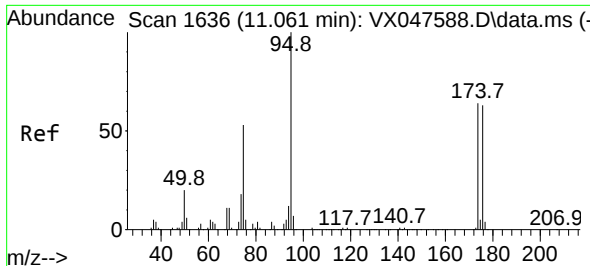

#62
4-Bromofluorobenzene
Concen: 52.213 ug/l
RT: 11.067 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 95 Resp: 112879
Ion Ratio Lower Upper
95 100
174 72.5 0.0 141.6
176 68.6 0.0 138.4

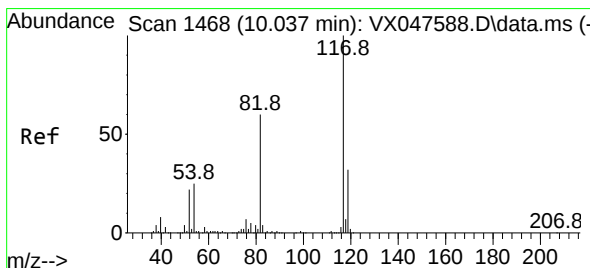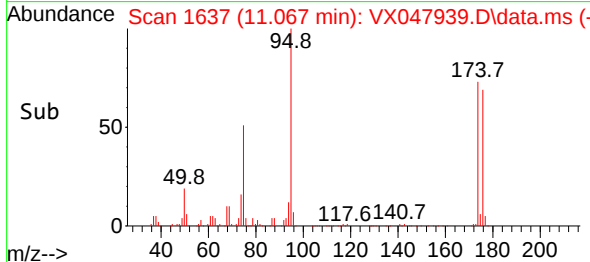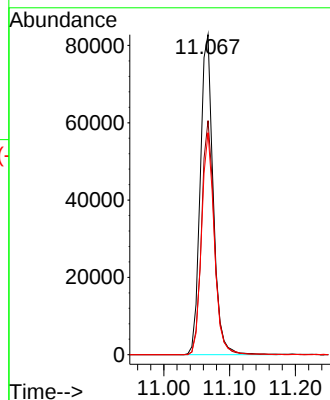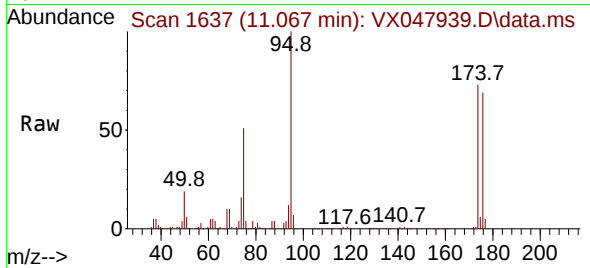

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 117 Resp: 248853
Ion Ratio Lower Upper
117 100
82 56.8 47.8 71.6
119 31.8 25.2 37.8


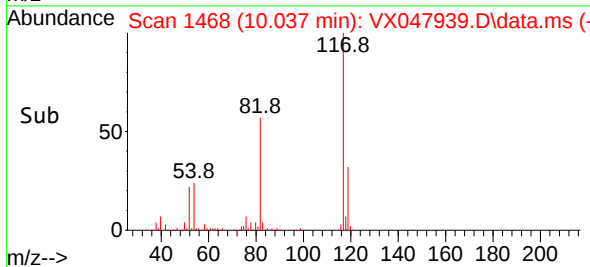
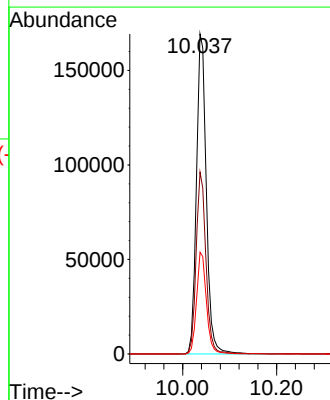
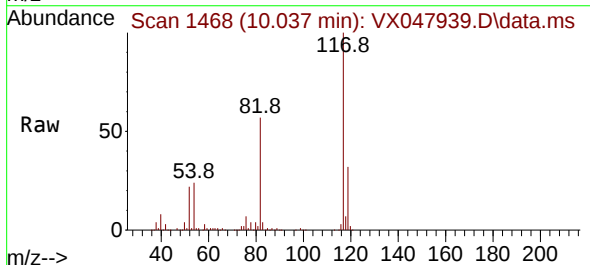




#64
Tetrachloroethene
Concen: 0.526 ug/l
RT: 9.256 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion:164 Resp: 853
Ion Ratio Lower Upper
164 100
166 95.7 100.2 150.2#
129 98.6 81.8 122.6
131 92.0 78.6 118.0

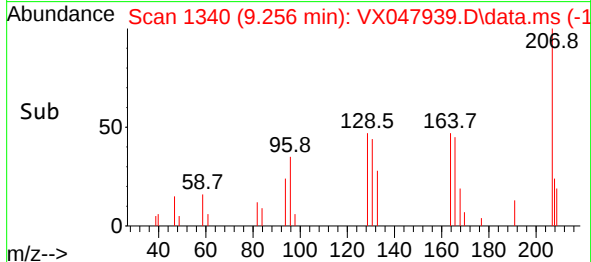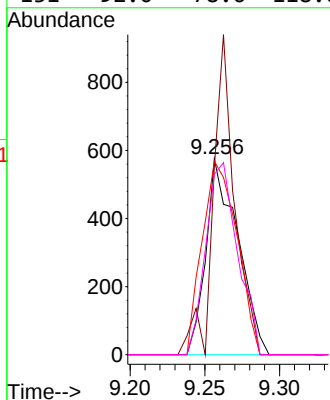

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion:152 Resp: 118778
Ion Ratio Lower Upper
152 100
115 62.3 44.9 134.5
150 156.6 0.0 352.0


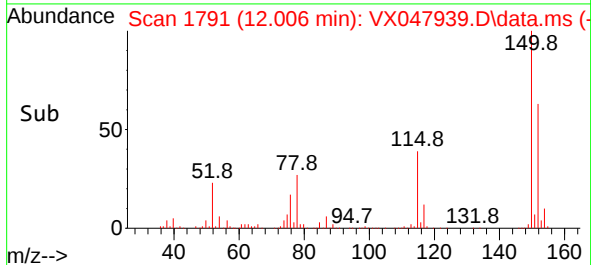
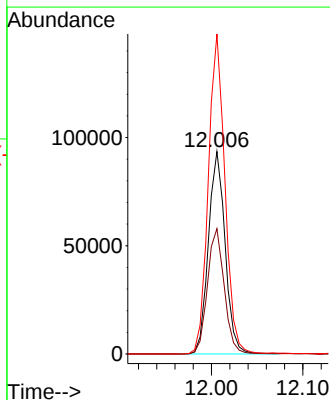





#76
1,2,3-Trichloropropane
Concen: 24.454 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. -0.153 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48




Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924


Tgt Ion: 75 Resp: 58810
Ion Ratio Lower Upper
75 100
77 1.4 18.8 56.4#

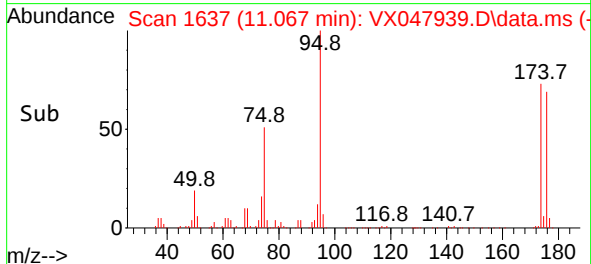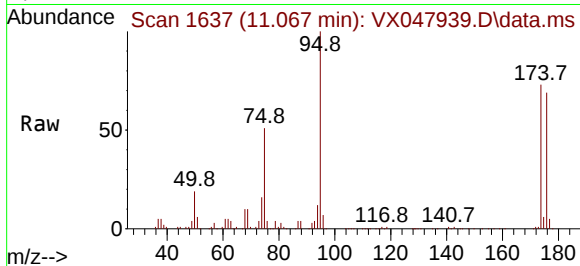

#81
trans-1,4-Dichloro-2-butene
Concen: 62.362 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.067 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion: 75 Resp: 58810
Ion Ratio Lower Upper
75 100
53 0.0 83.4 125.2#
89 0.0 36.3 54.5#

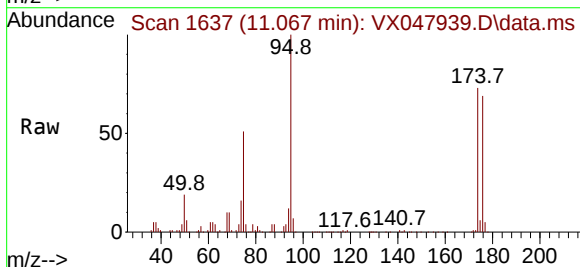



#86

p-Isopropyltoluene

Concen: 0.221 ug/l

RT: 11.994 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX047939.D


Acq: 01 Oct 2025 14:48

Instrument :

MSVOA_X

ClientSampleId :

TT162S1-20250924






Tgt Ion:119 Resp: 1688

Ion Ratio Lower Upper

119 100

134 27.8 12.6 37.8

91 44.1 12.6 37.6#



#89

n-Butylbenzene

Concen: 0.296 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. 0.006 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48




Tgt Ion: 91 Resp: 2095


Ion Ratio Lower Upper

91 100

92 55.5 27.6 82.7

134 25.7 12.6 37.8

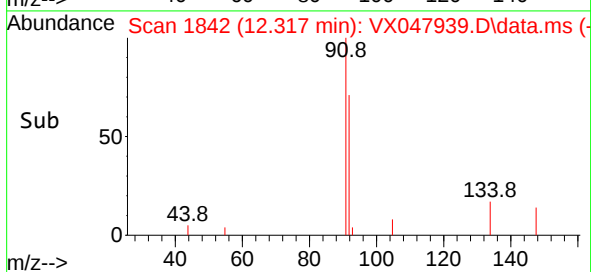



#93

1,2,4-Trichlorobenzene

Concen: 0.414 ug/l

RT: 13.573 min Scan# 2047

Delta R.T. 0.006 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48

Instrument :

MSVOA_X

ClientSampleId :

TT162S1-20250924





Tgt Ion:180 Resp: 1060

Ion Ratio Lower Upper

180 100

182 87.5 46.6 139.8

145 28.0 16.4 49.1

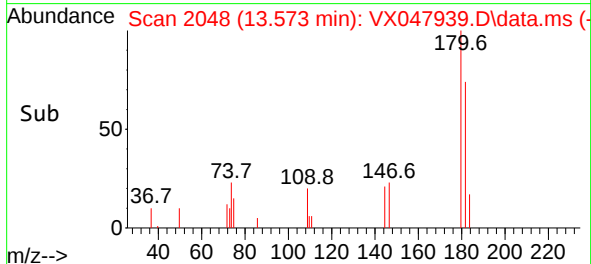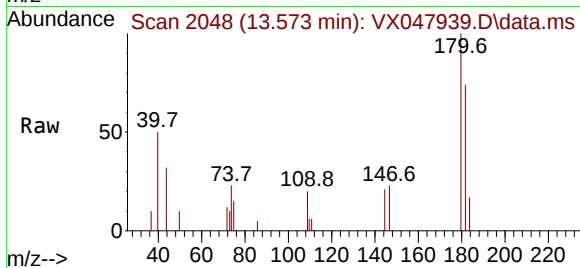

#94

Hexachlorobutadiene

Concen: 1.171 ug/l

RT: 13.707 min Scan# 2070

Delta R.T. -0.000 min

Lab File: VX047939.D

Acq: 01 Oct 2025 14:48




Tgt Ion:225 Resp: 1017


Ion Ratio Lower Upper

225 100

223 65.2 31.7 95.1

227 66.0 32.0 96.0




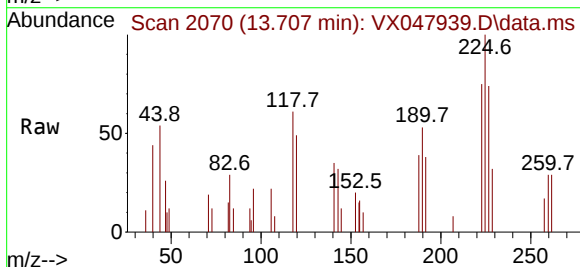




#95
Naphthalene
Concen: 0.329 ug/l
RT: 13.762 min Scan# 2078
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Instrument :
MSVOA_X
ClientSampleId :
TT162S1-20250924

Tgt Ion:	128	Resp:	2561
Ion Ratio	Lower	Upper	
128	100		
127	12.5	10.2	15.2
129	9.4	8.8	13.2



#96
1,2,3-Trichlorobenzene
Concen: 0.454 ug/l
RT: 13.945 min Scan# 2109
Delta R.T. 0.006 min
Lab File: VX047939.D
Acq: 01 Oct 2025 14:48

Tgt Ion:	180	Resp:	1081
Ion Ratio	Lower	Upper	
180	100		
182	87.6	47.6	142.8
145	31.5	17.9	53.7

